



SPECTRUM
INSTRUMENTATION

Perfect fit – modular designed solutions



M4i.23xx-x8

M4x.23xx-x4

**high-speed 7bit bit transient recorder,
A/D converter board
for PCI Express bus and PXI Express bus**

valid for all versions

**Hardware Manual
Software Driver Manual**

Latest revision: 23. April 2026

Digitizers | Transient Recorders | Arbitrary Waveform Generators | Digital Waveform Acquisition Cards
for PCI Express, PXI Express and LXI / Ethernet

(c) SPECTRUM INSTRUMENTATION GMBH
AHRENSFELDER WEG 13-17, 22927 GROSSHANS DORF, GERMANY

SBench, digitizerNETBOX, generatorNETBOX and hybridNETBOX are registered trademarks of Spectrum Instrumentation GmbH.
Microsoft, Visual C++, Windows, Windows 98, Windows NT, Windows 2000, Windows XP, Windows Vista, Windows 7, Windows 8, Windows 10, Windows 11 and Windows Server are trademarks/registered trademarks of Microsoft Corporation.
LabVIEW, DASyLab, Diadem and LabWindows/CVI are trademarks/registered trademarks of National Instruments Corporation.
MATLAB is a trademark/registered trademark of The Mathworks, Inc.
Delphi and C++Builder are trademarks or registered trademarks of Embarcadero Technologies, Inc.
Keysight VEE, VEE Pro and VEE OneLab are trademarks/registered trademarks of Keysight Technologies, Inc.
FlexPro is a registered trademark of Weisang GmbH & Co. KG.
PCIe, PCI Express, PCI-X and PCI-SIG are trademarks of PCI-SIG.
PICMG and CompactPCI are trademarks of the PCI Industrial Computer Manufacturers Group.
PXI is a trademark of the PXI Systems Alliance.
LXI is a registered trademark of the LXI Consortium.
IVI is a registered trademark of the IVI Foundation.
Oracle and Java are registered trademarks of Oracle and/or its affiliates.
Python is a trademark/registered trademark of Python Software Foundation.
Julia is a trademark/registered trademark of Julia Computing, Inc.
Intel and Intel Core i3, Core i5, Core i7, Core i9 and Xeon are trademarks and/or registered trademarks of Intel Corporation.
AMD, Opteron, Sempron, Phenom, FX, Ryzen and EPYC are trademarks and/or registered trademarks of Advanced Micro Devices.
Arm is a trademark or registered trademark of Arm Limited (or its subsidiaries).
NVIDIA, CUDA, GeForce, Quadro, Tesla and Jetson are trademarks and/or registered trademarks of NVIDIA Corporation.

Table of Contents

Table of Contents.....	3
Safety Instructions	10
Symbols and Safety Labels	10
General safety information	10
Requirements for users and duties for operators.....	10
General safety at work.....	10
Bringing the product into service	11
Intended use	11
Application area of the product.....	11
Requirements for the technical state of the product	11
Requirements for operation	11
Electrical safety and power supply.....	11
Requirements for the location	11
Requirements on the ventilation	11
Maintenance.....	11
Repair/Service.....	12
Cleaning the module housing (NETBOX devices, cables, amplifiers, systems only)	12
Opening the module (NETBOX devices, amplifiers only).....	12
Dismounting parts of the card (instrument card only)	12
Markings and Labelling.....	12
Packing list.....	13
PCIe (PCI Express) cards M4i.xxxx	13
PXIe (PXI Express) cards M4x.xxxx.....	13
Introduction.....	14
Preface	14
Overview	14
M4i cards for PCIe Express (PCIe)	14
M4x cards for PXI Express (PXIe)	14
General Information	15
Different models of the M4i.23xx series	16
Different models of the M4x.23xx series	17
Additional options.....	18
Star-Hub (M4i only)	18
Digital I/O with Dig-SMA (M4i.44xx only)	18
The Spectrum type plate	19
Hardware information.....	20
Block Diagrams.....	20
Technical Data	21
Dynamic Parameters	23
RMS Noise Level (Zero Noise).....	24
M4i Specific Technical Data	24
M4x specific Technical Data	25
Order Information	27
M4i Order Information	27
M4x Order Information	28
Hardware Installation	29
ESD Precautions	29
Sources of noise.....	29
Cooling Precautions.....	29
Connector Handling Precautions	29
M4i PCIe Cards	30
System Requirements.....	30
Installing the M4i board in the system	30
Additional notes on PCIe x16 slot retention.....	31
Providing additional power to M4i.xxxx-x8 cards.....	31
Installing a M4i.44xx board with digital inputs/outputs mounted on an extra bracket	31
Installing multiple boards synchronized by star-hub option	32
Shipment of systems with Spectrum cards installed.....	33
M4x PXIe Cards.....	33
System Requirements.....	33
Installing the M4x board in the system	33

Software Driver Installation and Driver Update.....	34
Windows	34
Before initial installation	34
Running the driver Installer/Update.....	34
After installation	35
Linux.....	36
Overview	36
Driver Installation with Installation Script.....	36
Standard Driver Update	37
Compilation of kernel driver sources (optional and local cards only)	37
Update of a self compiled kernel driver	37
Installing the library only without a kernel (for remote devices)	38
Installation from Spectrum Repository	38
Control Center	39

Software	41
Software Overview	41
Card Control Center	41
Discovery of Remote Cards, digitizerNETBOX/generatorNETBOX/hybridNETBOX products	42
Enter IP Address of digitizerNETBOX/generatorNETBOX/hybridNETBOX manually	42
Wake On LAN of digitizerNETBOX/generatorNETBOX/hybridNETBOX	42
Netbox Monitor	43
Device identification	43
Hardware information	44
Firmware information	44
Software License information	45
Driver information	45
Installing and removing Demo cards	46
Feature upgrade	46
Software license upgrade	46
Performing card calibration	46
Performing memory test	47
Transfer speed test	47
Debug logging for support cases	48
Device mapping	48
Firmware upgrade	49
Firmware switch	49
Accessing the hardware with SBench 6	50
Accessing the hardware with DDS Control (DDS firmware required)	51
C/C++ Driver Interface	51
Header files	52
General Information on Windows 64 bit drivers	52
Microsoft Visual C++ 6.0, 2005 and newer 32 Bit	52
Microsoft Visual C++ 2005 and newer 64 Bit	52
Linux Gnu C/C++ 32/64 Bit	53
C++ for .NET	53
Other Windows C/C++ compilers 32 Bit	53
Other Windows C/C++ compilers 64 Bit	53
Driver functions	53
.....	58
Delphi (Pascal) Programming Interface	58
Driver interface	58
Examples	60
.NET programming languages	61
Library	61
Declaration	61
Using C#	61
Using Managed C++/CLI	63
Using VB.NET	63
Using J#	63
Python Programming Interface and Examples	64
High-level object oriented Python package spcm	64
Low-level driver interface	64
Examples	65
Java Programming Interface and Examples	65
Driver interface	65
Examples	66
Julia Programming Interface and Examples	66
Driver interface	66
Examples	67
LabVIEW driver and examples	67
MATLAB driver and examples	67
SCAPP – CUDA GPU based data processing	68

Programming the Board	69
Overview	69
Register tables	69
Programming examples.....	69
Initialization.....	70
Initialization of Remote Products	70
Error handling.....	71
Printing custom strings to the driver debug log	71
Gathering information from the card.....	72
Card type.....	72
Hardware and PCB version	72
Reading currently used PXI slot No. (M4x only)	73
Firmware versions.....	73
Production date.....	74
Last calibration date (A/D and D/A cards only)	74
Serial number	74
Maximum possible sampling rate	74
Installed memory	74
Installed features and options	75
Miscellaneous Card Information	76
Function type of the card	76
Used type of driver	76
Custom modifications	77
Reset.....	77
Analog Inputs.....	79
Channel Selection	79
Important note on channel selection	80
Setting up the inputs	80
Input ranges.....	80
Input offset.....	81
AC/DC offset compensation	82
Read out of input features	82
Input coupling	83
Anti aliasing filter (Bandwidth limit).....	83
Automatic on-board calibration of the offset and gain settings	83
Acquisition modes	85
Overview	85
Setup of the mode	85
Commands.....	86
Card Status.....	88
Acquisition cards status overview	88
Generation card status overview	88
Data Transfer	88
Standard Single acquisition mode	91
Card mode.....	91
Memory, Pre- and Posttrigger	91
.....	92
Example	92
FIFO Single acquisition mode	92
Card mode.....	92
Length and Pretrigger	92
Difference to standard single acquisition mode.....	92
Example FIFO acquisition	93
Limits of pre trigger, post trigger, memory size	93
Buffer handling	94
Data organization	98
Sample format.....	98
Converting ADC samples to voltage values	98
Enabling hardware sample conversion to offset-binary	99

Clock generation	100
Overview	100
Clock Mode Register	100
The different clock modes	100
Details on the different clock modes	101
Programming the sampling rate	101
Standard internal sampling clock (PLL)	101
Using Quartz2 with PLL (optional, M4i cards only)	102
Oversampling	102
External clock (reference clock)	102
PXI Reference Clock (M4x cards only)	103
Trigger modes and appendant registers	105
General Description	105
Trigger Engine Overview	105
Trigger masks	106
Trigger OR mask	106
Trigger AND mask	107
Combining multiple trigger sources by OR/AND masks	108
Software trigger	109
Force- and Enable trigger	109
Trigger delay	110
Trigger Counter	110
Main external window trigger (Ext0/Trg0)	111
Trigger Mode	111
Trigger Input Termination	111
Trigger Input Coupling	112
Secondary external level trigger (Ext1/Trg1)	112
Trigger Mode	112
Trigger level	112
Detailed description of the external analog trigger modes	113
Channel Trigger	117
Overview of the channel trigger registers	117
Channel trigger level	118
Detailed description of the channel trigger modes	119
PXI Trigger (M4x PXIe cards only)	126
PXI Trigger Mode Registers	126
PXI Trigger Sources within the Trigger Masks	127
PXI Trigger Setup Example	128
Multi Purpose I/O Lines	129
On-board I/O lines (X0, X1, X2)	129
Programming the behavior	129
Using asynchronous I/O	130
Special behavior of trigger output	130
Synchronous digital inputs	131
Mode Multiple Recording	132
Recording modes	132
Standard Mode	132
FIFO Mode	132
Limits of pre trigger, post trigger, memory size	133
Multiple Recording and Timestamps	134
Trigger Modes	134
Programming examples	135
Mode Gated Sampling	136
Acquisition modes	136
Standard Mode	136
FIFO Mode	136
Limits of pre trigger, post trigger, memory size	137
Gate-End Alignment	138
Gated Sampling and Timestamps	138
Trigger	139
Detailed description of the external analog trigger modes	139
Channel triggers modes	143
Programming examples	148

Timestamps	149
General information	149
Example for setting timestamp mode:	150
Timestamp modes.....	150
Standard mode	150
StartReset mode.....	150
Refclock mode.....	151
Reading out the timestamps	152
General.....	152
Data Transfer using DMA	153
Data Transfer using Polling	154
Comparison of DMA and polling commands.....	155
Data format	155
Combination of Memory Segmentation Options with Timestamps	157
Multiple Recording and Timestamps	157
Gate-End Alignment.....	157
Gated Sampling and Timestamps	158
ABA Mode and Timestamps.....	159
ABA mode (dual timebase)	160
General information	160
Standard Mode.....	160
FIFO Mode	161
Limits of pre trigger, post trigger, memory size	161
Example for setting ABA mode:	162
Reading out ABA data	162
General.....	162
Data Transfer using DMA	163
Data Transfer using Polling	165
Comparison of DMA and polling commands.....	166
ABA Mode and Timestamps.....	166
Option Remote Server	168
Introduction	168
Installing and starting the Remote Server	168
Windows	168
Linux	168
Detecting the digitizerNETBOX/generatorNETBOX/hybridNETBOX	168
Discovery Function.....	168
Finding the digitizerNETBOX/generatorNETBOX/hybridNETBOX in the network	169
Troubleshooting.....	170
Accessing remote cards	170
Pulse Generator (Firmware Option)	171
General Information	171
Principle of Operation.....	172
Setting up the Pulse Generator	173
Enabling, disabling and resetting a pulse generator.....	173
Defining the basic pulse parameters.....	173
Delaying (phase shifting) the Outputs	174
Defining the trigger behavior	174
Configuring the pulse generator's trigger source.....	175
Configuring Multi Purpose lines to output generated pulses	177
Programming Example	178
Option Star-Hub (M3i and M4i only)	179
Star-Hub introduction	179
Star-Hub trigger engine	179
Star-Hub clock engine	179
Software Interface	179
Star-Hub Initialization.....	179
Setup of Synchronization	181
Setup of Trigger	182
Run the synchronized cards	182
SH-Direct: using the Star-Hub clock directly without synchronization	183
Error Handling	184

Mode Block Average (Firmware Option)	185
Overview	185
General Information	185
Principle of operation	185
Simplified Block Diagram	186
Setting up the Acquisition	186
Recording modes	186
Standard Mode	186
FIFO Mode	187
Limits of pre trigger, post trigger, memory size	187
For cards with 12bit, 14bit and 16bit ADC resolution (firmware V14 and above):	188
For cards with 8bit ADC resolution, 32 bit data mode (firmware V14 and above):	188
For cards with 8bit ADC resolution, 16 bit data mode (firmware V14 and above):	188
Trigger Modes	188
Output Data Format	188
Data organization	189
Programming examples	189
Mode Block Statistics (Firmware Option)	190
Overview	190
General Information	190
Waveform Block Statistics	190
Simplified Block Diagram	191
Setting up the Acquisition	191
Recording modes	191
Standard Mode	191
FIFO Mode	192
Limits of pre trigger, post trigger, memory size	192
For cards with 12bit, 14bit and 16bit ADC resolution:	193
For cards with 8bit ADC resolution:	193
Trigger Modes	193
Information Set Format	193
Data organization	193
Programming examples	194
Appendix	195
Error Codes	195
Spectrum Knowledge Base	196
Temperature sensors	197
Temperature read-out registers	197
Temperature hints	197
23xx temperatures and limits	197
Details on M4i/M4x cards I/O lines	198
Multi-Purpose I/O Lines	198
Interfacing with clock input	198
Interfacing with clock output	198
Details on M4i/M4x cards status LED	200
Turning on card identification LED	200
Continuous memory for increased data transfer rate	201
Background	201
Setup on Linux systems	202
Setup on Windows systems	203
Usage of the buffer	203
List Of Figures	205
List Of Tables	207

Safety Instructions

This chapter contains information about the following topics:

- General safety information
- Requirements for users and duties for operators
- Intended use
- Markings and Labelling

Symbols and Safety Labels

Table 1: Symbols and Safety Labels

Label	Where	Description
	Cards	ESD symbol Parts can be damaged by electrostatic discharge. Follow these precautions: Avoid touching pins, leads, or circuitry. Always be properly grounded when touching a static-sensitive component or assembly.
	NETBOX chassis	GND symbol To enhance the immunity of the equipment against conducted and radiated RF disturbance, sensitive electrical circuits are connected to the chassis.
		Protective Conductor Class I This movable devices of protection class I is equipped with a cable with additional protective conductor and a protective contact plug. The device may only be connected to the protective conductor system of the fixed electrical installation, which is at ground potential.
	Products	Labelling for CE conformity Spectrum confirms with the CE marking affixed to the product or its packaging that the product complies with the product-specific applicable European directives. The CE declaration of conformity for the product is available upon request.
	Products	Labelling for WEEE The WEEE symbol on the product or its packaging indicates that the product must not be disposed of with other waste. The user is obliged to collect the old devices separately and to make them available to the WEEE take-back system for recycling.
	NETBOX chassis	Labelling for battery disposal Batteries must not be disposed of with household waste. You are legally obliged to return old batteries so that proper disposal can be guaranteed. You can dispose of used batteries at a municipal collection point or in local stores
	Manual	Important part of the manual with safety related content
	Manual	Additional information inside the manual which helps to understand a topic in more detail

General safety information

Carefully read the documentation (Installation manual and hardware manual) that belongs to the product prior to the start-up. Please observe the product safety instructions and the following safety notices to avoid health issues or damage to the device.

The manufacturer does not assume any liability for damages resulting from improper handling, unintended use or non-observance of the safety precautions.

Applicable regulations and laws governing the location and use of the product must be observed and all accident prevention and occupational safety regulations must be complied with.

Requirements for users and duties for operators

The product may be assembled, operated and maintained only if you have the necessary qualification and experience for this product. Improper use or use by a user without sufficient qualification can lead to damages or injuries to one's health or damages to property. The assembler of the system is responsible for the safety of any system incorporating the equipment.

General safety at work

The existing regulations for safety at work and accident prevention must be followed. All applicable regulations and statutes regarding operation must be strictly followed when using this product.

Bringing the product into service

The following steps need to be done when first bringing the product into service:

- Please check the content of the delivery against the above stated packing list upon first opening of the package
- Check the products before connecting them to any power source for any damages. Do not connect a damaged product to any power source
- Be sure to have the correct knowledge to install this product
- Carefully read the installation manual and take the stated precautions
- Follow the installation process step by step as described in this manual
- The product relies on proper cooling as described in this manual. Make sure to avoid to restrict the airflow to any part. Do not cover or block any cooling fans or cooling vents.

Intended use

Application area of the product

The device has been developed for indoor use in controlled laboratory and industrial environments not exceeding an operating height of 2000 m and for an ambient temperature of 0°C to +40°C with non-condensing humidity up to 10% to 90%.

Requirements for the technical state of the product

The product is designed in accordance with state-of-the-art technology and recognized safety rules. The product may be operated only in a technically flawless condition and according to the intended purpose and with regard to safety and dangers as stated in the respective product documentation. If the product is not used according to its intended purpose, the protection of the product may be impaired.

Requirements for operation

Use the product only according to the specifications in the corresponding User's Guide. With any deviating operation, the product safety is no longer ensured.

The use of the product is permitted only in accordance with the specifications and information of the respective user manual. Product safety is not guaranteed in the event of deviating use. Use in wet or humid environments or in potentially explosive areas is not permitted.

The installer is responsible for the safety of the system in which the device is installed.

Electrical safety and power supply

Observe the regulations applicable at the operating location concerning electrical safety as well as the laws and regulations concerning work safety! Connect only current circuits with safety extra-low voltage in accordance with EN 61140 (degree of protection III) to the connections of the module.

Ensure that the connection and setting values are being followed (see the information in the chapter "Technical data"). Do not apply any voltages to the connections of the module that do not correspond to the specifications of the respective connection. When setting up the appliance, care must be taken to ensure that the power plug of the chassis is easily accessible and the power cable can be unplugged in the event of an emergency shut-down.

Use only approved cables at the connections of the product. Adhere to the maximum permissible cable lengths! Do not use any damaged cables! Never apply force to insert a plug into a socket. Ensure that there is no contamination in and on the connection, that the plug fits the socket, and that you correctly aligned the plugs with the connection.

There is no danger from the device in case of power supply interruption or shut down.

Requirements for the location

The housing and the connectors of the module as well as the plug connectors of the cables meet the degree of protection IP20. Position the module on a smooth, level and solid underground. The module or the module stack must always be securely fastened.

The functionality and safety of the device is only guaranteed at operation conditions of IP20 and contamination class II up to a light contamination by non-conductive materials.

Requirements on the ventilation

Keep the module away from heat sources and protect it against direct exposure to the sun. The free space above and behind the module must be selected so that sufficient air circulation is ensured. During normal operation there are no hot surfaces that pose any danger to the operator.

Maintenance

The product is maintenance-free.

Repair/Service

In the event of a necessary repair, the product must be returned to the manufacturer. Before returning any good get in contact with the support group and obtain a RMA code. The support group can be reached by email: Support@spec.de

Please ensure suitable packaging to avoid damage during transport.

World-wide service address is:

Spectrum Instrumentation GmbH
Ahrensfelder Weg 13-17
22927 Grosshansdorf
Germany

Cleaning the module housing (NETBOX devices, cables, amplifiers, systems only)

Use a dry or lightly moistened, soft cloth for cleaning the module housing. Do not use any sprays, solvents or abrasive cleaners which could damage the housing. Ensure that no moisture enters the housing. Never spray cleaning agents directly onto the module.

Opening the module (NETBOX devices, amplifiers only)

Do not open or change the module housing! Work on the module housing may only be performed by the manufacturer.

Dismounting parts of the card (instrument card only)

Do not dismount any part of the card like modules, front plates or internal cable connections.

Markings and Labelling

The product complies with the current European directives on CE marking. A CE declaration of conformity is available on request.

The product complies with the current European Directives on the Use of Certain Hazardous Substances (RoHS-3) 2015/863/EU).

According to the European directive WEEE (Waste Electrical and Electronic Equipment), the user is obliged to return the product to the system for collection, treatment and recycling of waste electronic equipment. Disposal via residual waste is not permitted.

Up-to-date information on notifiable substances according to REACH regulation (EC) No 1907 /2006 can be quoted on request.

Packing list

The following items are containing in the packing. Some of these items need to be ordered separately as an option.

PCIe (PCI Express) cards M4i.xxxx

Table 2: Packing List M4i card (PCI Express)

Item	Contained	Description
Card	Yes	Ordered card type inside ESD safety bag
Star-Hub M4i.xxxx-SH8ex, -SH8tm	Optional	Star-Hub mounted on card, containing 8 sync-cables
Digital Option M4i.44xx-DigSMB	Optional (M4i.44xx only)	Digital option, mounted on card
Manual	Yes	Printed Installation Manual
USB Stick	Yes	Containing drivers, software and programming manuals
Cables	Optional	Ordered cables, each packed in own bag

PXIe (PXI Express) cards M4x.xxxx

Table 3: Packing List M4x card (PXI Express)

Item	Contained	Description
Card	Yes	Ordered card type inside ESD safety bag
Manual	Yes	Printed Installation Manual
USB Stick	Yes	Containing drivers, software and programming manuals
Cables	Optional	Ordered cables, each packed in own bag

Introduction

Preface

This manual provides detailed information on the hardware features of your Spectrum board. This information includes technical data, specifications, block diagram and a connector description.

In addition, this guide takes you through the process of installing your board and also describes the installation of the delivered driver package for each operating system.

Finally this manual provides you with the complete software information of the board and the related driver. The reader of this manual will be able to integrate the board in any PC system with one of the supported bus and operating systems.

Please note that this manual provides no description for specific driver parts such as those for IVI, LabVIEW or MATLAB. These driver manuals are available on USB-Stick or on the Spectrum website.

For any new information on the board as well as new available options or memory upgrades please contact our website www.spectrum-instrumentation.com. You will also find the current driver package with the latest bug fixes and new features on our site.

Please read this manual carefully before you install any hardware or software. Spectrum is not responsible for any hardware failures resulting from incorrect usage.



Overview

M4i cards for PCIe Express (PCIe)



The M4i generation is the fast streaming and high performance platform from Spectrum. The 3/4 length cards are available in different speed grades and resolutions with best performance.

The cards have been optimized for extremely fast data transfer and allow to read data for online analysis or offline storage with more than 3 GB/s using the PCI Express x8 Gen 2 bus interface. Mechanically the card family needs x8 or x16 lane PCI Express connectors with any PCI Express generation. Electrically the card can handle smaller number of PCI Express lanes with reduced transfer speed.



When using high sampling rates the 4 GiByte standard on-board memory (2 GiSamples for cards with 12/14/16 bit resolution) is sufficient to acquire up to several seconds of high-speed data. The M4i cards are carefully designed and offer an optimized clock section, a wide range of trigger possibilities, new and improved features, easy usability and programming as well as an outstanding software support.

The PCI Express bus was first introduced in 2004. In today's standard PC there are usually two to six slots available for instrumentation boards. Special industrial PCs offer up to a maximum of 16 slots. The PCI Express Gen2 standard theoretically delivers up to 8 GByte/s data transfer rate per x16 slot. The Spectrum M4i boards are available as PCI Express x8 (eight lane) Gen2, 3/4 length card.

Within this document the name M4i or M4i.xxxx is used as a synonym for the PCI Express version with the full name of M4i.xxxx-x8 to enhance readability. The exact order information can be found in the related passage in this manual.



M4x cards for PXI Express (PXIe)



The M4x platform takes the features of the M4i series of PCIe cards to an industrial bus standard. The 3U two slot cards are available in different speed grades and resolutions with best performance.

Based on Spectrums proven M4i series of PCIe products the new M4x PXIe modules deliver the same advanced features and signal quality.

It also allows the new modules to share a common software interface and offer the same FPGA based averaging and statistics options.



Compared to PCIe, PXIe systems come with superior mechanical design, better connectors and a defined air flow for cooling. This makes it the ideal platform for many industrial and mobile applications.



The M4x cards have been optimized for extremely fast data transfer and allow to read data for online analysis or offline storage with more than 1.5 GB/s using the PCI Express x4 Gen 2 bus interface.

When using high sampling rates the 4 GiByte standard on-board memory (2 GiSamples for cards with 12/14/16 bit resolution) is sufficient to acquire up to several seconds of high-speed data. The M4x cards are carefully designed and offer an optimized clock section, a wide range of trigger possibilities, new and improved features, easy usability and programming as well as an outstanding software support.

Within this document the name M4x or M4x.xxxx is used as a synonym for the PXI Express version with the full name of M4x.xxxx-x4 to enhance readability. The exact order information can be found in the related passage in this manual.



General Information

The M4i.23xx and M4x.23xx is best suitable for applications that need ultra high sample rates as well as a high input bandwidth. All six models are available with 1.5 GHz bandwidth .

On the M4i.23xx and M4x.23xx every of the up to four channels has its own amplifier and 1.25 GS/s A/D converter core, that can be combined to two channels sampling at 2.5 GS/s or even one channel with 5 GS/s. Each input channel can be adapted to a wide variety of signal sources. This is done by software selecting a matching input range and input coupling. The user will easily find a matching solution from the six offered models. These versions are working with sample rates of 1.25 GS/s up to 5 GS/s and have one, two or four channels and can also be updated to a multi-channel system using the internal synchronization bus.


Data is written in the internal 4 GiSample large memory. This memory can also be used as a FIFO buffer. In FIFO mode data will be transferred online into the PC RAM or to hard disk.

Application examples: Automatic test systems, Supersonics, CCD imaging systems, Vibration analysis, Radar, Sonar.


Different models of the M4i.23xx series

The following overview shows the different available models of the M4i.23xx series. They differ in the number of available channels. You can also see the model dependent location of the input connectors.


- **M4i.2320-x8**
- **M4i.2330-x8**

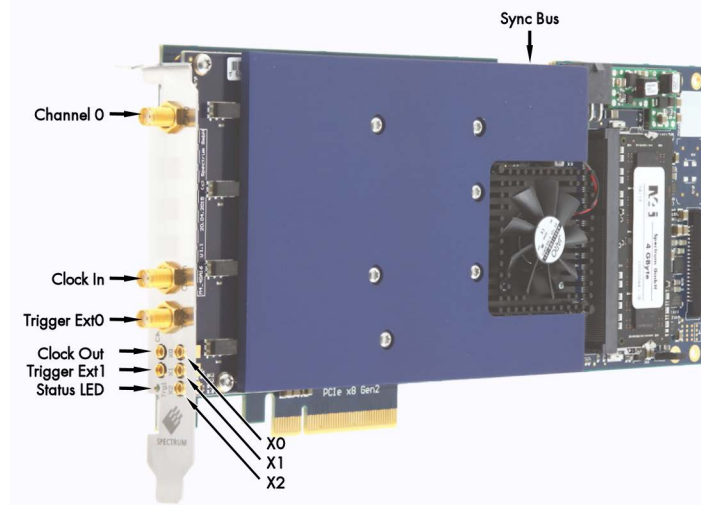

- **M4i.2321-x8**
- **M4i.2323-x8**
- **M4i.2333-x8**

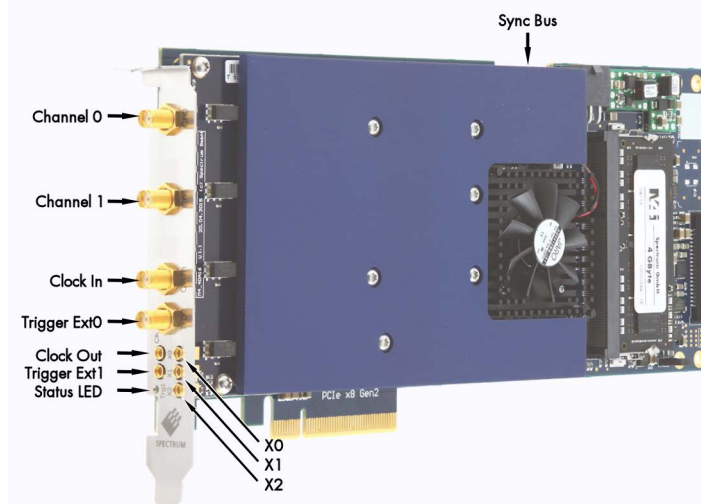


- **M4i.2334-x8**

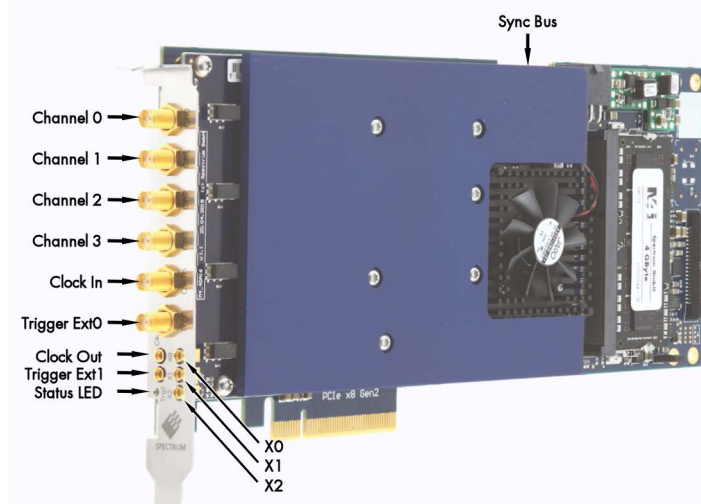


Different models of the M4x.23xx series

The following overview shows the different available models of the M4x.23xx series. They differ in the number of available channels. You can also see the model dependent location of the input connectors.


- **M4x.2320-x4**
- **M4x.2330-x4**

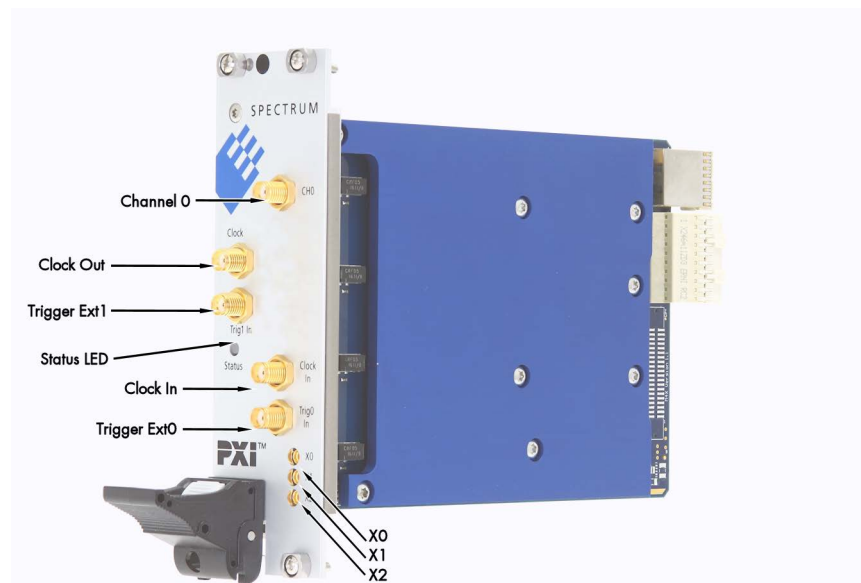

- **M4x.2321-x4**
- **M4x.2323-x4**
- **M4x.2333-x4**

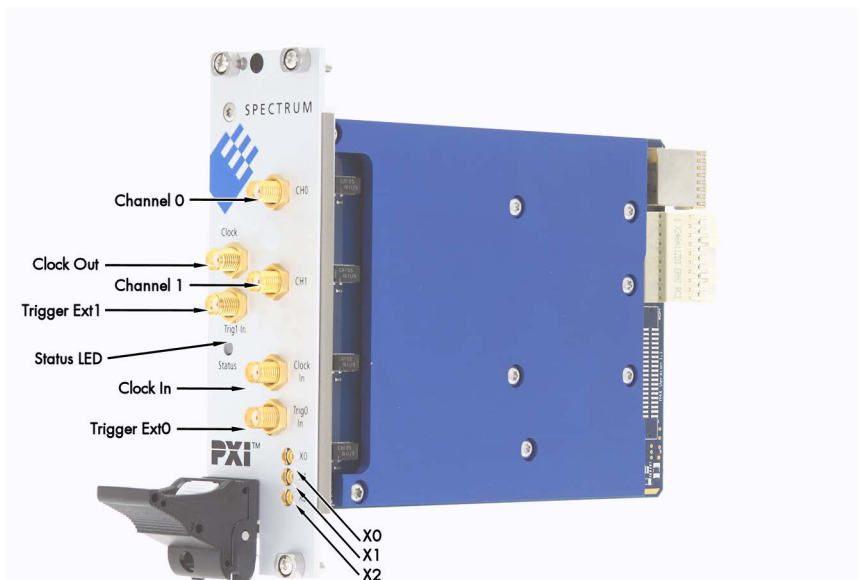

- **M4x.2234-x4**

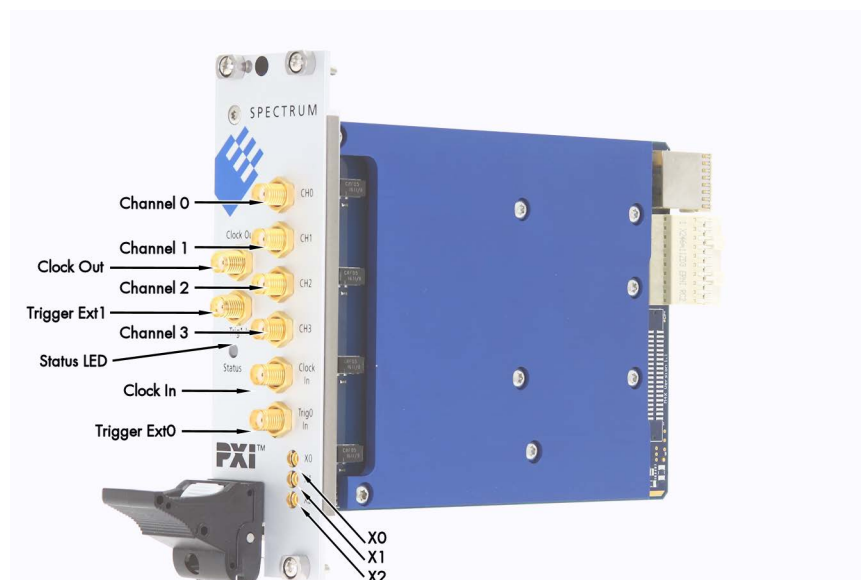

Additional options

Star-Hub (M4i only)

The star hub module allows the synchronization of up to 8 M4i cards. It is possible to synchronize only cards of the same family with each other.

Two different versions of the star-hub module allowing the synchronization of up to 8 cards are available. A version that is mounted on top of the carrier card as a piggy-back module (option SH8tm) extending the width of the card to two slots.

The second version (option SH8ex) is mounted behind the card and extends the M4i base card to a full-length PCI Express card. Therefore it requires the availability of a full-length slot in the system but does not need the space of an additional slot.

The module acts as a star hub for clock and trigger signals. Each board is connected with a small cable of the same length, even the master board. That minimizes the clock skew between the different cards. The picture shows the piggy-back module mounted on the base board schematically without any cables to achieve a better visibility.

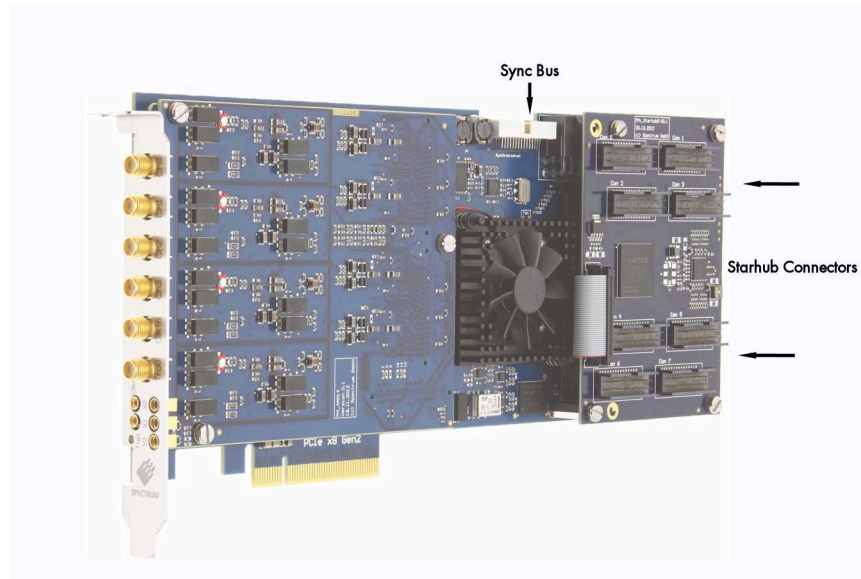


Image 1: M4i card showing mounted star-hub and sync bus connector

The carrier card acts as the clock master and the same or any other card can be the trigger master. All trigger modes that are available on the master card are also available if the synchronization star-hub is used.

The cable connection of the boards is automatically recognized and checked by the driver when initializing the star-hub module. So no care must be taken on how to cable the cards. The star-hub module itself is handled as an additional device just like any other card and the programming consists of only a few additional commands.

Digital I/O with Dig-SMA (M4i.44xx only)

The Digital I/O options „Dig-SMA“ adds eight additional Multi-Purpose I/O lines to the card.

All eight lines are provided via SMA miniature coaxial connectors, just like the analog channels or clock and trigger input.

All of these lines are mounted on the PCI bracket and are hence accessible from the outside of the PC.

These lines extend the already existing Multi-Purpose I/O lines that come standard with the main card (X0 .. X2) and are intended to expand the number of available digital lines, that can be recorded synchronously alongside the analog channels.

Although the capabilities of these additional lines are not identical to those on the main card, they are consistently named (X3 .. X10).

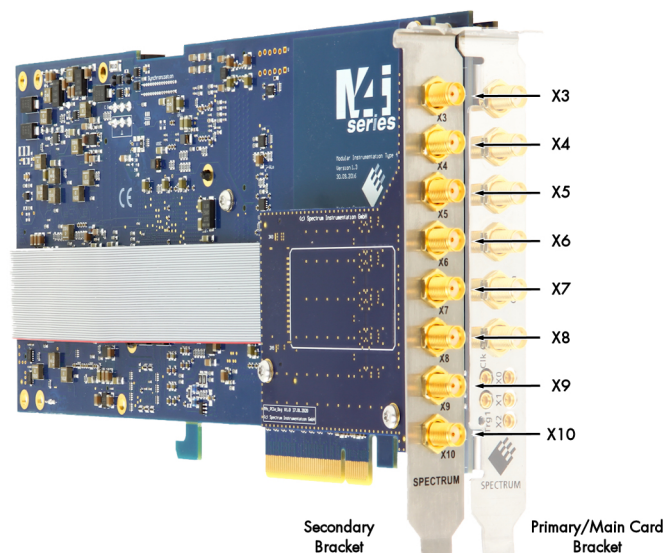


Image 2: M4i card showing mounted digital option

Either one of the two Star-Hub or the DigSMA option can be mounted on any board physically at any given time. It is not possible to mount a Star-Hub and a digital option DigSMA onto the same board.



The Spectrum type plate

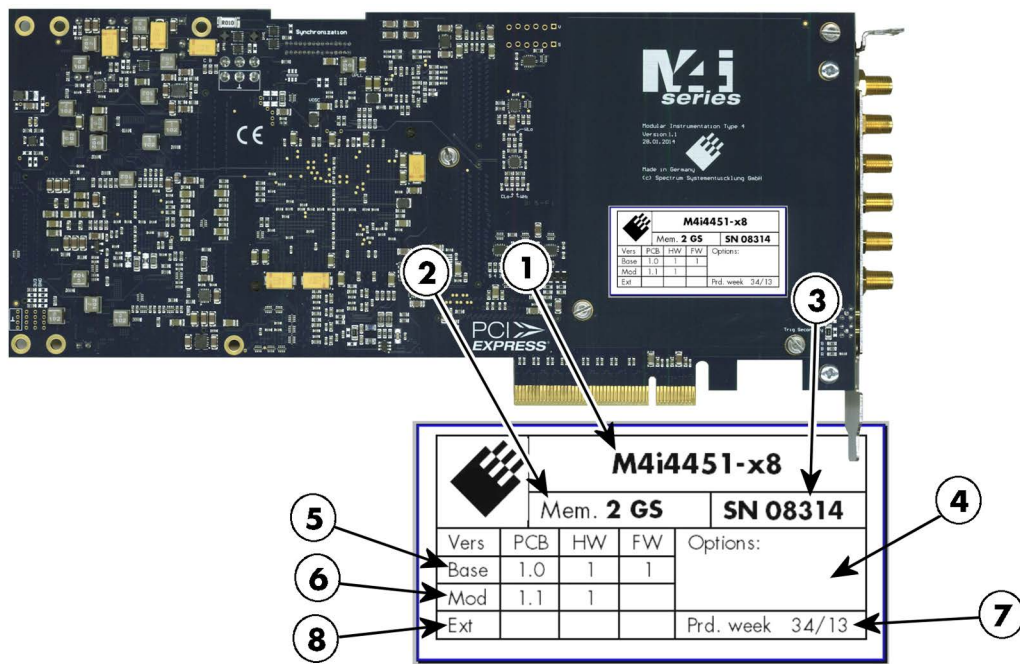


Image 3: M4i card backside showing type plate location and content

The Spectrum type plate, which consists of the following components, can be found on all of our boards. Please check whether the printed information is the same as the information on your delivery note. All this information can also be read out by software:


- ① The board type, consisting of the two letters describing the bus (in this case M4i for the PCI Express x8 bus) and the model number.
- ② The size of the on-board installed memory in MiSample or GiSample. In this example there are 2 GiS = 2048 MiSample (4 GiByte = 4096 MiByte) installed. (please note that on the label the "old" incorrect definition 2 GS = 2 x 1024 x 1024 x 1024 Samples is used).
- ③ The serial number of your Spectrum board. Every board has a unique serial number.
- ④ A list of the installed options. A complete list of all available options is shown in the order information. In this example no additional options are installed.
- ⑤ The base card version, consisting of the printed circuit board (PCB) version, the hardware version and the firmware version.
- ⑥ The version of the analog/digital front-end module, consisting of the printed circuit board (PCB) version, the hardware version and the firmware version (if available). If no programmable device is located on the module, the firmware field is left empty.
- ⑦ The date of production, consisting of the calendar week and the year.
- ⑧ The version of the extension module (such as a Starhub) if one is installed, consisting of the printed circuit board (PCB) version, the hardware version and the firmware version. If no extension module is installed this part is left empty.

Please always supply us with the above information, especially the serial number in case of support request. That allows us to answer your questions as soon as possible. Thank you.


Hardware information

Block Diagrams

M4i.23xx Block Diagram

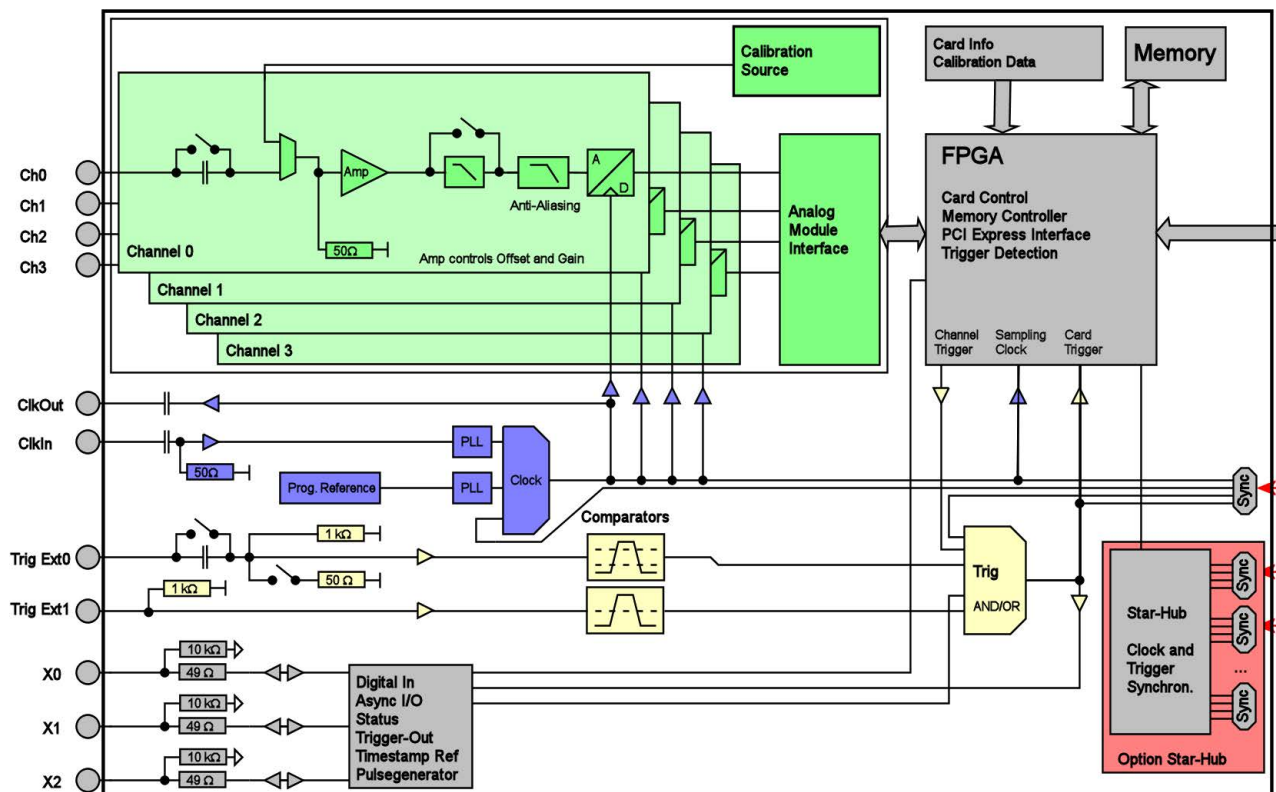

M4x.23xx Block Diagram

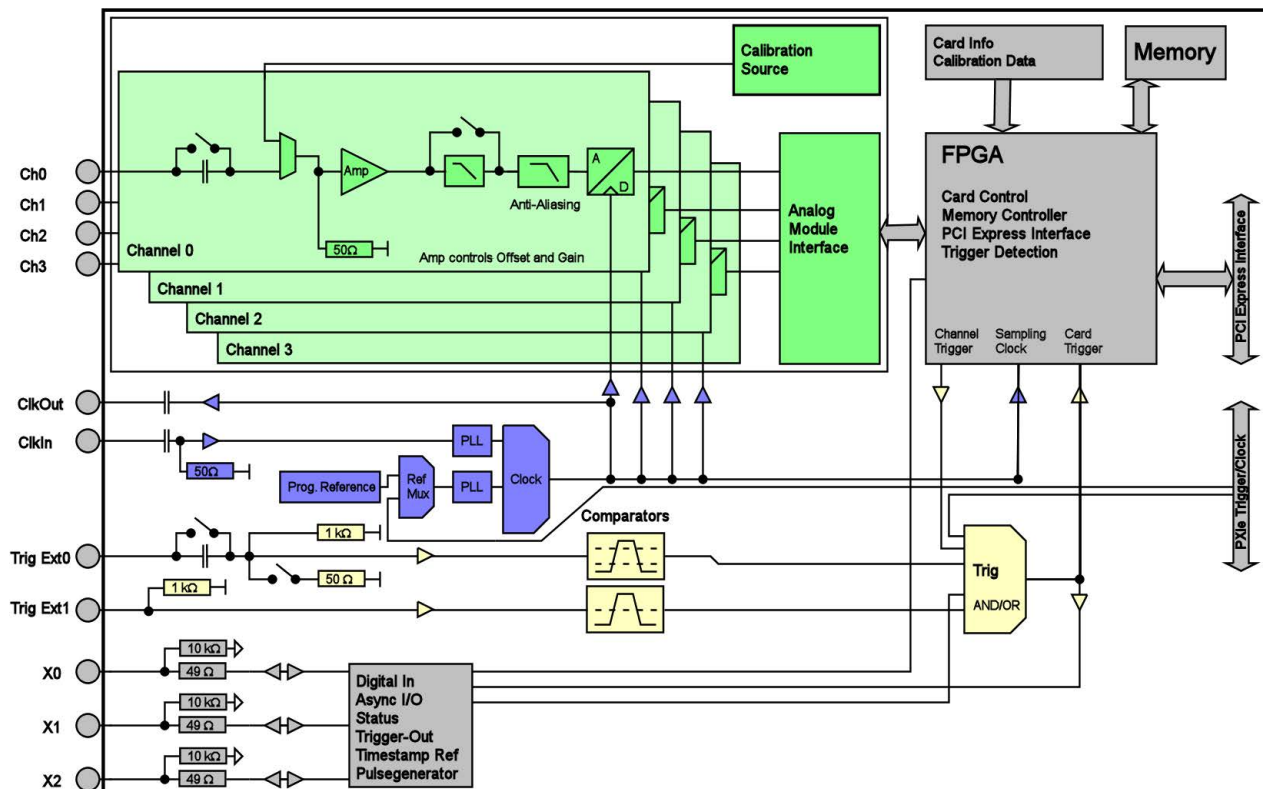

Technical Data



Only figures that are given with a maximum reading or with a tolerance reading are guaranteed specifications. All other figures are typical characteristics that are given for information purposes only. Figures are valid for products stored for at least 2 hours inside the specified operating temperature range, after a 30 minute warm-up, after running an on-board calibration and with proper cooled products. All figures have been measured in lab environment with an environmental temperature between 20 °C and 25 °C and an altitude of less than 100 m.

Analog Inputs

Resolution (nom)		7 Bit			
Input Type		Single-ended			
ADC Differential non linearity (nom)	DNL, ADC only	±0.35 LSB			
ADC Integral non linearity (nom)	INL, ADC only	±0.9 LSB			
ADC Bit Error Rate, BER (nom)	sampling rate 1.25 GS/s	10 ⁻¹⁶			
Channel selection	software programmable	1, 2, or 4 (maximum is model dependent)			
Analog Input impedance (nom)	fixed	50 Ω			
Input Ranges, standard ranges (nom)	software programmable	±200 mV, ±500 mV, ±1 V, ±2.5 V (programmable input offset at 0%)			
Input Ranges, Low Voltage Option (nom)	software programmable	±40 mV, ±100 mV, ±200 mV, ±500 mV (programmable input offset at 0%)			
Programmable Input Offset (nom)	software programmable	±200% of input range (allowing bi-polar ranges to become uni-polar)			
Input Coupling	software programmable	AC/DC			
Max DC voltage if AC coupling active (meas)		±30 V			
Offset error at full speed (spec)	after warm-up and calibration	<0.5% of range			
Gain error at full speed (spec)	after warm-up and calibration	<1% of reading			
Input offset error at full speed (spec)	after warm-up and calibration	<3% of programmed input offset			
Offset temperature drift (meas)	after warm-up and calibration	typical 5 ppm/K of range			
Gain temperature drift (meas)	after warm-up and calibration	typical 45 ppm/K of reading			
Crosstalk 20 MHz sine signal (meas)	≥ ±500 mV standard range	< -96 dB (all channel same input range)			
Crosstalk 20 MHz sine signal (meas)	= ±200 mV standard range	< -88 dB (all channel same input range)			
Crosstalk 100 MHz sine signal (meas)	≥ ±500 mV standard range	< -78 dB (all channel same input range)			
Crosstalk 100 MHz sine signal (meas)	= ±200 mV standard range	< -65 dB (all channel same input range)			
Over voltage protection (standard ranges)	input range	±200 mV	±500 mV	±1 V	±2.5 V
	max. continuous input power (nom)	22.5 dBm	27.0 dBm	27.0 dBm	27.0 dBm
	max. peak input voltage (nom)	±3 V	±7.5 V	±15 V	±30 V
Over voltage protection (low voltage option)	input range	±40 mV	±100 mV	±200 mV	±500 mV
	max. continuous input power (nom)	21.0 dBm	27.0 dBm	22.5 dBm	27.0 dBm
	max. peak input voltage (nom)	±2.5 V	±6.25 V	±3 V	±7.5 V
Calibration	Internal	Self-calibration is done on software command and corrects against the on-board references. Self-calibration should be issued after warm-up time.			
Calibration	External	External calibration calibrates the on-board references used in self-calibration. All calibration constants are stored in non-volatile memory. Optional ISO/IEC17025-compliant certificate. A yearly external calibration is recommended.			

Trigger

Available trigger modes	software programmable	Channel Trigger, External, Software, Window, Re-Arm, Or/And, Delay, PXI (M4x only)
Channel trigger level resolution	software programmable	7 bit
Trigger engines		1 engine per channel with two individual levels, 2 external triggers
Trigger edge	software programmable	Rising edge, falling edge or both edges
Trigger delay	software programmable	0 to (8 GiSamples - 32) = 8589934560 Samples in steps of 32 samples
Multi, ABA, Gate: re-arming time (nom)	1.25 GS/s or below 2.5 GS/s 5 GS/s	80 samples (+ programmed pretrigger) 160 samples (+ programmed pretrigger) 320 samples (+ programmed pretrigger)
Pretrigger at Multi, ABA, Gate, FIFO	software programmable	32 up to 8192 Samples in steps of 32
Posttrigger	software programmable	32 up to 16 GiSamples in steps of 32 (defining pretrigger in standard scope mode)
Memory depth	software programmable	64 up to [installed memory / number of active channels] samples in steps of 32
Multiple Recording/ABA segment size	software programmable	64 up to [installed memory / 2 / active channels] samples in steps of 32
Trigger accuracy (all sources)		1 sample
Timestamp modes	software programmable	Standard, Startreset, external reference clock on X0 (e.g. PPS from GPS, IRIG-B)
Data format		Std., Startreset: 64 bit counter, increments with sample clock (reset manually or on start) RefClock: 24 bit upper counter (increment with RefClock) 40 bit lower counter (increments with sample clock, reset with RefClock)
Extra data	software programmable	none, acquisition of X0/X1/X2 inputs at trigger time, trigger source (for OR trigger)
Size per stamp		128 bit = 16 bytes
External trigger		Ext0
External trigger impedance (typ)	software programmable	50 Ω / 1 kΩ
External trigger coupling (nom)	software programmable	AC or DC
External trigger type		Window comparator
External input level (nom)		±10 V (1 kΩ), ±2.5 V (50 Ω),
External trigger sensitivity, min signal swing (nom)		2.5% of full scale range
External trigger level (nom)	software programmable	±10 V in steps of 10 mV
External trigger maximum voltage (nom)		±30V
External trigger bandwidth DC (meas)	50 Ω 1 kΩ	DC to 200 MHz DC to 150 MHz
External trigger bandwidth AC (meas)	50 Ω	20 kHz to 200 MHz
Minimum external trigger pulse width		≥ 2 samples

Ext1

1 kΩ
fixed DC
Single level comparator
±10 V
2.5% of full scale range = 0.5 V
±10 V in steps of 10 mV
±30 V
n.a.
DC to 200 MHz
n.a.
≥ 2 samples

External trigger
Minimum pause between external triggers
Resulting max. detectable trigger frequency

Ext0
≥ 2 samples
[Current Samplerate]/4

Ext1
≥ 2 samples
[Current Samplerate]/4

Clock

Clock Modes	software programmable	internal PLL, external reference clock, Star-Hub sync (M4i only), PXI Reference Clock (M4x only)
Internal clock accuracy (spec)		≤ ±5 ppm
Clock setup range	standard mode	all clock modes and all cards, single or synchronized by star-hub: maximum sampling clock 5 GS/s or 2.5 GS/s or 1.25 GS/s (depending on type) divider: maximum sampling rate divided by: 1, 2, 4, 8, 16, ... up to 262144
Clock setup range	special clock mode	internal clock only, single cards only, digitizerNETBOX with one internal digitizer only: maximum sampling clock 4 GS/s or 2 GS/s or 1 GS/s (depending on type) divider: maximum sampling rate divided by: 1, 2, 4, 8, 16, ... up to 262144
External reference clock range	software programmable	≥ 10 MHz and ≤ 1.25 GHz
External reference clock input impedance (typ)		50 Ω fixed
External reference clock input coupling		AC coupling
External reference clock input edge		Rising edge
External reference clock input type		Single-ended, sine wave or square wave
External reference clock input swing (nom)	square wave	0.3 V peak-peak up to 3.0 V peak-peak
External reference clock input swing (nom)	sine wave	1.0 V peak-peak up to 3.0 V peak-peak
External reference clock input max DC voltage (nom)		±30 V (with max 3.0 V difference between low and high level)
External reference clock input duty cycle (nom)		45% to 55%
Clock setup granularity when using reference clock		divider: maximum sampling rate divided by: 1, 2, 4, 8, 16, ... up to 262144
Internal reference clock output type (nom)		Single-ended, AC-coupled, LVPECL, 750 mVpp (typical)
Internal reference clock output frequency		2.5 GHz / 64 = 39.0625 MHz
Star-Hub synchronization clock modes	software selectable	Internal clock (standard clock mode only), External reference clock
ABA mode clock divider for slow clock	software programmable	16 up to (128 Ki - 16) in steps of 16
Channel to channel skew on one card (meas)		< 60 ps (typical)
Skew between star-hub synchronized cards (meas)		< 130 ps (typical, preliminary)

	M4i.233xx / M4x.233xx DN2.233-xx DN2.235-xx DN6.235-xx	M4i.232xx / M4x.232xx DN2.232-xx
ADC Resolution	7 bit	7 bit
max sampling clock	5 GS/s	2.5 GS/s
min sampling clock	4.768 kS/s	4.768 kS/s
lower bandwidth limit, DC coupling (meas)	0 Hz	0 Hz
lower bandwidth limit, AC coupling (meas)	< 30 kHz	< 30 kHz
-3 dB bandwidth (no filter active), Standard input ranges (meas)	1.5 GHz	1.5 GHz
-3 dB bandwidth (no filter active), small input ranges, ir40m option installed (meas)	1.2 GHz	1.2 GHz
-3 dB bandwidth, BW filter active (meas)	~400 MHz	~400 MHz

Block Average Signal Processing Option M4i.23xx/DN2.23x/DN6.23x Series

Data Mode (resulting sample width)	software programmable	32 bit mode	16 bit mode
Minimum Waveform Length		64 samples	128 samples
Minimum Waveform Stepsize		32 samples	64 samples
Maximum Waveform Length	1 channel active	64 KiSamples	128 KiSamples
Maximum Waveform Length	2 channels active	32 KiSamples	64 KiSamples
Maximum Waveform Length	4 or more channels active	16 KiSamples	32 KiSamples
Minimum Number of Averages		2	2
Maximum Number of Averages		16777216 (16Mi)	256
Data Output Format	fixed	32 bit signed integer	16 bit signed integer
Re-Arming Time between waveforms (nom)	1.25 GS/s or below	80 samples (+ programmed pretrigger)	
Re-Arming Time between waveforms (nom)	2.5 GS/s	160 samples (+ programmed pretrigger)	
Re-Arming Time between waveforms (nom)	5 GS/s	320 samples (+ programmed pretrigger)	
Re-Arming Time between end of average to start of next average (nom)		Depending on programmed segment length, max 50 µs	

Block Statistics Signal Processing Option M4i.23xx/DN2.23x Series/DN6.23x Series

Minimum Waveform Length		64 samples
Minimum Waveform Stepsize		32 samples
Maximum Waveform Length	Standard Acquisition	2 GiSamples / channels
Maximum Waveform Length	FIFO Acquisition	2 GiSamples
Data Output Format	fixed	32 bytes statistics summary
Statistics Information Set per Waveform		Average, Minimum, Maximum, Position Minimum, Position Maximum, Trigger Timestamp
Re-Arming Time between Segments (nom)	1.25 GS/s or below	80 samples (+ programmed pretrigger)
Re-Arming Time between Segments (nom)	2.5 GS/s	160 samples (+ programmed pretrigger)
Re-Arming Time between Segments (nom)	5 GS/s	320 samples (+ programmed pretrigger)

Multi Purpose I/O lines (front-plate)

Number of multi purpose lines		three, named X0, X1, X2
Input: available signal types	software programmable	Asynchronous Digital-In, Synchronous Digital-In, Timestamp Reference Clock
Input: impedance (nom)		10 k Ω to 3.3 V
Input: maximum voltage level (nom)		-0.5 V to +4.0 V
Input: signal levels (nom)		3.3 V LVTTTL (Low $\leq$ 0.8 V, High $\geq$ 2.0 V)
Input: bandwidth (nom)		125 MHz
Output: available signal types	software programmable	Asynchronous Digital-Out, Trigger Output, Run, Arm, PLL Refclock, System Clock
Output: impedance (nom)		50 Ω
Output: signal levels (nom)		3.3 V LVTTTL
Output: type (nom)		3.3 V LVTTTL, TTL compatible for high impedance loads
Output: drive strength (nom)		Capable of driving 50 Ω loads, maximum drive strength $\pm$ 48 mA
Output: update rate (nom)	14/16 bit ADC resolution	sampling clock
Output: update rate (nom)	7/8 bit ADC resolution	Current sampling clock $\leq$ 1.25 GS/s : sampling clock Current sampling clock $>$ 1.25 GS/s and $\leq$ 2.50 GS/s : $\frac{1}{2}$ sampling clock Current sampling clock $>$ 2.50 GS/s and $\leq$ 5.00 GS/s : $\frac{1}{4}$ sampling clock

Option M4i.xxxx-PulseGen

Number of internal pulse generators	4
Number of pulse generator output lines	3 (Existing multi-purpose outputs X0 to X2)
Time resolution of pulse generator	Pulse generator's sampling rate is derived from instrument's sampling rate and value can be read out. Maximum possible pulse generator update rate is 22xx: 156.25 MS/s (6.4 ns) 23xx: 156.25 MS/s (6.4 ns) 44xx: 125.00 MS/s (8.0 ns) 66xx: 156.25 MS/s (6.4 ns) 96xx: 156.25 MS/s (6.4 ns)
Programmable output modes	Single-shot, multiple repetitions on trigger, gated
Programmable trigger sources	Software, Card Trigger, Other Pulse Generator, XIO lines.
Programmable trigger gate	None, ARM state, RUN state
Programmable length (frequency)	2 to 4Gi samples in steps of 1 (32 bit)
Programmable width (duty cycle)	1 to 4Gi samples in steps of 1 (32 bit)
Programmable delay	0 to 4Gi samples in steps of 1 (32 bit)
Programmable loops	0 to 4Gi samples in steps of 1 (32 bit) with 0 = infinite loops
Output level of digital pulse generators	Please see section of multi-purpose I/O lines.

Dynamic Parameters

M4i.233x, M4x.233x and DN2.233-xx, DN2.235-xx and DN6.235-xx, 7 Bit 5 GS/s												
Input Path	DC or AC coupled, fixed 50 Ohm											
Test signal frequency	10 MHz				40 MHz		70 MHz		240 MHz		600 MHz	
Input Range	±200 mV	±500 mV	±1 V	±2.5 V	±200 mV	±1V	±200 mV	±1V	±200 mV	±1V	±200 mV	±1V
THD (typ)	<56.5 dB	<56.5 dB	<56.8 dB	<57.1 dB	<56.9 dB	<56.9 dB	<56.5 dB	<56.5 dB	<51.9 dB	<51.9 dB	<47.60 dB	<47.0 dB
SNR (typ)	>42.1 dB	>42.2 dB	>42.2 dB	>42.1 dB	>42.0 dB	>42.0 dB	>41.9 dB	>41.9 dB	>41.5 dB	>41.6 dB	>40.5 dB	>40.9 dB
SFDR, excl. harmonics (typ)	>57.3 dB	>58.7 dB	>58.8 dB	>58.8 dB	>57.1 dB	>57.1 dB	>56.9 dB	>56.9 dB	>54.1 dB	>59.5 dB	>52.2 dB	>52.2 dB
SFDR, incl. harmonics (typ)	>57.1 dB	>58.2 dB	>58.3 dB	>58.3 dB	>57.1 dB	>57.1 dB	>56.9 dB	>56.9 dB	>53.3 dB	>53.1 dB	>49.9 dB	>49.9 dB
SINAD/THD+N (typ)	>42.1 dB	>42.2 dB	>42.2 dB	>42.2 dB	>41.9 dB	>41.9 dB	>41.7 dB	>41.7 dB	>41.1 dB	>41.4 dB	>40.0 dB	>40.1 dB
ENOB based on SINAD (bit)	>6.7 bit	>6.7 bit	>6.7 bit	>6.7 bit	>6.7 bit	>6.7 bit	>6.6 bit	>6.7 bit	>6.5 bit	>6.6 bit	>6.3 bit	>6.3 bit
ENOB based on SNR (bit)	>6.7 bit	>6.7 bit	>6.7 bit	>6.7 bit	>6.7 bit	>6.7 bit	>6.6 bit	>6.7 bit	>6.6 bit	>6.6 bit	>6.3 bit	>6.3 bit

Input Path	M4i.232x, M4x.232x and DN2.232-xx, 7 Bit 2.5 GS/s											
	DC or AC coupled, fixed 50 Ohm											
	10 MHz				40 MHz		70 MHz		240 MHz		600 MHz	
	±200 mV	±500 mV	±1 V	±2.5 V	±200 mV	±1V	±200 mV	±1V	±200 mV	±1V	±200 mV	±1V
Test signal frequency												
Input Range												
THD (typ)	<56.5 dB	<56.5 dB	<56.8 dB	<57.1 dB	<56.9 dB	<56.9 dB	<56.5 dB	<56.5 dB	<51.9 dB	<51.9 dB	<47.60 dB	<47.0 dB
SNR (typ)	>42.1 dB	>42.2 dB	>42.2 dB	>42.1 dB	>42.0 dB	>42.0 dB	>41.9 dB	>41.9 dB	>41.5 dB	>41.6 dB	>40.5 dB	>40.9 dB
SFDR, excl. harmonics (typ)	>57.3 dB	>58.7 dB	>58.8 dB	>58.8 dB	>57.1 dB	>57.1 dB	>56.9 dB	>56.9 dB	>54.1 dB	>59.5 dB	>52.2 dB	>52.2 dB
SFDR, incl. harmonics (typ)	>57.1 dB	>58.2 dB	>58.3 dB	>58.3 dB	>57.1 dB	>57.1 dB	>56.9 dB	>56.9 dB	>53.3 dB	>53.1 dB	>49.9 dB	>49.9 dB
SINAD/THD+N (typ)	>42.1 dB	>42.2 dB	>42.2 dB	>42.2 dB	>41.9 dB	>41.9 dB	>41.7 dB	>41.7 dB	>41.1 dB	>41.4 dB	>40.0 dB	>40.1 dB
ENOB based on SINAD (bit)	>6.7 bit	>6.7 bit	>6.7 bit	>6.7 bit	>6.7 bit	>6.7 bit	>6.6 bit	>6.7 bit	>6.5 bit	>6.6 bit	>6.3 bit	>6.3 bit
ENOB based on SNR (bit)	>6.7 bit	>6.7 bit	>6.7 bit	>6.7 bit	>6.7 bit	>6.7 bit	>6.6 bit	>6.7 bit	>6.6 bit	>6.6 bit	>6.3 bit	>6.3 bit

	M4i.23xx, DN2.23x-xx and DN6.23x-xx - low voltage input ranges									
Input Path	DC or AC coupled, fixed 50 Ohm									
Test signal frequency	10 MHz				40 MHz		70 MHz		240 MHz	
Input Range	±40 mV	±100 mV	±200 mV	±500 mV	±40 mV	±100 mV	±40 mV	±100 mV	±40 mV	±100 mV
THD (typ)										
SNR (typ)										
SFDR, excl. harmonics (typ)										
SFDR, incl. harmonics (typ)										
SINAD/THD+N (typ)										
ENOB based on SINAD (bit)										
ENOB based on SNR (bit)										

Dynamic parameters are measured at ± 1 V input range (if no other range is stated) and 50 Ω termination with the samplerate specified in the table. Measured parameters are averaged 20 times to get typical values. Test signal is a pure sine wave generated by a signal generator and a matching bandpass filter. Amplitude is >99% of FSR. SNR and RMS noise parameters may differ depending on the quality of the used PC. SNR = Signal to Noise Ratio, THD = Total Harmonic Distortion, SFDR = Spurious Free Dynamic Range, SINAD = Signal Noise and Distortion, ENOB = Effective Number of Bits.

RMS Noise Level (Zero Noise)

M4i.233x, M4x.233x and DN2.233-xx, DN2.235-xx, DN6.235-xx, 7 Bit 5 GS/s								
Input Range	± 200 mV		± 500 mV		± 1		± 2.5 V	
Voltage resolution (1 LSB)	3.1 mV		7.8 mV		15.6 mV		39.0 mV	
DC, fixed 50 Ω (typ)	<0.2 LSB	<0.5 mV	<0.2 LSB	<1.2 mV	<0.2 LSB	<2.3 mV	<0.2 LSB	<5.9 mV
DC, fixed 50 Ω (max)	<0.3 LSB	<0.9 mV	<0.3 LSB	<2.3 mV	<0.3 LSB	<4.7 mV	<0.3 LSB	<11.7 mV

M4i.232x, M4x.232x, DN2.232-xx and DN6.232-xx, 7 Bit 2.5 GS/s								
Input Range	± 200 mV		± 500 mV		± 1		± 2.5 V	
Voltage resolution (1 LSB)	3.1 mV		7.8 mV		15.6 mV		39.0 mV	
DC, fixed 50 Ω (typ)	<0.2 LSB	<0.5 mV	<0.2 LSB	<1.2 mV	<0.2 LSB	<2.3 mV	<0.2 LSB	<5.9 mV
DC, fixed 50 Ω (max)	<0.3 LSB	<0.9 mV	<0.3 LSB	<2.3 mV	<0.3 LSB	<4.7 mV	<0.3 LSB	<11.7 mV

Low Voltage Version M4i.23xx, M4x.23xx, DN2.23x-xx and DN6.23x-xx, 7 Bit 1.25 GS/s								
Input Range	± 40 mV		± 100 mV		± 200 mV		± 500 mV	
Voltage resolution (1 LSB)	0.6 mV		1.6 mV		3.1 mV		7.8 mV	
DC, fixed 50 Ω (typ)	<0.2 LSB	<0.2 mV	<0.2 LSB	<0.3 mV	<0.2 LSB	<0.6 mV	<0.2 LSB	<1.6 mV
DC, fixed 50 Ω (max)	<0.3 LSB	<0.2 mV	<0.3 LSB	<0.4 mV	<0.3 LSB	<0.8 mV	<0.3 LSB	<2.0 mV

M4i Specific Technical Data

Connectors

Analog Inputs/Analog Outputs	SMA female (one for each single-ended input)	Cable-Type: Cab-3mA-xx-xx
Trigger 0 Input	SMA female	Cable-Type: Cab-3mA-xx-xx
Clock Input	SMA female	Cable-Type: Cab-3mA-xx-xx
Trigger 1 Input	MMCX female	Cable-Type: Cab-1m-xx-xx
Clock Output	MMCX female	Cable-Type: Cab-1m-xx-xx
Multi Purpose I/O	MMCX female (3 lines)	Cable-Type: Cab-1m-xx-xx

Connection Cycles

All connectors have an expected lifetime as specified below. Please avoid to exceed the specified connection cycles or use connector savers.

SMA connector	500 connection cycles
MMCX connector	500 connection cycles
PCIe connector	50 connection cycles
PCIe power connector	30 connection cycles

Environmental and Physical Details

Dimension (Single Card)	L x H x W: 241 mm (¾ PCIe length) x 107 mm x 20 mm (single slot width)
Dimension (Card with option SH8tm installed)	241 mm (¾ PCIe length) x 107 mm x 40 mm (double slot width, extends W by 1 slot right of the main card's bracket, on „component side“ of the PCIe card.)
Dimension (Card with option SH8ex installed)	Extends L to 312 mm (full PCIe length) x 107 mm x 20 mm (single slot width)
Dimension (Card with option M4i.44xx-DigSMA installed)	241 mm (¾ PCIe length) x 107 mm x 40 mm (double slot width, extends W by 1 slot left of the main card's bracket, on „solder side“ of the PCIe card.)
Weight (M4i.44xx series)	maximum 290 g
Weight (M4i.22xx, M4i.23xx, M4i.66xx, M4i.77xx, M4i.96xx series)	maximum 420 g
Weight (Option star-hub -sh8ex, -sh8tm)	including 8 sync cables 130 g
Weight (Option M4i.44xx-DigSMA)	320 g
Warm up time (meas)	30 minutes
Operating temperature (nom)	0°C to 50°C
Storage temperature (nom)	-10°C to 70°C
Humidity (nom)	10% to 90%
Dimension of packing	1 or 2 cards 470 mm x 250 mm x 130 cm
Volume weight of packing	1 or 2 cards 4 kg

PCI Express specific details

PCIe slot type	x8 Generation 2 (Gen2)
PCIe slot compatibility (physical)	x8/x16
PCIe slot compatibility (electrical)	x1, x2, x4, x8, x16 with PCIe Gen1, Gen2, Gen3, Gen4 or Gen5
Sustained streaming mode (meas): M4i.22xx, M4i.23xx, M4i.44xx, M4i.77xx	Card-to-System > 3.4 GB/s (measured with a chipset supporting a TLP size of 256 bytes, using PCIe x8 Gen2)
Sustained streaming mode (meas): M4i.66xx, M4i.96xx	System-to-Card > 2.8 GB/s (measured with a chipset supporting a TLP size of 256 bytes, using PCIe x8 Gen2)

Certification, Compliance, Warranty

Conformity Declaration	EN 17050-1:2010	General Requirements
EU Directives	2014/30/EU 2014/35/EU 2011/65/EU 2006/1907/EC 2012/19/EU	EMC - Electromagnetic Compatibility LVD - Electrical equipment designed for use within certain voltage limits RoHS - Restriction of the use of certain hazardous substances in electrical and electronic equipment REACH - Registration, Evaluation, Authorisation and Restriction of Chemicals WEEE - Waste from Electrical and Electronic Equipment
Compliance Standards	EN 61010-1: 2010 EN 61187:1994 EN 61326-1:2021 EN 61326-2-1:2021 EN IEC 63000:2018	Safety regulations for electrical measuring, control, regulating and laboratory devices - Part 1: General requirement Electrical and electronic measuring equipment - Documentation Electrical equipment for measurement, control and laboratory use EMC requirements - Part 1: General requirements EMC requirements - Part 2-1: Particular requirements - Test configurations, operational conditions and performance criteria for sensitive test and measurement equipment for EMC unprotected applications Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances
Product warranty	5 years starting with the day of delivery	
Software and firmware updates	Life-time, free of charge	

Power Consumption

	PCI EXPRESS		
	3.3V	12 V	Total
M4i.2330/2320-x8 (meas)	0.2 A	2.6 A	32 W
M4i.2333/2321-x8/2323-x8 (meas)	0.2 A	2.7 A	33 W
M4i.2334-x8 (meas)	0.2 A	2.9 A	35 W

MTBF

MTBF (typ)	200000 hours
------------	--------------

M4x specific Technical Data

Connectors

Analog Inputs/Analog Outputs	SMA female (one for each single-ended input)	Cable-Type: Cab-3mA-xx-xx
Trigger 0 Input	SMA female	Cable-Type: Cab-3mA-xx-xx
Clock Input	SMA female	Cable-Type: Cab-3mA-xx-xx
Trigger 1 Input	SMA female	Cable-Type: Cab-3mA-xx-xx
Clock Output	SMA female	Cable-Type: Cab-3mA-xx-xx
Multi Purpose I/O	MMCX female (3 lines)	Cable-Type: Cab-1m-xx-xx

Connection Cycles

All connectors have an expected lifetime as specified below. Please avoid to exceed the specified connection cycles or use connector savers.

SMA connector	500 connection cycles
MMCX connector	500 connection cycles
PXIe connector	250 connection cycles

Environmental and Physical Details

Dimension (Single Card)	(PCB only)	160 mm x 100 mm (Standard 3U)
Width		2 slots
Weight (M4x.44xx series)	maximum	340 g
Weight (M4x.22xx, M4x.66xx series)	maximum	450 g
Warm up time (meas)		30 minutes
Operating temperature (nom)		0°C to 50°C
Storage temperature (nom)		-10°C to 70°C
Humidity (nom)		10% to 90%
Dimension of packing	1 or 2 cards	470 mm x 250 mm x 130 cm
Volume weight of packing	1 or 2 cards	4 kg

PXI Express specific details

PXIe slot type	4 Lanes, PCIe Gen2 (x4 Gen2)
PXIe hybrid slot compatibility	Fully compatible
Sustained streaming mode (meas) (Card-to-System: M4x.22xx, M4x.44xx)	> 1.7 GB/s (measured with a chipset supporting a TLP size of 256 bytes, using PXIe x4 Gen2)
Sustained streaming mode (meas) (System-to-Card: M4x.66xx, M4x.96xx)	> 1.4 GB/s (measured with a chipset supporting a TLP size of 256 bytes, using PXIe x4 Gen2)

Certification, Compliance, Warranty

Conformity Declaration	EN 17050-1:2010	General Requirements
EU Directives	2014/30/EU	EMC - Electromagnetic Compatibility
	2014/35/EU	LVD - Electrical equipment designed for use within certain voltage limits
	2011/65/EU	RoHS - Restriction of the use of certain hazardous substances in electrical and electronic equipment
	2006/1907/EC	REACH - Registration, Evaluation, Authorisation and Restriction of Chemicals
	2012/19/EU	WEEE - Waste from Electrical and Electronic Equipment
Compliance Standards	EN 61010-1: 2010	Safety regulations for electrical measuring, control, regulating and laboratory devices - Part 1: General requirement
	EN 61187:1994	Electrical and electronic measuring equipment - Documentation
	EN 61326-1:2021	Electrical equipment for measurement, control and laboratory use
	EN 61326-2-1:2021	EMC requirements - Part 1: General requirements
		EMC requirements - Part 2-1: Particular requirements - Test configurations, operational conditions and performance criteria for sensitive test and measurement equipment for EMC unprotected applications
	EN IEC 63000:2018	Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances
Product warranty	5 years starting with the day of delivery	
Software and firmware updates	Life-time, free of charge	

Power Consumption

	PCI EXPRESS		
	3.3V	12 V	Total
M4x.2330-x4, M4x.2320-x4	0.25 A	2.6 A	32 W
M4x.2333-x4, M4x.2321-x4, M4x.2323-x4	0.25 A	2.7 A	33 W
M4x.2334-x4	0.25 A	2.9 A	35 W

MTBF

MTBF	100000 hours
------	--------------

Order Information

M4i Order Information

The card is delivered with 4 GiSample on-board memory and supports standard acquisition (Scope), FIFO acquisition (streaming), Multiple Recording, Gated Sampling, ABA mode and Timestamps. Operating system drivers for Windows/Linux 32 bit and 64 bit, examples for C/C++, LabVIEW (Windows), MATLAB (Windows and Linux), IVI, .NET, Delphi, Java, Python, Julia and a Base license of the oscilloscope software SBench 6 are included.

Adapter cables are not included. Please order separately!

PCI Express x8

Order no.	Bandwidth Standard	Bandwidth ir40m option	Standard mem	1 channel	2 channels	4 channels
M4i.2320-x8	1.5 GHz	1.2 GHz	4 GiSample	2.5 GS/s		
M4i.2323-x8	1.5 GHz	1.2 GHz	4 GiSample	2.5 GS/s	1.25 GS/s	
M4i.2321-x8	1.5 GHz	1.2 GHz	4 GiSample	2.5 GS/s	2.5 GS/s	
M4i.2330-x8	1.5 GHz	1.2 GHz	4 GiSample	5 GS/s		
M4i.2333-x8	1.5 GHz	1.2 GHz	4 GiSample	5 GS/s	2.5 GS/s	
M4i.2334-x8	1.5 GHz	1.2 GHz	4 GiSample	5 GS/s	2.5 GS/s	1.25 GS/s

Options

Order no.	Option
M4i.23xx-ir40m	Low voltage input range option for 23xx series. 4 Input ranges with ± 40 mV, ± 100 mV, ± 200 mV, ± 500 mV, bandwidth limited.

Options

Order no.	Option
M4i.xxxx-SH8ex ⁽¹⁾	Synchronization Star-Hub for up to 8 cards (extension), only one slot width, extension of the card to full PCI Express length (312 mm). 8 synchronization cables included.
M4i.xxxx-SH8tm ⁽¹⁾	Synchronization Star-Hub for up to 8 cards (top mount), two slots width, top mounted on card. 8 synchronization cables included.
M4i-upgrade	Upgrade for M4i.xxxx: Later installation of option Star-Hub

Firmware Options

Order no.	Option
M4i.xxxx-spavg	Signal Processing Firmware Option: Block Average (later firmware-upgrade available)
M4i.xxxx-spstat	Signal Processing Firmware Option: Block Statistics/Peak Detect (later firmware-upgrade available)
M4i.xxxx-PulseGen	Firmware Option: adds 4 freely programmable digital pulse generators that use the XIO lines for output (later installation by firmware -upgrade available)

Services

Order no.	
Recal	Recalibration at Spectrum incl. calibration protocol
Card-Prot-17025	ISO 17025 Calibration Certificate for one card; add-on for new cards or for recalibration

Standard Cables

for Connections	Length	Order no.	to BNC male	to BNC female	to SMA male	to SMA female	to SMB female
Analog/Clock-In/Trig-In	80 cm	Cab-3mA-9m-80		Cab-3mA-9f-80	Cab-3mA-3mA-80		Cab-3f-3mA-80
Analog/Clock-In/Trig-In	200 cm	Cab-3mA-9m-200		Cab-3mA-9f-200	Cab-3mA-3mA-200		Cab-3f-3mA-200
Probes (short)	5 cm			Cab-3mA-9f-5			
Clk-Out/Trig-Out/Extra	80 cm	Cab-1m-9m-80		Cab-1m-9f-80	Cab-1m-3mA-80	Cab-1m-3fA-80	Cab-1m-3f-80
Clk-Out/Trig-Out/Extra	200 cm	Cab-1m-9m-200		Cab-1m-9f-200	Cab-1m-3mA-200	Cab-1m-3fA-200	Cab-1m-3f-200
Information	The standard adapter cables are based on RG174 cables and have a nominal attenuation of 0.3 dB/m at 100 MHz and 0.5 dB/m at 250 MHz. For high speed signals we recommend the low loss cables series CHF						

Low Loss Cables

Order No.	Option
CHF-3mA-3mA-200	Low loss cables SMA male to SMA male 200 cm
CHF-3mA-9m-200	Low loss cables SMA male to BNC male 200 cm
Information	The low loss adapter cables are based on MF141 cables and have an attenuation of 0.3 dB/m at 500 MHz and 0.5 dB/m at 1.5 GHz. They are recommended for signal frequencies of 200 MHz and above.

Amplifiers

Order no.	Bandwidth	Connection	Input Impedance	Coupling	Amplification
SPA.1841 ⁽²⁾	2 GHz	SMA	50 Ohm	AC	x100 (40 dB)
SPA.1801 ⁽²⁾	2 GHz	SMA	50 Ohm	AC	x10 (20 dB)
SPA.1601 ⁽²⁾	500 MHz	BNC	50 Ohm	DC	x10 (20 dB)
Information	External Amplifiers with one channel, BNC/SMA female connections on input and output, manually adjustable offset, manually switchable settings. An external power supply for 100 to 240 VAC is included. Please be sure to order an adapter cable matching the amplifier connector type and matching the connector type for your A/D card input.				

Software SBench6

Order no.	
SBench6	Base version included in delivery. Supports standard mode for one card.
SBench6-Pro	Professional version for one card: FIFO mode, export/import, calculation functions, ...
SBench6-Multi	Option multiple cards: Needs SBench6-Pro. Handles multiple synchronized cards in one system.
Volume Licenses	Please ask Spectrum for details.

Software Options

Order no.	
SPc-RServer	Remote Server Software Package - LAN remote access for M2i/M3i/M4i/M4x/M2p/M5i cards
SPc-SCAPP	Spectrum's CUDA Access for Parallel Processing - SDK for direct data transfer between Spectrum card and CUDA GPU. Includes RDMA activation and examples. Only working for Data Acquisition or AWG mode, not usable for DDS mode

⁽¹⁾ : Just one of the options can be installed on a card at a time.

⁽²⁾ : Third party product with warranty differing from our export conditions. No volume rebate possible.

M4x Order Information

The card is delivered with 4 GiSample on-board memory and supports standard acquisition (Scope), FIFO acquisition (streaming), Multiple Recording, Gated Sampling, ABA mode and Timestamps. Operating system drivers for Windows/Linux 32 bit and 64 bit, examples for C/C++, LabVIEW (Windows), MATLAB (Windows and Linux), IVI, .NET, Delphi, Java, Python, Julia and a Base license of the oscilloscope software SBench 6 are included.

Adapter cables are not included. Please order separately!

PXI Express x4

	Bandwidth					
M4x.2320-x4	1.5 GHz	4 GiSample	2.5 GS/s			
M4x.2323-x4	1.5 GHz	4 GiSample	2.5 GS/s	1.25 GS/s		
M4x.2321-x4	1.5 GHz	4 GiSample	2.5 GS/s	2.5 GS/s		
M4x.2330-x4	1.5 GHz	4 GiSample	5 GS/s			
M4x.2333-x4	1.5 GHz	4 GiSample	5 GS/s	2.5 GS/s		
M4x.2334-x4	1.5 GHz	4 GiSample	5 GS/s	2.5 GS/s	1.25 GS/s	

Options

Order no.	Option
M4i.23xx-ir40m	Low voltage input range option for 23xx series. 4 Input ranges with ± 40 mV, ± 100 mV, ± 200 mV, ± 500 mV, bandwidth limited.

Firmware Options

Order no.	Option
M4i.xxxx-spavg	Signal Processing Firmware Option: Block Average (later firmware-upgrade available)
M4i.xxxx-spstat	Signal Processing Firmware Option: Block Statistics/Peak Detect (later firmware-upgrade available)
M4i.xxxx-PulseGen	Firmware Option: adds 4 freely programmable digital pulse generators that use the XIO lines for output (later installation by firmware -upgrade available)

Services

Order no.	
Recal	Recalibration at Spectrum incl. calibration protocol
Card-Prot-17025	ISO 17025 Calibration Certificate for one card; add-on for new cards or for recalibration

Standard Cables

for Connections	Length	Order no.				
		to BNC male	to BNC female	to SMA male	to SMA female	to SMB female
Analog/Clock-In/Trig-In	80 cm	Cab-3mA-9m-80	Cab-3mA-9f-80	Cab-3mA-3mA-80		Cab-3f-3mA-80
Analog/Clock-In/Trig-In	200 cm	Cab-3mA-9m-200	Cab-3mA-9f-200	Cab-3mA-3mA-200		Cab-3f-3mA-200
Probes (short)	5 cm		Cab-3mA-9f-5			
Clk-Out/Trig-Out/Extra	80 cm	Cab-1m-9m-80	Cab-1m-9f-80	Cab-1m-3mA-80	Cab-1m-3fA-80	Cab-1m-3f-80
Clk-Out/Trig-Out/Extra	200 cm	Cab-1m-9m-200	Cab-1m-9f-200	Cab-1m-3mA-200	Cab-1m-3fA-200	Cab-1m-3f-200
Information	The standard adapter cables are based on RG174 cables and have a nominal attenuation of 0.3 dB/m at 100 MHz and 0.5 dB/m at 250 MHz. For high speed signals we recommend the low loss cables series CHF					

Low Loss Cables

Order No.	Option
CHF-3mA-3mA-200	Low loss cables SMA male to SMA male 200 cm
CHF-3mA-9m-200	Low loss cables SMA male to BNC male 200 cm
Information	The low loss adapter cables are based on MF141 cables and have an attenuation of 0.3 dB/m at 500 MHz and 0.5 dB/m at 1.5 GHz. They are recommended for signal frequencies of 200 MHz and above.

Amplifiers

Order no.	Bandwidth	Connection	Input Impedance	Coupling	Amplification
SPA.1841 ⁽²⁾	2 GHz	SMA	50 Ohm	AC	x100 (40 dB)
SPA.1801 ⁽²⁾	2 GHz	SMA	50 Ohm	AC	x10 (20 dB)
SPA.1601 ⁽²⁾	500 MHz	BNC	50 Ohm	DC	x10 (20 dB)
Information	External Amplifiers with one channel, BNC/SMA female connections on input and output, manually adjustable offset, manually switchable settings. An external power supply for 100 to 240 VAC is included. Please be sure to order an adapter cable matching the amplifier connector type and matching the connector type for your A/D card input.				

Software SBench6

Order no.	
SBench6	Base version included in delivery. Supports standard mode for one card.
SBench6-Pro	Professional version for one card: FIFO mode, export/import, calculation functions, ...
SBench6-Multi	Option multiple cards: Needs SBench6-Pro. Handles multiple synchronized cards in one system.
Volume Licenses	Please ask Spectrum for details.

Software Options

Order no.	
SPc-RServer	Remote Server Software Package - LAN remote access for M2i/M3i/M4i/M4x/M2p/M5i cards
SPc-SCAPP	Spectrum's CUDA Access for Parallel Processing - SDK for direct data transfer between Spectrum card and CUDA GPU. Includes RDMA activation and examples. Only working for Data Acquisition or AWG mode, not usable for DDS mode

⁽¹⁾ : Just one of the options can be installed on a card at a time.

⁽²⁾ : Third party product with warranty differing from our export conditions. No volume rebate possible.

Hardware Installation

ESD Precautions

All Spectrum boards contain electronic components that can be damaged by electrostatic discharge (ESD).

Before installing the board in your system or protective conductive packaging, discharge yourself by touching a grounded bare metal surface or approved anti-static mat before picking up this ESD sensitive product.



Sources of noise

Noise sensitive analog devices, such as analog acquisition and generator boards should be placed physically as far away from any noise producing source (like e.g. the power supply) as possible. It should especially be avoided to place the board in the slot directly adjacent to another fast board like e.g. a graphics controller.

Cooling Precautions

The boards of the M4i.xxxx-x8 and M4x.xxxx-x4 series operate with components having very high power consumption at high speeds. For this reason it is absolutely required to cool the boards sufficiently.

For all M4i cards it is absolutely mandatory to have installed cooling fans specifically providing a stream of air across the board's surface.



- Make absolutely sure, that the on-board fan on the M4i card is not blocked by PC internal cabling or any other means.
- Ensure that there is plenty of space around the PC chassis fan's intake and exhaust vents, both inside and outside the chassis.
- If your chassis includes fan filters, make sure that these are regularly cleaned.
- Set the rotation speed for all chassis fans and especially those providing air for the PCIe/PXle cards to highest setting in the BIOS/UEFI.
- Whenever possible leave the slot adjacent to the M4i/M4x card empty. This allows for best possible air flow over the card's surface.
- If you do need to use any adjacent slots, preferably install cards, that grant the most clearance between the devices, such as low-profile adapters.
- If available install filler panels with ventilation holes for all unused PCI or PCI Express slots to allow for additional air flow for the M4i cards and serve as an additional outtake.

Connector Handling Precautions

The connectors used on this product are designed for high signal quality and good shielding. Due to the limited space on the front-panel they have to be as small as possible to fit the needed signal connections on the front panel. Therefore these connectors are vulnerable to mechanical damages when used not properly. Especially SMB and MMCX connectors may be broken when not operated correctly.

Always dismount the connections by operating the connector itself and not the cable. Always move the cable connector in a straight line from the board connector. Do not cant the connector when opening the connection. A broken connector can only be replaced in factory and is not covered by warranty.



M4i PCIe Cards

System Requirements

All Spectrum M4i.xxxx-x8 instrumentation cards are compliant to the PCI Express 2.0 standard and require in general one free 3/4 length PCI Express slot. This can mechanically either be a x8 or x16 slot, electrically all lane widths are supported, be it x1, x4, x8 or x16. Please consult your mainboard manual for details. Depending on the installed options additional free slots can be necessary.

Installing the M4i board in the system

Please be sure that the system is powered-down and all power cables are disconnected from the system before starting with the installation process.

Installing a single board without any options

Before installing the board you first need to unscrew and remove the dedicated blind-bracket usually mounted to cover unused slots of your PC. Please keep the screw in reach to fasten your Spectrum card afterwards. All Spectrum M4i cards mechanically require one PCI Express x8 or x16 slot (electrically either x1, x4, x8 or x16). Now insert the board slowly into your computer. This is done best with one hand each at both fronts of the board.

Please take especial care to not bend the card in any direction while inserting it into the system. Bending of the card may damage the PCB totally and is not covered by the standard warranty.



Please be very careful when inserting the board in the slot, as most of the mainboards are mounted with spacers and therefore might be damaged if they are exposed to high pressure.



After the insertion of the board fasten the screw of the bracket carefully, without overdoing.

Installing the M4i.xxxx-x8 PCI Express card in a PCIe x8 or x16 slot:

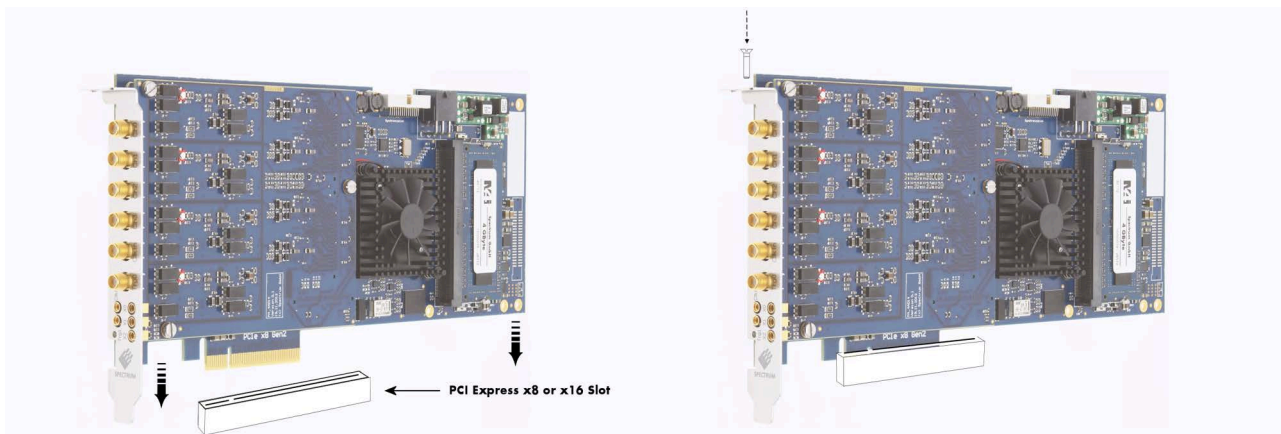


Image 4: Mounting M4i PCIe card into connector

Additional notes on PCIe x16 slot retention

M4i-xxx-x8 cards starting with hardware version V7 (which includes the new PCB revision V1.2) do have an additional PCIe retention hook (hockey stick) added to the PCB.

That allows the card to be additionally locked when being installed into a PCIe x16 slot.

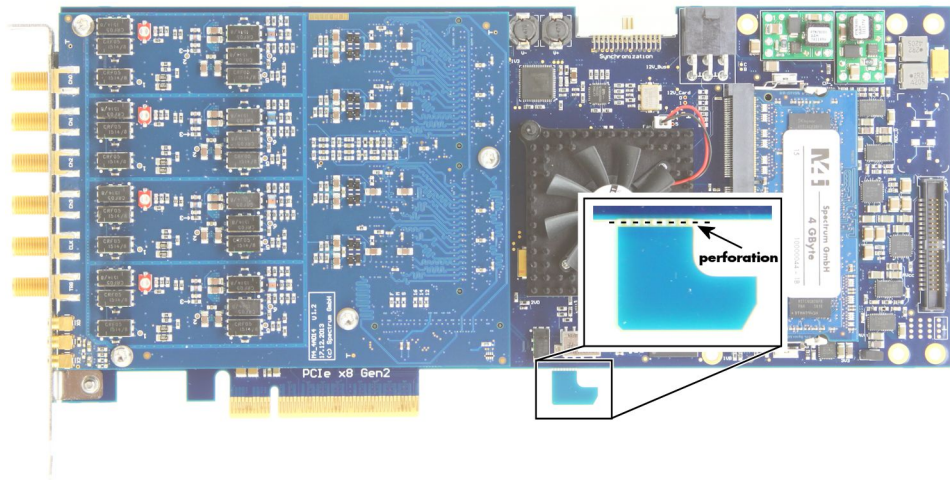


Image 5: M4i card slot retention with perforation

When installing the card in a x16 slot, make sure that the locking mechanism of the slots properly lock in place with the retention hook.



In the case that there are any components on the mainboard in the way of the retention hook when installing the card in an x8 slot, you can remove the hook by carefully breaking it off at its perforation line.



Providing additional power to M4i.xxxx-x8 cards

All PCI Express cards, with the exception of graphic adapters, are per specification only allowed to consume a maximum power of 25W per card. While some of the M4i PCIe cards are specified with a power consumption to meet these power limits, many do consume more than 25W of total power.

This is why all M4i cards can be optionally supplied with the required voltages via a dedicated PCIe 6-pin power connector directly from the system power supply.

As part of its power-on routine, the card will automatically detect, whether a cable is plugged or not and will give preference to the cable-supplied voltages.

Although it would be considered good practice to always provide the power via cable in case the card's rated power consumption is above the 25W limit, in typical system setups with one or at maximum two cards installed, not doing so and using just the slot power usually works out perfectly fine. Having more M4i cards in a system will definitely require a separate power cable per card.

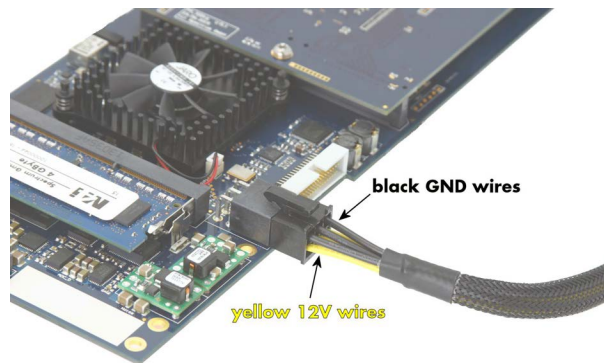


Image 6: M4i card additional power connection usage

Please only connect 6-pin PCIe power cables to the M4i cards power connector and make absolutely sure, that its three lower row wires are marked yellow (hence providing 12V) and the three upper row wires (the side of the connectors retention hook) are marked black providing a connection to system ground (GND), as shown on the picture.



Installing a M4i.44xx board with digital inputs/outputs mounted on an extra bracket

Before installing the board you first need to unscrew and remove the dedicated blind-bracket usually mounted to cover unused slots of your PC. Please keep the screw in reach to fasten your Spectrum card afterwards. All Spectrum M4i cards mechanically require one PCI Express x8 or x16 slot (electrically either x1, x4, x8 or x16). Now insert the board with it's attached extra bracket slowly into your computer. This is done best with one hand each at both fronts of the board.

Please take special care to not bend the card in any direction while inserting it into the system. A bending of the card may damage the PCB totally and is not covered by the standard warranty.



Please be very carefully when inserting the board in the PCI slot, as most of the mainboards are mounted with spacers and therefore might be damaged they are exposed to high pressure.



After the board's insertion fasten the screws of both brackets carefully, without overdoing. The figure shows a board with the option installed.



Image 7: M4i card with digital option mechanical installation and position of screws

Installing multiple boards synchronized by star-hub option

Precautions M4i cards with Star-Hub option (SH8ex)

Due to the length of the SMA connectors on the card's bracket in combination with the full-length of a card having the option SH8ex installed, it may be necessary with some computer case designs, to remove the black plastic retainer bracket from the end of the M4i card's main PCB to properly plug the card into the PCIe slot.

In case the retainer must be removed, an alternative to steadily holding the back of the PCB should then be implemented (if not already present in the case design).

This is especially critical, when the probability exists that the computer may be subject to sudden movement, shock or during shipment!

When fitting the card, please take care not to damage the motherboard with the lower edge of the metal front connector bracket.



Hooking up the boards

Before mounting several synchronized boards for a multi channel system into the PC you can hook up the cards with their synchronization cables first. If there is enough space in your computer's case (e.g. a big tower case) you can also mount the boards first and hook them up afterwards. Spectrum ships the card carrying the star-hub option together with the needed amount of synchronization cables. All of them are matched to the same length, to achieve a zero clock delay between the cards.

Only use the included flat ribbon cables.

All of the cards, **including the one that carries the star-hub piggy-back module**, must be wired to the star-hub.

It does not matter which of the available connectors on the star-hub module you use for which board. The software driver will detect the types and order of the synchronized boards automatically.

All of the synchronization cables are secured against wrong plugging, but nonetheless you should take care to have the pin 1 markers on the connector and on the cable on the same side, as the figure on the right is showing.


Mounting the wired boards

Before installing the cards you first need to unscrew and remove the dedicated blind-brackets usually mounted to cover unused slots of your PC. Please keep the screws in reach to fasten your Spectrum cards afterwards.

Spectrum M4i cards with the option „M4i.xxxx-SH8tm“ installed require two slots with $\frac{3}{4}$ PCIe length, whilst M4i cards with the option „M4i.xxxx-SH8ex“ installed require one single full length PCIe slot with a track at the backside to guide the card by its retainer.



Image 8: M4i cards with star-hub ex installed and connecting cables



Now insert the cards slowly into your computer. This is done best with one hand each at both fronts of the board.

While inserting the board take care not to tilt the retainer in the track. Please take especial care to not bend the card in any direction while inserting it in the system. A bending of the card may damage the PCB totally and is not covered by the standard warranty.



Please be very careful when inserting the cards in the slots, as most of the mainboards are mounted with spacers and therefore might be damaged if they are exposed to high pressure.



Shipment of systems with Spectrum cards installed

When shipping complete systems with Spectrum cards installed make sure that the cards are properly secured and cannot bend while being transported. When using freight forwarders, the transport and handling processes can be quite rough potentially subjecting the shipped PC system to quite large shocks. If the installed spectrum cards are not well mounted, secured correctly at the front and - if applicable for your model - back of the card, it's possible that they can bend when subjected to strong forces, such when a shipment container is dropped.

If damage occurs during a transport, we do not consider this to be covered by the warranty.

To avoid this we strongly recommend that when shipping these systems, customers either:

- Install the cards securely - with separate protection - so they cannot bend, or
- Remove the cards and ship them separately in their original shipping boxes (or similar packaging)

Please note that a sole fixing of the card at the front panel may not be sufficient to avoid damages in case of a mechanical shock!

M4x PXle Cards

System Requirements

The Spectrum M4x PXle 3U cards run in dedicated 3U PXle slots as well as 3U PXI/PXle hybrid slots. The M4x series of cards occupies two slots width, so up to eight cards can be installed in a large chassis providing 16 PXle slots for peripheral cards.

The M4x cards cannot be installed in either the CPU system slot nor in the dedicated system timing slot. Only a peripheral slot marked with the „circle“ symbol is suited for the cards.



Installing the M4x board in the system

Installing a single board without any options

The locks on the bottom side of PXle boards need to be unlocked and opened before installing the board into a free slot of the system. Therefore you need to press the little button on the inside of the fastener and move it outwards (see figure). Now slowly insert the card into the host system using the key ways until the lock snaps in with a „click“.

While inserting the board take care not to tilt it.



After the board's insertion fasten the four screws carefully, without overdoing.



Image 9: Installation of PXle cards with connector handling and mounting screws

Software Driver Installation and Driver Update

Before using the board, a driver must be installed that matches the operating system. Later on the same principles for the initial installation also apply, when updating an existing driver on the system to a newer version.

Since driver V3.33 (released on install-disk V3.48 in August 2017) the installation is done via an installer executable rather than manually via the Windows Device Manager. The steps for manually installing a card has since been moved to a separate application note „AN008 - Legacy Windows Driver Installation“.



This new installer is common on all currently supported Windows platforms (Windows 7, Windows 8, Windows 10 and Windows 11) both 32bit and 64bit. The driver from the USB-Stick supports all cards of the M2i/M3i, M4i/M4x, M2p and M5i series, meaning that you can use the same driver for all cards of these families. This driver installer is also available from the Spectrum homepage under <https://spectrum-instrumentation.com/support/downloads.php>

Windows

Before initial installation

When you install a card for the very first time, Windows will discover the new hardware and might try to search the Microsoft Website for available matching driver modules (where no matching driver will be found).

Prior to running the Spectrum installer, the card will hence appear in the Windows device manager as a generalized card, shown here is the device manager of a Windows 10 as an example.

- M2i and M3i cards will be shown as „DPIO module“
- M5i, M4i, M4x and M2p cards will be shown as „PCI Data Acquisition and Signal Processing Controller“

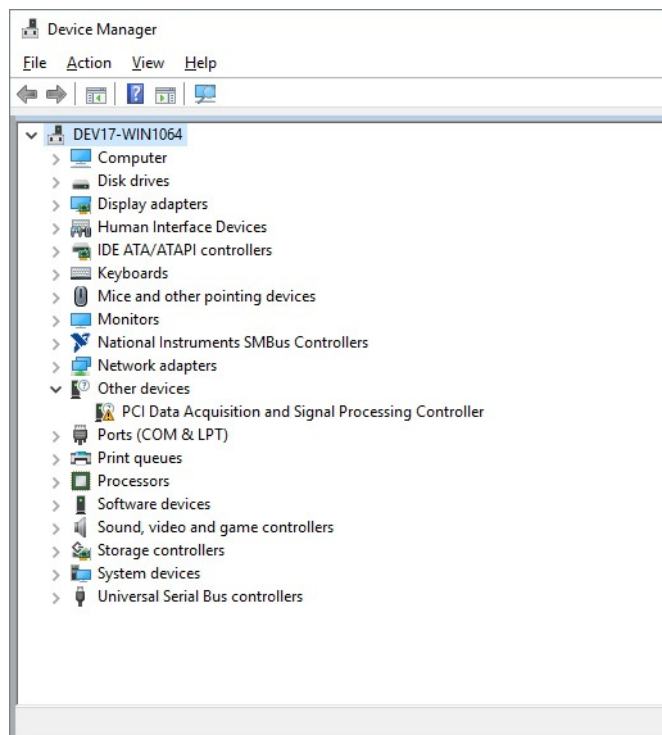


Image 10: Windows Device Manager showing a new Spectrum card

Running the driver Installer/Update

Simply run the installer supplied either on the USB-Stick "Driver\windows" folder or download it from our homepage and run it.

The installer can be run on a fresh system for the first install or also later on, when updating an already existing driver on the system.

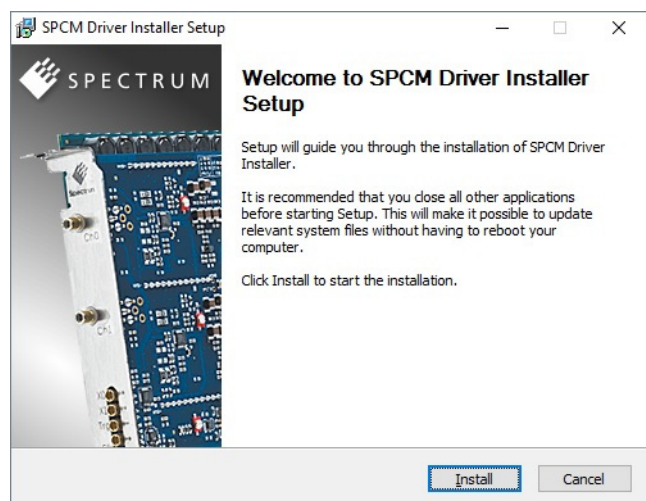


Image 11: Spectrum Driver Installer Welcome Screen

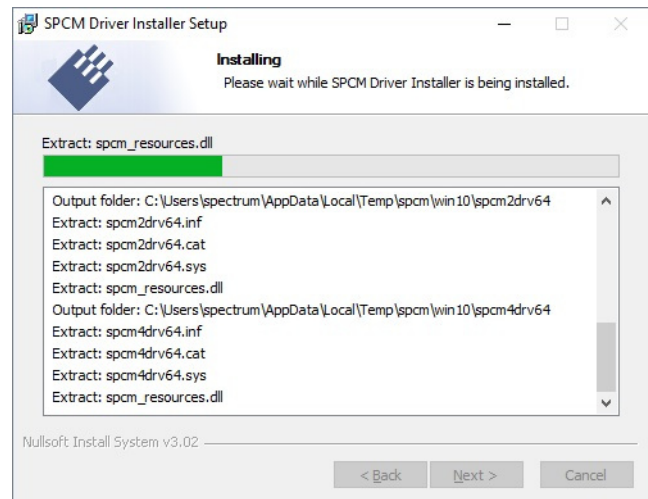


Image 12: Spectrum Driver Installer - Progress

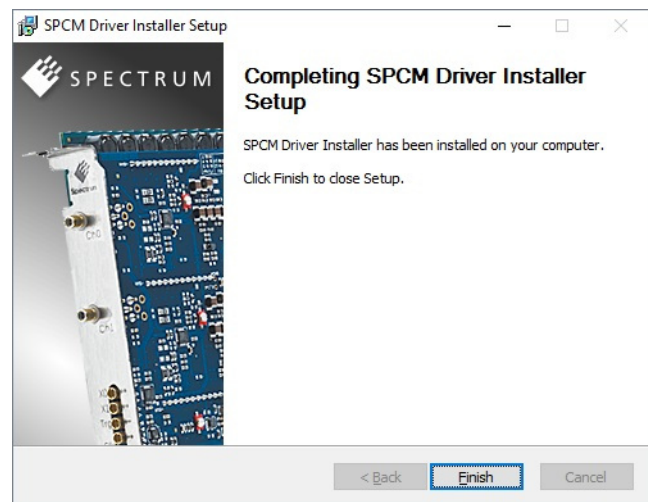


Image 13: Spectrum Driver Installer - finished

After installation

After running the Spectrum driver installer, the card will appear in the Windows device manager with its name matching the card series.

The card is now ready to be used with the new or updated driver.

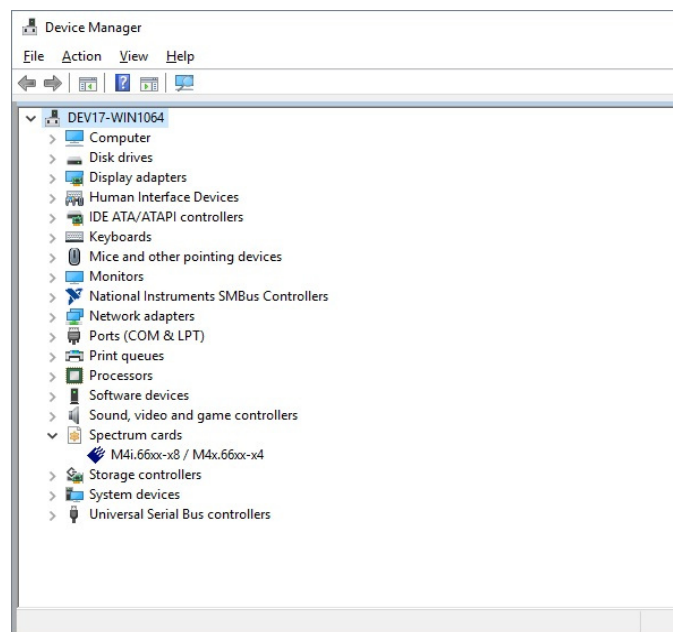


Image 14: Windows Device Manager showing properly installed Spectrum card

Linux

Overview

The Spectrum M2i/M3i/M4i/M4x/M2p/M5i cards and digitizerNETBOX/generatorNETBOX or hybridNETBOX products are delivered with Linux drivers for 64 bit systems. As each Linux distribution contains different kernel versions and different system setup it is in nearly every case necessary, to have a directly matching kernel driver for card level products to run it on a specific system.

For digitizerNETBOX/generatorNETBOX or hybridNETBOX products the library is sufficient and no kernel driver has to be installed.

Spectrum delivers pre-compiled kernel driver modules for a number of common distributions with the cards. You may try to use one of these kernel modules for different distributions which have a similar kernel version. Unfortunately this won't work in most cases as most Linux system refuse to load a driver which is not exactly matching. In this case it is possible to get the kernel driver sources from Spectrum. Please contact your local sales representative to get more details on this procedure.

The Standard delivery contains the pre-compiled kernel driver modules for the most popular Linux distributions, like Suse, Debian, Fedora and Ubuntu. The list with all pre-compiled and readily supported distributions and their respective kernel version can be found under: https://spectrum-instrumentation.com/support/knowledgebase/software/Supported_Linux_Distributions.php or via the shown QR code.

The Linux drivers have been tested with all above mentioned distributions by Spectrum. Each of these distributions has been installed with the default setup using no kernel updates. A lot more different distributions are used by customers with self compiled kernel driver modules.



Driver Installation with Installation Script

The driver is delivered as installable kernel modules together with libraries to access the kernel driver. The installation script will help you with the installation of the kernel module and the library.

This installation is only needed if you are operating real locally installed cards. For software emulated demo cards, remotely installed cards or for digitizerNETBOX/generatorNETBOX/hybridNETBOX products it is only necessary to install the libraries without a kernel as explained further below.



Login as root

It is necessary to have the root rights for installing a driver.

Call the `install.sh <install_path>` script

This script will try to use the package management of the system to install the kernel module and user-space driver library packages:

- the kernel driver package is called „`spcm`“ (M2i, M3i) or „`spcm4`“ (M4i, M4x, M2p, M5i)
- the driver library package is called „`libspcm_linux`“

Udev support

Once the driver is loaded it automatically generates the device nodes under `/dev`. The cards are automatically named to `/dev/spcm0`, `/dev/spcm1`,...

You may use all the standard naming and rules that are available with udev.

Start the driver

The kernel driver should be loaded automatically when the system boots. If you need to load the kernel driver manually use the „`modprobe`“ command (as root or using `sudo`):

For M2i and M3i cards:

```
modprobe spcm
```

For M5i, M4i, M4x and M2p cards:

```
modprobe spcm4
```

Get first driver info

After the driver has been loaded successfully some information about the installed boards can be found in the matching `/proc/` file as shown below. Some basic information from the on-board EEPROM is listed for every card.

For M2i and M3i cards:

```
cat /proc/spcm_cards
```

For M5i, M4i, M4x and M2p cards:

```
cat /proc/spcm4_cards
```

Stop the driver

You can unload the kernel driver using the „modprobe -r“ command (as root or using sudo):

For M2i and M3i cards:

```
modprobe -r spcm
```

For M5i, M4i, M4x and M2p cards:

```
modprobe -r spcm4
```

Standard Driver Update

A driver update is done with the same commands as shown above. Please make sure that the driver has been stopped before updating it. To stop the driver you may use the proper “modprobe -r” command as shown above.

Compilation of kernel driver sources (optional and local cards only)

The driver sources are only available for existing customers upon special request. Please send an email to Support@spec.de to receive the kernel driver sources. The driver sources are not part of the standard delivery. The driver source package contains only the sources of the kernel module, not the sources of the library.

Please do the following steps for compilation and installation of the kernel driver module:

Login as root

It is necessary to have the root rights for installing a driver.

Call the compile script

The compile script depends on the type of card that you have installed:

- for M2i and M3i cards: make_spcm_linux_kerneldrv.sh
- for M5i, M4i, M4x and M2p cards: make_spcm4_linux_kerneldrv.sh

This script will examine the type of system you use and compile the kernel with the correct settings. The compilation of the kernel driver modules requires the kernel sources of the running kernel. These are normally available as a package with a name like kernel-devel, kernel-dev, kernel-source and need to match the running kernel.

The compiled driver module will be copied to the module directory of the kernel (/lib/modules/\$(uname -r)/kernel/drivers/), and will be loaded automatically at the next boot. To load or unload the kernel driver module manually use the modprobe command as explained above in “Start the driver” and “Stop the driver”.

Update of a self compiled kernel driver

If the kernel driver has changed, one simply has to perform the same steps as shown above and recompile the kernel driver module. However the kernel driver module isn't changed very often.

Normally an update only needs new libraries. To update the libraries only you can either download the full Linux driver (spcm_linux_drv_v123b4567) and only use the libraries out of this or one downloads the library package which is much smaller and doesn't contain the pre-compiled kernel driver module (spcm_linux_lib_v123b4567).

The update is done with a dedicated script which only updates the library file. This script is present in both driver archives:

```
sh install_libonly.sh
```

Installing the library only without a kernel (for remote devices)

The kernel driver module only contains the basic hardware functions that are necessary to access locally installed card level products. The main part of the driver is located inside a dynamically loadable library that is delivered with the driver. This library is available in two different versions:

- `spcm_linux_32bit_std++6.so` - supporting `libstdc++6` on 32 bit systems
- `spcm_linux_64bit_std++6.so` - supporting `libstdc++6` on 64 bit systems

The matching version is installed automatically in the `"/usr/lib"` or `"/usr/lib64/"` or `"/usr/lib/x86_64-linux-gnu"` directory (depending on your Linux distribution) by the kernel driver install script for card level products. The library is renamed for easy access to `libspcm_linux.so`.

For digitizerNETBOX/generatorNETBOX/hybridNETBOX products and also for evaluating or using only the software simulated demo cards the library is installed with a separate install script:

```
sh install_libonly.sh
```

To access the driver library one must include the library in the compilation:

```
gcc -o test_prg -lspcm_linux test.cpp
```

To start programming the cards under Linux please use the standard C/C++ examples which are all running under Linux and Windows.

Installation from Spectrum Repository

The driver library, Spectrum Control Center and SBench6 can be easily installed and updated from our online repositories. Adding the repository to the system and installing software differs depending on the package format used by the Linux distribution.

DEB based distributions (like Debian, Ubuntu and derived distributions)

Execute the following commands to get the Spectrum repository key and convert it for local use:

```
wget http://spectrum-instrumentation.com/dl/repo-key.asc  
gpg --dearmor -o repo-key.gpg repo-key.asc  
cp repo-key.gpg /etc/apt/spectrum-instrumentation.gpg
```

To add the repository create a new file `/etc/apt/sources.list.d/spectrum-instrumentation.list` with this content. Please note that there is a mandatory blank between URL and `"/"`:

```
deb [signed-by=/etc/apt/spectrum-instrumentation.gpg] http://spectrum-instrumentation.com/dl/ ./
```

Alternatively this line can be added to `/etc/apt/sources.list`

Then run

```
sudo apt update
```

to update the repository information.

To install the software (e.g. SBench6) run

```
sudo apt install sbench6
```

An overview of DEB based distributions can be found here: https://en.wikipedia.org/wiki/Category:Debian-based_distributions

RPM based distributions

On distributions using Zypper (such as openSUSE, SLES, ...) to add the repository run:

```
sudo zypper ar --repo http://spectrum-instrumentation.com/dl/spectrum_instrumentation.repo
```

The repository information will be updated automatically.

To install the software (e.g. SBench6) run

```
sudo zypper install SBench6
```

On distributions using DNF (such as Fedora, CentOS Stream, RHEL, ...) to add the repository run

```
sudo dnf config-manager --add-repo http://spectrum-instrumentation.com/dl/spectrum_instrumentation.repo
```

The repository information will be updated automatically.

To install the software (e.g. SBench6) run

```
sudo dnf install SBench6
```

An overview of RPM based distributions can be found here: https://en.wikipedia.org/wiki/Category:RPM-based_Linux_distributions

Control Center

The Spectrum Control Center is also available for Linux and needs to be installed separately. The features of the Control Center are described in a later chapter in deeper detail. The Control Center has been tested under all Linux distributions for which Spectrum delivers pre-compiled kernel modules. The following packages need to be installed to run the Control Center:

- X-Server
- expat
- freetype
- fontconfig
- libpng
- libspcm_linux (the Spectrum Linux driver library)

Installation

Use the supplied packages in either *.deb or *.rpm format found in the driver section of the USB stick by double clicking the package file root rights from a X-Windows window.

The Control Center is installed under KDE, Gnome or Unity in the system/system tools section. It may be located directly in this menu or under a „More Programs“ menu. The final location depends on the used Linux distribution. The program itself is installed as /usr/bin/spcmcontrol and may be started directly from here.

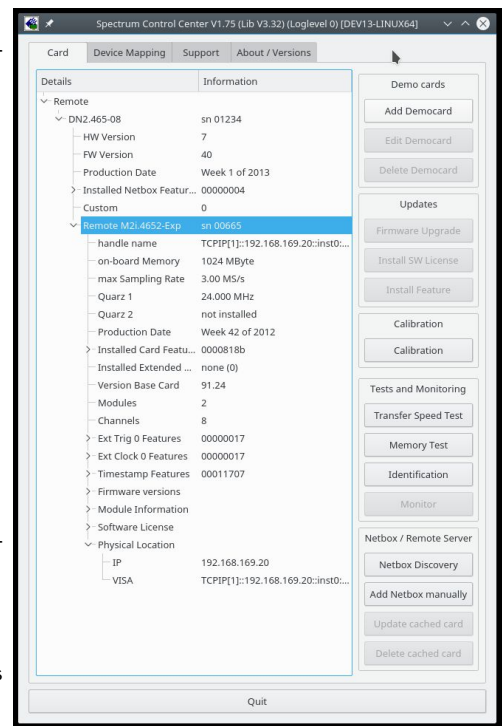


Image 15: Device Manager showing a new Spectrum card

Manual Installation

To manually install the Control Center, first extract the files from the rpm matching your distribution:

```
rpm2cpio spcmcontrol-{Version}.rpm > ~/spcmcontrol-{Version}.cpio
cd ~/
cpio -id < spcmcontrol-{Version}.cpio
```

You get the directory structure and the files contained in the rpm package. Copy the binary spcmcontrol to /usr/bin. Copy the .desktop file to /usr/share/applications. Run ldconfig to update your systems library cache. Finally you can run spcmcontrol.

Troubleshooting

If you get a message like the following after starting spcmcontrol:

```
spcm_control: error while loading shared libraries: libz.so.1: cannot open shared object file: No such file or directory
```

Run `ldd spcm_control` in the directory where `spcm_control` resides to see the dependencies of the program. The output may look like this:

```
libXext.so.6 => /usr/X11R6/lib/libXext.so.6 (0x4019e000)
libX11.so.6 => /usr/X11R6/lib/libX11.so.6 (0x401ad000)
libz.so.1 => not found
libdl.so.2 => /lib/libdl.so.2 (0x402ba000)
libpthread.so.0 => /lib/tls/libpthread.so.0 (0x402be000)
libstdc++.so.6 => /usr/lib/libstdc++.so.6 (0x402d0000)
```

As seen in the output, one of the libraries isn't found inside the library cache of the system. Be sure that this library has been properly installed. You may then run `ldconfig`. If this still doesn't help please add the library path to `/etc/ld.so.conf` and run `ldconfig` again.

If the `libspcm_linux.so` is quoted as missing please make sure that you have installed the card driver properly before. If any other library is stated as missing please install the matching package of your distribution.

Software

This chapter gives you an overview about the structure of the drivers and the software, where to find and how to use the examples. It shows in detail, how the drivers are included using different programming languages and deals with the differences when calling the driver functions from them.

This manual only shows the use of the standard driver API. For further information on programming drivers for third-party software like LabVIEW, MATLAB, IVI or SCAPP an additional manual is required that is available on the USB stick or by download from our homepage.



Software Overview

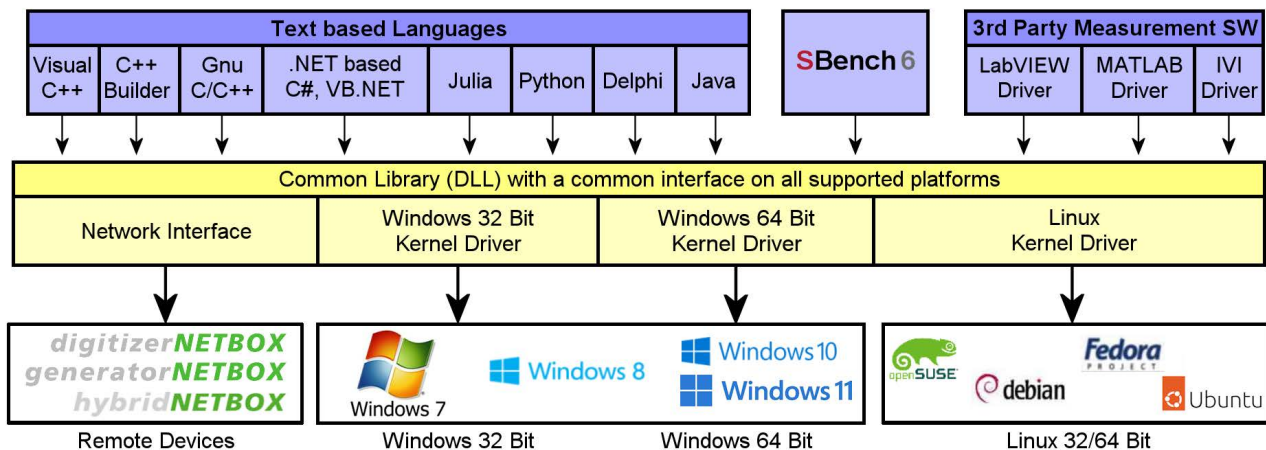


Image 16: Spectrum Kernel Driver, API Library and Software structure

The Spectrum drivers offer you a common and fast API for using all of the board hardware features. This API is the same on all supported operating systems. Based on this API one can write own programs using any programming language that can access the driver API. This manual describes in detail the driver API, providing you with the necessary information to write your own programs. The drivers for third-party products like LabVIEW or MATLAB, IVI or SCAPP are also based on this API. The special functionality of these drivers is not subject of this document and is described with separate manuals available on the USB stick or on the website.

Card Control Center

A special Card Control Center is available on the USB stick and from the internet for all Spectrum M2i/M3i/M4i/M4x/M2p/M5i cards and for all digitizerNETBOX, generatorNETBOX or hybridNETBOX products. Windows users find the Control Center installer on the USB stick under „Install\win\spcmcontrol_install.exe“.

Linux users find the versions for the different stdc++ libraries under /Install/linux/spcm_control_center/ as RPM packages.

When using a digitizerNETBOX/generatorNETBOX/hybridNETBOX the Card Control Center installers for Windows and Linux are also directly available from the integrated webserver.

The Control Center under Windows and Linux is available as an executive program. Under Windows it is also linked as a system control and can be accessed directly from the Windows control panel. Under Linux it is also available from the KDE System Settings, the Gnome or Unity Control Center. The different functions of the Spectrum Card Control Center are explained in detail in the following passages.

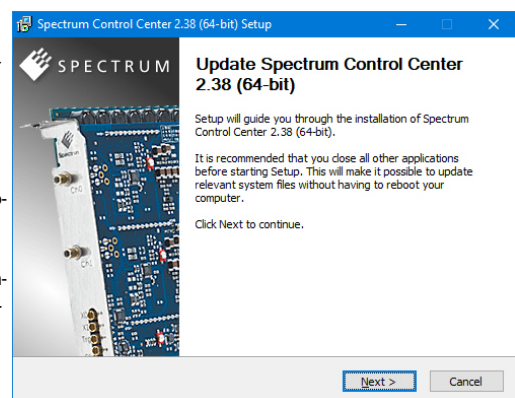


Image 17: Spectrum Control Center Installer



To install the Spectrum Control Center you will need to be logged in with administrator rights for your operating system. On all Windows versions, starting with Windows Vista, installations with enabled UAC will ask you to start the installer with administrative rights (run as administrator).

Discovery of Remote Cards, digitizerNETBOX/generatorNETBOX/hybridNETBOX products

The Discovery function helps you to find and identify the Spectrum LXI instruments like digitizerNETBOX, generatorNETBOX or hybridNETBOX available to your computer on the network. The Discovery function will also locate Spectrum card products handled by an installed Spectrum Remote Server somewhere on the network. The function is not needed if you only have locally installed cards.

Please note that only remote products are found that are currently not used by another program. Therefore in a bigger network the number of Spectrum products found may vary depending on the current usage of the products.

Execute the Discovery function by pressing the „Discovery“ button. There is no progress window shown. After the discovery function has been executed the remotely found Spectrum products are listed under the node Remote as separate card level products. Inhere you find all hardware information as shown in the next topic and also the needed VISA resource string to access the remote card.

Please note that these information is also stored on your system and allows Spectrum software like SBench 6 to access the cards directly once found with the Discovery function.

After closing the control center and re-opening it the previously found remote products are shown with the prefix cached, only showing the card type and the serial number. This is the stored information that allows other Spectrum products to access previously found cards. Using the „Update cached cards“ button will try to re-open these cards and gather information of it. Afterwards the remote cards may disappear if they're in use from somewhere else or the complete information of the remote products is shown again.

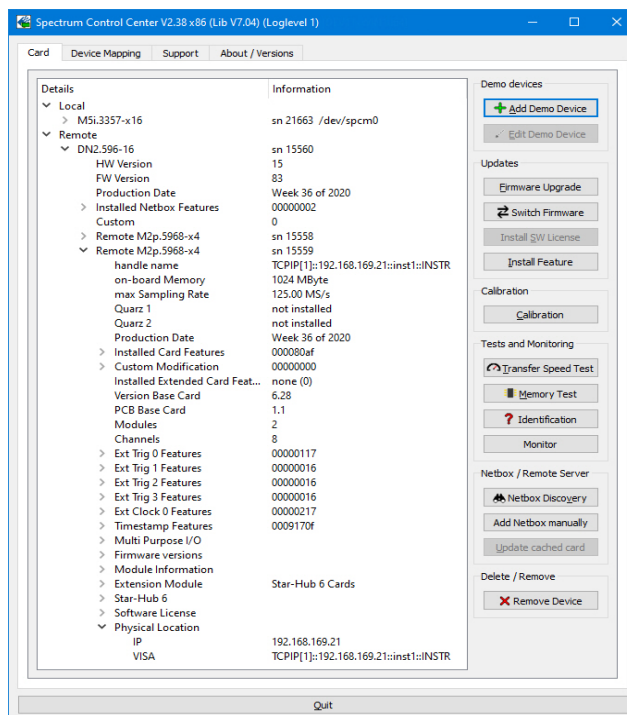


Image 18: Spectrum Control Center showing detail card information

Enter IP Address of digitizerNETBOX/generatorNETBOX/hybridNETBOX manually

If for some reason an automatic discovery is not suitable, such as the case where the remote device is located in a different subnet, it can also be manually accessed by its type and IP address.

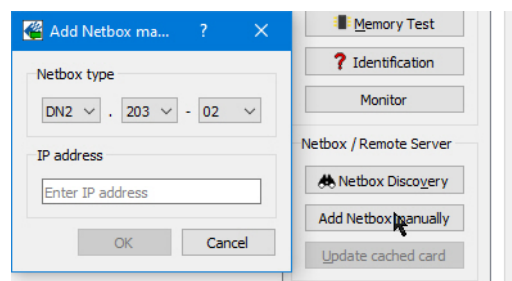


Image 19: Spectrum Control Center - entering an IP address for a NETBOX

Wake On LAN of digitizerNETBOX/generatorNETBOX/hybridNETBOX

Cached digitizerNETBOX/generatorNETBOX/hybridNETBOX products that are currently in standby mode can be woken up by using the „Wake remote device“ entry from the context menu.

The Control Center will broadcast a standard Wake On LAN „Magic Packet“, that is sent to the device's MAC address.

It is also possible to use any other Wake On LAN software to wake e.g. a digitizerNETBOX by sending such a „Magic Packet“ to the MAC address, which must be then entered manually.

It is also possible to wake a remote device from your own application software by using the SPC_NETBOX_WAKEONLAN register. To wake a digitizerNETBOX, generatorNETBOX or hybridNETBOX with the MAC address „00:03:2d:20:48:ec“, the following command can be issued:

```
spcm_dwSetParam_i64 (NULL, SPC_NETBOX_WAKEONLAN, 0x00032d2048ec);
```

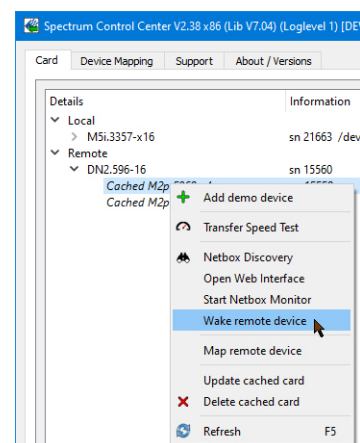


Image 20: Spectrum Control Center: wake on LAN for a cached card

Netbox Monitor

The Netbox Monitor permanently monitors whether the digitizerNETBOX/generatorNETBOX/hybridNETBOX is still available through LAN. This tool is helpful if e.g. the digitizerNETBOX is located somewhere in the company LAN or located remotely or directly mounted inside another device. Starting the Netbox Monitor can be done in two different ways:

- Starting manually from the Spectrum Control Center using the context menu as shown above
- Starting from command line. The Netbox Monitor program is automatically installed together with the Spectrum Control Center and is located in the selected install folder. Using the command line tool one can place a simple script into the autostart folder to have the Netbox Monitor running automatically after system boot. The command line tool needs the IP address of the digitizerNETBOX/generatorNETBOX/hybridNETBOX to monitor:

```
NetboxMonitor 192.168.169.22
```

The Netbox Monitor is shown as a small window with the type of digitizerNETBOX/generatorNETBOX in the title and the IP address under which it is accessed in the window itself. The Netbox Monitor runs completely independent of any other software and can be used in parallel to any application software. The background of the IP address is used to display the current status of the device. Pressing the Escape key or alt + F4 (Windows) terminates the Netbox Monitor permanently.



After starting the Netbox Monitor it is also displayed as a tray icon under Windows. The tray icon itself shows the status of the digitizerNETBOX/generatorNETBOX/hybridNETBOX as a color. Please note that the tray icon may be hidden as a Windows default and need to be set to visible using the Windows tray setup.

Left clicking on the tray icon will hide/show the small Netbox Monitor status window. Right clicking on the tray icon as shown in the picture on the right will open up a context menu. In here one can again select to hide/show the Netbox Monitor status window, one can directly open the web interface from here or quit the program (including the tray icon) completely.




Image 21: Netbox Monitor activation

The checkbox „Show Status Message“ controls whether the tray icon should emerge a status message on status change. If enabled (which is default) one is notified with a status message if for example the LAN connection to the digitizerNETBOX/generatorNETBOX/hybridNETBOX is lost.

The status colors:

- Green: digitizerNETBOX/generatorNETBOX/hybridNETBOX available and accessible over LAN
- Cyan: digitizerNETBOX/generatorNETBOX/hybridNETBOX is used from my computer
- Yellow: digitizerNETBOX/generatorNETBOX/hybridNETBOX is used from a different computer
- Red: LAN connection failed, digitizerNETBOX/generatorNETBOX/hybridNETBOX is no longer accessible

Device identification

Pressing the *Identification* button helps to identify a certain device in either a remote location, such as inside a 19" rack where the back of the device with the type plate is not easily accessible, or a local device installed in a certain slot. Pressing the button starts flashing a visible LED on the device, until the dialog is closed, for:

- On a digitizerNETBOX/generatorNETBOX/hybridNETBOX: the LAN LED light on the front plate of the device
- On local or remote M5i, M4i, M4x or M2p card: the indicator LED on the card's bracket

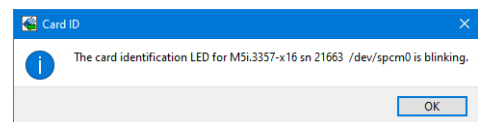


Image 22: Device Identification

This feature is not available for M2i/M3i cards, either local or remote, other than inside a digitizerNETBOX or generatorNETBOX.

Hardware information

Through the Control Center you can easily get the main information about all the installed Spectrum hardware. For each installed card there is a separate tree of information available. The picture shows the information for one installed card by example. This given information contains:

- Basic information as the type of card, the production date and its serial number, as well as the installed memory, the hardware revision of the base card, the number of available channels and installed acquisition modules.
- Information about the maximum sampling clock and the available quartz clock sources.
- The installed features/options in a sub-tree. The shown card is equipped for example with the option Multiple Recording, Gated Sampling, Timestamp and ABA-mode.
- Detailed Information concerning the installed acquisition modules. In case of the shown analog acquisition card the information consists of the module's hardware revision, of the converter resolution and the last calibration date as well as detailed information on the available analog input ranges, offset compensation capabilities and additional features of the inputs.

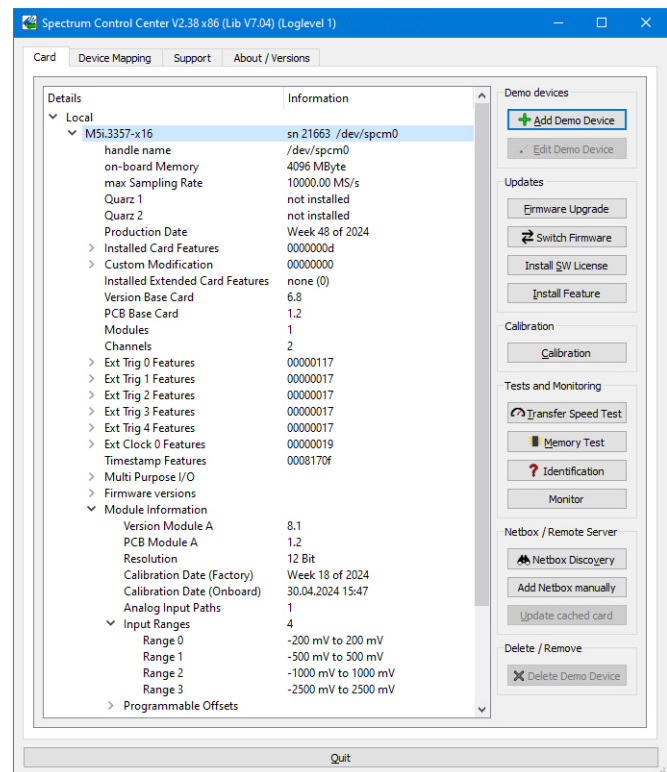


Image 23: Spectrum Control Center: detailed hardware information on installed card

Firmware information

Another sub-tree is informing about the cards firmware version. As all Spectrum cards consist of several programmable components, there is one firmware version per component.

Nearly all of the components firmware can be updated by software. The only exception is the configuration device, which only can receive a factory update.

The procedure on how to update the firmware of your Spectrum card with the help of the card control center is described in a dedicated section later on.

The procedure on how to update the firmware of your digitizerNETBOX/generatorNETBOX/hybridNETBOX with the help of the integrated Webserver is described in a dedicated chapter later on.

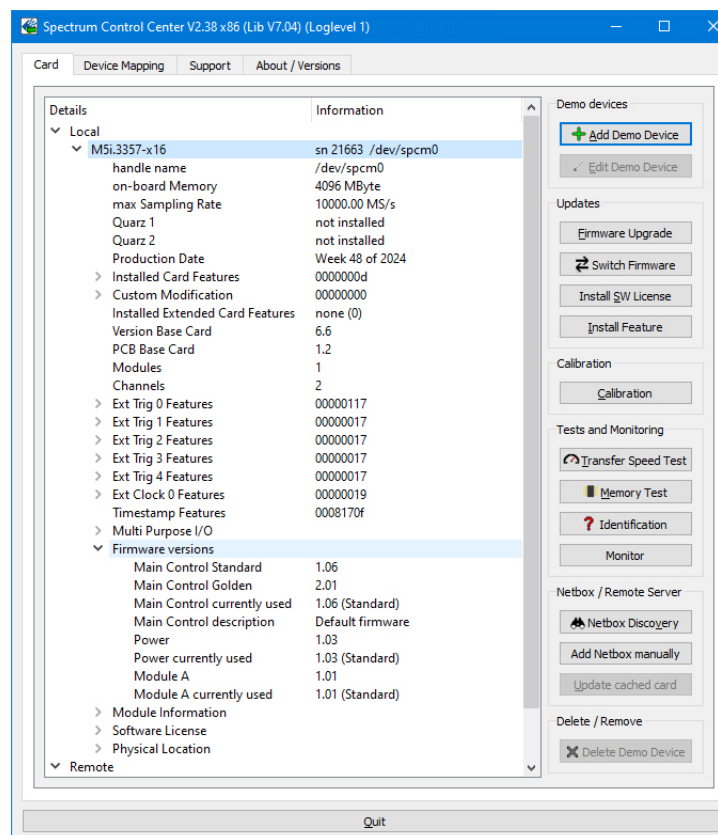


Image 24: Spectrum Control Center - showing firmware information of an installed card

Software License information

This sub-tree is informing about installed possible software licenses.

As a default all cards come with the demo professional license of SBench6, that is limited to 30 starts of the software with all professional features unlocked.

The number of demo starts left can be seen here.

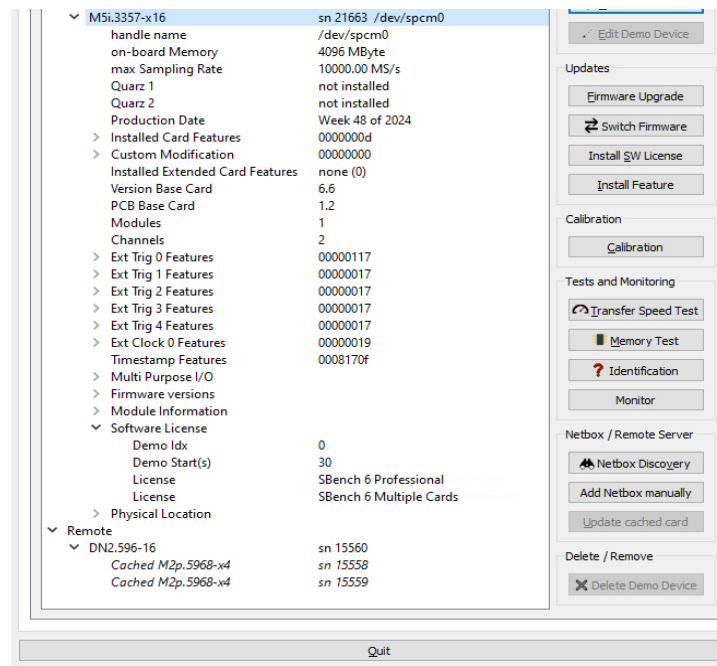


Image 25: Spectrum Control Center - showing software license information of an installed card

Driver information

The Spectrum card control center also offers a way to gather information on the installed and used Spectrum driver.

The information on the driver is available through a dedicated tab, as the picture is showing in the example.

The provided information informs about the used type, distinguishing between Windows or Linux driver and the 32 bit or 64 bit type.

It also gives direct information about the version of the installed Spectrum kernel driver, separately for M2i/ M3i cards and M4i/M4x/M2p/M5i cards and the version of the library (which is the *.dll file under Windows).

The information given here can also be found under Windows using the device manager from the control panel. For details in driver details within the control panel please stick to the section on driver installation in your hardware manual.

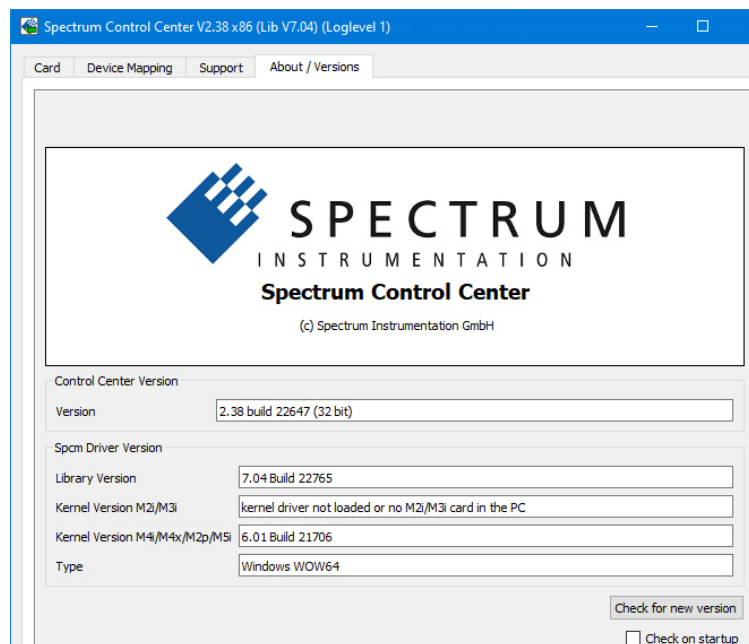


Image 26: Spectrum Control Center - showing driver information details

Installing and removing Demo cards

With the help of the card control center one can install demo cards in the system. A demo card is simulated by the Spectrum driver including data production for acquisition cards. As the demo card is simulated on the lowest driver level all software can be tested including SBench, own applications and drivers for third-party products like LabVIEW. The driver supports up to 64 demo cards at the same time. The simulated memory as well as the simulated software options can be defined when adding a demo card to the system.

Please keep in mind that these demo cards are only meant to test software and to show certain abilities of the software. They do not simulate the complete behavior of a card, especially not any timing concerning trigger, recording length or FIFO mode notification. The demo card will calculate data every time directly after been called and give it to the user application without any more delay. As the calculation routine isn't speed optimized, generating demo data may take more time than acquiring real data and transferring them to the host PC.

Installed demo cards are listed together with the real hardware in the main information tree as described above. Existing demo cards can be deleted by clicking the related button. The demo card details can be edited by using the edit button. It is for example possible to virtually install additional feature to one card or to change the type to test with a different number of channels.

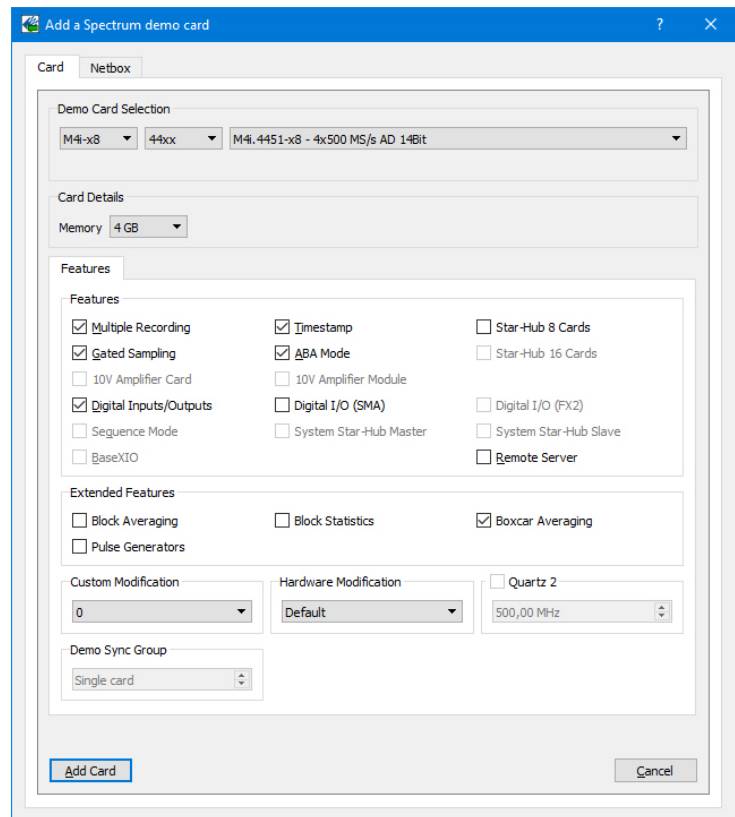


Image 27: Spectrum Control Center - adding a demo card to the system

For installing demo cards on a system without real hardware simply run the Control Center installer. If the installer is not detecting the necessary driver files normally residing on a system with real hardware, it will simply install the Spcm_driver.



Feature upgrade

All optional features of the M2i/M3i/M4i/M4x/M2p/M5i cards that do not require any hardware modifications can be installed on fielded cards. After Spectrum has received the order, the customer will get a personalized upgrade code. Just start the card control center, click on „install feature“ and enter that given code. After a short moment the feature will be installed and ready to use. No restart of the host system is required.

For details on the available options and prices please contact your local Spectrum distributor.

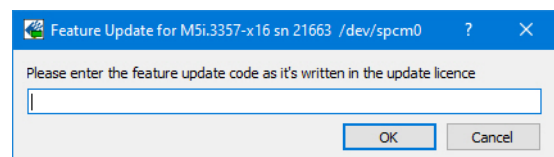


Image 28: Spectrum Control Center - feature update, code entry

Software License upgrade

The software license for SBench 6 Professional is installed on the hardware. If ordering a software license for a card that has already been delivered you will get an upgrade code to install that software license. The upgrade code will only match for that particular card with the serial number given in the license. To install the software license please click the „Install SW License“ button and type in the code exactly as given in the license.

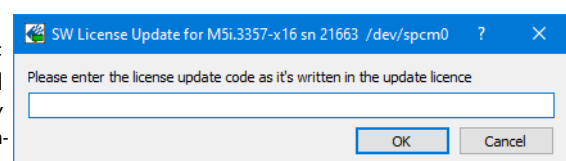


Image 29: Spectrum Control Center - software license install

Performing card calibration

The Card Control Center also provides an easy way to access the automatic card calibration routines of the Spectrum Cards, if that feature is supported by the hardware.

On-board calibration is supported by all A/D converter cards and some D/A converter cards. Depending on the used card family this can affect offset calibration only or also might include gain calibration. Please refer to the dedicated chapter in your hardware manual for details.

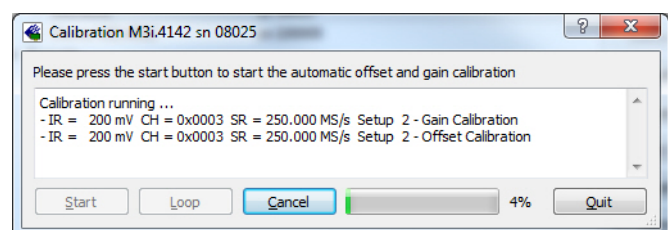


Image 30: Spectrum Control Center - running an on-board calibration

This function is not available for digital I/O cards and some D/A cards.

Performing memory test

The complete on-board memory of the Spectrum M2i/M3i/M4i/M4x/M2p/M5i cards can be tested by the memory test included with the card control center.

When starting the test, randomized data is generated and written to the on-board memory. After a complete write cycle all the data is read back and compared with the generated pattern.

Depending on the amount of installed on-board memory, and your computer's performance this operation might take a while.

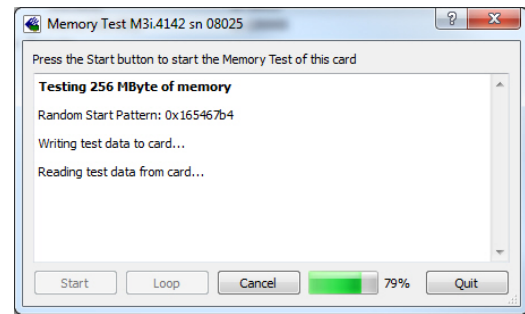


Image 31: Spectrum Control Center - performing memory test

Transfer speed test

The control center allows to measure the bus transfer speed of an installed Spectrum card. Therefore different setup is run multiple times and the overall bus transfer speed is measured. To get reliable results it is necessary that you disable debug logging as shown below. It is also highly recommended that no other software or time-consuming background threads are running on that system. The speed test program runs the following two tests:

- Repetitive Memory Transfers: single DMA data transfers are repeated and measured. This test simulates the measuring of pulse repetition frequency when doing multiple single-shots. The test is done using different block sizes. One can estimate the transfer in relation to the transferred data size on multiple single-shots.
- FIFO mode streaming: this test measures the streaming speed in FIFO mode. The test can only use the same direction of transfer the card has been designed for (card to PC = read for all DAQ (data acquisition) cards, PC to card = write for all generator cards and both directions for I/O cards). The streaming speed is tested without using the front-end to measure the maximum bus speed that can be reached. The Speed in FIFO mode depends on the selected notify size which is explained later in this manual in greater detail.

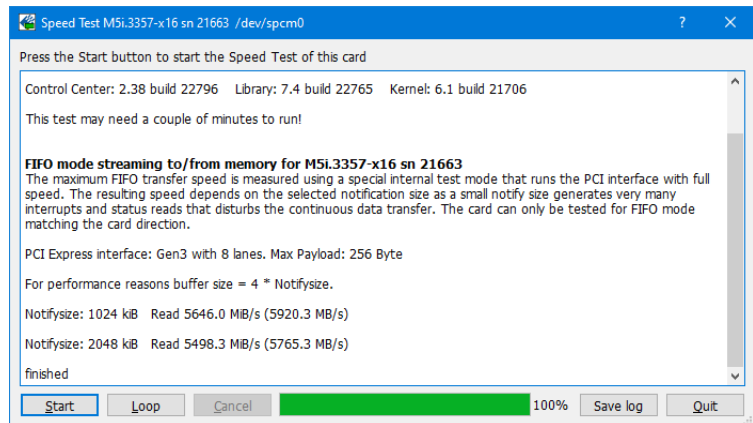


Image 32: Spectrum Control Center - running a transfer speed test of one card

The results are given in MiB/s (Mebibyte = 1024 * 1024 bytes) and MB/s (Megabyte = 1000 * 1000 bytes). To estimate whether a desired acquisition speed is possible to reach, one has to calculate the transfer speed in bytes. There are a few things that have to be put into the calculation:

- 12, 14 and 16 bit analog cards need two bytes for each sample.
- 16 channel digital cards need 2 bytes per sample while 32 channel digital cards need 4 bytes and 64 channel digital cards need 8 bytes.
- The sum of analog channels must be used to calculate the total transfer rate.
- The figures in the Speed Test Utility are given as MiBytes, meaning 1024 * 1024 Bytes, 1 MiByte = 1048576 Bytes

As an example running a card with two 16 bit analog channels with 28 MSps produces a transfer rate of $[2 \text{ channels} * 2 \text{ Bytes/Sample} * 28000000] = 112000000 \text{ Bytes/second} = 112 \text{ MB/s}$. When expressing this in Mebibytes, this would equal to $[112000000 / 1024 / 1024] = 106.8 \text{ MiB/s}$. For convenience, the Control Center presents both values.

Unfortunately it is not possible to measure transfer speed on a system without having a Spectrum card installed.

Debug logging for support cases

For answering your support questions as fast as possible, the setup of the card, driver and firmware version and other information is very helpful.

Therefore the card control center provides an easy way to gather all that information automatically.

Different debug log levels are available through the graphical interface. By default the log level is set to „no logging“ for maximum performance.

The customer can select different log levels and the path of the generated ASCII text file. One can also decide to delete the previous log file first before creating a new one automatically or to append different logs to one single log file.

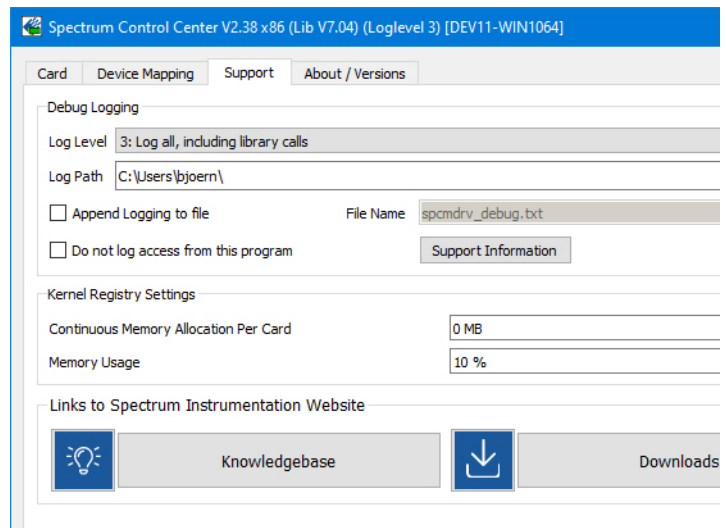


Image 33: Spectrum Control Center - activate debug logging for support cases



For maximum performance of your hardware, please make sure that the debug logging is set to „no logging“ for normal operation. Please keep in mind that a detailed logging in append mode can quickly generate huge log files.

Device mapping

Within the „Device mapping“ tab of the Spectrum Control Center, one can enable the re-mapping of Spectrum devices, be it either local cards, remote instruments such as a digitizerNETBOX, generatorNETBOX, hybridNETBOX or even cards in a remote PC and accessed via the Spectrum remote server option.

In the left column the re-mapped device name is visible that is given to the device in the right column with its original un-mapped device string.

In this example the two local cards „spcm0“ and „spcm1“ are re-mapped to „spcm1“ and „spcm0“ respectively, so that their names are simply swapped.

The remote digitizerNETBOX device is mapped to spcm2.

The application software can then use the re-mapped name for simplicity instead of the quite long VISA string.

Changing the order of devices within one group (either local cards or remote devices) can simply be accomplished by dragging&dropping the cards to their desired position in the same table.

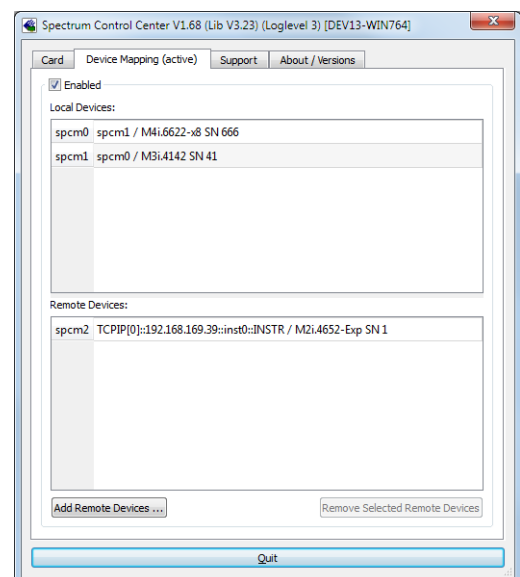


Image 34: Spectrum Control Center - using device mapping

Firmware upgrade

One of the major features of the card control center is the ability to update the card's firmware by an easy-to-use software. The latest firmware revisions can be found in the download section of our homepage under <http://www.spectrum-instrumentation.com>.

A new firmware version is provided there as an installer, that copies the latest firmware to your system. All files are located in a dedicated subfolder „FirmwareUpdate“ that will be created inside the Spectrum installation folder. Under Windows this folder by default has been created in the standard program installation directory.

Please do the following steps when wanting to update the firmware of your M2i/M3i/M4i/M4x/M2p/M5i card:

- Download the latest software driver for your operating system provided on the Spectrum homepage.
- Install the new driver as described in the driver install section of your hardware manual or install manual. All manuals can also be found on the Spectrum homepage in the literature download section.
- Download and run the latest Spectrum Control Center installer.
- Download the installer for the new firmware version.
- Start the installer and follow the instructions given there.
- Start the card control center, select the „card“ tab, select the card from the listbox and press the „firmware update“ button on the right side.

The dialog then will inform you about the currently installed firmware version for the different devices on the card and the new versions that are available. All devices that will be affected with the update are marked as „update needed“. Simply start the update or cancel the operation now, as a running update cannot be aborted.

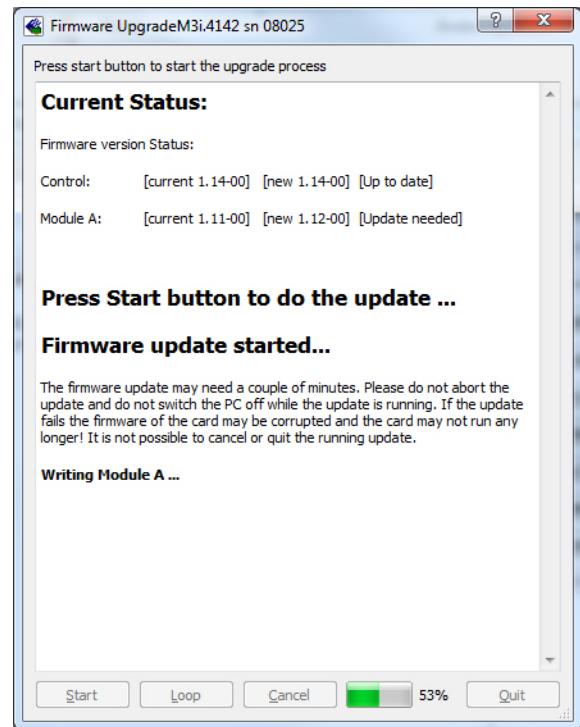


Image 35: Spectrum Control Center - doing a firmware update for one device



Please keep in mind that you have to start the update for each card installed in your system separately. Select one card after the other from the listbox and press the „firmware update“ button. The firmware installer on the other hand only needs to be started once prior to the update.



Do not abort or shut down the computer while the firmware update is in progress. After a successful update please shut down your PC completely (remove power). The re-powering is required to finally activate the new firmware version of your Spectrum card.

Firmware switch

Most Spectrum cards come with just a single, default firmware configuration, that supports all of the device features. But some of the cards require different firmware configurations (different firmware images) for certain operating modes or for a certain set of features.

For such cards the firmware configuration can be changed by using the “Firmware Switch” function of the Spectrum Control Center:

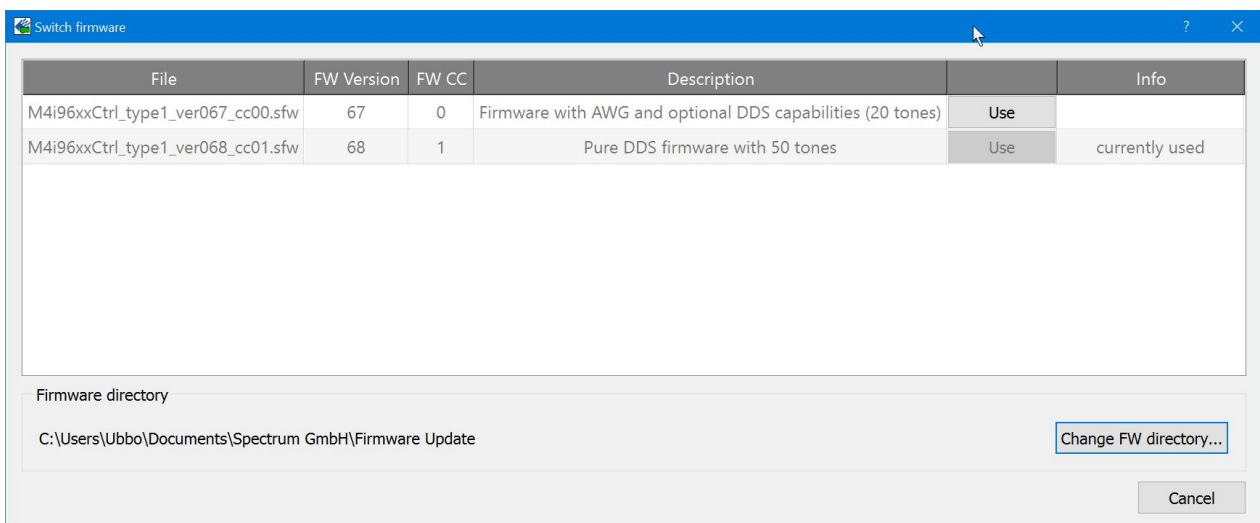


Image 36: Spectrum Control Center - selecting a firmware configuration for one card

The dialog shows a list of available firmware configurations for the current hardware and provides information:

- Info: which firmware is currently used
- FW Version: The firmware version of this particular firmware configuration
- FW CC: The number of the firmware configuration. Most cards have only one single default configuration 0.
- Description: A more detailed information of what each configuration is capable of

The firmware directory is by default set to the path to which the FW-Installer has installed the firmware files. This folder can be changed however to a specific location, if required.

For switching to a different configuration, press the "Use" button. The firmware will be applied to the hardware, similar to a firmware update. Afterwards



Please keep in mind that you have to switch the configuration for each card installed in your system separately. Select one card after the other from the listbox and press the „firmware switch“ button. The firmware installer on the other hand only needs to be started once prior to the update.



Certain firmware configurations might only be available, when a certain feature/license is installed. In case that a separate license is required, the switch dialog will still display all available configurations, but might not allow to select certain configurations. This information will be shown in the "Description" column.



Do not abort or shut down the computer while the firmware switch is in progress. After a successful firmware switch please shut down your PC completely (remove power). The re-powering is required to finally activate the new firmware version of your Spectrum card.

Accessing the hardware with SBench 6

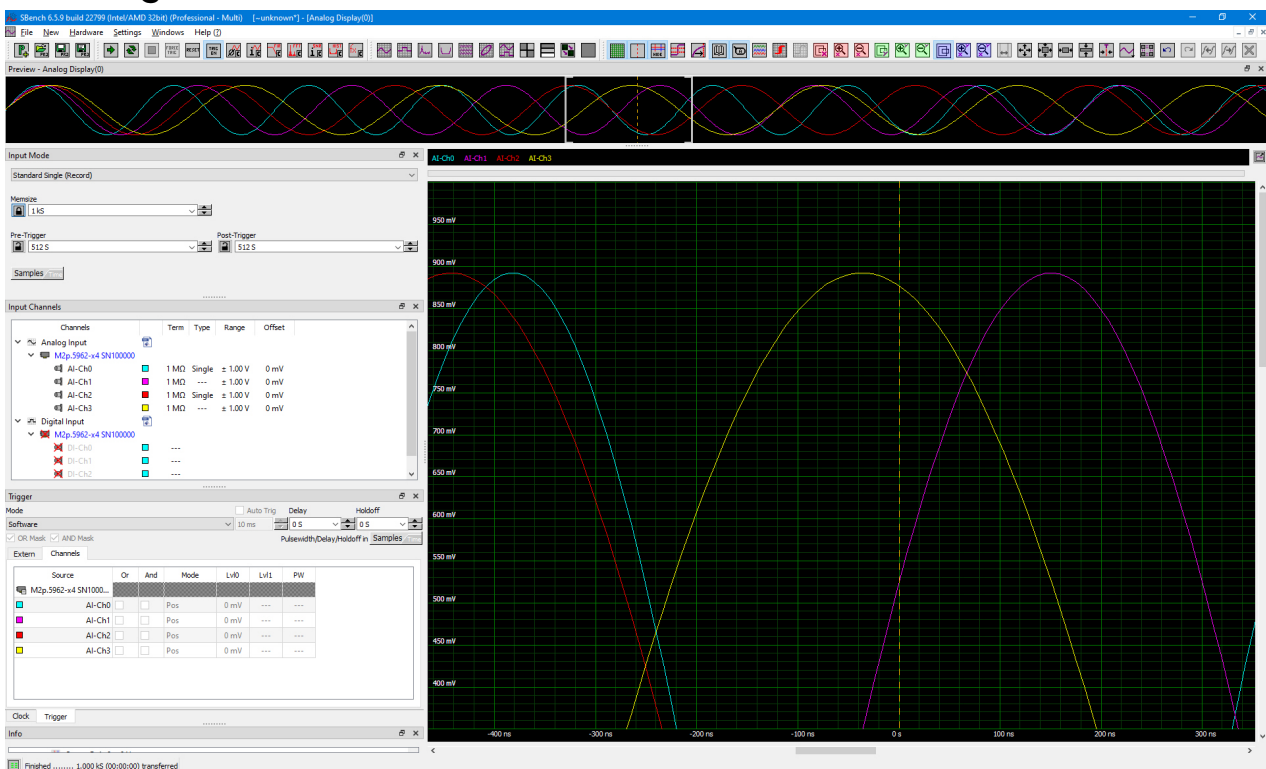


Image 37: SBench 6 overview of main functionality with demo data

After the installation of the cards and the drivers it can be useful to first test the card function with a ready to run software before starting with programming. If accessing a digitizerNETBOX/generatorNETBOX a full SBench 6 Professional license is installed on the system and can be used without any limitations. For plug-in card level products a base version of SBench 6 is delivered with the card on USB stick also including a 30 starts Professional demo version for plain card products. If you already have bought a card prior to the first SBench 6 release please contact your local dealer to get a SBench 6 Professional demo version. All digitizerNETBOX/generatorNETBOX products come with a pre-installed full SBench 6 Professional.

SBench 6 supports all current acquisition and generation cards and digitizerNETBOX/generatorNETBOX products from Spectrum. Depending on the used product and the software setup, one can use SBench as a digital storage oscilloscope, a spectrum analyzer, a signal generator, a pattern generator, a logic analyzer or simply as a data recording front end. Different export and import formats allow the use of SBench 6 together with a variety of other programs.

On the USB stick you'll find an install version of SBench 6 in the directory „/Install/SBench6“.

The current version of SBench 6 is available free of charge directly from the Spectrum website: www.spectrum-instrumentation.com. Please go to the download section and get the latest version there.

SBench 6 has been designed to run under Windows 7, 8, 10 and Windows 11 as well as Linux using KDE, Gnome or Unity Desktop.

Accessing the hardware with DDS Control (DDS firmware required)



If you have purchased an Arbitrary Waveform Generator (AWG) with Direct Digital Synthesis (DDS) firmware option, the DDS Control tool enables you to use and test the DDS functionality of your card. DDS Control supports the following cards:

- M2p.65xx
- M4i.66xx and M4i.96xx as well as the PXIe versions M4x.66xx and M4x.96xx
- M5i.63xx.

Additionally, all Spectrum generatorNETBOX and hybridNETBOX products with installed DDS feature are supported.

DDS control can program these DDS controls statically with DDS dialogs, or it allows the user to program full sequences (or patterns) of commands in an exact timed manner.

The current DDS control software is free to download from our website, and all the features are available without additional fees. Both Windows and Linux are supported.

C/C++ Driver Interface

C/C++ is the main programming language for which the drivers have been designed for. Therefore the interface to C/C++ is the best match. All the small examples of the manual showing different parts of the hardware programming are done with C. As the libraries offer a standard interface it is easy to access the libraries also with other programming languages like Delphi, Basic, Python or Java. Please read the following chapters for additional information on this.

Header files

The basic task before using the driver is to include the header files that are delivered on USB stick together with the board. The header files are found in the directory /Driver/c_header. Please don't change them in any way because they are updated with each new driver version to include the new registers and new functionality.

Table 4: list of C/C++ header files in driver

dlltyp.h	Includes the platform specific definitions for data types and function declarations. All data types are based on these definitions. The use of this type definition file allows the use of examples and programs on different platforms without changes to the program source. The header file supports Microsoft Visual C++, Borland C++ Builder and GNU C/C++ directly. When using other compilers it might be necessary to make a copy of this file and change the data types according to this compiler.
regs.h	Defines all registers and commands which are used in the Spectrum driver for the different boards. The registers a board uses are described in the board specific part of the documentation. This header file is common for all cards. Therefore this file also contains a huge number of registers used on other card types than the one described in this manual. Please stick to the manual to see which registers are valid for your type of card.
spcm_drv.h	Defines the functions of the used SpcM driver. All definitions are taken from the file dlltyp.h. The functions themselves are described below.
spcerr.h	Contains all error codes used with the Spectrum driver. All error codes that can be given back by any of the driver functions are also described here briefly. The error codes and their meaning are described in detail in the appendix of this manual.


Example for including the header files:

```
// ----- driver includes -----
#include "dlltyp.h"      // 1st include
#include "regs.h"        // 2nd include
#include "spcerr.h"      // 3rd include
#include "spcm_drv.h"    // 4th include
```



Please always keep the order of including the four Spectrum header files. Otherwise some or all of the functions do not work properly or compiling your program will be impossible!

General Information on Windows 64 bit drivers



After installation of the Spectrum 64 bit driver there are two general ways to access the hardware and to develop applications. If you're going to develop a real 64 bit application it is necessary to access the 64 bit driver dll (spcm_win64.dll) as only this driver dll is supporting the full 64 bit address range.

But it is still possible to run 32 bit applications or to develop 32 bit applications even under Windows 64 bit. Therefore the 32 bit driver dll (spcm_win32.dll) is also installed in the system. The Spectrum SBench5 software is for example running under Windows 64 bit using this driver. The 32 bit dll of course only offers the 32 bit address range and is therefore limited to access only 4 GByte of memory. Beneath both drivers the 64 bit kernel driver is running.

Mixing of 64 bit application with 32 bit dll or vice versa is not possible.

Microsoft Visual C++ 6.0, 2005 and newer 32 Bit

Include Driver

The driver files can be directly included in Microsoft C++ by simply using the library file spcm_win32_msvcpp.lib that is delivered together with the drivers. The library file can be found on the CD in the path /examples/c_cpp/c_header. Please include the library file in your Visual C++ project as shown in the examples. All functions described below are now available in your program.

Examples

Examples can be found on CD in the path /examples/c_cpp. This directory includes a number of different examples that can be used with any card of the same type (e.g. A/D acquisition cards, D/A acquisition cards). You may use these examples as a base for own programming and modify them as you like. The example directories contain a running workspace file for Microsoft Visual C++ 6.0 (*.dsw) as well as project files for Microsoft Visual Studio 2005 and newer (*.vcproj) that can be directly loaded or imported and compiled. There are also some more board type independent examples in separate subdirectory. These examples show different aspects of the cards like programming options or synchronization and can be combined with one of the board type specific examples.

As the examples are build for a card class there are some checking routines and differentiation between cards families. Differentiation aspects can be number of channels, data width, maximum speed or other details. It is recommended to change the examples matching your card type to obtain maximum performance. Please be informed that the examples are made for easy understanding and simple showing of one aspect of programming. Most of the examples are not optimized for maximum throughput or repetition rates.

Microsoft Visual C++ 2005 and newer 64 Bit

Depending on your version of the Visual Studio suite it may be necessary to install some additional 64 bit components (SDK) on your system. Please follow the instructions found on the MSDN for further information.

Include Driver

The driver files can be directly included in Microsoft C++ by simply using the library file spcm_win64_msvcpp.lib that is delivered together with the drivers. The library file can be found on the CD in the path /examples/c_cpp/c_header. All functions described below are now available in your program.

Linux Gnu C/C++ 32/64 Bit

Include Driver

The interface of the linux drivers does not differ from the windows interface. Please include the "libspcm_linux.so" library in your makefile using the below shown "LIBS = -lspcm_linux" line, to have access to all driver functions. A makefile may look like this:

```
COMPILER = gcc
EXECUTABLE = test_prg
LIBS = -lspcm_linux

OBJECTS = test.o\
          test2.o

all: $(EXECUTABLE)

$(EXECUTABLE): $(OBJECTS)
    $(COMPILER) $(CFLAGS) -o $(EXECUTABLE) $(LIBS) $(OBJECTS)

%.o: %.cpp
    $(COMPILER) $(CFLAGS) -o $*.o -c $*.cpp
```

Examples

The Gnu C/C++ examples share the source with the Visual C++ examples. Please see above chapter for a more detailed documentation of the examples. Each example directory contains a makefile for the Gnu C/C++ examples.

C++ for .NET

Please see the next chapter for more details on the .NET inclusion.

Other Windows C/C++ compilers 32 Bit

Include Driver

To access the driver using a compiler such as e.g. MinGW or Borland, the driver functions must be loaded from the 32 bit driver DLL. Most compilers offer special tools to generate a matching library (e.g. Borland offers the implib tool that generates a matching library out of the windows driver DLL). If such a tool is available it is recommended to use it. Otherwise the driver functions need to be loaded from the dll using standard Windows functions. There is one example in the example directory /examples/c_cpp/dll_loading that shows the process.

Example of function loading:

```
hDLL = LoadLibrary ("spcm_win32.dll"); // Load the 32 bit version of the Spcm driver
pfn_spcm_hOpen = (SPCM_HOPEN*) GetProcAddress (hDLL, "_spcm_hOpen@4");
pfn_spcm_vClose = (SPCM_VCLOSE*) GetProcAddress (hDLL, "_spcm_vClose@4");
```

Other Windows C/C++ compilers 64 Bit

Include Driver

To access the driver using a compiler such as e.g. MinGW or Borland, the driver functions must be loaded from the 64 bit the driver DLL. Most compilers offer special tools to generate a matching library (e.g. Borland offers the implib tool that generates a matching library out of the windows driver DLL). If such a tool is available it is recommended to use it. Otherwise the driver functions need to be loaded from the dll using standard Windows functions. There is one example in the example directory /examples/c_cpp/dll_loading that shows the process for 32 bit environments. The only line that needs to be modified is the one loading the DLL:

Example of function loading:

```
hDLL = LoadLibrary ("spcm_win64.dll"); // Modified: Load the 64 bit version of the Spcm driver here
pfn_spcm_hOpen = (SPCM_HOPEN*) GetProcAddress (hDLL, "spcm_hOpen");
pfn_spcm_vClose = (SPCM_VCLOSE*) GetProcAddress (hDLL, "spcm_vClose");
```

Driver functions

The driver contains seven main functions to access the hardware.

Own types used by our drivers

To simplify the use of the header files and our examples with different platforms and compilers and to avoid any implicit type conversions we decided to use our own type declarations. This allows us to use platform independent and universal examples and driver interfaces. If you do not stick to these declarations please be sure to use the same data type width. However it is strongly recommended that you use our defined

type declarations to avoid any hard to find errors in your programs. If you're using the driver in an environment that is not natively supported by our examples and drivers, please be sure to use a type declaration that represents a similar data width

Table 5: C/C++ type declarations for drivers and examples

Declaration	Type	Declaration	Type
int8	8 bit signed integer (range from -128 to +127)	uint8	8 bit unsigned integer (range from 0 to 255)
int16	16 bit signed integer (range from -32768 to 32767)	uint16	16 bit unsigned integer (range from 0 to 65535)
int32	32 bit signed integer (range from -2147483648 to 2147483647)	uint32	32 bit unsigned integer (range from 0 to 4294967295)
int64	64 bit signed integer (full range)	uint64	64 bit unsigned integer (full range)
drv_handle	handle to driver, implementation depends on operating system platform		

Notation of variables and functions

In our header files and examples we use a common and reliable form of notation for variables and functions. Each name also contains the type as a prefix. This notation form makes it easy to see implicit type conversions and minimizes programming errors that result from using incorrect types. Feel free to use this notation form for your programs as well-

Table 6: C/C++ type naming convention throughout drivers and examples

Declaration	Notation	Declaration	Notation
int8	c Name (character)	uint8	by Name (byte)
int16	n Name	uint16	w Name (word)
int32	l Name (long)	uint32	dw Name (double word)
int64	ll Name (long long)	uint64	qw Name (quad word)
float	f Name	double	d Name
void	v Name	bool	b Name
int8*	pc Name (character)	uint8*	pby Name (byte)
int16*	pn Name	uint16*	pw Name (word)
int32*	pl Name (long)	uint32*	pdw Name (double word)
int64*	pll Name (long long)	uint64*	pqw Name (quad word)
float*	pf Name	double*	pd Name
void*	pv Name		
drv_handle	h Name	char*	sz Name (string with zero termination)

Function spcm_hOpen

This function initializes and opens an installed card supporting the new SpcM driver interface, which at the time of printing, are all cards of the M2i/M3i/M4i/M4x/M2p/M5i series and the related digitizerNETBOX/generatorNETBOX/hybridNETBOX devices. The function returns a handle that has to be used for driver access. If the card can't be found or the loading of the driver generated an error the function returns a NULL. When calling this function all card specific installation parameters are read out from the hardware and stored within the driver. It is only possible to open one device by one software as concurrent hardware access may be very critical to system stability. As a result when trying to open the same device twice an error will be raised and the function returns NULL.

Function spcm_hOpen (const char* szDeviceName):

```
drv_handle _stdcall spcm_hOpen (           // tries to open the device and returns handle or error code
    const char* szDeviceName);           // name of the device to be opened
```

Under Linux the device name in the function call needs to be a valid device name. Please change the string according to the location of the device if you don't use the standard Linux device names. The driver is installed as default under /dev/spcm0, /dev/spcm1 and so on. The kernel driver numbers the devices starting with 0.

Under Windows the only part of the device name that is used is the trailing number. The rest of the device name is ignored. Therefore to keep the examples simple we use the Linux notation in all our examples. The trailing number gives the index of the device to open. The Windows kernel driver numbers all devices that it finds on boot time starting with 0.

Example for local installed cards

```
drv_handle hDrv;                               // returns the handle to the opened driver or NULL in case of error
hDrv = spcm_hOpen ("/dev/spcm0");             // open the first card (spcm0) and get a handle to this card
if (!hDrv)
    printf ("open of driver failed\n");
```

Example for digitizerNETBOX/generatorNETBOX and remote installed cards

```
drv_handle hDrv;                               // returns the handle to the opened driver or NULL in case of error
hDrv = spcm_hOpen ("TCP/IP::192.168.169.14::INST0::INSTR");
if (!hDrv)
    printf ("open of driver failed\n");
```

If the function returns a NULL it is possible to read out the error description of the failed open function by simply passing this NULL to the error function. The error function is described in one of the next topics.

Function `spcm_vClose`

This function closes the driver and releases all allocated resources. After closing the driver handle it is not possible to access this driver any more. Be sure to close the driver if you don't need it any more to allow other programs to get access to this device.

Function `spcm_vClose`:

```
void __stdcall spcm_vClose (           // closes the device
    drv_handle hDevice);              // handle to an already opened device
```

Example:

```
spcm_vClose (hDrv);
```

Function `spcm_dwSetParam`

All hardware settings are based on software registers that can be set by one of the functions `spcm_dwSetParam`. These functions set a register to a defined value or execute a command. The board must first be initialized by the `spcm_hOpen` function. The parameter `lRegister` must have a valid software register constant as defined in `regs.h`. The available software registers for the driver are listed in the board specific part of the documentation below. The function returns a 32 bit error code if an error occurs. If no error occurs the function returns `ERR_OK`, what is zero.

Function `spcm_dwSetParam`

```
uint32 __stdcall spcm_dwSetParam_i32 ( // Return value is an error code
    drv_handle hDevice,                // handle to an already opened device
    int32 lRegister,                   // software register to be modified
    int32 lValue);                     // the value to be set

uint32 __stdcall spcm_dwSetParam_i64m ( // Return value is an error code
    drv_handle hDevice,                // handle to an already opened device
    int32 lRegister,                   // software register to be modified
    int32 lValueHigh,                 // upper 32 bit of the value. Containing the sign bit !
    uint32 dwValueLow);                // lower 32 bit of the value.

uint32 __stdcall spcm_dwSetParam_i64 ( // Return value is an error code
    drv_handle hDevice,                // handle to an already opened device
    int32 lRegister,                   // software register to be modified
    int64 llValue);                    // the value to be set

uint32 __stdcall spcm_dwSetParam_d64 ( // Return value is an error code
    drv_handle hDevice,                // handle to an already opened device
    int32 lRegister,                   // software register to be modified
    double dValue);                    // the value to be set

uint32 __stdcall spcm_dwSetParam_ptr ( // Return value is an error code
    drv_handle hDevice,                // handle to an already opened device
    int32 lRegister,                   // software register to be modified
    void* pvValue,                     // pointer to the value to be set
    unit64 qwLen);                     // length of the buffer behind the pvValue
```

The functions `spcm_dwSetParam_d64` and `spcm_dwSetParam_ptr` have been added with driver release V 7.00

Example:

```
if (spcm_dwSetParam_i64 (hDrv, SPC_MEMSIZE, 16384) != ERR_OK)
    printf ("Error when setting memory size\n");
```

This example sets the memory size to 16 KiSamples (16384). If an error occurred the example will show a short error message

Function `spcm_dwGetParam`

All hardware settings are based on software registers that can be read by one of the functions `spcm_dwGetParam`. These functions read an internal register or status information. The board must first be initialized by the `spcm_hOpen` function. The parameter `lRegister` must have a valid software register constant as defined in the `regs.h` file. The available software registers for the driver are listed in the board specific part of the documentation below. The function returns a 32 bit error code if an error occurs. If no error occurs the function returns `ERR_OK`, what is zero.

Function `spcm_dwGetParam`

```

uint32 _stdcall spcm_dwGetParam_i32 ( // Return value is an error code
    drv_handle hDevice,                // handle to an already opened device
    int32 lRegister,                   // software register to be read out
    int32* pIValue);                  // pointer for the return value

uint32 _stdcall spcm_dwGetParam_i64m ( // Return value is an error code
    drv_handle hDevice,                // handle to an already opened device
    int32 lRegister,                   // software register to be read out
    int32* pIValueHigh,               // pointer for the upper part of the return value
    uint32* pDValueLow);              // pointer for the lower part of the return value

uint32 _stdcall spcm_dwGetParam_i64 ( // Return value is an error code
    drv_handle hDevice,                // handle to an already opened device
    int32 lRegister,                   // software register to be read out
    int64* pIValue);                  // pointer for the return value

uint32 _stdcall spcm_dwGetParam_d64 ( // Return value is an error code
    drv_handle hDevice,                // handle to an already opened device
    int32 lRegister,                   // software register to be modified
    double* dValue);                 // pointer for the return value

uint32 _stdcall spcm_dwGetParam_ptr ( // Return value is an error code
    drv_handle hDevice,                // handle to an already opened device
    int32 lRegister,                   // software register to be modified
    void* pvValue,                    // pointer for the return value
    unit64 qwLen);                   // length of the buffer behind the pvValue

```

The functions `spcm_dwGetParam_d64` and `spcm_dwGetParam_ptr` have been added with driver release V 7.00

Example:

```

int32 lSerialNumber;
spcm_dwGetParam_i32 (hDrv, SPC_PCISERIALNO, &lSerialNumber);
printf ("Your card has serial number: %05d\n", lSerialNumber);

```

The example reads out the serial number of the installed card and prints it. As the serial number is available under all circumstances there is no error checking when calling this function.

Different call types of `spcm_dwSetParam` and `spcm_dwGetParam`: `i32`, `i64`, `i64m`, `d64`

The four functions only differ in the type of the parameters that are used to call them. As some of the registers can exceed the 32 bit integer range (like memory size or post trigger) it is recommended to use the `_i64` function to access these registers. However as there are some programs or compilers that don't support 64 bit integer variables there are two functions that are limited to 32 bit integer variables. In case that you do not access registers that exceed 32 bit integer please use the `_i32` function. In case that you access a register which exceeds 64 bit value please use the `_i64m` calling convention. Inhere the 64 bit value is split into a low double word part and a high double word part. Please be sure to fill both parts with valid information.

As some registers need to be read/written in double precision and can't be read/written as integer values, two additional new functions for accessing double values have been added with the suffix `_d64`.

If accessing 64 bit registers with 32 bit functions the behaviour differs depending on the real value that is currently located in the register. Please have a look at this table to see the different reactions depending on the size of the register:

Table 7: Spectrum driver API functions overview and differentiation between 32 bit and 64 bit registers

Internal register	read/write	Function type	Behavior
32 bit register	read	<code>spcm_dwGetParam_i32</code>	value is returned as 32 bit integer in <code>pIValue</code>
32 bit register	read	<code>spcm_dwGetParam_i64</code>	value is returned as 64 bit integer in <code>pIValue</code>
32 bit register	read	<code>spcm_dwGetParam_i64m</code>	value is returned as 64 bit integer, the lower part in <code>pIValueLow</code> , the upper part in <code>pIValueHigh</code> . The upper part can be ignored as it's only a sign extension
32 bit register	read	<code>spcm_dwGetParam_d64</code>	value is returned as 64 bit double in <code>pdValue</code>
32 bit register	write	<code>spcm_dwSetParam_i32</code>	32 bit value can be directly written
32 bit register	write	<code>spcm_dwSetParam_i64</code>	64 bit value can be directly written, please be sure not to exceed the valid register value range
32 bit register	write	<code>spcm_dwSetParam_i64m</code>	32 bit value is written as <code>lValueLow</code> , the value <code>lValueHigh</code> needs to contain the sign extension of this value. In case of <code>lValueLow</code> being a value ≥ 0 <code>lValueHigh</code> can be 0, in case of <code>lValueLow</code> being a value < 0 , <code>lValueHigh</code> has to be -1.
32 bit register	write	<code>spcm_dwSetParam_d64</code>	32 bit value needs to be converted to double. Please make sure not to exceed the valid register range
64 bit register	read	<code>spcm_dwGetParam_i32</code>	If the internal register has a value that is inside the 32 bit integer range $[-2Gi$ up to $(2Gi - 1)]$ the value is returned normally. If the internal register exceeds this size an error code <code>ERR_EXCEEDSINT32</code> is returned. As an example: reading back the installed memory will work as long as this memory is < 2 GiByte. If the installed memory is ≥ 2 GiByte the function will return an error.
64 bit register	read	<code>spcm_dwGetParam_i64</code>	value is returned as 64 bit integer value in <code>pIValue</code> independent of the value of the internal register.
64 bit register	read	<code>spcm_dwGetParam_i64m</code>	the internal value is split into a low and a high part. As long as the internal value is within the 32 bit range, the low part <code>pIValueLow</code> contains the 32 bit value and the upper part <code>pIValueHigh</code> can be ignored. If the internal value exceeds the 32 bit range it is absolutely necessary to take both value parts into account.
64 bit register	read	<code>spcm_dwGetParam_d64</code>	value is returned as 64 bit double in <code>pdValue</code> . Please note that double values are limited to 2^{48} . Any larger value is not returned with full precision.
64 bit register	write	<code>spcm_dwSetParam_i32</code>	the value to be written is limited to 32 bit range. If a value higher than the 32 bit range should be written, one of the other function types need to be used.

Table 7: Spectrum driver API functions overview and differentiation between 32 bit and 64 bit registers

Internal register	read/write	Function type	Behavior
64 bit register	write	spcm_dwSetParam_i64	the value has to be split into two parts. Be sure to fill the upper part lValueHigh with the correct sign extension even if you only write a 32 bit value as the driver every time interprets both parts of the function call.
64 bit register	write	spcm_dwSetParam_i64m	the value can be written directly independent of the size.
64 bit register	write	spcm_dwSetParam_d64	the value need to be converted to double. Any value up to 2^48 can be written directly. Larger values need to be written using the _i64 function

Function spcm_dwGetContBuf

This function reads out the internal continuous memory buffer in bytes, in case one has been allocated. If no buffer has been allocated the function returns a size of zero and a NULL pointer. You may use this buffer for data transfers. As the buffer is continuously allocated in memory the data transfer will speed up by up to 15% - 25%, depending on your specific kind of card. Please see further details in the appendix of this manual.

```
uint32_stdcall spcm_dwGetContBuf_i64 ( // Return value is an error code
    drv_handle hDevice,                // handle to an already opened device
    uint32 dwBufType,                  // type of the buffer to read as listed above under SPCM_BUF_XXXX
    void** ppvDataBuffer,              // address of available data buffer
    uint64* pqwContBufLen);            // length of available continuous buffer

uint32_stdcall spcm_dwGetContBuf_i64m (// Return value is an error code
    drv_handle hDevice,                // handle to an already opened device
    uint32 dwBufType,                  // type of the buffer to read as listed above under SPCM_BUF_XXXX
    void** ppvDataBuffer,              // address of available data buffer
    uint32* pdwContBufLenH,            // high part of length of available continuous buffer
    uint32* pdwContBufLenL);           // low part of length of available continuous buffer
```



These functions have been added in driver version 1.36. The functions are not available in older driver versions.



These functions also only have effect on locally installed cards and are neither useful nor usable with any digitizerNETBOX or generatorNETBOX products, because no local kernel driver is involved in such a setup. For remote devices these functions will return a NULL pointer for the buffer and 0 Bytes in length.

Function spcm_dwDefTransfer

The spcm_dwDefTransfer function defines a buffer for a following data transfer. This function only defines the buffer, there is no data transfer performed when calling this function. Instead the data transfer is started with separate register commands that are documented in a later chapter. At this position there is also a detailed description of the function parameters.

Please make sure that all parameters of this function match. It is especially necessary that the buffer address is a valid address pointing to memory buffer that has at least the size that is defined in the function call. Please be informed that calling this function with non valid parameters may crash your system as these values are base for following DMA transfers.

The use of this function is described in greater detail in a later chapter.

Function spcm_dwDefTransfer

```
uint32_stdcall spcm_dwDefTransfer_i64m(// Defines the transfer buffer by 2 x 32 bit unsigned integer
    drv_handle hDevice,                // handle to an already opened device
    uint32 dwBufType,                  // type of the buffer to define as listed above under SPCM_BUF_XXXX
    uint32 dwDirection,                // the transfer direction as defined above
    uint32 dwNotifySize,               // no. of bytes after which an event is sent (0=end of transfer)
    void* pvDataBuffer,                // pointer to the data buffer
    uint32 dwBrdOffsH,                 // high part of offset in board memory (zero when using FIFO mode)
    uint32 dwBrdOffsL,                 // low part of offset in board memory (zero when using FIFO mode)
    uint32 dwTransferLenH,             // high part of transfer buffer length
    uint32 dwTransferLenL);            // low part of transfer buffer length

uint32_stdcall spcm_dwDefTransfer_i64 (// Defines the transfer buffer by using 64 bit unsigned integer values
    drv_handle hDevice,                // handle to an already opened device
    uint32 dwBufType,                  // type of the buffer to define as listed above under SPCM_BUF_XXXX
    uint32 dwDirection,                // the transfer direction as defined above
    uint32 dwNotifySize,               // no. of bytes after which an event is sent (0=end of transfer)
    void* pvDataBuffer,                // pointer to the data buffer
    uint64 qwBrdOffs,                  // offset for transfer in board memory (zero when using FIFO mode)
    uint64 qwTransferLen);             // buffer length
```

This function is available in two different formats as the spcm_dwGetParam and spcm_dwSetParam functions are. The background is the same. As long as you're using a compiler that supports 64 bit integer values please use the _i64 function. Any other platform needs to use the _i64m function and split offset and length in two 32 bit words.

Example:

```
int16* pnBuffer = (int16*) pvAllocMemPageAligned (16384);
if (spcm_dwDefTransfer_i64 (hDrv, SPCM_BUF_DATA, SPCM_DIR_CARDTOPC, 0, (void*) pnBuffer, 0, 16384) != ERR_OK)
    printf ("DefTransfer failed\n");
```

The example defines a data buffer of 8 KiSamples of 16 bit integer values = 16 KiByte (16384 byte) for a transfer from card to PC memory. As notify size is set to 0 we only want to get an event when the transfer has finished.

Function `spcm_dwInvalidateBuf`

The invalidate buffer function is used to tell the driver that the buffer that has been set with `spcm_dwDefTransfer` call is no longer valid. It is necessary to use the same buffer type as the driver handles different buffers at the same time. Call this function if you want to delete the buffer memory after calling the `spcm_dwDefTransfer` function. If the buffer already has been transferred after calling `spcm_dwDefTransfer` it is not necessary to call this function. When calling `spcm_dwDefTransfer` any previously defined buffer of this type is automatically invalidated.

Function `spcm_dwInvalidateBuf`

```
uint32_stdcall spcm_dwInvalidateBuf ( // invalidate the transfer buffer
    drv_handle hDevice,              // handle to an already opened device
    uint32      dwBufType);          // type of the buffer to invalidate as
                                     // listed above under SPCM_BUF_XXXX
```

Function `spcm_dwGetErrorInfo`

The function returns complete error information on the last error that has occurred. The error handling itself is explained in a later chapter in greater detail. When calling this function please be sure to have a text buffer allocated that has at least `ERRORTXTLEN` length. The error text function returns a complete description of the error including the register/value combination that has raised the error and a short description of the error details. In addition it is possible to get back the error generating register/value for own error handling. If not needed the buffers for register/value can be left to NULL.

Note that the timeout event (`ERR_TIMEOUT`) is not counted as an error internally as it is not locking the driver but as a valid event. Therefore the `GetErrorInfo` function won't return the timeout event even if it had occurred in between. You can only recognize the `ERR_TIMEOUT` as a direct return value of the wait function that was called.



Function `spcm_dwGetErrorInfo`

```
// for reading errors that occur during hOpen(), leave the drv_handle parameter NULL

uint32_stdcall spcm_dwGetErrorInfo_i32 (
    drv_handle hDevice,          // handle to an already opened device
    uint32*    pdwErrorReg,      // address of the error register (can be NULL if not of interest)
    int32*     plErrorValue,     // address of the error value (can be NULL if not of interest)
    char       pszErrorTextBuffer[ERRORTXTLEN]); // text buffer for text error

uint32_stdcall spcm_dwGetErrorInfo_i64 (
    drv_handle hDevice,          // handle to an already opened device
    uint32*    pdwErrorReg,      // address of the error register (can be NULL if not of interest)
    int64*     pllErrorValue,    // address of the error value (can be NULL if not of interest)
    char       pszErrorTextBuffer[ERRORTXTLEN]); // text buffer for text error

uint32_stdcall spcm_dwGetErrorInfo_d64 (
    drv_handle hDevice,          // handle to an already opened device
    uint32*    pdwErrorReg,      // address of the error register (can be NULL if not of interest)
    double*    pdErrorValue,     // address of the error value (can be NULL if not of interest)
    char       pszErrorTextBuffer[ERRORTXTLEN]); // text buffer for text error
```

The functions `spcm_dwGetErrorInfo_i64` and `spcm_dwGetErrorInfo_d64` have been added with driver release V 7.00

Example:

```
char szErrorBuf[ERRORTXTLEN];
if (spcm_dwSetParam_i64 (hDrv, SPC_MEMSIZE, -1))
{
    spcm_dwGetErrorInfo_i64 (hDrv, NULL, NULL, szErrorBuf);
    printf ("Set of memSize failed with error message: %s\n", szErrorBuf);
}
```

Delphi (Pascal) Programming Interface

Driver interface

The driver interface is located in the sub-directory `d_header` and contains the following files. The files need to be included in the delphi project and have to be put into the „uses“ section of the source files that will access the driver. Please do not edit any of these files as they're regularly updated if new functions or registers have been included.

file `spcm_win32.pas`

The file contains the interface to the driver library and defines some needed constants and variable types. All functions of the delphi library are similar to the above explained standard driver functions:

```
// ----- device handling functions -----
function spcm_hOpen (strName: pchar): int32; stdcall; external 'spcm_win32.dll' name '_spcm_hOpen@4';
procedure spcm_vClose (hDevice: int32); stdcall; external 'spcm_win32.dll' name '_spcm_vClose@4';

function spcm_dwGetErrorInfo_i32 (hDevice: int32; var lErrorReg, lErrorValue: int32; strError: pchar): uint32;
stdcall; external 'spcm_win32.dll' name '_spcm_dwGetErrorInfo_i32@16';

function spcm_dwGetErrorInfo_i64 (hDevice: int32; var plErrorReg: int32; var pllErrorValue: int64; strError:
PAnsiChar): uint32; stdcall; external 'spcm_win32.dll' name '_spcm_dwGetErrorInfo_i64@16';

function spcm_dwGetErrorInfo_d64 (hDevice: int32; var plErrorReg: int32; var pdErrorValue: double; strError:
PAnsiChar): uint32; stdcall; external 'spcm_win32.dll' name '_spcm_dwGetErrorInfo_d64@16';

// ----- register access functions -----
function spcm_dwSetParam_i32 (hDevice, lRegister, lValue: int32): uint32;
stdcall; external 'spcm_win32.dll' name '_spcm_dwSetParam_i32@12';

function spcm_dwSetParam_i64 (hDevice, lRegister: int32; llValue: int64): uint32;
stdcall; external 'spcm_win32.dll' name '_spcm_dwSetParam_i64@16';

function spcm_dwSetParam_d64 (hDevice, lRegister: int32; dValue: double): uint32;
stdcall; external 'spcm_win32.dll' name '_spcm_dwSetParam_d64@16';

function spcm_dwGetParam_i32 (hDevice, lRegister: int32; var plValue: int32): uint32;
stdcall; external 'spcm_win32.dll' name '_spcm_dwGetParam_i32@12';

function spcm_dwGetParam_i64 (hDevice, lRegister: int32; var pllValue: int64): uint32;
stdcall; external 'spcm_win32.dll' name '_spcm_dwGetParam_i64@12';

function spcm_dwGetParam_d64 (hDevice, lRegister: int32; var pdValue: double): uint32;
stdcall; external 'spcm_win32.dll' name '_spcm_dwGetParam_d64@12';

// ----- data handling -----
function spcm_dwDefTransfer_i64 (hDevice, dwBufType, dwDirection, dwNotifySize: int32; pvDataBuffer: Pointer;
llBrdOffs, llTransferLen: int64): uint32;
stdcall; external 'spcm_win32.dll' name '_spcm_dwDefTransfer_i64@36';

function spcm_dwInvalidateBuf (hDevice, lBuffer: int32): uint32;
stdcall; external 'spcm_win32.dll' name '_spcm_dwInvalidateBuf@8';
```

The file also defines types used inside the driver and the examples. The types have similar names as used under C/C++ to keep the examples more simple to understand and allow a better comparison.

file spcm_win64.pas

The file contains the interface to the driver library and defines some needed constants and variable types. All functions of the delphi library are similar to the above explained standard driver functions:

```
// ----- device handling functions -----
function spcm_hOpen (strName: pchar): int32; stdcall; external 'spcm_win32.dll' name '_spcm_hOpen@4';
procedure spcm_vClose (hDevice: int32); stdcall; external 'spcm_win32.dll' name '_spcm_vClose@4';

function spcm_dwGetErrorInfo_i32 (hDevice: int32; var lErrorReg: lErrorValue: int32; strError: pchar): uint32;
stdcall; external 'spcm_win32.dll' name '_spcm_dwGetErrorInfo_i32@16';

function spcm_dwGetErrorInfo_i64 (hDevice: int32; var plErrorReg: int32; var pllErrorValue: int64; strError:
PAnsiChar): uint32; stdcall; external 'spcm_win32.dll' name '_spcm_dwGetErrorInfo_i64@16';

function spcm_dwGetErrorInfo_d64 (hDevice: int32; var plErrorReg: int32; var pdErrorValue: double; strError:
PAnsiChar): uint32; stdcall; external 'spcm_win32.dll' name '_spcm_dwGetErrorInfo_d64@16';

// ----- register access functions -----
function spcm_dwSetParam_i32 (hDevice, lRegister, lValue: int32): uint32;
stdcall; external 'spcm_win32.dll' name '_spcm_dwSetParam_i32@12';

function spcm_dwSetParam_i64 (hDevice, lRegister: int32; llValue: int64): uint32;
stdcall; external 'spcm_win32.dll' name '_spcm_dwSetParam_i64@16';

function spcm_dwSetParam_d64 (hDevice, lRegister: int32; dValue: double): uint32;
stdcall; external 'spcm_win32.dll' name '_spcm_dwSetParam_d64@16';

function spcm_dwGetParam_i32 (hDevice, lRegister: int32; var plValue: int32): uint32;
stdcall; external 'spcm_win32.dll' name '_spcm_dwGetParam_i32@12';

function spcm_dwGetParam_i64 (hDevice, lRegister: int32; var pllValue: int64): uint32;
stdcall; external 'spcm_win32.dll' name '_spcm_dwGetParam_i64@12';

function spcm_dwGetParam_d64 (hDevice, lRegister: int32; var pdValue: double): uint32;
stdcall; external 'spcm_win32.dll' name '_spcm_dwGetParam_d64@12';

// ----- data handling -----
function spcm_dwDefTransfer_i64 (hDevice, dwBufType, dwDirection, dwNotifySize: int32; pvDataBuffer: Pointer;
llBrdOffs, llTransferLen: int64): uint32;
stdcall; external 'spcm_win32.dll' name '_spcm_dwDefTransfer_i64@36';

function spcm_dwInvalidateBuf (hDevice, lBuffer: int32): uint32;
stdcall; external 'spcm_win32.dll' name '_spcm_dwInvalidateBuf@8';
```

file SpcRegs.pas

The SpcRegs.pas file defines all constants that are used for the driver. The constant names are the same names as used under the C/C++ examples. All constants names will be found throughout this hardware manual when certain aspects of the driver usage are explained. It is recommended to only use these constant names for better visibility of the programs:

```
const SPC_M2CMD                = 100;                { write a command }
const M2CMD_CARD_RESET        = $00000001;          { hardware reset   }
const M2CMD_CARD_WRITESETUP    = $00000002;          { write setup only }
const M2CMD_CARD_START        = $00000004;          { start of card (including writesetup) }
const M2CMD_CARD_ENABLETRIGGER = $00000008;          { enable trigger engine }
...
```

file SpcErr.pas

The SpcErr.pas file contains all error codes that may be returned by the driver.

Including the driver files

To use the driver function and all the defined constants it is necessary to include the files into the project as shown in the picture on the right. The project overview is taken from one of the examples delivered on the USB stick. Besides including the driver files in the project it is also necessary to include them in the uses section of the source files where functions or constants should be used:

```
uses
  Windows, Messages, SysUtils, Classes, Graphics, Controls, Forms, Dialogs,
  StdCtrls, ExtCtrls,

  SpcRegs, SpcErr, spcm_win32;
```

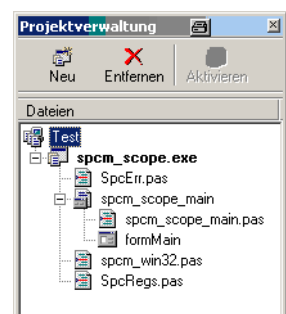


Image 39: Structure of the Delphi examples

Examples

Examples for Delphi can be found on the USB stick in the directory /examples/delphi. The directory contains the above mentioned delphi header files and a couple of universal examples, each of them working with a certain type of card. Please feel free to use these examples as a base for your programs and to modify them in any kind.

spcm_scope

The example implements a very simple scope program that makes single acquisitions on button pressing. A fixed setup is done inside the example. The spcm_scope example can be used with any analog data acquisition card from Spectrum. It covers cards with 1 byte per sample (8 bit resolution) as well as cards with 2 bytes per sample (12, 14 and 16 bit resolution)

The program shows the following steps:

- Initialization of a card and reading of card information like type, function and serial number
- Doing a simple card setup
- Performing the acquisition and waiting for the end interrupt
- Reading of data, re-scaling it and displaying waveform on screen

.NET programming languages

Library

For using the driver with a .NET based language Spectrum delivers a special library that encapsulates the driver in a .NET object. By adding this object to the project it is possible to access all driver functions and constants from within your .NET environment.

There is one small console based example for each supported .NET language that shows how to include the driver and how to access the cards. Please combine this example with the different standard examples to get the different card functionality.

Declaration

The driver access methods and also all the type, register and error declarations are combined in the object Spcm and are located in one of the two DLLs either SpcmDrv32.NET.dll or SpcmDrv64.NET.dll delivered with the .NET examples.



For simplicity, either file is simply called „SpcmDrv.NET.dll“ in the following passages and the actual file name must be replaced with either the 32bit or 64bit version according to your application.

Spectrum also delivers the source code of the DLLs as a C# project. These sources are located in the directory SpcmDrv.NET.

```
namespace Spcm
{
    public class Drv
    {
        [DllImport("spcm_win32.dll")]public static extern IntPtr spcm_hOpen (string szDeviceName);
        [DllImport("spcm_win32.dll")]public static extern void spcm_vClose (IntPtr hDevice);
    }
    ...
    public class CardType
    {
        public const int TYP_M2I2020 = unchecked ((int)0x00032020);
        public const int TYP_M2I2021 = unchecked ((int)0x00032021);
        public const int TYP_M2I2025 = unchecked ((int)0x00032025);
    }
    ...
    public class Regs
    {
        public const int SPC_M2CMD = unchecked ((int)100);
        public const int M2CMD_CARD_RESET = unchecked ((int)0x00000001);
        public const int M2CMD_CARD_WRITESETUP = unchecked ((int)0x00000002);
    }
    ...
}
```

Using C#

The SpcmDrv.NET.dll needs to be included within the Solution Explorer in the References section. Please use right mouse and select „AddReference“. After this all functions and constants of the driver object are available.

Please see the example in the directory CSharp as a start:

```
// ----- open card -----
hDevice = Drv.spcm_hOpen("/dev/spcm0");
if ((int)hDevice == 0)
{
    Console.WriteLine("Error: Could not open card\n");
    return 1;
}

// ----- get card type -----
dwErrorCode = Drv.spcm_dwGetParam_i32(hDevice, Regs.SPC_PCITYP, out lCardType);
dwErrorCode = Drv.spcm_dwGetParam_i32(hDevice, Regs.SPC_PCISERIALNR, out lSerialNumber);
```

Example for digitizerNETBOX/generatorNETBOX and remotely installed cards:

```
// ----- open remote card -----  
hDevice = Drv.spcm_hOpen("TCPIP::192.168.169.14::INST0::INSTR");
```

Using Managed C++/CLI

The SpcmDrv.NET.dll needs to be included within the project options. Please select „Project“ - „Properties“ - „References“ and finally „Add new Reference“. After this all functions and constants of the driver object are available.

Please see the example in the directory CppCLR as a start:

```
// ----- open card -----
hDevice = Drv::spcm_hOpen("/dev/spcm0");
if ((int)hDevice == 0)
{
    Console::WriteLine("Error: Could not open card\n");
    return 1;
}

// ----- get card type -----
dwErrorCode = Drv::spcm_dwGetParam_i32(hDevice, Regs::SPC_PCITYP, lCardType);
dwErrorCode = Drv::spcm_dwGetParam_i32(hDevice, Regs::SPC_PCISERIALNR, lSerialNumber);
```

Example for digitizerNETBOX/generatorNETBOX and remotely installed cards:

```
// ----- open remote card -----
hDevice = Drv::spcm_hOpen("TCPIP::192.168.169.14::INST0::INSTR");
```

Using VB.NET

The SpcmDrv.NET.dll needs to be included within the project options. Please select „Project“ - „Properties“ - „References“ and finally „Add new Reference“. After this all functions and constants of the driver object are available.

Please see the example in the directory VB.NET as a start:

```
' ----- open card -----
hDevice = Drv.spcm_hOpen("/dev/spcm0")

If (hDevice = 0) Then
    Console.WriteLine("Error: Could not open card\n")
Else

    ' ----- get card type -----
    dwError = Drv.spcm_dwGetParam_i32(hDevice, Regs.SPC_PCITYP, lCardType)
    dwError = Drv.spcm_dwGetParam_i32(hDevice, Regs.SPC_PCISERIALNR, lSerialNumber)
```

Example for digitizerNETBOX/generatorNETBOX and remotely installed cards:

```
' ----- open remote card -----
hDevice = Drv.spcm_hOpen("TCPIP::192.168.169.14::INST0::INSTR")
```

Using J#

The SpcmDrv.NET.dll needs to be included within the Solution Explorer in the References section. Please use right mouse and select „AddReference“. After this all functions and constants of the driver object are available.

Please see the example in the directory JSharp as a start:

```
// ----- open card -----
hDevice = Drv.spcm_hOpen("/dev/spcm0");

if (hDevice.ToInt32() == 0)
    System.out.println("Error: Could not open card\n");
else
{
    // ----- get card type -----
    dwErrorCode = Drv.spcm_dwGetParam_i32(hDevice, Regs.SPC_PCITYP, lCardType);
    dwErrorCode = Drv.spcm_dwGetParam_i32(hDevice, Regs.SPC_PCISERIALNR, lSerialNumber);
```

Example for digitizerNETBOX/generatorNETBOX and remotely installed cards:

```
' ----- open remote card -----
hDevice = Drv.spcm_hOpen("TCPIP::192.168.169.14::INST0::INSTR")
```

Python Programming Interface and Examples

The Spectrum Instrumentation API has extensive support for Python. There is an implementation for both low- and high-level Python programming. The low-level API is closely related to C and optimized for speed. The high-level general-purpose object-oriented API is located on Github and available through the pip repository and optimized for usability and learning how to use the cards.

High-level object oriented Python package spcm

Build on top of the low-level Python API, there is a general purpose high-level object oriented Python package. This spcm package is available through the PIP repository and is easily installed using the straight-forward installation command:

```
pip install spcm
```

The package automatically handles correct opening and closing of cards and Netbox devices, including sets of synchronizes cards. It also implements error handling through exceptions.

Moreover, the package handles allocation of memory and provides a direct interface to numpy and support for physical quantities and units through pint. A multitude of card functionalities are implemented in easy-to-use classes and examples. The spcm package can be found here:

- Spectrum Instrumentation Python package on GitHub: <https://github.com/SpectrumInstrumentation/spcm>
- Spectrum Instrumentation Python examples on GitHub: <https://github.com/SpectrumInstrumentation/spcm/tree/master/src/examples>
- Spectrum Instrumentation Python repository on GitHub: <https://pypi.org/project/spcm/>
- Spectrum Instrumentation Python reference documentation on GitHub: <https://spectruminstrumentation.github.io/spcm/spcm.html>

The spcm is free-to-use and freely available to all Spectrum Instrumentation card users under the MIT-license. The package is only available for Python 3 starting with version 3.9.

Low-level driver interface

The driver interface contains the following files. The files need to be included in the python project. Please do not edit any of these files as they are regularly updated if new functions or registers have been included. To use pyspcm you need either python 2 (2.4, 2.6 or 2.7) or python 3 (3.x) and ctypes, which is included in python 2.6 and newer and needs to be installed separately for Python 2.4.

file pyspcm.py

The file contains the interface to the driver library and defines some needed constants. All functions of the python library are similar to the above explained standard driver functions and use ctypes as input and return parameters:

```
# ----- Windows -----
# Load DLL into memory.

# use windll because all driver access functions use _stdcall calling convention under windows
if (bIs64Bit == 1):
    spcmDll = windll.LoadLibrary ("spcm_win64.dll")
else:
    spcmDll = windll.LoadLibrary ("spcm_win32.dll")

# load spcm_hOpen
if (bIs64Bit):
    spcm_hOpen = getattr(spcmDll, "spcm_hOpen")
else:
    spcm_hOpen = getattr(spcmDll, "_spcm_hOpen@4")
spcm_hOpen.argtype = [c_char_p]
spcm_hOpen.restype = drv_handle

# load spcm_vClose
if (bIs64Bit):
    spcm_vClose = getattr(spcmDll, "spcm_vClose")
else:
    spcm_vClose = getattr(spcmDll, "_spcm_vClose@4")
spcm_vClose.argtype = [drv_handle]
spcm_vClose.restype = None

# load spcm_dwGetErrorInfo_i32
if (bIs64Bit):
    spcm_dwGetErrorInfo_i32 = getattr(spcmDll, "spcm_dwGetErrorInfo_i32")
else:
    spcm_dwGetErrorInfo_i32 = getattr(spcmDll, "_spcm_dwGetErrorInfo_i32@16")
spcm_dwGetErrorInfo_i32.argtype = [drv_handle, uptr32, ptr32, c_char_p]
spcm_dwGetErrorInfo_i32.restype = uint32

...
```

file regs.py

The regs.py file defines all constants that are used for the driver. The constant names are the same names compared to the C/C++ examples. All constant names will be found throughout this hardware manual when certain aspects of the driver usage are explained. It is recommended to only use these constant names for better readability of the programs:

```
SPC_M2CMD = 1001                # write a command
M2CMD_CARD_RESET = 0x000000011  # hardware reset
M2CMD_CARD_WRITESETUP = 0x000000021 # write setup only
M2CMD_CARD_START = 0x000000041  # start of card (including writesetup)
M2CMD_CARD_ENABLETRIGGER = 0x000000081 # enable trigger engine
...
```

file spcerr.py

The spcerr.py file contains all error codes that may be returned by the driver.

Examples

Examples for Python can be found on the USB stick in the directory /examples/python. The directory contains the above mentioned header files and some examples, each of them working with a certain type of card. Please feel free to use these examples as a base for your programs and to modify them in any kind.

When allocating the buffer for DMA transfers, use the following function to get a mutable character buffer:
ctypes.create_string_buffer(init_or_size[, size])

**Java Programming Interface and Examples****Driver interface**

The driver interface contains the following Java files (classes). The files need to be included in your Java project. Please do not edit any of these files as they are regularly updated if new functions or registers have been included. The driver interface uses the Java Native Access (JNA) library.

This library is licensed under the LGPL (<https://www.gnu.org/licenses/lgpl-3.0.en.html>) and has also to be included to your Java project.

To download the latest jna.jar package and to get more information about the JNA project please check the projects GitHub page under: <https://github.com/java-native-access/jna>

The following files can be found in the „SpcmDrv“ folder of your Java examples install path.

SpcmDrv32.java / SpcmDrv64.java

The files contain the interface to the driver library and defines some needed constants. All functions of the driver interface are similar to the above explained standard driver functions. Use the SpcmDrv32.java for 32 bit and the SpcmDrv64.java for 64 bit projects:

```
...

public interface SpcmWin64 extends StdCallLibrary {

    SpcmWin64 INSTANCE = (SpcmWin64)Native.loadLibrary ("spcm_win64"), SpcmWin64.class);

    long spcm_hOpen (String sDeviceName);
    void spcm_vClose (long hDevice);
    int spcm_dwSetParam_i64 (long hDevice, int lRegister, long llValue);
    int spcm_dwGetParam_i64 (long hDevice, int lRegister, LongByReference pllValue);
    int spcm_dwSetParam_ptr (long hDevice, int lRegister, Pointer pValue, long llLen);
    int spcm_dwGetParam_ptr (long hDevice, int lRegister, Pointer pValue, long llLen);
    int spcm_dwSetParam_d64 (int hDevice, int lRegister, double dValue);
    int spcm_dwGetParam_d64 (int hDevice, int lRegister, DoubleByReference pdValue);
    int spcm_dwDefTransfer_i64 (long hDevice, int lBufType, int lDirection, int lNotifySize, Pointer pDataBuffer,
    long llBrdOffs, long llTransferLen);

    int spcm_dwInvalidateBuf (long hDevice, int lBufType);

    int spcm_dwGetErrorInfo_i32 (long hDevice, IntByReference plErrorReg, IntByReference plErrorValue, Pointer sErrorTextBuffer);

    int spcm_dwGetErrorInfo_i64 (long hDevice, IntByReference plErrorReg, LongByReference pllErrorValue, Pointer sErrorTextBuffer);

    int spcm_dwGetErrorInfo_d64 (long hDevice, IntByReference plErrorReg, DoubleByReference pdErrorValue, Pointer sErrorTextBuffer);
}
...
```

SpcmRegs.java

The SpcmRegs class defines all constants that are used for the driver. The constants names are the same names compared to the C/C++ examples. All constant names will be found throughout this hardware manual when certain aspects of the driver usage are explained. It is recommended to only use these constant names for better readability of the programs:

```
...
public static final int SPC_M2CMD = 100;
public static final int M2CMD_CARD_RESET = 0x00000001;
public static final int M2CMD_CARD_WRITESETUP = 0x00000002;
public static final int M2CMD_CARD_START = 0x00000004;
public static final int M2CMD_CARD_ENABLETRIGGER = 0x00000008;
...
```

SpcmErrors.java

The SpcmErrors class contains all error codes that may be returned by the driver.

Examples

Examples for Java can be found on the USB stick in the directory /examples/java. The directory contains the above mentioned header files and some examples, each of them working with a certain type of card. Please feel free to use these examples as a base for your programs and to modify them in any kind.

Julia Programming Interface and Examples**Driver interface**

The driver interface contains the following files. The files need to be included in the julia project. Please do not edit any of these files as they are regularly updated if new functions or registers have been included.

file spcm_drv.jl

The file contains the interface to the driver library and defines some needed constants. All functions of the Julia library are similar to the above explained standard driver functions.

```
hDevice::Int64 = spcm_hOpen(sDeviceName::String)
Cvoid spcm_vClose(hDevice::Int64)

dwErr::UInt32, lValue::Int32 = spcm_dwGetParam_i32(hDevice::Int64, lRegister::Int32)
dwErr::UInt32, llValue::Int64 = spcm_dwGetParam_i64(hDevice::Int64, lRegister::Int32)
dwErr::UInt32, dValue::Float64 = spcm_dwGetParam_d64(hDevice::Int64, lRegister::Int32)

dwErr::UInt32 = spcm_dwSetParam_i32(hDevice::Int64, lRegister::Int32, lValue::Int32)
dwErr::UInt32 = spcm_dwSetParam_i64(hDevice::Int64, lRegister::Int32, llValue::Int64)
dwErr::UInt32 = spcm_dwSetParam_d64(hDevice::Int64, lRegister::Int32, dValue::Float64)

dwErr::UInt32 = spcm_dwDefTransfer_i64(hDevice::Int64, lBufType::Int32, lDirection::Int32,
                                     dwNotifySize::UInt32, pDataBuffer::Array{Int16,1},
                                     qwBrdOffs::UInt64, qwTransferLen::UInt64)

dwErr::UInt32 = spcm_dwDefTransfer_i64(hDevice::Int64, lBufType::Int32, lDirection::Int32,
                                     dwNotifySize::UInt32, pDataBuffer::Array{Int8,1},
                                     qwBrdOffs::UInt64, qwTransferLen::UInt64)

dwErr::UInt32 = spcm_dwInvalidateBuf(hDevice::Int64, lBufType::Int32)

dwErr::UInt32, dwErrReg::UInt32, lErrVal::Int32, sErrText::String = spcm_dwGetErrorInfo_i32(hDevice::Int64)
dwErr::UInt32, dwErrReg::UInt32, llErrVal::Int64, sErrText::String = spcm_dwGetErrorInfo_i64(hDevice::Int64)
dwErr::UInt32, dwErrReg::UInt32, dErrVal::Float64, sErrText::String = spcm_dwGetErrorInfo_d64(hDevice::Int64)
```

file regs.jl

The regs.jl file defines all constants that are used for the driver. The constant names are the same names compared to the C/C++ examples. All constant names will be found throughout this hardware manual when certain aspects of the driver usage are explained. It is recommended to only use these constant names for better readability of the programs:

```
const SPC_M2CMD = Int32(100) # write a command
const M2CMD_CARD_RESET = Int32(1) # 0x00000001 # hardware reset
const M2CMD_CARD_WRITESETUP = Int32(2) # 0x00000002 # write setup only
const M2CMD_CARD_START = Int32(4) # 0x00000004 # start of card (including writesetup)
const M2CMD_CARD_ENABLETRIGGER = Int32(8) # 0x00000008 # enable trigger engine
# ...
```

file spcerr.il

The spcerr.il file contains all error codes that may be returned by the driver.

Examples

Examples for Julia can be found on USB-Stick in the directory /examples/julia. The directory contains the above mentioned include files and some examples, each of them working with a certain type of card. Please feel free to use these examples as a base for your programs and to modify them in any kind.

LabVIEW driver and examples

A full set of drivers and examples is available for LabVIEW for Windows. LabVIEW for Linux is currently not supported. The LabVIEW drivers have their own manual. The LabVIEW drivers, examples and the manual are found on the USB stick that has been included in the delivery. The latest version is also available on our webpage www.spectrum-instrumentation.com

Please follow the description in the LabVIEW manual for installation and usage of the LabVIEW drivers for this card.

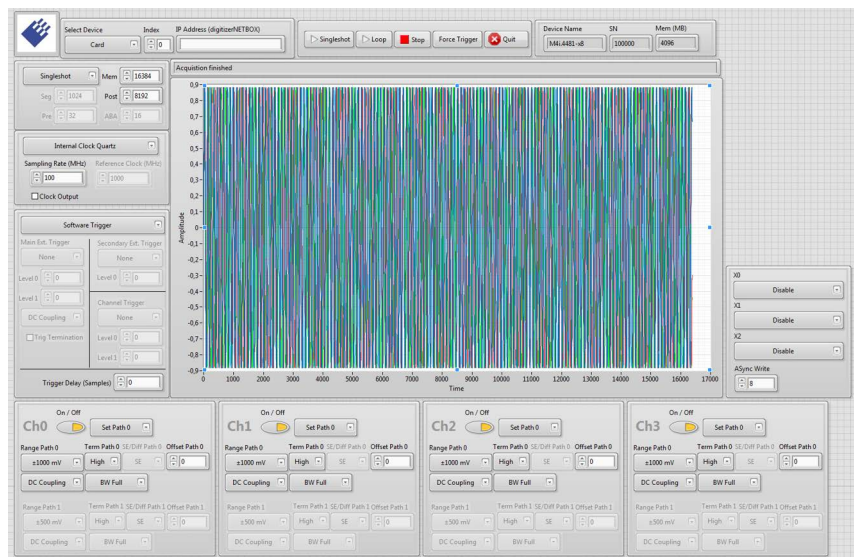


Image 40: LabVIEW driver oscilloscope example

MATLAB driver and examples

A full set of drivers and examples is available for Mathworks MATLAB for Windows (32 bit and 64 bit versions) and also for MATLAB for Linux (64 bit version). There is no additional toolbox needed to run the MATLAB examples and drivers.

The MATLAB drivers have their own manual. The MATLAB drivers, examples and the manual are found on the USB stick that has been included in the delivery. The latest version is also available on our webpage www.spectrum-instrumentation.com

Please follow the description in the MATLAB manual for installation and usage of the MATLAB drivers for this card.

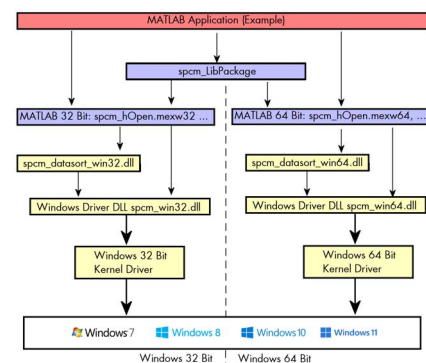


Image 41: Spectrum MATLAB driver structure

SCAPP – CUDA GPU based data processing

Spectrum's CUDA Access for Parallel Processing

Modern GPUs (Graphic Processing Units) are designed to handle a large number of parallel operations. While a CPU offers only a few cores for parallel calculations, a GPU can offer thousands of cores. This computing capabilities can be used for calculations using the Nvidia CUDA interface.

Since bus bandwidth and CPU power are often a bottleneck in calculations, CUDA Remote Direct

Memory Access (RDMA) can be used to directly transfer data from/to a Spectrum Digitizer/Generator to/from a GPU card for processing, thus avoiding the transfer of raw data to the host memory and benefiting from the computational power of the GPU.

For applications requiring high performance signal and data processing Spectrum offers SCAPP (Spectrum's CUDA Access for Parallel Processing).

The SCAPP SDK allows a direct link between Spectrum digitizers or generators and CUDA based GPU cards. Once data is available to the GPU, users can harness the processing power of the GPU's massive number of processing cores and large, ultra-high-speed GPU memory. SCAPP uses an RDMA (Linux only) process to send data at the digitizers full PCIe transfer speed to the GPU card. The SDK includes a set of examples for interaction between the digitizer or generator and the GPU card and another set of CUDA parallel processing examples with easy building blocks for basic functions like filtering, averaging, data de-multiplexing, data conversion or FFT. All the software is based on C/C++ and can easily be implemented, expanded and modified with normal programming skills.

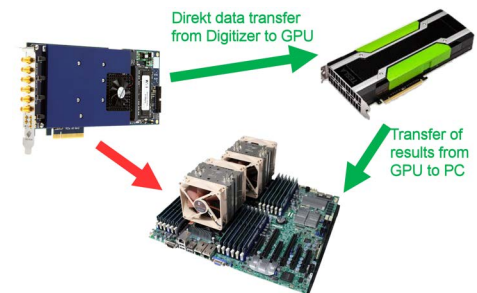


Image 42: GPU usage with SCAPP SDK: data transfer options

Please follow the description in the SCAPP manual for installation and usage of the SCAPP drivers for this card.



Please note that the DDS commands for cards that support one of the DDS features cannot be directly streamed from the GPU to the card, since the necessary re-calculation of the hardware's DDS registers requires calculation to be done under control of the host CPU.

Programming the Board

Overview

The following chapters show you in detail how to program the different aspects of the board. For every topic there's a small example. For the examples we focused on Visual C++. However as shown in the last chapter the differences in programming the board under different programming languages are marginal. This manual describes the programming of the whole hardware family. Some of the topics are similar for all board versions. But some differ a little bit from type to type. Please check the given tables for these topics and examine carefully which settings are valid for your special kind of board.

Register tables

The programming of the boards is totally software register based. All software registers are described in the following form:

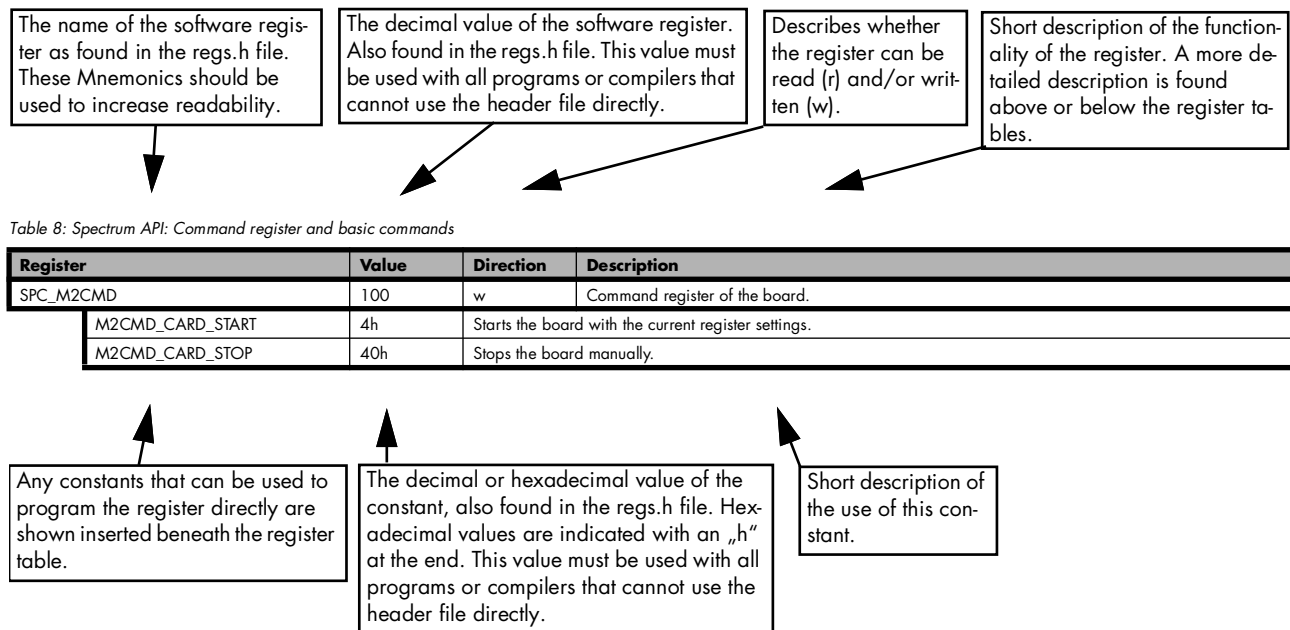


Table 8: Spectrum API: Command register and basic commands

Register	Value	Direction	Description
SPC_M2CMD	100	w	Command register of the board.
M2CMD_CARD_START	4h		Starts the board with the current register settings.
M2CMD_CARD_STOP	40h		Stops the board manually.

If no constants are given below the register table, the dedicated register is used as a switch. All such registers are activated if written with a "1" and deactivated if written with a "0".



Programming examples

In this manual a lot of programming examples are used to give you an impression on how the actual mentioned registers can be set within your own program. All of the examples are located in a separated colored box to indicate the example and to make it easier to differ it from the describing text.

All of the examples mentioned throughout the manual are written in C/C++ and can be used with any C/C++ compiler for Windows or Linux.

Complete C/C++ Example

```

#include "../c_header/dlltyp.h"
#include "../c_header/regs.h"
#include "../c_header/spcm_drv.h"

#include <stdio.h>

int main()
{
    drv_handle hDrv;                // the handle of the device
    int32 lCardType;                // a place to store card information

    hDrv = spcm_hOpen ("/dev/spcm0"); // Opens the board and gets a handle
    if (!hDrv)                       // check whether we can access the card
        return -1;

    spcm_dwGetParam_i32 (hDrv, SPC_PCITYP, &lCardType); // simple command, read out of card type
    printf ("Found card M2i/M3i/M4i/M4x/M2p/M5i.%04x in the system\n", lCardType & TYP_VERSIONMASK);
    spcm_vClose (hDrv);

    return 0;
}

```

Initialization

Before using the card it is necessary to open the kernel device to access the hardware. It is only possible to use every device exclusively using the handle that is obtained when opening the device. Opening the same device twice will only generate an error code. After ending the driver use the device has to be closed again to allow later re-opening. Open and close of driver is done using the `spcm_hOpen` and `spcm_vClose` function as described in the "Driver Functions" chapter before.

Open/Close Example

```

drv_handle hDrv;                // the handle of the device

hDrv = spcm_hOpen ("/dev/spcm0"); // Opens the board and gets a handle
if (!hDrv)                       // check whether we can access the card
{
    printf "Open failed\n";
    return -1;
}

... do any work with the driver

spcm_vClose (hDrv);
return 0;

```

Initialization of Remote Products

The only step that is different when accessing remotely controlled cards or digitizerNETBOXes is the initialization of the driver. Instead of the local handle one has to open the VISA string that is returned by the discovery function. Alternatively it is also possible to access the card directly without discovery function if the IP address of the device is known.

```

drv_handle hDrv;                // the handle of the device

hDrv = spcm_hOpen ("TCPIP::192.168.169.14::INSTR"); // Opens the remote board and gets a handle
if (!hDrv)                                       // check whether we can access the card
{
    printf "Open of remote card failed\n";
    return -1;
}

...

```

Multiple cards are opened by indexing the remote card number:

```

hDrv = spcm_hOpen ("TCPIP::192.168.169.14::INSTR"); // Opens the remote board #0
hDrv = spcm_hOpen ("TCPIP::192.168.169.14::INST0::INSTR"); // or alternatively
hDrv = spcm_hOpen ("TCPIP::192.168.169.14::INST0::INSTR"); // Opens the remote board #0
hDrv = spcm_hOpen ("TCPIP::192.168.169.14::INST1::INSTR"); // all other boards require an index:
hDrv = spcm_hOpen ("TCPIP::192.168.169.14::INST2::INSTR"); // Opens the remote board #1
hDrv = spcm_hOpen ("TCPIP::192.168.169.14::INST2::INSTR"); // Opens the remote board #2

```

Error handling

If one action caused an error in the driver this error and the register and value where it occurs will be saved.

The driver is then locked until the error is read out using the error function `spcm_dwGetErrorInfo_i32`. Any calls to other functions will just return the error code `ERR_LASTERR` showing that there is an error to be read out.



This error locking functionality will prevent the generation of unseen false commands and settings that may lead to totally unexpected behavior. For sure there are only errors locked that result on false commands or settings. Any error code that is generated to report a condition to the user won't lock the driver. As example the error code `ERR_TIMEOUT` showing that the a timeout in a wait function has occurred won't lock the driver and the user can simply react to this error code without reading the complete error function.

As a benefit from this error locking it is not necessary to check the error return of each function call but just checking the error function once at the end of all calls to see where an error occurred. The enhanced error function returns a complete error description that will lead to the call that produces the error.

Example for error checking at end using the error text from the driver:

```
char szErrorText[ERRORTXTLEN];

spcm_dwSetParam_i64 (hDrv, SPC_SAMPLERATE, 1000000);           // correct command
spcm_dwSetParam_i64 (hDrv, SPC_MEMSIZE, -345);                // faulty command
spcm_dwSetParam_i64 (hDrv, SPC_POSTTRIGGER, 1024);            // correct command
if (spcm_dwGetErrorInfo_i32 (hDrv, NULL, NULL, szErrorText) != ERR_OK) // check for an error
{
    printf (szErrorText);                                       // print the error text
    spcm_vClose (hDrv);                                         // close the driver
    exit (0);                                                  // and leave the program
}
```

This short program then would generate a printout as:

```
Error occurred at register SPC_MEMSIZE with value -345: value not allowed
```

All error codes are described in detail in the appendix. Please refer to this error description and the description of the software register to examine the cause for the error message.



Any of the parameters of the `spcm_dwGetErrorInfo_i32` function can be used to obtain detailed information on the error. If one is not interested in parts of this information it is possible to just pass a `NULL` (zero) to this variable like shown in the example. If one is not interested in the error text but wants to install its own error handler it may be interesting to just read out the error generating register and value.

Example for error checking with own (simple) error handler:

```
uint32 dwErrorReg;
int32 lErrorValue;
uint32 dwErrorCode;

spcm_dwSetParam_i64 (hDrv, SPC_SAMPLERATE, 1000000);           // correct command
spcm_dwSetParam_i64 (hDrv, SPC_MEMSIZE, -345);                // faulty command
spcm_dwSetParam_i64 (hDrv, SPC_POSTTRIGGER, 1024);            // correct command
dwErrorCode = spcm_dwGetErrorInfo_i32 (hDrv, &dwErrorReg, &lErrorValue, NULL);
if (dwErrorCode) // check for an error
{
    printf ("Errorcode: %d in register %d at value %d\n", lErrorValue, dwErrorReg, lErrorValue);
    spcm_vClose (hDrv);                                         // close the driver
    exit (0);                                                  // and leave the program
}
```

Printing custom strings to the driver debug log

The detailed driver debug logfile has proven to not only being a great help for support issues, but also for one's own debugging during application development. To additionally help the user in debugging, the driver allows to print output lines initiated by the application software.

This feature requires the `scm_dwSetParam_ptr` to be implemented, which has been added with driver version V7.00

The following example shows how to print a custom message to the logfile:

```
const char* szText = "My custom log file entry";
spcm_dwSetParam_ptr (NULL, SPC_WRITE_TO_LOG, szText, strlen(szText)); // print line to debug log file
```

Gathering information from the card

When opening the card the driver library internally reads out a lot of information from the on-board eeprom. The driver also offers additional information on hardware details. All of this information can be read out and used for programming and documentation. This chapter will show all general information that is offered by the driver. There is also some more information on certain parts of the card, like clock machine or trigger machine, that is described in detail in the documentation of that part of the card.

All information can be read out using one of the `spcm_dwGetParam` functions. Please stick to the “Driver Functions” chapter for more details on this function.

Card type

The card type information returns the specific card type that is found under this device. When using multiple cards in one system it is highly recommended to read out this register first to examine the ordering of cards. Please don't rely on the card ordering as this is based on the BIOS, the bus connections and the operating system.

Table 9: Spectrum API: Card Type Register

Register	Value	Direction	Description
SPC_PCITYP	2000	read	Type of board as listed in the table below.

The SPC_PCITYP register can be used to read the numeric card type as well as a full name of the card using the `spcm_dwGetParam_ptr` function:

```
// read out the numeric card type as shown in the list below
spcm_dwGetParam_i32 (hDrv, SPC_PCITYP, &lCardType);

// read out the official name of the card
char acCardType[20] = {};
spcm_dwGetParam_ptr (hCard, SPC_PCITYP, acCardType, sizeof (acCardType));

// printout both information:
printf ("Found: %s (decimal: %d)\n", acCardType, lCardType);
```

One of the following values is returned, when reading this register. Each card has its own card type constant defined in `regs.h`. Please note that when reading the card information as a hex value, the lower word shows the digits of the card name while the upper word is a indication for the used bus type.

Card type	Card type as defined in regs.h	Value hexadecimal	Value decimal	Card type	Card type as defined in regs.h	Value hexadecimal	Value decimal
M4i.2320-x8	TYP_M4I2320_X8	72320h	467744	M4i.2330-x8	TYP_M4I2330_X8	72330h	467760
M4i.2321-x8	TYP_M4I2321_X8	72321h	467745	M4i.2333-x8	TYP_M4I2333_X8	72333h	467763
M4i.2323-x8	TYP_M4I2323_X8	72323h	467747	M4i.2334-x8	TYP_M4I2334_X8	72334h	467764

Hardware and PCB version

Since all of the boards from Spectrum are modular boards, they consist of one base board and one piggy-back front-end module and eventually of an extension module like the star-hub. Each of these three kinds of hardware has its own version register. Normally you do not need this information but if you have a support question, please provide the revision together with it.

Table 10: Spectrum API: hardware and PCB version register overview

Register	Value	Direction	Description
SPC_PCIVERSION	2010	read	Base card version: the upper 16 bit show the hardware version, the lower 16 bit show the firmware version.
SPC_BASEPCBVERSION	2014	read	Base card PCB version: the lower 16 bit are divided into two 8 bit values containing pre/post decimal point version information. For example a lower 16 bit value of 0106h represents a PCB version V1.6. The upper 16 bit are always zero.
SPC_PCIMODULEVERSION	2012	read	Module version: the upper 16 bit show the hardware version, the lower 16 bit show the firmware version.
SPC_MODULEPCBVERSION	2015	read	Module PCB version: the lower 16 bit are divided into two 8 bit values containing pre/post decimal point version information. For example a lower 16 bit value of 0106h represents a PCB version V1.6. The upper 16 bit are always zero.

If your board has an additional piggy-back extension module mounted you can get the hardware version with the following register.

Table 11: Spectrum API: extension module hardware and PCB version register

Register	Value	Direction	Description
SPC_PCIEXTVERSION	2011	read	Extension module version: the upper 16 bit show the hardware version, the lower 16 bit show the firmware version.
SPC_EXTPCBVERSION	2017	read	Extension module PCB version: the lower 16 bit are divided into two 8 bit values containing pre/post decimal point version information. For example a lower 16 bit value of 0106h represents a PCB version V1.6. The upper 16 bit are always zero.

Reading currently used PXI slot No. (M4x only)

For the PXIe cards of the M4x.xxxx series it is possible to read out the current slot number, in which the card is installed within the chassis:

Table 12: Spectrum API: register for reading back the PXIe card slot number

Register	Value	Direction	Description
SPC_PXIHWSLOTNO	2055	read	Returns the currently used slot number of the chassis.

Firmware versions

All the cards from Spectrum typically contain multiple programmable devices such as FPGAs, CPLDs and the like. Each of these have their own dedicated firmware version. This version information is readable for each device through the various version registers. Normally you do not need this information but if you have a support question, please provide us with this information. Please note that number of devices and hence the readable firmware information is card series dependent:

Table 13: Spectrum API: Register overview of firmware versions

Register	Value	Direction	Description	Available for					
				M2i	M3i	M4i	M4x	M2p	M5i
SPCM_FW_CTRL	210000	read	Main control FPGA version: the upper 16 bit show the firmware type, the lower 16 bit show the firmware version. For the standard release firmware, the type has always a value of 1.	X	X	X	X	X	X
SPCM_FW_CTRL_GOLDEN	210001	read	Main control FPGA golden version: the upper 16 bit show the firmware type, the lower 16 bit show the firmware version. For the golden (recovery) firmware, the type has always a value of 2.	—	—	X	X	X	X
SPCM_FW_CLOCK	210010	read	Clock distribution version: the upper 16 bit show the firmware type, the lower 16 bit show the firmware version. For the standard release firmware, the type has always a value of 1.	X	—	—	—	—	—
SPCM_FW_CONFIG	210020	read	Configuration controller version: the upper 16 bit show the firmware type, the lower 16 bit show the firmware version. For the standard release firmware, the type has always a value of 1.	X	X	—	—	—	—
SPCM_FW_MODULEA	210030	read	Front-end module A version: the upper 16 bit show the firmware type, the lower 16 bit show the firmware version. For the standard release firmware, the type has always a value of 1.	X	X	X	X	X	X
SPCM_FW_MODULEB	210031	read	Front-end module B version: the upper 16 bit show the firmware type, the lower 16 bit show the firmware version. For the standard release firmware, the type has always a value of 1. The version is zero if no second front-end module is installed on the card.	X	—	—	—	X	—
SPCM_FW_MODEXTRA	210050	read	Extension module (Star-Hub) version: the upper 16 bit show the firmware type, the lower 16 bit show the firmware version. For the standard release firmware, the type has always a value of 1. The version is zero if no extension module is installed on the card.	X	X	X	—	X	X
SPCM_FW_POWER	210060	read	Power controller version: the upper 16 bit show the firmware type, the lower 16 bit show the firmware version. For the standard release firmware, the type has always a value of 1.	—	—	X	X	X	X

Cards that do provide a golden recovery image for the main control FPGA, the currently booted firmware can additionally read out:

Table 14: Spectrum API: Register overview of reading current firmware

Register	Value	Direction	Description	Available for					
				M2i	M3i	M4i	M4x	M2p	M5i
SPCM_FW_CTRL_ACTIVE	210002	read	Cards that do provide a golden (recovery) firmware additionally have a register to read out the version information of the currently loaded firmware image, to determine if it is a standard or golden image, and which kind of standard version is booted, in case that different configurations are available. The hexadecimal 32bit format is: TVVCCUUh T: the currently booted type (1: standard, 2: golden) V: the version C: configuration : for different kinds of firmware (0: default) U: unused , in production versions always zero	—	—	X	X	X	X
SPC_NUM_FW_CONFIGS	210100	read	Allows to read out the number of different firmware images available for the current card series. Each available firmware will have a different configuration .	—	—	X	X	X	X

The following example shows how to read out the number of available firmware configurations for the card series and displays which configuration is currently used.

```
spcm_dwGetParam_i32 (hDrv, SPCM_FW_CTRL_ACTIVE, &lActiveFW);

int32 lTyp = ((lActiveFW >> 28) & 0xf);
int32 lVer = ((lActiveFW >> 16) & 0xffff);
int32 lCfg = ((lActiveFW >> 8) & 0xff);

spcm_dwGetParam_i32 (hDrv, SPC_NUM_FW_CONFIGS, &lNumOfFW);
printf ("%d FW configs available. Active FW T:%d, V:%d, C:%d\n", lNumOfFW, lTyp, lVer, lCfg);
```



Most cards only have one “Default” firmware configuration available. Hence the number returned when reading SPC_NUM_FW_CONFIGS is 1 for most cards and the active configuration is typically 0.

If more than just the one default firmware configuration is available, switching images can be done with the help of the Spectrum Control Center. Please see “Firmware switching” paragraph in the “Card Control Center” section for details.

Production date

This register informs you about the production date, which is returned as one 32 bit long word. The lower word is holding the information about the year, while the upper word informs about the week of the year.

Table 15: Spectrum API: production date register

Register	Value	Direction	Description
SPC_PCIDATE	2020	read	Production date: week in bits 31 to 16, year in bits 15 to 0

The following example shows how to read out a date and how to interpret the value:

```
spcm_dwGetParam_i32 (hDrv, SPC_PCIDATE, &lProdDate);
printf ("Production: week %d of year %d\n", (lProdDate >> 16) & 0xffff, lProdDate & 0xffff);
```

Last calibration date (A/D and D/A cards only)

This register informs you about the date of the last factory calibration. When receiving a new card this date is similar to the delivery date when the production calibration is done. When returning the card to calibration this information is updated. This date is not updated when the user does an on-board calibration. The date is returned as one 32 bit long word. The lower word is holding the information about the year, while the upper word informs about the week of the year.

Table 16: Spectrum API: calibration date register

Register	Value	Direction	Description
SPC_CAIBDATE	2025	read	Last calibration date: week in bit 31 to 16, year in bit 15 to 0

Serial number

This register holds the information about the serial number of the board. This number is unique and should always be sent together with a support question. Normally you use this information together with the register SPC_PCITYP to verify that multiple measurements are done with the exact same board.

Table 17: Spectrum API: hardware serial number register

Register	Value	Direction	Description
SPC_PCISERIALNO	2030	read	Serial number of the board

Maximum possible sampling rate

This register gives you the maximum possible sampling rate the board can run. The information provided here does not consider any restrictions in the maximum speed caused by special channel settings. For detailed information about the correlation between the maximum sampling rate and the number of activated channels please refer to the according chapter.

Table 18: Spectrum API: maximum sampling rate register

Register	Value	Direction	Description
SPC_PCISAMPLERATE	2100	read	Maximum sampling rate in Hz as a 64 bit integer value

Installed memory

This register returns the size of the installed on-board memory in bytes as a 64 bit integer value. If you want to know the amount of samples you can store, you must regard the size of one sample of your card. All 7 bit and 8 bit A/D and D/A cards use only one byte per sample,

while all other A/D and D/A cards with 12, 14 and 16 bit resolution use two bytes to store one sample. All digital cards need one byte to store 8 data bits.

Table 19: Spectrum API: installed memory registers

Register	Value	Direction	Description
SPC_PCIMEMSIZE	2110	read_i32	Installed memory in bytes as a 32 bit integer value. Maximum return value will 1 GiByte. If more memory is installed this function will return the error code ERR_EXCEEDINT32.
SPC_PCIMEMSIZE	2110	read_i64	Installed memory in bytes as a 64 bit integer value

The following example is written for a „two bytes“ per sample card (12, 14 or 16 bit board), on any 8 bit card memory in MiSamples is similar to memory in MiBytes.

```
spcm_dwGetParam_i64 (hDrv, SPC_PCIMEMSIZE, &llInstMemsize);
printf ("Memory on card: %d MiBytes\n", (int32) (llInstMemsize /1024/1024));
printf ("          : %d MiSamples\n", (int32) (llInstMemsize /1024/1024/2));
```

Installed features and options

The SPC_PCIFEATURES register informs you about the features, that are installed on the board. If you want to know about one option being installed or not, you need to read out the 32 bit value and mask the interesting bit. In the table below you will find every feature that may be installed on a M2i/M3i/M4i/M4x/M2p/M5i card. Please refer to the ordering information to see which of these features are available for your card series.

Table 20: Spectrum API: Feature Register and available feature flags

Register	Value	Direction	Description
SPC_PCIFEATURES	2120	read	PCI feature register. Holds the installed features and options as a bitfield. The read value must be masked out with one of the masks below to get information about one certain feature.
SPCM_FEAT_MULTI	1h		Is set if the feature Multiple Recording / Multiple Replay is available.
SPCM_FEAT_GATE	2h		Is set if the feature Gated Sampling / Gated Replay is available.
SPCM_FEAT_DIGITAL	4h		Is set if the feature Digital Inputs / Digital Outputs is available.
SPCM_FEAT_TIMESTAMP	8h		Is set if the feature Timestamp is available.
SPCM_FEAT_STARHUB6_EXTM	20h		Is set on the card, that carries the star-hub extension or piggy-back module for synchronizing up to 6 cards (M2p).
SPCM_FEAT_STARHUB8_EXTM	20h		Is set on the card, that carries the star-hub extension or piggy-back module for synchronizing up to 8 cards (M4i).
SPCM_FEAT_STARHUB4	20h		Is set on the card, that carries the star-hub piggy-back module for synchronizing up to 4 cards (M3i).
SPCM_FEAT_STARHUB5	20h		Is set on the card, that carries the star-hub piggy-back module for synchronizing up to 5 cards (M2i).
SPCM_FEAT_STARHUB16_EXTM	40h		Is set on the card, that carries the star-hub piggy-back module for synchronizing up to 16 cards (M2p).
SPCM_FEAT_STARHUB8	40h		Is set on the card, that carries the star-hub piggy-back module for synchronizing up to 8 cards (M3i and M5i).
SPCM_FEAT_STARHUB16	40h		Is set on the card, that carries the star-hub piggy-back module for synchronizing up to 16 cards (M2i).
SPCM_FEAT_ABA	80h		Is set if the feature ABA mode is available.
SPCM_FEAT_BASEXIO	100h		Is set if the extra BaseXIO option is installed. The lines can be used for asynchronous digital I/O, extra trigger or timestamp reference signal input.
SPCM_FEAT_AMPLIFIER_10V	200h		Arbitrary Waveform Generators only: card has additional set of calibration values for amplifier card.
SPCM_FEAT_STARHUBSYSMASTER	400h		Is set in the card that carries a System Star-Hub Master card to connect multiple systems (M2i).
SPCM_FEAT_DIFFMODE	800h		M2i.30xx series only: card has option -diff installed for combining two SE channels to one differential channel.
SPCM_FEAT_SEQUENCE	1000h		Only available for output cards or I/O cards: Replay sequence mode available.
SPCM_FEAT_AMPMODULE_10V	2000h		Is set on the card that has a special amplifier module for mounted (M2i.60xx/61xx only).
SPCM_FEAT_STARHUBSYSLAVE	4000h		Is set in the card that carries a System Star-Hub Slave module to connect with System Star-Hub master systems (M2i).
SPCM_FEAT_NETBOX	8000h		The card is physically mounted within a digitizerNETBOX, generatorNETBOX or hybridNETBOX.
SPCM_FEAT_REMOTESERVER	10000h		Support for the Spectrum Remote Server option is installed on this card.
SPCM_FEAT_SCAPP	20000h		Support for the SCAPP option allowing CUDA RDMA access to supported graphics cards for GPU calculations (M5i, M4i and M2p)
SPCM_FEAT_DIG16_SMB	40000h		M2p: Set if option M2p.xxxx-DigSMB is installed, adding 16 additional digital I/Os via SMB connectors.
SPCM_FEAT_DIG16_FX2	80000h		M2p: Set if option M2p.xxxx-DigFX2 is installed, adding 16 additional digital I/Os via FX2 multipin connectors.
SPCM_FEAT_DIGITALBWFILTER	100000h		A digital (boxcar) bandwidth filter is available that can be globally enabled/disabled for all channels.
SPCM_FEAT_CUSTOMMOD_MASK	F0000000h		The upper 4 bit of the feature register is used to mark special custom modifications. This is only used if the card has been specially customized. Please refer to the extra documentation for the meaning of the custom modifications. (M2i/M3i). For M5i, M4i, M4x and M2p cards see „Custom modifications“ chapter instead.

The following example demonstrates how to read out the information about one feature.

```
spcm_dwGetParam_i32 (hDrv, SPC_PCIFEATURES, &lFeatures);
if (lFeatures & SPCM_FEAT_DIGITAL)
    printf("Option digital inputs/outputs is installed on your card");
```

The following example demonstrates how to read out the custom modification code.

```
spcm_dwGetParam_i32 (hDrv, SPC_PCIFEATURES, &lFeatures);
lCustomMod = (lFeatures >> 28) & 0xF;
if (lCustomMod != 0)
    printf("Custom modification no. %d is installed.", lCustomMod);
```

Installed extended Options and Features

Some cards (such as M5i/M4i/M4x/M2p cards) can have advanced features and options installed. This can be read out with the following register:

Table 21: Spectrum API: Extended feature register and available extended feature flags

Register	Value	Direction	Description
SPC_PCIEXTFEATURES	2121	read	PCI extended feature register. Holds the installed extended features and options as a bitfield. The read value must be masked out with one of the masks below to get information about one certain feature.
SPCM_FEAT_EXTFW_SEGSTAT	1h		Is set if the firmware option "Block Statistics" is installed on the board, which allows certain statistics to be on-board calculated for data being recorded in segmented memory modes, such as Multiple Recording or ABA.
SPCM_FEAT_EXTFW_SEGAVERAGE	2h		Is set if the firmware option "Block Average" is installed on the board, which allows on-board hardware averaging of data being recorded in segmented memory modes, such as Multiple Recording or ABA.
SPCM_FEAT_EXTFW_BOXCAR	4h		Is set if the firmware mode "Boxcar Average" is supported in the installed firmware version.
SPCM_FEAT_EXTFW_PULSEGEN	8h		Is set if the firmware mode "Pulse Generator" is installed on the board, which allows generation of pulses for output on the card's multi-purpose I/O lines (XIO).
SPCM_FEAT_EXTFW_DDS20	10h		If set, the firmware option "DDS20" (20 tone DDS) is installed. Prior to the introduction of the "DDS50", this feature was named "SPCM_FEAT_EXTFW_DDS". This register has been renamed, whilst the associated value remained unchanged.
SPCM_FEAT_EXTFW_DDS50	20h		If set, the firmware option "DDS50" (50 tone DDS) is installed.
SPCM_FEAT_EXTFW_AWG	40h		If set, the firmware option "AWG" (arbitrary waveform generator) is installed.

Miscellaneous Card Information

Some more detailed card information, that might be useful for the application to know, can be read out with the following registers:

Table 22: Spectrum API: register overview of miscellaneous cards information

Register	Value	Direction	Description
SPC_MIINST_MODULES	1100	read	Number of the installed front-end modules on the card.
SPC_MIINST_CHPERMODULE	1110	read	Number of channels installed on one front-end module.
SPC_MIINST_BYTESPERSAMPLE	1120	read	Number of bytes used in memory by one sample.
SPC_MIINST_BITSPERSAMPLE	1125	read	Resolution of the samples in bits.
SPC_MIINST_MAXADCVALUE	1126	read	Decimal code of the full scale value.
SPC_MIINST_MINEXTCLOCK	1145	read	Minimum external clock that can be fed in for direct external clock (if available for card model).
SPC_MIINST_MAXEXTCLOCK	1146	read	Maximum external clock that can be fed in for direct external clock (if available for card model).
SPC_MIINST_MINEXTREFCLOCK	1148	read	Minimum external clock that can be fed in as a reference clock.
SPC_MIINST_MAXEXTREFCLOCK	1149	read	Maximum external clock that can be fed in as a reference clock.
SPC_MIINST_ISDEMOCARD	1175	read	Returns a value other than zero, if the card is a demo card.

Function type of the card

This register returns the basic type of the card:

Table 23: Spectrum API: register card function type and possible types

Register	Value	Direction	Description
SPC_FNCATYPE	2001	read	Gives information about what type of card it is.
SPCM_TYPE_AI	1h		Analog input card (analog acquisition; the M2i.4028 and M2i.4038 also return this value)
SPCM_TYPE_AO	2h		Analog output card (arbitrary waveform generators)
SPCM_TYPE_DI	4h		Digital input card (logic analyzer card)
SPCM_TYPE_DO	8h		Digital output card (pattern generators)
SPCM_TYPE_DIO	10h		Digital I/O (input/output) card, where the direction is software selectable.

Used type of driver

This register holds the information about the driver that is actually used to access the board. Although the driver interface doesn't differ between Windows and Linux systems it may be of interest for a universal program to know on which platform it is working.

Table 24: Spectrum API: register driver type information and possible driver types

Register	Value	Direction	Description
SPC_GETDRVTYPE	1220	read	Gives information about what type of driver is actually used
DRVTYPE_LINUX32	1		Linux 32bit driver is used
DRVTYPE_WDM32	4		Windows WDM 32bit driver is used (XP/Vista/Windows 7/8/10/11).
DRVTYPE_WDM64	5		Windows WDM 64bit driver is used by 64bit application (XP64/Vista/Windows 7/8/10/11).
DRVTYPE_WOW64	6		Windows WDM 64bit driver is used by 32bit application (XP64/Vista/Windows 7/8/10/11).
DRVTYPE_LINUX64	7		Linux 64bit driver is used

Driver version

This register holds information about the currently installed driver library. As the drivers are permanently improved and maintained and new features are added user programs that rely on a new feature are requested to check the driver version whether this feature is installed.

Table 25: Spectrum API: driver version read register

Register	Value	Direction	Description
SPC_GETDRVVERSION	1200	read	Gives information about the driver library version

The resulting 32 bit value for the driver version consists of the three version number parts shown in the table below:

Driver Major Version	Driver Minor Version	Driver Build
8 Bit wide: bit 24 to bit 31	8 Bit wide, bit 16 to bit 23	16 Bit wide, bit 0 to bit 15

Kernel Driver version

This register informs about the actually used kernel driver. Windows users can also get this information from the device manager. Please refer to the „Driver Installation“ chapter. On Linux systems this information is also shown in the kernel message log at driver start time.

Table 26: Spectrum API: kernel driver version read register

Register	Value	Direction	Description
SPC_GETKERNELVERSION	1210	read	Gives information about the kernel driver version.

The resulting 32 bit value for the driver version consists of the three version number parts shown in the table below:

Driver Major Version	Driver Minor Version	Driver Build
8 Bit wide: bit 24 to bit 31	8 Bit wide, bit 16 to bit 23	16 Bit wide, bit 0 to bit 15

The following example demonstrates how to read out the kernel and library version and how to print them.

```
spcm_dwGetParam_i32 (hDrv, SPC_GETDRVVERSION, &lLibVersion);
spcm_dwGetParam_i32 (hDrv, SPC_GETKERNELVERSION, &lKernelVersion);
printf("Kernel V %d.%d build %d\n", lKernelVersion >> 24, (lKernelVersion >> 16) & 0xff, lKernelVersion & 0xffff);
printf("Library V %d.%d build %d\n", lLibVersion >> 24, (lLibVersion >> 16) & 0xff, lLibVersion & 0xffff);
```

This small program will generate an output like this:

```
Kernel V 1.11 build 817
Library V 1.1 build 854
```

Custom modifications

Since all of the boards from Spectrum are modular boards, they consist of one base board and one piggy-back front-end module and eventually of an extension module like the Star-Hub. Each of these three kinds of hardware has its own version register. Normally you do not need this information but if you have a support question, please provide the revision together with it.

Table 27: Spectrum API: custom modification register and different bitmasks to split the register in various hardware parts

Register	Value	Direction	Description
SPCM_CUSTOMMOD	3130	read	Dedicated feature register used to mark special custom modifications of the base card and/or the front-end module and/or the Star-Hub module. This is only used if the card has been specially customized. Please refer to the extra documentation for the meaning of the custom modifications. This register is supported for all M5i, M4i, M4x, M2p cards and all digitizerNETBOX, generatorNETBOX or hybridNETBOX based upon these series of cards.
SPCM_CUSTOMMOD_BASE_MASK	000000Fh		Mask for the custom modification of the base card.
SPCM_CUSTOMMOD_MODULE_MASK	0000FF00h		Mask for the custom modification of the front-end module(s).
SPCM_CUSTOMMOD_STARHUB_MASK	00FF0000h		Mask out custom modification of the Star-Hub module.

Reset

Every Spectrum card can be reset by software. Concerning the hardware, this reset is the same as the power-on reset when starting the host computer. In addition to the power-on reset, the reset command also brings all internal driver settings to a defined default state. A software reset is automatically performed, when the driver is first loaded after starting the host system.

Performing a board reset can be easily done by the related board command mentioned in the following table.

Table 28: Spectrum API: command register and reset command

Register	Value	Direction	Description
SPC_M2CMD	100	w	Command register of the board.

M2CMD_CARD_RESET	1h	A software and hardware reset is done for the board. All settings are set to the default values. The data in the board's on-board memory will be no longer valid. Any output signals like trigger or clock output will be disabled.
------------------	----	---

Analog Inputs

Channel Selection

One key setting that influences all other possible settings is the channel enable register. A unique feature of the Spectrum cards is the possibility to program the number of channels you want to use. All on-board memory can then be used by these activated channels.

This description shows you the channel enable register for the complete card family. However, your specific board may have less channels depending on the card type that you have purchased and therefore does not allow you to set the maximum number of channels shown here.

Table 29: Spectrum API: channel enable register and register settings

Register	Value	Direction	Description
SPC_CHENABLE	11000	read/write	Sets the channel enable information for the next card run.
CHANNEL0	1	Activates channel 0	
CHANNEL1	2	Activates channel 1	
CHANNEL2	4	Activates channel 2	
CHANNEL3	8	Activates channel 3	

The channel enable register is set as a bitmap. That means that one bit of the value corresponds to one channel to be activated. To activate more than one channel the values have to be combined by a bitwise OR.

Example showing how to activate 4 channels:

```
spcm_dwSetParam_i64 (hDrv, SPC_CHENABLE, CHANNEL0 | CHANNEL1 | CHANNEL2 | CHANNEL3);
```

The following table shows all allowed settings for the channel enable register when your card has a maximum of 1 channel.

Channels to activate				
Ch0		Values to program	Value as hex	Value as decimal
X		CHANNEL0	1h	1

The following table shows all allowed settings for the channel enable register when your card has a maximum of 2 channels.

Channels to activate				
Ch0	Ch1	Values to program	Value as hex	Value as decimal
X		CHANNEL0	1h	1
	X	CHANNEL1	2h	2
X	X	CHANNEL0 CHANNEL1	3h	3

The following table shows all allowed settings for the channel enable register in case that you have a four channel card.

Channels to activate						
Ch0	Ch1	Ch2	Ch3	Values to program	Value as hex	Value as decimal
X				CHANNEL0	1h	1
	X			CHANNEL1	2h	2
		X		CHANNEL2	4h	4
			X	CHANNEL3	8h	8
X	X			CHANNEL0 CHANNEL1	3h	3
X		X		CHANNEL0 CHANNEL2	5h	5
X			X	CHANNEL0 CHANNEL3	9h	9
	X	X		CHANNEL1 CHANNEL2	6h	6
	X		X	CHANNEL1 CHANNEL3	Ah	10
		X	X	CHANNEL2 CHANNEL3	Ch	12
X	X	X	X	CHANNEL0 CHANNEL1 CHANNEL2 CHANNEL3	Fh	15

Any channel activation mask that is not shown here is not valid. If programming an other channel activation, the driver will return with an error code ERR_VALUE.



To help user programs it is also possible to read out the number of activated channels that correspond to the currently programmed bitmap.

Table 30: Spectrum API: channel count register

Register	Value	Direction	Description
SPC_CHCOUNT	11001	read	Reads back the number of currently activated channels.

Reading out the channel enable information can be done directly after setting it or later like this:

```
spcm_dwSetParam_i32 (hDrv, SPC_CHENABLE, CHANNEL0 | CHANNEL1);
spcm_dwGetParam_i32 (hDrv, SPC_CHENABLE, &lActivatedChannels);
spcm_dwGetParam_i32 (hDrv, SPC_CHCOUNT, &lChCount);

printf ("Activated channels bitmask is: 0x%08x\n", lActivatedChannels);
printf ("Number of activated channels with this bitmask: %d\n", lChCount);
```

Assuming that the two channels are available on your card the program will have the following output:

```
Activated channels bitmask is: 0x00000003
Number of activated channels with this bitmask: 2
```


Important note on channel selection

As some of the manuals passages are used in more than one hardware manual most of the registers and channel settings throughout this handbook are described for the maximum number of possible channels that are available on one card of the current series. There can be less channels on your actual type of board or bus-system. Please refer to the technical data section to get the actual number of available channels.




Setting up the inputs

This analog acquisition board uses separate input stages and converters on each channel. This gives you the possibility to set up the desired and concerning your application best suiting input range also separately for each channel. All input stage related settings can easily be set by the corresponding input registers. The table below shows the available input stage registers and possible standard values for your type of board. As there are also modified versions available with different input ranges it is recommended to read out the currently available input ranges as shown later in this chapter.

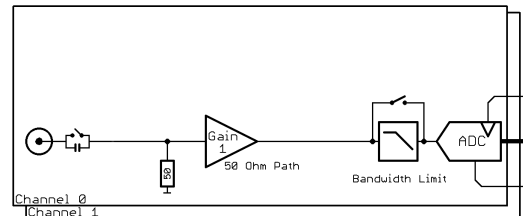

Input ranges

This analog acquisition board has several different input ranges for each channel. This gives you the possibility to set up the desired and concerning your application best suiting input range also separately for each channel. The input ranges can easily be set by the corresponding input registers. The table below shows the available input registers and possible standard ranges for your type of board. As there are also modified versions available with different input ranges it is recommended to read out the currently available input ranges as shown later in this chapter.

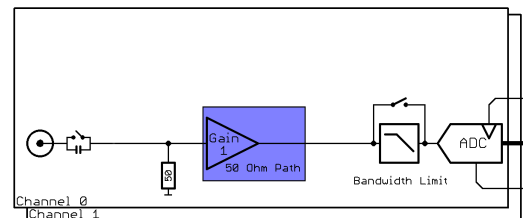

The available input ranges are read out using the following registers.

Table 31: Spectrum API: registers for reading the installed input ranges from card EEPROM

Register	Value	Direction	Description
SPC_READIRCOUNT	3000	read	Returns the number of available input ranges.
SPC_READRANGEMIN0	4000	read	Reads the lower border of input range 0 in mV
SPC_READRANGEMIN1	4001	read	Reads the lower border of input range 1 in mV
...	...	...	...
SPC_READRANGEMAX0	4100	read	Reads the upper border of input range 0 in mV
SPC_READRANGEMAX1	4101	read	Reads the upper border of input range 1 in mV
...	...	...	...

The following example reads out the number of available input ranges and reads and prints the minimum and maximum value of all input ranges.

```
spcm_dwGetParam_i32 (hDrv, SPC_READIRCOUNT, &lNumberOfRanges);
for (i = 0; i < lNumberOfRanges; i++)
{
    spcm_dwGetParam_i32 (hDrv, SPC_READRANGEMIN0 + i, &lMinimumInputRange);
    spcm_dwGetParam_i32 (hDrv, SPC_READRANGEMAX0 + i, &lMaximumInputRange);
    printf („Range %d: %d mV to %d mV\n", i, lMinimumInputRange, lMaximumInputRange);
}
```

The input range is selected individually for each channel. Please note that the correct input path needs to be set

Table 32: Spectrum API: input range settings register and available vales depending on installed low-voltage option

Register	Value	Direction	Description
SPC_AMP0	30010	read/write	Defines the input range of channel0.
SPC_AMP1	30110	read/write	Defines the input range of channel1.
SPC_AMP2	30210	read/write	Defines the input range of channel2.
SPC_AMP3	30310	read/write	Defines the input range of channel3.

Standard Input ranges:

200	± 200 mV calibrated input range for the appropriate channel.
500	± 500 mV calibrated input range for the appropriate channel.
1000	± 1 V calibrated input range for the appropriate channel.
2500	± 2.5 V calibrated input range for the appropriate channel.

Low-voltage Input ranges (option M4i.22xx-ir40m or M4i.23xx-ir40m installed):

40	± 40 mV calibrated input range for the appropriate channel.
100	± 100 mV calibrated input range for the appropriate channel.
200	± 200 mV calibrated input range for the appropriate channel.
500	± 500 mV calibrated input range for the appropriate channel.

For detailed information on how to deal with data coming from multiple channels, how to unpack possible digital data acquired along the analog data or on how to convert the RAW samples into voltage values, please consult the “Data Organization” section in this manual.



Input offset

In most cases the external signals will not be symmetrically related to ground. If you want to acquire such asymmetrical signals, it is possible to use the smallest input range that matches the biggest absolute signal amplitude without exceeding the range.

The figure at the right shows this possibility. But in this example you would leave half of the possible resolution unused.

It is much more efficient if you shift the signal on-board to be as symmetrical as possible and to acquire it within the best possible range.

This results in a much better use of the converters resolution.

On this acquisition boards from Spectrum you have the possibility to adjust the input offset separately for each channel.

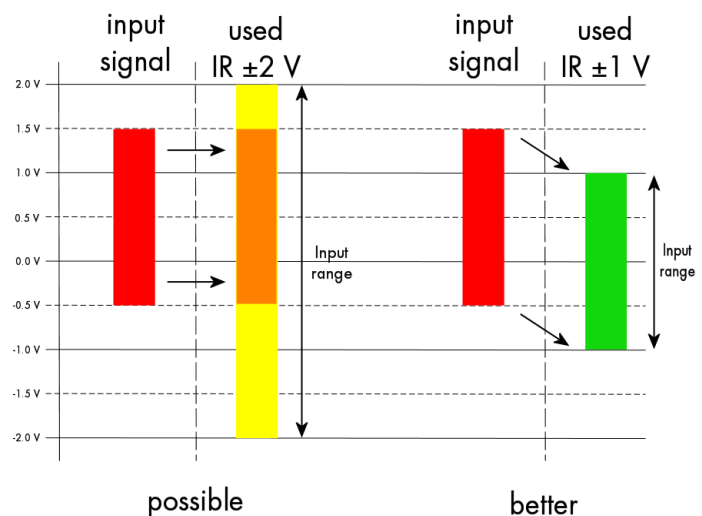


Image 43: Spectrum API: using the input offset shifting to optimize the usage of the input range

The example in the right figure shows signals with a range of ± 1.0 V that have offsets up to ± 1.0 V. So related to the desired input range these signals have offsets of ± 100 %.

For compensating such offsets you can use the offset register for each channel separately. If you want to compensate the $+100$ % offset of the outer left signal, you would have to set the offset to -100 % to compensate it.

As the offset levels are relatively to the related input range, you have to calculate and set your offset again when changing the input's range.

The table below shows the offset registers and the possible offset ranges for your specific type of board.

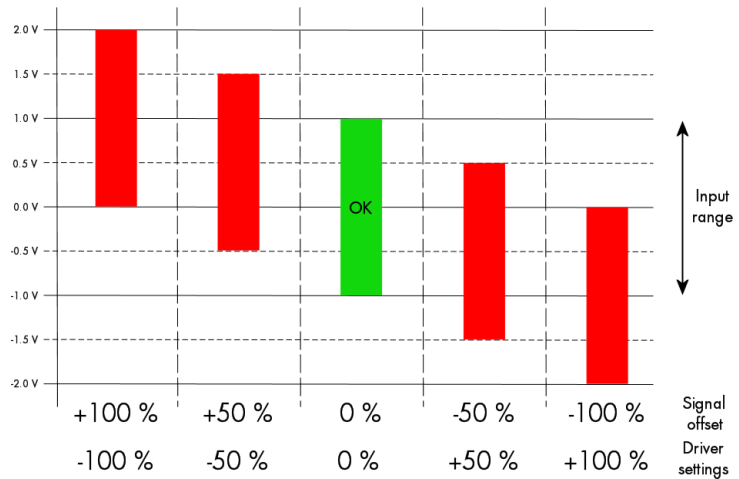


Image 44: Spectrum API: effects of different input offset setting

Image 45: Spectrum API: input offset registers and available register settings

Register	Value	Direction	Description	Offset range
SPC_OFFS0	30000	read/write	Defines the input's offset and therefore shifts the input of channel0.	± 200 % in steps of 1 %
SPC_OFFS1	30100	read/write	Defines the input's offset and therefore shifts the input of channel1.	± 200 % in steps of 1 %
SPC_OFFS2	30200	read/write	Defines the input's offset and therefore shifts the input of channel2.	± 200 % in steps of 1 %
SPC_OFFS3	30300	read/write	Defines the input's offset and therefore shifts the input of channel3.	± 200 % in steps of 1 %

AC/DC offset compensation

When using the input offset other than 0% an offset voltage will be visible in case DC coupling is selected for the channel and the signal source is externally AC coupled. This offset can be compensated for by setting the compensation registers:

Table 33: Spectrum API: AC/DC compensation register for offset settings with an AC coupled signal

Register	Value	Direction	Description
SPC_ACDC_OFFS_COMPENSATION0	30021	read/write	A „1“ enables the compensation. A „0“ disables the compensation (default).
SPC_ACDC_OFFS_COMPENSATION1	30121	read/write	A „1“ enables the compensation. A „0“ disables the compensation (default).
SPC_ACDC_OFFS_COMPENSATION2	30221	read/write	A „1“ enables the compensation. A „0“ disables the compensation (default).
SPC_ACDC_OFFS_COMPENSATION3	30321	read/write	A „1“ enables the compensation. A „0“ disables the compensation (default).

Read out of input features

Each input path (if multiple paths are available on the card) has different features that can be read out to make the software more general. If you only operate one single card type in your software it is not necessary to read out these features.

Please note that the following table shows all input features settings that are available throughout all Spectrum acquisition cards. Some of these features are not installed on your specific hardware:

Table 34: Spectrum API: register to read the analog input features and the meaning of the feature flags

Register	Value	Direction	Description
SPC_READAIFEATURES	3101	read	Returns a bit map with the available features of that input path. The possible return values are listed below.

	Value	Path 0	Description
SPCM_AI_TERM	00000001h		Programmable input termination available
SPCM_AI_SE	00000002h	fixed	Input is single-ended. If available together with SPC_AI_DIFF: input type is software selectable
SPCM_AI_DIFF	00000004h		Input is differential. If available together with SPC_AI_SE: input type is software selectable
SPCM_AI_OFFSPERCENT	00000008h	x	Input offset programmable in per cent of input range
SPCM_AI_OFFSMV	00000010h		Input offset programmable in mV
SPCM_AI_OVERRANGEDETECT	00000020h		Programmable over-range detection available
SPCM_AI_DCCOUPLING	00000040h	x	Input is DC coupled. If available together with AC coupling: coupling is software selectable
SPCM_AI_ACCOUPLING	00000080h	x	Input is AC coupled. If available together with DC coupling: coupling is software selectable
SPCM_AI_LOWPASS	00000100h		Input has a individually per channel selectable low pass filter (bandwidth limit)
SPCM_AI_ACDC_OFFS_COMP	00000200h		Input has a selectable offset compensation for HF-Path with AC/DC coupling/source mismatch.
SPCM_AI_GLOBALLOWPASS	00000800h	x	Card has a globally selectable low pass (affects all channels with the same setting)
SPCM_AI_AUTOCALOFS	00001000h	x	Input offset can be auto calibrated on the card

	Value	Path 0	Description
SPCM_AI_AUTOCALGAIN	00002000h		Input gain can be auto calibrated on the card
SPCM_AI_AUTOCALOFFSNOIN	00004000h		Input offset can auto calibrated on the card if inputs are left open
SPCM_AI_HIGHIMP	00008000h		Input has a high impedance mode available
SPCM_AI_LOWIMP	00010000h	fixed	Input has a low impedance mode (50 Ohm) available
SPCM_AI_INDIVPULSEWIDTH	00100000h		Trigger pulse-width is individually per channel programmable

The following example shows a setup of the input range of a two channel card.

Please note that this is a general example and the number of input channels may not match your card channels.

```
spcm_dwSetParam_i32 (hDrv, SPC_AMP0 , 1000); // Set up channel0 to the range of ± 1.0 V
spcm_dwSetParam_i32 (hDrv, SPC_AMP1 , 500); // Set up channel1 to the range of ± 0.5 V
```

Input coupling

All inputs can be set separately switched to AC or DC coupling. Please refer to the technical data section to see the signal frequency range that is available for the different settings.

Using the AC coupling will eliminate all DC and low frequency parts of the input signal and allows best quality measurements in the frequency domain even if the DC level of the signal varies over the time.

The following table shows the corresponding register to set the input coupling.

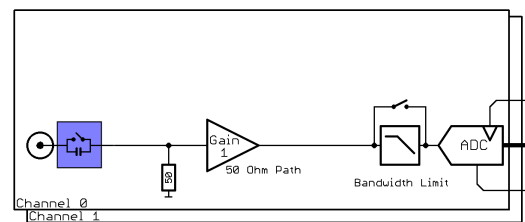


Table 35: Spectrum API: AC/DC setup registers and available register settings

Register	Value	Direction	Description
SPC_ACDC0	30020	read/write	A „1“ sets the AC coupling for channel0. A „0“ sets the DC coupling (default is AC)
SPC_ACDC1	30120	read/write	A „1“ sets the AC coupling for channel1. A „0“ sets the DC coupling (default is AC)
SPC_ACDC2	30220	read/write	A „1“ sets the AC coupling for channel2. A „0“ sets the DC coupling (default is AC)
SPC_ACDC3	30320	read/write	A „1“ sets the AC coupling for channel3. A „0“ sets the DC coupling (default is AC)

Anti aliasing filter (Bandwidth limit)

All inputs share a global selectable anti aliasing filter (bandwidth limit) that will cut of any aliasing effects and will reduce signal noise.

Please note that this bandwidth limit filter will also cut of any distortion or high frequency spurious signals parts that are within the frequency spectrum of the input.

Please refer to the technical data section to see the cut off frequency and the type of filter used. The following table shows the corresponding register to activate the bandwidth limit.

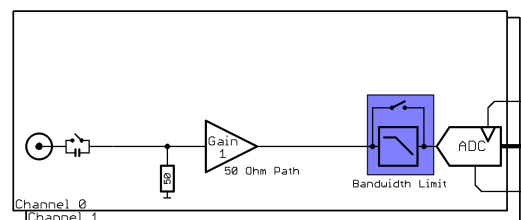


Table 36: Spectrum API: anti-aliasing filter setup register

Register	Value	Direction	Description
SPC_FILTER0	30080	read/write	A „1“ selects the bandwidth limit for all channels. A „0“ sets all channels to full bandwidth (default).

Automatic on-board calibration of the offset and gain settings

All of the channels are calibrated in factory before the board is shipped. These values are stored in the on-board EEPROM under the default settings. An automatic on-board calibration can be initiated with the corresponding registers of the inputs as shown before.

To start the automatic offset adjustment, simply write the register, mentioned in the following table.

Before you start an automatic on-board calibration it is recommended, that no signal is connected to any input. Leave all the analog channel connectors open and then start the adjustment. All the internal settings of the driver are changed, when the automatic on-board calibration is engaged and must be set/restored afterwards.



Table 37: Spectrum API: automatic offset compensation register and valid register settings

Register	Value	Direction	Description
SPC_ADJ_AUTOADJ	50020	write	Performs the automatic on-board calibration within the driver.
ADJ_ALL	0		A/D cards: Automatic on-board calibration for all input channels and all input ranges. D/A cards: Automatic on-board calibration for all output channels.

As all corrections are temporarily stored in the driver, the automatic adjustments are volatile at first. After exiting your program, all calibration information will be lost. To give you a possibility to save your own settings, the Spectrum card have at least one set of user settings that can be saved within the on-board EEPROM.

You can easily either save adjustment settings to the EEPROM with SPC_ADJ_SAVE or recall them with SPC_ADJ_LOAD. These two registers are shown in the table below.

Table 38: Spectrum API: loading and storing calibration values to the EEPROM

Register	Value	Direction	Description
SPC_ADJ_LOAD	50000	write	Loads the specified set of settings from the EEPROM. The default settings are automatically loaded, when the driver is started.
		read	Reads out, what kind of settings have been loaded last.
SPC_ADJ_SAVE	50010	write	Stores the current settings to the specified set in the EEPROM.
		read	Reads out, what kind of settings have been saved last.
ADJ_DEFAULT	0		Default storage location for the calibration values.

If you want to make an on-board offset/gain calibration on all the channels and store the data to the ADJ_DEFAULT set of the EEPROM you can do this the way, the following example shows.

```
spcm_dwSetParam_i32 (hDrv, SPC_ADJ_AUTOADJ, ADJ_ALL ); // Activate on-board calibration on all channels
spcm_dwSetParam_i32 (hDrv, SPC_ADJ_SAVE , ADJ_DEFAULT); // and store values to DEFAULT set in the EEPROM
```

Every time the on-board calibration is started, the UTC time is stored in the on-board EEPROM. That value can be read out via the following register:

Table 39: Spectrum API: read out when last on-board calibration has been engaged

Register	Value	Direction	Description
SPC_CALIBDATEONBOARD	2026	read	Reads out the UTC time of when the last on-board calibration has been engaged.

Acquisition modes

Your card is able to run in different modes. Depending on the selected mode there are different registers that each define an aspect of this mode. The single modes are explained in this chapter. Any further modes that are only available if an option is installed on the card is documented in a later chapter.

Overview

This chapter gives you a general overview on the related registers for the different modes. The use of these registers throughout the different modes is described in the following chapters.

Setup of the mode

The mode register is organized as a bitmap. Each mode corresponds to one bit of this bitmap. When defining the mode to use, please be sure just to set one of the bits. All other settings will return an error code.

The main difference between all standard and all FIFO modes is that the standard modes are limited to on-board memory and therefore can run with full sampling rate. The FIFO modes are designed to transfer data continuously over the bus to PC memory or to hard disk and can therefore run much longer. The FIFO modes are limited by the maximum bus transfer speed the PC can use. The FIFO mode uses the complete installed on-board memory as a FIFO buffer.

However as you'll see throughout the detailed documentation of the modes the standard and the FIFO mode are similar in programming and behavior and there are only a very few differences between them.

Table 40: Spectrum API: card mode and read out of available card mode software registers

Register	Value	Direction	Description
SPC_CARDMODE	9500	read/write	Defines the used operating mode, a read command will return the currently used mode.
SPC_AVAILCARDMODES	9501	read	Returns a bitmap with all available modes on your card. The modes are listed below.

Acquisition modes

Table 41: Spectrum API: possible values for the card mode register. Description of the different card modes

Mode	Value	Available on	Description
SPC_REC_STD_SINGLE	1h	all cards	Data acquisition to on-board memory for one single trigger event.
SPC_REC_STD_MULTI	2h	all cards	Data acquisition to on-board memory for multiple trigger events. Each recorded segment has the same size. This mode is described in greater detail in a special chapter about the Multiple Recording option.
SPC_REC_STD_GATE	4h	all M2p and M4i digitizers and NETBOXes	Data acquisition to on-board memory using an external Gate signal. Acquisition is only done as long as the gate signal has a programmed level. The mode is described in greater detail in a special chapter about the Gated Sampling option.
SPC_REC_STD_ABA	8h	all M2p and M4i digitizers and NETBOXes	Data acquisition to on-board memory for multiple trigger events. While the multiple trigger events are stored with programmed sampling rate the inputs are sampled continuously with a slower sampling speed. The mode is described in a special chapter about ABA mode option.
SPC_REC_STD_SEGSTATS	10000h	M4i/M4x.2xxx M4i/M4x.44xx DN2/DN6.2xx DN2/DN6.44x digitizers only	Data acquisition to on-board memory for multiple trigger events, using Block/Segment Statistic Module (FPGA firmware Option).
SPC_REC_STD_AVERAGE	20000h	M4i/M4x.2xxx M4i/M4x.44xx M5i.33xx DN2/DN6.2xx DN2/DN6.44x DN2/DN6.33x digitizers only	Data acquisition to on-board memory for multiple trigger events, using Block Average Module (FPGA firmware Option).
SPC_REC_STD_BOXCAR	800000h	M4i/M4x.44xx DN2/DN6.44x digitizers only	Enables Boxcar Averaging for standard acquisition. Requires digitizer module with firmware version V29 or newer.
SPC_REC_FIFO_SINGLE	10h	all cards	Continuous data acquisition for one single trigger event. The on-board memory is used completely as FIFO buffer.
SPC_REC_FIFO_MULTI	20h	all cards	Continuous data acquisition for multiple trigger events.
SPC_REC_FIFO_GATE	40h	all M2p and M4i digitizers and NETBOXes	Continuous data acquisition using an external gate signal.
SPC_REC_FIFO_ABA	80h	all M2p and M4i digitizers and NETBOXes	Continuous data acquisition for multiple trigger events together with continuous data acquisition with a slower sampling clock.
SPC_REC_FIFO_SEGSTATS	100000h	M4i/M4x.2xxx M4i/M4x.44xx DN2/DN6.2xx DN2/DN6.44x digitizers only	Enables Block/Segment Statistic for FIFO acquisition (FPGA firmware Option).
SPC_REC_FIFO_AVERAGE	200000h	M4i/M4x.2xxx M4i/M4x.44xx M5i.33xx DN2/DN6.2xx DN2/DN6.44x DN2/DN6.33x digitizers only	Enables Block Averaging for FIFO acquisition (FPGA firmware Option).
SPC_REC_FIFO_BOXCAR	1000000h	M4i/M4x.44xx DN2/DN6.44x digitizers only	Enables Boxcar Averaging for FIFO acquisition. Requires digitizer module firmware version V29 or newer.
SPC_REC_FIFO_SINGLE_MONITOR	2000000h	all M2p and M4i digitizers and NETBOXes	Combination of SPC_REC_FIFO_SINGLE mode with additional slower sampling clock data stream for monitoring purposes (same as A-data of SPC_REC_FIFO_ABA mode).

Commands

The data acquisition/data replay is controlled by the command register. The command register controls the state of the card in general and also the state of the different data transfers. Data transfers are explained in an extra chapter later on.

The commands are split up into two types of commands: execution commands that fulfill a job and wait commands that will wait for the occurrence of an interrupt. Again the commands register is organized as a bitmap allowing you to set several commands together with one call. As not all of the command combinations make sense (like the combination of reset and start at the same time) the driver will check the given command and return an error code ERR_SEQUENCE if one of the given commands is not allowed in the current state.

Table 42: Spectrum API: card command register and different commands with descriptions

Register	Value	Direction	Description
SPC_M2CMD	100	write only	Executes a command for the card or data transfer.

Card execution commands

M2CMD_CARD_RESET	1h	Performs a hard and software reset of the card as explained further above.
M2CMD_CARD_WRITESETUP	2h	Writes the current setup to the card without starting the hardware. This command may be useful if changing some internal settings like clock frequency and enabling outputs.
M2CMD_CARD_START	4h	Starts the card with all selected settings. This command automatically writes all settings to the card if any of the settings has been changed since the last one was written. After card has been started, only some of the settings might be changed while the card is running, such as e.g. output level and offset for D/A replay cards.
M2CMD_CARD_ENABLETRIGGER	8h	The trigger detection is enabled. This command can be either sent together with the start command to enable trigger immediately or in a second call after some external hardware has been started.
M2CMD_CARD_FORCETRIGGER	10h	This command forces a trigger even if none has been detected so far. Sending this command together with the start command is similar to using the software trigger.
M2CMD_CARD_DISABLETRIGGER	20h	The trigger detection is disabled. All further trigger events are ignored until the trigger detection is again enabled. When starting the card the trigger detection is started disabled.
M2CMD_CARD_STOP	40h	Stops the current run of the card. If the card is not running this command has no effect.

Card wait commands

These commands do not return until either the defined state has been reached which is signaled by an interrupt from the card or the timeout counter has expired. If the state has been reached the command returns with an ERR_OK. If a timeout occurs the command returns with ERR_TIMEOUT. If the card has been stopped from a second thread with a stop or reset command, the wait function returns with ERR_ABORT.

M2CMD_CARD_WAITPREFULL	1000h	Acquisition modes only: the command waits until the pretrigger area has once been filled with data. After pretrigger area has been filled the internal trigger engine starts to look for trigger events if the trigger detection has been enabled.
M2CMD_CARD_WAITTRIGGER	2000h	Waits until the first trigger event has been detected by the card. If using a mode with multiple trigger events like Multiple Recording or Gated Sampling there only the first trigger detection will generate an interrupt for this wait command.
M2CMD_CARD_WAITREADY	4000h	Waits until the card has completed the current run. In an acquisition mode receiving this command means that all data has been acquired. In a generation mode receiving this command means that the output has stopped.

Wait command timeout

If the state for which one of the wait commands is waiting isn't reached any of the wait commands will either wait forever if no timeout is defined or it will return automatically with an ERR_TIMEOUT if the specified timeout has expired.

Table 43: Spectrum API: timeout definition register

Register	Value	Direction	Description
SPC_TIMEOUT	295130	read/write	Defines the timeout for any following wait command in a millisecond resolution. Writing a zero to this register disables the timeout.

As a default the timeout is disabled. After defining a timeout this is valid for all following wait commands until the timeout is disabled again by writing a zero to this register.

A timeout occurring should not be considered as an error. It did not change anything on the board status. The board is still running and will complete normally. You may use the timeout to abort the run after a certain time if no trigger has occurred. In that case a stop command is necessary after receiving the timeout. It is also possible to use the timeout to update the user interface frequently and simply call the wait function afterwards again.

Example for card control:

```
// card is started and trigger detection is enabled immediately
spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_CARD_START | M2CMD_CARD_ENABLETRIGGER);

// we wait a maximum of 1 second for a trigger detection. In case of timeout we force the trigger
spcm_dwSetParam_i32 (hDrv, SPC_TIMEOUT, 1000);
if (spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_CARD_WAITTRIGGER) == ERR_TIMEOUT)
{
    printf ("No trigger detected so far, we force a trigger now!\n");
    spcm_dwSetParam (hDrv, SPC_M2CMD, M2CMD_CARD_FORCETRIGGER);
}

// we disable the timeout and wait for the end of the run
spcm_dwSetParam_i32 (hDrv, SPC_TIMEOUT, 0);
spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_CARD_WAITREADY);
printf ("Card has stopped now!\n");
```

In case that a firmware update has gone wrong and the card has booted its golden recovery firmware (either automatically or by manual selection), all M2CMD_CARD_START commands will be returned with an ERR_GOLDENIMAGE error. The sole intention for the golden image is to provide a backup for safely updating the standard firmware image.



Card Status

In addition to the wait for an interrupt mechanism or completely instead of it one may also read out the current card status by reading the SPC_M2STATUS register. The status register is organized as a bitmap, so that multiple bits can be set, showing the status of the card and also of the different data transfers.

Table 44: Spectrum API: card status register and possible status values with descriptions of the status

Register	Value	Direction	Description
SPC_M2STATUS	110	read only	Reads out the current status information
M2STAT_CARD_PRETRIGGER	1h		Acquisition modes only: the first pretrigger area has been filled. In Multi/ABA/Gated acquisition this status is set only for the first segment and will be cleared at the end of the acquisition.
M2STAT_CARD_TRIGGER	2h		The first trigger has been detected.
M2STAT_CARD_READY	4h		The card has finished its run and is ready.
M2STAT_CARD_SEGMENT_PRETRG	8h		This flag will be set for each completed pretrigger area including the first one of a Single acquisition. Additionally for a Multi/ABA/Gated acquisition of M4i/M4x/M2p only, this flag will be set when the pretrigger area of a segment has been filled and will be cleared after the trigger for a segment has been detected.

Acquisition cards status overview

The following drawing gives you an overview of the card commands and card status information. After start of card with M2CMD_CARD_START the card is acquiring pretrigger data until one time complete pretrigger data has been acquired. Then the status bit M2STAT_CARD_PRETRIGGER is set. Either the trigger has been enabled together with the start command or the card now waits for trigger enable command M2CMD_CARD_ENABLETRIGGER. After receiving this command the trigger engine is enabled and card checks for a trigger event. As soon as the trigger event is received the status bit M2STAT_CARD_TRIGGER is set and the card acquires the programmed posttrigger data. After all post trigger data has been acquired the status bit M2STAT_CARD_READY is set and data can be read out:

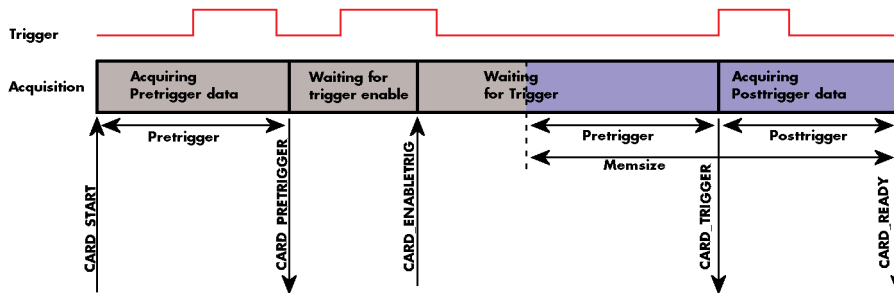


Image 46: Acquisition cards: graphical overview of acquisition status and card command interaction

Generation card status overview

This drawing gives an overview of the card commands and status information for a simple generation mode. After start of card with the M2CMD_CARD_START the card is armed and waiting. Either the trigger has been enabled together with the start command or the card now waits for trigger enable command M2CMD_CARD_ENABLETRIGGER. After receiving this command the trigger engine is enabled and card checks for a trigger event. As soon as the trigger event is received the status bit M2STAT_CARD_TRIGGER is set and the card starts with the data replay. After replay has been finished - depending on the programmed mode - the status bit M2STAT_CARD_READY is set and the card stops.

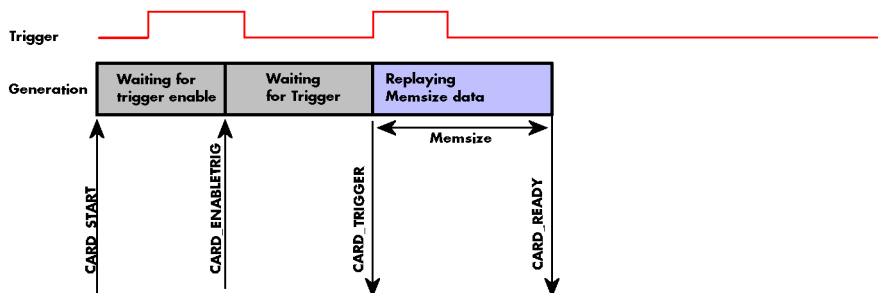


Image 47: Generation cards: graphical overview of generation status and card command interaction

Data Transfer

Data transfer consists of two parts: the buffer definition and the commands/status information that controls the transfer itself. Data transfer shares the command and status register with the card control commands and status information. In general the following details on the data transfer are valid for any data transfer in any direction:

- The memory size register (SPC_MEMSIZE) must be programmed before starting the data transfer.
- When the hardware buffer is adjusted from its default (see „Output latency“ section later in this manual), this must be done before defining the transfer buffers in the next step via the spcm_dwDefTransfer function.
- Before starting a data transfer the buffer must be defined using the spcm_dwDefTransfer function.
- Each defined buffer is only used once. After transfer has ended the buffer is automatically invalidated.
- If a buffer has to be deleted although the data transfer is in progress or the buffer has at least been defined it is necessary to call the spc-

`m_dwInvalidateBuf` function.

Definition of the transfer buffer

Before any data transfer can start it is necessary to define the transfer buffer with all its details. The definition of the buffer is done with the `spcm_dwDefTransfer` function as explained in an earlier chapter.

```
uint32 _stdcall spcm_dwDefTransfer_i64 (// Defines the transfer buffer by using 64 bit unsigned integer values
    drv_handle hDevice,                // handle to an already opened device
    uint32 dwBufType,                  // type of the buffer to define as listed below under SPCM_BUF_XXXX
    uint32 dwDirection,                // the transfer direction as defined below
    uint32 dwNotifySize,               // number of bytes after which an event is sent (0=end of transfer)
    void* pvDataBuffer,                // pointer to the data buffer
    uint64 qwBrdOffs,                  // offset for transfer in board memory
    uint64 qwTransferLen);              // buffer length
```

This function is used to define buffers for standard sample data transfer as well as for extra data transfer for additional ABA or timestamp information. Therefore the `dwBufType` parameter can be one of the following:

SPCM_BUF_DATA	1000	Buffer is used for transfer of standard sample data
SPCM_BUF_ABA	2000	Buffer is used to read out slow ABA data. Details on this mode are described in the chapter about the ABA mode option
SPCM_BUF_TIMESTAMP	3000	Buffer is used to read out timestamp information. Details on this mode are described in the chapter about the timestamp option.

The `dwDirection` parameter defines the direction of the following data transfer:

SPCM_DIR_PCTOCARD	0	Transfer is done from PC memory to on-board memory of card
SPCM_DIR_CARDTOPC	1	Transfer is done from card on-board memory to PC memory.
SPCM_DIR_CARDTGPU	2	RDMA transfer from card memory to GPU memory, SCAPP option needed, Linux only
SPCM_DIR_GPUTCARD	3	RDMA transfer from GPU memory to card memory, SCAPP option needed, Linux only

The direction information used here must match the currently used mode. While an acquisition mode is used there's no transfer from PC to card allowed and vice versa. It is possible to use a special memory test mode to come beyond this limit. Set the `SPC_MEMTEST` register as defined further below.



The `dwNotifySize` parameter defines the amount of bytes after which an interrupt should be generated. If leaving this parameter zero, the transfer will run until all data is transferred and then generate an interrupt. Filling in notify size > zero will allow you to use the amount of data that has been transferred so far. The notify size is used on FIFO mode to implement a buffer handshake with the driver or when transferring large amount of data where it may be of interest to start data processing while data transfer is still running. Please see the chapter on handling positions further below for details.

M2i, M3i, M4i, M4x and M2p cards:

The Notify size sticks to the page size which is defined by the PC hardware and the operating system. Therefore the notify size must be a multiple of 4 KiByte. For main data transfer it may also be a fraction of 4Ki in the range of 16, 32, 64, 128, 256, 512, 1Ki or 2Ki. No other values are allowed. For ABA and timestamp the notify size can be 2Ki as a minimum. If you need to work with ABA or timestamp data in smaller chunks please use the polling mode as described later.



M5i:

The Notify size sticks to the page size which is defined by the PC hardware and the operating system. Therefore the notify size must be a multiple of 4 KiByte. For main data transfer it may also be a fraction of 4Ki in the range of 64, 128, 256, 512, 1Ki or 2Ki. No other values are allowed. For timestamp the notify size can be 2Ki as a minimum. If you need to work with timestamp data in smaller chunks please use the polling mode as described later.



The `pvDataBuffer` must point to an allocated data buffer for the transfer. Please be sure to have at least the amount of memory allocated that you program to be transferred. If the transfer is going from card to PC this data is overwritten with the current content of the card on-board memory.

The `pvDataBuffer` needs to be aligned to a page size (4096 bytes). Please use appropriate software commands when allocating the data buffer. Using a non-aligned buffer may result in data corruption.



When not doing FIFO mode one can also use the `qwBrdOffs` parameter. This parameter defines the starting position for the data transfer as byte value in relation to the beginning of the card memory. Using this parameter allows it to split up data transfer in smaller chunks if one has acquired a very large on-board memory.

The `qwTransferLen` parameter defines the number of bytes that has to be transferred with this buffer. Please be sure that the allocated memory has at least the size that is defined in this parameter. In standard mode this parameter cannot be larger than the amount of data defined with memory size.

M5i cards only:

On M5i cards the `qwTransferLen` parameter needs to be an integer multiple of 64 bytes.

**Memory test mode**

In some cases it might be of interest to transfer data in the opposite direction. Therefore a special memory test mode is available which allows random read and write access of the complete on-board memory. While memory test mode is activated no normal card commands are processed:

Table 45: Spectrum API: memory test register

Register	Value	Direction	Description
SPC_MEMTEST	200700	read/write	Writing a 1 activates the memory test mode, no commands are then processed. Writing a 0 deactivates the memory test mode again.

Invalidation of the transfer buffer

The command can be used to invalidate an already defined buffer if the buffer is about to be deleted by user. This function is automatically called if a new buffer is defined or if the transfer of a buffer has completed

```
uint32 _stdcall spcm_dwInvalidateBuf ( // invalidate the transfer buffer
    drv_handle hDevice,              // handle to an already opened device
    uint32      dwBufType);          // type of the buffer to invalidate as listed above under SPCM_BUF_XXXX
```

The `dwBufType` parameter need to be the same parameter for which the buffer has been defined:

SPCM_BUF_DATA	1000	Buffer is used for transfer of standard sample data
SPCM_BUF_ABA	2000	Buffer is used to read out slow ABA data. Details on this mode are described in the chapter about the ABA mode option. The ABA mode is only available on analog acquisition cards.
SPCM_BUF_TIMESTAMP	3000	Buffer is used to read out timestamp information. Details on this mode are described in the chapter about the timestamp option. The timestamp mode is only available on analog or digital acquisition cards.

Commands and Status information for data transfer buffers.

As explained above the data transfer is performed with the same command and status registers like the card control. It is possible to send commands for card control and data transfer at the same time as shown in the examples further below.

Table 46: Spectrum API: Command register and commands for DMA transfers

Register	Value	Direction	Description
SPC_M2CMD	100	write only	Executes a command for the card or data transfer
M2CMD_DATA_STARTDMA	10000h		Starts the DMA transfer for an already defined buffer. In acquisition mode it may be that the card hasn't received a trigger yet, in that case the transfer start is delayed until the card receives the trigger event
M2CMD_DATA_WAITDMA	20000h		Waits until the data transfer has ended or until at least the amount of bytes defined by notify size are available. This wait function also takes the timeout parameter described above into account.
M2CMD_DATA_STOPDMA	40000h		Stops a running DMA transfer. Data is invalid afterwards.

The data transfer can generate one of the following status information:

Table 47: Spectrum API: status register and status codes for DMA data transfer

Register	Value	Direction	Description
SPC_M2STATUS	110	read only	Reads out the current status information
M2STAT_DATA_BLOCKREADY	100h		The next data block as defined in the notify size is available. It is at least the amount of data available but it also can be more data.
M2STAT_DATA_END	200h		The data transfer has completed.
M2STAT_DATA_OVERRUN	400h		The data transfer had on overrun (acquisition) or underrun (replay) while doing FIFO transfer.
M2STAT_DATA_ERROR	800h		An internal error occurred while doing data transfer.

Example of data transfer

```
void* pvData = pvAllocMemPageAligned (1024);

// transfer data from PC memory to card memory (on replay cards) ...
spcm_dwDefTransfer_i64 (hDrv, SPCM_BUF_DATA, SPCM_DIR_PCTOCARD, 0, pvData, 0, 1024);
spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_DATA_STARTDMA | M2CMD_DATA_WAITDMA);

// ... or transfer data from card memory to PC memory (acquisition cards)
spcm_dwDefTransfer_i64 (hDrv, SPCM_BUF_DATA, SPCM_DIR_CARDTOPC, 0, pvData, 0, 1024);
spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_DATA_STARTDMA | M2CMD_DATA_WAITDMA);

// explicitly stop DMA tranfer prior to invalidating buffer
spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_DATA_STOPDMA);
spcm_dwInvalidateBuf (hDrv, SPCM_BUF_DATA);
vFreeMemPageAligned (pvData, 1024);
```

To keep the example simple it does no error checking. Please be sure to check for errors if using these command in real world programs!

Users should take care to explicitly send the M2CMD_DATA_STOPDMA command prior to invalidating the buffer, to avoid crashes due to race conditions when using higher-latency data transportation layers, such as to remote Ethernet devices.



Standard Single acquisition mode

The standard single mode is the easiest and mostly used mode to acquire analog data with a Spectrum acquisition card. In standard single recording mode the card is working totally independent from the PC, after the card setup is done. The advantage of the Spectrum boards is that regardless to the system usage the card will sample with equidistant time intervals.

The sampled and converted data is stored in the on-board memory and is held there for being read out after the acquisition. This mode allows sampling at very high conversion rates without the need to transfer the data into the memory of the host system at high speed. After the recording is done, the data can be read out by the user and is transferred via the bus into PC memory.

This standard recording mode is the most common mode for all analog and digital acquisition and oscilloscope boards. The data is written to a programmed amount of the on-board memory (memsize). That part of memory is used as a ring buffer, and recording is done continuously until a trigger event is detected. After the trigger event, a certain programmable amount of data is recorded (post trigger) and then the recording finishes. Due to the continuous ring buffer recording, there are also samples prior to the trigger event in the memory (pretrigger).

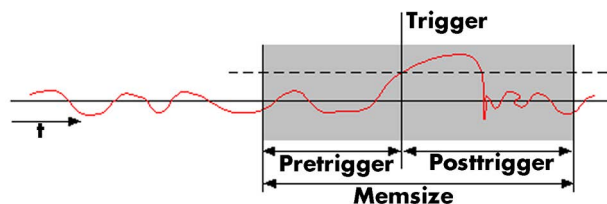


Image 48: standard acquisition mode and pretrigger/posttrigger/trigger relation

When the card is started the pre trigger area is filled up with data first. While doing this the board's trigger detection is not armed. If you use a huge pre trigger size and a slow sample rate it can take some time after starting the board before a trigger event will be detected.



Card mode

The card mode has to be set to the correct mode SPC_REC_STD_SINGLE.

Table 48: Spectrum API: card mode register and standard single mode setup

Register	Value	Direction	Description
SPC_CARDMODE	9500	read/write	Defines the used operating mode, a read command will return the currently used mode.
SPC_REC_STD_SINGLE	1h		Data acquisition to on-board memory for one single trigger event.

Memory, Pre- and Posttrigger

At first you have to define, how many samples are to be recorded at all and how many of them should be acquired after the trigger event has been detected.

Table 49: Spectrum API: memory size and posttrigger registers for standard single mode

Register	Value	Direction	Description
SPC_MEMSIZE	10000	read/write	Sets the memory size in samples per channel.
SPC_POSTTRIGGER	10100	read/write	Sets the number of samples to be recorded per channel after the trigger event has been detected.

You can access these settings by the register SPC_MEMSIZE, which sets the total amount of data that is recorded, and the register SPC_POSTTRIGGER, that defines the number of samples to be recorded after the trigger event has been detected. The size of the pretrigger results on the simple formula:

$$\text{pretrigger} = \text{memsize} - \text{posttrigger}$$

The maximum memsize that can be use for recording is of course limited by the installed amount of memory and by the number of channels to be recorded. Please have a look at the topic "Limits of pre, post memsize, loops" later in this chapter.

-

Example

The following example shows a simple standard single mode data acquisition setup with the read out of data afterwards. To keep this example simple there is no error checking implemented.

```
int32 lMemsize = 16384; // recording length is set to 16 KiSamples

spcm_dwSetParam_i32 (hDrv, SPC_CHENABLE, CHANNEL0); // only one channel activated
spcm_dwSetParam_i32 (hDrv, SPC_CARDMODE, SPC_REC_STD_SINGLE); // set the standard single recording mode
spcm_dwSetParam_i64 (hDrv, SPC_MEMSIZE, lMemsize); // recording length
spcm_dwSetParam_i64 (hDrv, SPC_POSTTRIGGER, 8192); // samples to acquire after trigger = 8Ki

// now we start the acquisition and wait for the interrupt that signalizes the end
spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_CARD_START | M2CMD_CARD_ENABLETRIGGER | M2CMD_CARD_WAITREADY);

void* pvData = pvAllocMemPageAligned (2 * lMemsize); // assuming 2 bytes per sample

// read out the data
spcm_dwDefTransfer_i64 (hDrv, SPCM_BUF_DATA, SPCM_DIR_CARDTOPC, 0, pvData, 0, 2 * lMemsize);
spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_DATA_STARTDMA | M2CMD_DATA_WAITDMA);
```

FIFO Single acquisition mode

The FIFO single mode does a continuous data acquisition using the on-board memory as a FIFO buffer and transferring data continuously to PC memory. One can make on-line calculations with the acquired data, store the data continuously to disk for later use or even have a data logger functionality with on-line data display.

Card mode

The card mode has to be set to the correct mode SPC_REC_FIFO_SINGLE.

Table 50: Spectrum API: card mode register and standard FIFO mode setup

Register	Value	Direction	Description
SPC_CARDMODE	9500	read/write	Defines the used operating mode, a read command will return the currently used mode.
SPC_REC_FIFO_SINGLE	10h		Continuous data acquisition to PC memory. Complete on-board memory is used as FIFO buffer.

Length and Pretrigger

Even in FIFO mode it is possible to program a pretrigger area. In general FIFO mode can run forever until it is stopped by an explicit user command or one can program the total length of the transfer by two counters Loop and Segment size

Table 51: Spectrum API: setup registers for standard FIFO mode

Register	Value	Direction	Description
SPC_PRETRIGGER	10030	read/write	Programs the number of samples to be acquired before the trigger event detection
SPC_SEGMENTSIZE	10010	read/write	Length of segments to acquire.
SPC_LOOPS	10020	read/write	Number of segments to acquire in total. If set to zero the FIFO mode will run continuously until it is stopped by the user.

The total amount of samples per channel that is acquired can be calculated by $[SPC_LOOPS * SPC_SEGMENTSIZE]$. Please stick to the below mentioned limitations of the registers.

Difference to standard single acquisition mode

The standard modes and the FIFO modes differ not very much from the programming side. In fact one can even use the FIFO mode to get the same behavior like the standard mode. The buffer handling that is shown in the next chapter is the same for both modes.

Pretrigger

When doing standard single acquisition memory is used as a circular buffer and the pre trigger can be up to the [installed memory] - [minimum post trigger]. Compared to this the pre trigger in FIFO mode is limited by a special pre trigger FIFO and hence considerably shorter.

Length of acquisition.

In standard mode the acquisition length is defined before the start and is limited to the installed on-board memory whilst in FIFO mode the acquisition length can either be defined or it can run continuously until user stops it.

Example FIFO acquisition

The following example shows a simple FIFO single mode data acquisition setup with the read out of data afterwards. To keep this example simple there is no error checking implemented.

```

spcm_dwSetParam_i32 (hDrv, SPC_CHENABLE, CHANNEL0); // only one channel activated
spcm_dwSetParam_i32 (hDrv, SPC_CARDMODE, SPC_REC_FIFO_SINGLE); // set the FIFO single recording mode
spcm_dwSetParam_i64 (hDrv, SPC_PRETRIGGER, 1024); // 1 KiSample of data before trigger

// in FIFO mode we need to define the buffer before starting the transfer
void* pvData = pvAllocMemPageAligned (llBufsizeInSamples * 2); // 2 bytes per sample
spcm_dwDefTransfer_i64 (hDrv, SPCM_BUF_DATA, SPCM_DIR_CARDTOPC, 4096,
    pvData, 0, 2 * llBufsizeInSamples);

// now we start the acquisition and wait for the first block
dwError = spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_CARD_START | M2CMD_CARD_ENABLETRIGGER);
dwError = spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_DATA_STARTDMA | M2CMD_DATA_WAITDMA);

// we acquire data in a loop. As we defined a notify size of 4Ki we'll get the data in >=4Ki chunks
llTotalBytes = 0;
while (!dwError)
{
    spcm_dwGetParam_i64 (hDrv, SPC_DATA_AVAIL_USER_LEN, &llAvailBytes); // read out the available bytes
    llTotalBytes += llAvailBytes;

    // here is the right position to do something with the data (printf is limited to 32 bit variables)
    printf ("Currently Available: %lld, total: %lld\n", llAvailBytes, llTotalBytes);

    // now we free the number of bytes and wait for the next buffer
    spcm_dwSetParam_i64 (hDrv, SPC_DATA_AVAIL_CARD_LEN, llAvailBytes);
    dwError = spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_DATA_WAITDMA);
}

```

Limits of pre trigger, post trigger, memory size

The maximum memory size parameter is only limited by the number of activated channels and by the amount of installed memory. Please keep in mind that each sample needs 1 bytes of memory to be stored. Minimum memory size as well as minimum and maximum post trigger limits are independent of the activated channels or the installed memory.

Due to the internal organization of the card memory there is a certain stepsize when setting these values that has to be taken into account. The following table gives you an overview of all limits concerning pre trigger, post trigger, memory size, segment size and loops. The table shows all values in relation to the installed memory size in samples. If more memory is installed the maximum memory size figures will increase according to the complete installed memory

Table 52: Spectrum API: Limits of pre trigger, post trigger and memory size

Activated Channels	Used Mode	Memory size SPC_MEMSIZE			Pre trigger SPC_PRETRIGGER			Post trigger SPC_POSTTRIGGER			Segment size SPC_SEGMENTSIZE			Loops SPC_LOOPS		
		Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step
1 Ch	Standard Single	64	Mem	32	32	Mem - 32 (defined by mem and post)	32	32	8Gi - 32	32	not used			not used		
	Standard Multi/ABA	64	Mem	32	32	8Ki (defined by segment and post)	32	32	Mem/2-32 (Limited by max pretrigger)	32	64	Mem/2	32	not used		
	Standard Gate	64	Mem	32	32	8Ki	32	32	Mem-32	32	not used			not used		
	Standard Average	For the limits in this mode please refer to the dedicated chapter in this manual.														
	FIFO Single	not used			32	8Ki	32	not used			64	8Gi - 32	32	0 (x)	4Gi - 1	1
	FIFO Multi/ABA	not used			32	8Ki (defined by segment and post)	32	32	8Gi-32 (Limited by max pretrigger)	32	64	pre+post	32	0 (x)	4Gi - 1	1
	FIFO Gate	not used			32	8Ki	32	32	8Gi - 32	32	not used			0 (x)	4Gi - 1	1
	FIFO Average	For the limits in this mode please refer to the dedicated chapter in this manual.														
2 Ch	Standard Single	64	Mem/2	32	32	Mem/2 - 32 (defined by mem and post)	32	32	8Gi - 32	32	not used			not used		
	Standard Multi/ABA	64	Mem/2	32	32	8Ki (defined by segment and post)	32	32	Mem/4-32 (Limited by max pretrigger)	32	64	Mem/4	32	not used		
	Standard Gate	64	Mem/2	32	32	8Ki	32	32	Mem/2-32	32	not used			not used		
	Standard Average	For the limits in this mode please refer to the dedicated chapter in this manual.														
	FIFO Single	not used			32	8Ki	32	not used			64	8Gi - 32	32	0 (x)	4Gi - 1	1
	FIFO Multi/ABA	not used			32	8Ki (defined by segment and post)	32	32	8Gi-32 (Limited by max pretrigger)	32	64	pre+post	32	0 (x)	4Gi - 1	1
	FIFO Gate	not used			32	8Ki	32	32	8Gi - 32	32	not used			0 (x)	4Gi - 1	1
	FIFO Average	For the limits in this mode please refer to the dedicated chapter in this manual.														
4 Ch	Standard Single	64	Mem/4	32	32	Mem/4 - 32 (defined by mem and post)	32	32	8Gi - 16	32	not used			not used		
	Standard Multi/ABA	64	Mem/4	32	32	8Ki (defined by segment and post)	32	32	Mem/4-32 (Limited by max pretrigger)	32	64	Mem/8	32	not used		
	Standard Gate	64	Mem/4	32	32	8Ki	32	32	Mem/4-16	32	not used			not used		
	Standard Average	For the limits in this mode please refer to the dedicated chapter in this manual.														
	FIFO Single	not used			32	8Ki	32	not used			64	8Gi - 32	32	0 (x)	4Gi - 1	1
	FIFO Multi/ABA	not used			32	8Ki	32	32	8Gi-32	32	64	pre+post	32	0 (x)	4Gi - 1	1

Table 52: Spectrum API: Limits of pre trigger, post trigger and memory size

Activated Channels	Used Mode	Memory size SPC_MEMSIZE			Pre trigger SPC_PRETRIGGER			Post trigger SPC_POSTTRIGGER			Segment size SPC_SEGMENTSIZE			Loops SPC_LOOPS		
		Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step
	FIFO Multi/ABA	not used			32	8Ki	32	32	8Gi-32	32	64	pre+post	32	0 (∞)	4Gi - 1	1
	FIFO Gate	not used			32	8Ki	32	32	8Gi - 32	32	not used			0 (∞)	4Gi - 1	1
	FIFO Average	For the limits in this mode please refer to the dedicated chapter in this manual.														

All figures listed here are given in samples. An entry of [8Gi - 32] means [8 GiB Samples - 32] = 8,589,934,560 samples.

The given memory and memory / divider figures depend on the installed on-board memory as listed below:

	Installed Memory	
	2 GiSample	8 GiSample (Option: M5i.xxx-MEM8GS)
Mem	2 GiSample	8 GiSample
Mem / 2	1 GiSample	4 GiSample
Mem / 4	512 MiSample	2 GiSample
Mem / 8	256 MiSample	1 GiSample

Please keep in mind that this table shows all values at once. Only the absolute maximum and minimum values are shown. There might be additional limitations. Which of these values is programmed depends on the used mode. Please read the detailed documentation of the mode.

Buffer handling

To handle the huge amount of data that can possibly be acquired with the M5i/M4i/M4x/M2p series cards, there is a very reliable two step buffer strategy set up. The on-board memory of the card can be completely used as a real FIFO buffer. In addition a part of the PC memory can be used as an additional software buffer. Transfer between hardware FIFO and software buffer is performed interrupt driven and automatically by the driver to get best performance. The following drawing will give you an overview of the structure of the data transfer handling:

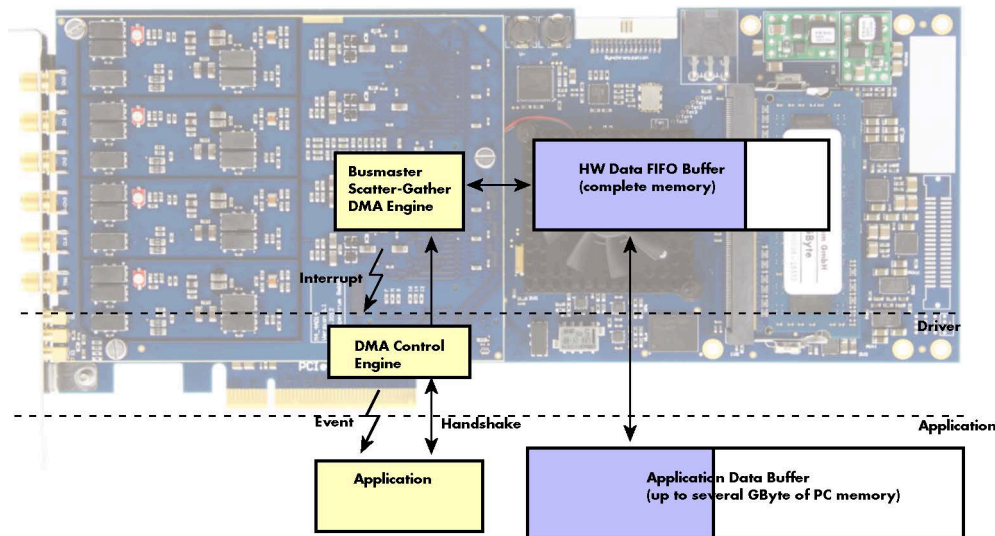


Image 49: Overview of buffer handling for DMA transfers showing and the interaction with the DMA engine

Although an M4i is shown here, this applies to M5i, M4x and M2p cards as well. A data buffer handshake is implemented in the driver which allows to run the card in different data transfer modes. The software transfer buffer is handled as one large buffer which is on the one side controlled by the driver and filled automatically by busmaster DMA from/to the hardware FIFO buffer and on the other hand it is handled by the user who set's parts of this software buffer available for the driver for further transfer. The handshake is fulfilled with the following 3 software registers:

Table 53: Spectrum API: registers for DMA buffer handling

Register	Value	Direction	Description
SPC_DATA_AVAIL_USER_LEN	200	read	Returns the number of currently to the user available bytes inside a sample data transfer.
SPC_DATA_AVAIL_USER_POS	201	read	Returns the position as byte index where the currently available data samples start.
SPC_DATA_AVAIL_CARD_LEN	202	write	Writes the number of bytes that the card can now use for sample data transfer again
SPC_FILLSIZEPROMILLE	200910	read	The register holds the current fill size of the on-board memory (FIFO buffer) in per mill (1/1000) of the full on-board memory.

Internally the card handles two counters, a user counter and a card counter. Depending on the transfer direction the software registers have slightly different meanings:

Table 54: Spectrum API: content of DMA buffer handling registers for different use cases

Transfer direction	Register	Direction	Description
Write to card	SPC_DATA_AVAIL_USER_LEN	read	This register contains the currently available number of bytes that are free to write new data to the card. The user can now fill this amount of bytes with new data to be transferred.
	SPC_DATA_AVAIL_CARD_LEN	write	After filling an amount of the buffer with new data to transfer to card, the user tells the driver with this register that the amount of data is now ready to transfer.
Read from card	SPC_DATA_AVAIL_USER_LEN	read	This register contains the currently available number of bytes that are filled with newly transferred data. The user can now use this data for own purposes, copy it, write it to disk or start calculations with this data.
	SPC_DATA_AVAIL_CARD_LEN	write	After finishing the job with the new available data the user needs to tell the driver that this amount of bytes is again free for new data to be transferred.
Any direction	SPC_DATA_AVAIL_USER_POS	read	The register holds the current byte index position where the available bytes start. The register is just intended to help you and to avoid own position calculation
Any direction	SPC_FILLSIZEPROMILLE	read	The register holds the current fill size of the on-board memory (FIFO buffer) in promille (1/1000) of the full on-board memory. Please note that the hardware reports the fill size only in 1/16 parts of the full memory. The reported fill size is therefore only shown in $1000/16 = 63$ promille steps.

Directly after start of transfer the SPC_DATA_AVAIL_USER_LEN is every time zero as no data is available for the user and the SPC_DATA_AVAIL_CARD_LEN is every time identical to the length of the defined buffer as the complete buffer is available for the card for transfer.

The counter that is holding the user buffer available bytes (SPC_DATA_AVAIL_USER_LEN) is related to the notify size at the DefTransfer call. Even when less bytes already have been transferred you won't get notice of it in case the notify size is programmed to a higher value.



Remarks

- The transfer between hardware FIFO buffer and application buffer is done with scatter-gather DMA using a busmaster DMA controller located on the card. Even if the PC is busy with other jobs data is still transferred until the application data buffer is completely used.
- Even if application data buffer is completely used there's still the hardware FIFO buffer that can hold data until the complete on-board memory is used. Therefore a larger on-board memory will make the transfer more reliable against any PC dead times.
- As you see in the above picture data is directly transferred between application data buffer and on-board memory. Therefore it is absolutely critical to delete the application data buffer without stopping any DMA transfers that are running actually. It is also absolutely critical to define the application data buffer with an unmatching length as DMA can than try to access memory outside the application data area.
- As shown in the drawing above the DMA control will announce new data to the application by sending an event. Waiting for an event is done internally inside the driver if the application calls one of the wait functions. Waiting for an event does not consume any CPU time and is therefore highly desirable if other threads do a lot of calculation work. However it is not necessary to use the wait functions and one can simply request the current status whenever the program has time to do so. When using this polling mode the announced available bytes still stick to the defined notify size!
- If the on-board FIFO buffer has an overrun (card to PC) or an underrun (PC to card) data transfer is stopped. However in case of transfer from card to PC there is still a lot of data in the on-board memory. Therefore the data transfer will continue until all data has been transferred although the status information already shows an overrun.
- For very small notify sizes, getting best bus transfer performance could be improved by using a „continuous buffer“. This mode is explained in the appendix in greater detail.

M2i, M3i, M4i, M4x and M2p cards:

The Notify size sticks to the page size which is defined by the PC hardware and the operating system. Therefore the notify size must be a multiple of 4 KiByte. For main data transfer it may also be a fraction of 4Ki in the range of 16, 32, 64, 128, 256, 512, 1Ki or 2Ki. No other values are allowed. For ABA and timestamp the notify size can be 2Ki as a minimum. If you need to work with ABA or timestamp data in smaller chunks please use the polling mode as described later.



M5i:


The Notify size sticks to the page size which is defined by the PC hardware and the operating system. Therefore the notify size must be a multiple of 4 KiByte. For main data transfer it may also be a fraction of 4Ki in the range of 64, 128, 256, 512, 1Ki or 2Ki. No other values are allowed. For timestamp the notify size can be 2Ki as a minimum. If you need to work with timestamp data in smaller chunks please use the polling mode as described later.



The following graphs will show the current buffer positions in different states of the transfer. The drawings have been made for the transfer from card to PC. However all the block handling is similar for the opposite direction, just the empty and the filled parts of the buffer are inverted.


Step 1: Buffer definition

Directly after buffer definition the complete buffer is empty (card to PC) or completely filled (PC to card). In our example we have a notify size which is 1/4 of complete buffer memory to keep the example simple. In real world use it is recommended to set the notify size to a smaller stepsize.

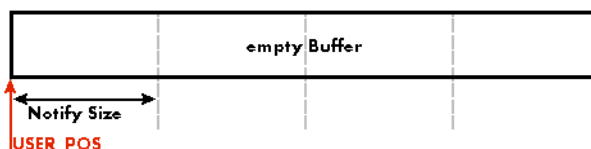

Step 2: Start and first data available


In between we have started the transfer and have waited for the first data to be available for the user. When there is at least one block of notify size in the memory we get an interrupt and can proceed with the data. Any data that already was transferred is announced. The USER_POS is still zero as we are right at the beginning of the complete transfer.

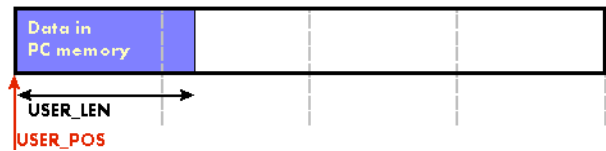**Step 3: set the first data available for card**


Now the data can be processed. If transfer is going from card to PC that may be storing to hard disk or calculation of any figures. If transfer is going from PC to card that means we have to fill the available buffer again with data. After the amount of data that has been processed by the user application we set it available for the card and for the next step.

**Step 4: next data available**


After reaching the next border of the notify size we get the next part of the data buffer to be available. In our example at the time when reading the USER_LEN even some more data is already available. The user position will now be at the position of the previous set CARD_LEN.

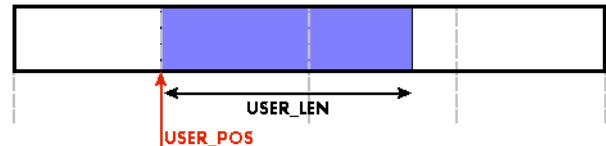**Step 5: set data available again**


Again after processing the data we set it free for the card use. In our example we now make something else and don't react to the interrupt for a longer time. In the background the buffer is filled with more data.

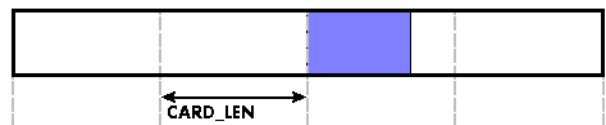**Step 6: roll over the end of buffer**

Now nearly the complete buffer is filled. Please keep in mind that our current user position is still at the end of the data part that we processed and marked in step 4 and step 5. Therefore the data to process now is split in two parts. Part 1 is at the end of the buffer while part 2 is starting with address 0.

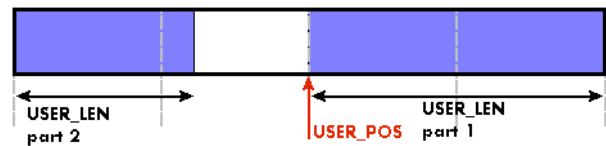**Step 7: set the rest of the buffer available**

Feel free to process the complete data or just the part 1 until the end of the buffer as we do in this example. If you decide to process complete buffer please keep in mind the roll over at the end of the buffer.

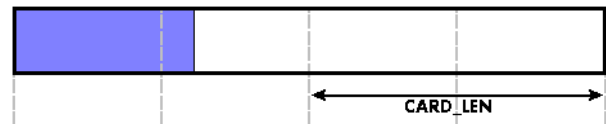

This buffer handling can now continue endless as long as we manage to set the data available for the card fast enough. The USER_POS and USER_LEN for step 8 would now look exactly as the buffer shown in step 2.

Buffer handling example for transfer from card to PC (Data acquisition)

```

int8* pcData = (int8*) pvAllocMemPageAligned (llBufferSizeInBytes);

// we now define the transfer buffer with the minimum notify size of one page = 4 KiByte
spcm_dwDefTransfer_i64 (hDrv, SPCM_BUF_DATA, SPCM_DIR_CARDTOPC, 4096, (void*) pcData, 0, llBufferSizeInBytes);

// we start the DMA transfer
dwError = spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_DATA_STARTDMA);

do
{
    if (!dwError)
    {
        // we wait for the next data to be available. After this call we get at least 4Ki of data to proceed
        dwError = spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_DATA_WAITDMA);

        // if there was no error we can proceed and read out the available bytes that are free again
        spcm_dwGetParam_i64 (hDrv, SPC_DATA_AVAIL_USER_LEN, &llAvailBytes);
        spcm_dwGetParam_i64 (hDrv, SPC_DATA_AVAIL_USER_POS, &llBytePos);

        printf ("We now have %lld new bytes available\n", llAvailBytes);
        printf ("The available data starts at position %lld\n", llBytePos);

        // we take care not to go across the end of the buffer, handling the wrap-around
        if ((llBytePos + llAvailBytes) >= llBufferSizeInBytes)
            llAvailBytes = llBufferSizeInBytes - llBytePos;

        // our do function gets a pointer to the start of the available data section and the length
        vDoSomething (&pcData[llBytePos], llAvailBytes);

        // the buffer section is now immediately set available for the card
        spcm_dwSetParam_i64 (hDrv, SPC_DATA_AVAIL_CARD_LEN, llAvailBytes);
    }
}
while (!dwError); // we loop forever if no error occurs

```

Buffer handling example for transfer from PC to card (Data generation)

```

int8* pcData = (int8*) pvAllocMemPageAligned (llBufferSizeInBytes);

// before starting transfer we first need to fill complete buffer memory with meaningful data
vDoGenerateData (&pcData[0], llBufferSizeInBytes);

// we now define the transfer buffer with the minimum notify size of one page = 4 KiByte
spcm_dwDefTransfer_i64 (hDrv, SPCM_BUF_DATA, SPCM_DIR_PCTOCARD, 4096, (void*) pcData, 0, llBufferSizeInBytes);

// and transfer some data to the hardware buffer before the start of the card
spcm_dwSetParam_i32 (hDrv, SPC_DATA_AVAIL_CARD_LEN, llBufferSizeInBytes);
dwError = spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_DATA_STARTDMA | M2CMD_DATA_WAITDMA);

do
{
    if (!dwError)
    {
        // if there was no error we can proceed and read out the current amount of available data
        spcm_dwGetParam_i64 (hDrv, SPC_DATA_AVAIL_USER_LEN, &llAvailBytes);
        spcm_dwGetParam_i64 (hDrv, SPC_DATA_AVAIL_USER_POS, &llBytePos);

        printf ("We now have %lld free bytes available\n", llAvailBytes);
        printf ("The available data starts at position %lld\n", llBytePos);

        // we take care not to go across the end of the buffer, handling the wrap-around
        if ((llBytePos + llAvailBytes) >= llBufferSizeInBytes)
            llAvailBytes = llBufferSizeInBytes - llBytePos;

        // our do function gets a pointer to the start of the available data section and the length
        vDoGenerateData (&pcData[llBytePos], llAvailBytes);

        // now we mark the number of bytes that we just generated for replay
        // and wait for the next free buffer
        spcm_dwSetParam_i64 (hDrv, SPC_DATA_AVAIL_CARD_LEN, llAvailBytes);
        dwError = spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_DATA_WAITDMA);
    }
}
while (!dwError); // we loop forever if no error occurs

```

Please keep in mind that you are using a continuous buffer writing/reading that will start again at the zero position if the buffer length is reached. However the `DATA_AVAIL_USER_LEN` register will give you the complete amount of available bytes even if one part of the free area is at the end of the buffer and the second half at the beginning of the buffer.



Data organization

Data is organized in a multiplexed way in the transfer buffer. If using 2 channels data of first activated channel comes first, then data of second channel.

Table 55: M4i and M4x cards data organization

Activated Channels	Ch0	Ch1	Ch2	Ch3	Samples ordering in buffer memory starting with data offset zero																
1 channel	X				A0	A1	A2	A3	A4	A5	A6	A7	A8	A9	A10	A11	A12	A13	A14	A15	A16
1 channel		X			B0	B1	B2	B3	B4	B5	B6	B7	B8	B9	B10	B11	B12	B13	B14	B15	B16
1 channel			X		C0	C1	C2	C3	C4	C5	C6	C7	C8	C9	C10	C11	C12	C13	C14	C15	C16
1 channel				X	D0	D1	D2	D3	D4	D5	D6	D7	D8	D9	D10	D11	D12	D13	D14	D15	D16
2 channels	X	X			A0	B0	A1	B1	A2	B2	A3	B3	A4	B4	A5	B5	A6	B6	A7	B7	A8
2 channels	X		X		A0	C0	A1	C1	A2	C2	A3	C3	A4	C4	A5	C5	A6	C6	A7	C7	A8
2 channels	X			X	A0	D0	A1	D1	A2	D2	A3	D3	A4	D4	A5	D5	A6	D6	A7	D7	A8
2 channels		X	X		B0	C0	B1	C1	B2	C2	B3	C3	B4	C4	B5	C5	B6	C6	B7	C7	B8
2 channels		X		X	B0	D0	B1	D1	B2	D2	B3	D3	B4	D4	B5	D5	B6	D6	B7	D7	B8
2 channels			X	X	C0	D0	C1	D1	C2	D2	C3	D3	C4	D4	C5	D5	C6	D6	C7	D7	C8
4 channels	X	X	X	X	A0	B0	C0	D0	A1	B1	C1	D1	A2	B2	C2	D2	A3	B3	C3	D3	A4

The samples are re-named for better readability. A0 is sample 0 of channel 0, B4 is sample 4 of channel 1, and so on.

Data in the transfer buffer is stored in little-endian format, so it can be easily processed by systems based on x86, x64 or others.



Sample format

The card is using 7 bit A/D samples, that are stored in two's complement in one 8 bit data byte. 7 bit resolution means that data is ranging from -64...to...+63:

	Standard Mode M4i.23xx	Digital inputs enabled SPCM_XMODE_DIGIN M4i.23xx
Data bit	8 bit ADC resolution	7 bit ADC resolution
D7	ADx Bit 6 (sign extension)	Ch3: Digital bit 0 (X0) Ch2: Digital bit 2 (X2) Ch1: Digital bit 1 (X1) Ch0: Digital bit 0 (X0)
D6	ADx Bit 6 (MSB)	ADx Bit 6 (MSB)
D5	ADx Bit 5	ADx Bit 5
D4	ADx Bit 4	ADx Bit 4
D3	ADx Bit 3	ADx Bit 3
D2	ADx Bit 2	ADx Bit 2
D1	ADx Bit 1	ADx Bit 1
D0	ADx Bit 0 (LSB)	ADx Bit 0 (LSB)

Converting ADC samples to voltage values

The Spectrum driver also contains a register that allows to read out the decimal value of cards ADC's full scale representation. This value should be read out and used for converting ADC values (in LSB) into real-world voltage values, because this register also automatically takes any specialities into account, such as card dependant slightly reduced ADC resolution with reserved codes for gain/offset compensation.

Register	Value	Direction	Description
SPC_MIINST_MAXADCVALUE	1126	read	Contains the decimal code (in LSB) of the ADC full scale value.

In case of a board that uses an 8 bit ADC that provides the full ADC code (without reserving any bits) the returned value would be 128. The peak value for a ± 1.0 V input range would be 1.0 V (or 1000 mV).

$$V_{In} = ADC_{Code} \times \frac{InputRange_{peak}}{ADC_{max}}$$

A returned sample value of for example +49 (decimal, two's complement, signed representation) would then convert to:

$$V_{in} = 49 \times \frac{1000 \text{ mV}}{128} = 382.81 \text{ mV}$$

A returned sample value of for example -55 (decimal) would then convert to:

$$V_{in} = -55 \times \frac{1000 \text{ mV}}{128} = -429.69 \text{ mV}$$

When converting samples that contain any additional data such as for example additional digital channels or over-range bits, this extra information must be first masked out and a proper sign-extension must be performed, before these values can be used as a signed two's complement value for above formulas.



Enabling hardware sample conversion to offset-binary

The data conversion modes allow the conversion of acquired sample data in on the fly within the firmware from the cards native two's complement representation to the offset binary mode. This feature was implemented beginning with firmware version V45. It is only intended to allow existing applications/data calculation routines relying on such encoding to be re-used. For all other situations the default two's complement signed integer format as described above should be used:

Table 56: Spectrum API: data conversion registers and valid register settings

Register	Value	Direction	Description
SPC_DATACONVERSION	201400	read/write	Defines the data conversion mode.
SPC_AVAIDATACONVERSION	201401	read	Read out the available data conversion modes.
SPCM_DC_NONE	0h		The original data format will be used and no hardware data conversion will be done.
SPCM_DC_TO_OFFSETBINARY	800h		Allows conversion of RAW 1 samples om two's complement to encoding to offset-binary encoding.

The conversion to offset-binary only works on the RAW original samples, as listed in the „Sample format“ table above. It cannot be combined with any other data conversion mode („Mode 8 bit Storage“) and also does not work on the output of any other firmware processing feature, such as „Block Average“, „Block Statistics“, or „Boxcar Average“. This conversion also only affects the samples of the main data stream (B-data) when using „ABA mode“.



Clock generation

Overview

The Spectrum M4i PCI Express (PCIe) and M4x PXI Express (PXIe) cards offer a wide variety of different clock modes to match all the customers' needs. All of the clock modes are described in detail with programming examples in this chapter.

The figure is showing an overview of the complete engine used on all M4i cards for clock generation.

The purpose of this chapter is to give you a guide to the best matching clock settings for your specific application and needs.

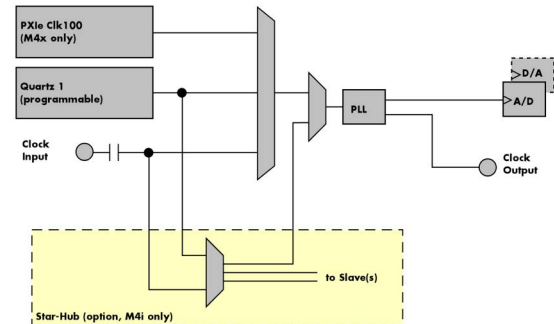


Image 50: M4i/M4x clock section overview

Clock Mode Register

The selection of the different clock modes has to be done by the SPC_CLOCKMODE register. All available modes, can be read out by the help of the SPC_AVAILCLOCKMODES register.

Table 57: Spectrum API: clock mode register and available clock modes

Register	Value	Direction	Description
SPC_AVAILCLOCKMODES	20201	read	Bitmask, in which all bits of the below mentioned clock modes are set, if available.
SPC_CLOCKMODE	20200	read/write	Defines the used clock mode or reads out the actual selected one.
SPC_CM_INTPLL	1		Enables internal programmable high precision Quartz 1 for sample clock generation
SPC_CM_EXTREFCLOCK	32		Enables internal PLL with external reference for sample clock generation
SPC_CM_PXIREFCLOCK	64		M4x cards only: Enables internal PLL with PXIe backplane clock as reference for sample clock generation

The different clock modes and all other related or required register settings are described on the following pages.

The different clock modes

Standard internal sample rate (programmable reference quartz 1)

This is the easiest and most common way to generate a sample rate with no need for additional external clock signals. The sample rate has low jitter and a high accuracy and on cards supporting fine granularity sample rate, this mode also provides a very fine resolution. The Quartz 1 is a high quality software programmable clock device acting as a reference to the internal PLL. The specification is found in the technical data section of this manual. This clock mode does require the sampling rate to be programmed as described in the upcoming "Programming the sampling rate" paragraph.

External Reference Clock

Any clock can be fed in that matches the specification of the board. The external clock signal can be used to synchronize the board on a system clock or to feed in an exact matching sample rate. The external clock is divided/multiplied using a PLL allowing a wide range of external clock modes. This clock mode does require the sampling rate to be programmed as described in the upcoming "Programming the sampling rate" paragraph.

PXIe Reference Clock (M4x cards only)

The PXIe reference clock is a 100 MHz high-quality differential clock signal with an accuracy of ± 100 ppm or better. This reference clock is located on the PXIe backplane and is routed to every PXIe slot with the same trace length on the mainboard's PCB. PXIe cards from Spectrum are able to use the PXIe reference clock for sampling clock generation. One big advantage of using the reference clock is the fact that all cards that are synchronized to the reference clock are running with the same clock frequency. This clock mode does require the sampling rate to be programmed as described in the upcoming "Programming the sampling rate" paragraph.

Synchronization Clock (option Star-Hub, M4i cards only)

The star-hub option allows the synchronization of up to 8 cards of the M4i series from Spectrum with a minimal phase delay between the different cards. The clock is distributed from the master card to all connected cards. As a source it is possible to either use the programmable Quartz 1 clock or the external Ext0 reference clock input of the master card. For details on the synchronization option please take a look at the dedicated chapter later in this manual. This clock mode does require the sampling rate to be programmed as described in the upcoming "Programming the sampling rate" paragraph.

Details on the different clock modes

Programming the sampling rate

Most clock modes require, that the sampling rate is explicitly programmed. Whether that is the case for a specific clock mode or not is mentioned in the "The different clock modes" paragraph.

When setting the sampling rate, the user does not have to care about how the desired sampling rate is generated by means of multiplying and dividing internally. You simply write the desired sample rate to the according register shown in the table below and the driver makes all the necessary calculations. If you want to make sure the sample rate has been set correctly you can also read out the register and the driver will give you back the sampling rate that is matching your desired one best.

Table 58: Spectrum API: samplerate register

Register	Value	Direction	Description
SPC_SAMPLERATE	20000	write	Defines the sample rate in Hz for internal sample rate generation.
		read	Read out the internal sample rate that is nearest matching to the desired one.

Standard internal sampling clock (PLL)

The internal sampling clock is generated in default mode by a programmable high precision quartz. You need to select the clock mode by the dedicated register shown in the table below:

Table 59: Spectrum API: clock mode register and internal clock mode

Register	Value	Direction	Description
SPC_CLOCKMODE	20200	read/write	Defines the used clock mode
SPC_CM_INTPLL	1		Enables internal programmable high precision Quartz 1 for sample clock generation

Independent of the used clock source it is possible to enable the clock output. The clock will be available on the external clock output connector and can be used to synchronize external equipment with the board.

Table 60: Spectrum API: clock output and clock output frequency register

Register	Value	Direction	Description
SPC_CLOCKOUT	20110	read/write	Writing a „1“ enables clock output on external clock output connector. Writing a „0“ disables the clock output (tristate)
SPC_CLOCKOUTFREQUENCY	20111	read	Allows to read out the frequency of an internally synthesized clock present at the clock output.

Example on writing and reading internal sampling rate

```

spcm_dwSetParam_i32 (hDrv, SPC_CLOCKMODE, SPC_CM_INTPLL); // Enables internal programmable quartz 1
spcm_dwSetParam_i64 (hDrv, SPC_SAMPLERATE, 62500000);      // Set internal sampling rate to 62.5 MHz
spcm_dwSetParam_i32 (hDrv, SPC_CLOCKOUT, 1);              // enable the clock output of the card
spcm_dwGetParam_i64 (hDrv, SPC_SAMPLERATE, &lSamplerate); // Read back the programmed sample rate and print
printf („Sample rate = %d\\n“, lSamplerate);                // it. Output should be „Sample rate = 62500000“

```

In all clock modes, the sampling rate can only be programmed as maximum samplingrate and divisions of this. Valid sampling rates are [max], [max/2], [max/4], [max/8], ... [max/131072]. Any programmed sampling rate in between will automatically be rounded to the next matching divided sampling clock.



Minimum internal sampling rate

The minimum internal sampling rates depend on the specific type of board. This value can be found in the technical data section of this manual.

Maximum internal sampling rate

activated Channels									
Ch0	Ch1	Ch2	Ch3	M4i.2320	M4i.2321	M4i.2323	M4i.2330	M4i.2333	M4i.2334
X	X	X	X	2.5 GS/s	2.5 GS/s	2.5 GS/s	5 GS/s	5 GS/s	5 GS/s
				n.a.	2.5 GS/s	2.5 GS/s	n.a.	5 GS/s	5 GS/s
				n.a.	n.a.	n.a.	n.a.	n.a.	5 GS/s
				n.a.	n.a.	n.a.	n.a.	n.a.	5 GS/s
X	X	X	X	n.a.	2.5 GS/s	1.25 GS/s	n.a.	2.5 GS/s	1.25 GS/s
X		X		n.a.	n.a.	n.a.	n.a.	n.a.	2.5 GS/s
X			X	n.a.	n.a.	n.a.	n.a.	n.a.	2.5 GS/s
	X	X		n.a.	n.a.	n.a.	n.a.	n.a.	2.5 GS/s
	X		X	n.a.	n.a.	n.a.	n.a.	n.a.	2.5 GS/s
		X	X	n.a.	n.a.	n.a.	n.a.	n.a.	1.25 GS/s
X	X	X	X	n.a.	n.a.	n.a.	n.a.	n.a.	1.25 GS/s

Using Quartz2 with PLL (optional, M4i cards only)

In some cases it is necessary to use a special high precision frequency for sampling rate generation. For these applications all cards of the M3i/M4i series can be equipped with a special customer quartz. Please contact Spectrum for details on available oscillators. If your card is equipped with a second oscillator you can enable it for sampling rate generation with the following register:

Table 61: Spectrum API: clock mode register and quartz 2 settings

Register	Value	Direction	Description
SPC_CLOCKMODE	20200	read/write	Defines the used clock mode
SPC_CM_QUARTZ2	4		Enables optional quartz2 for sample clock generation

The quartz 2 clock is routed through a PLL to allow the generation of sampling rates based on this reference clock. As with internal PLL mode it's also possible to program the clock mode first, set a desired sampling rate with the SPC_SAMPLERATE register and to read it back. The result will then again be the best matching sampling rate.

Independent of the used clock source it is possible to enable the clock output. The clock will be available on the external clock output connector and can be used to synchronize external equipment with the board.

Table 62: Spectrum API: clock output and clock output frequency register

Register	Value	Direction	Description
SPC_CLOCKOUT	20110	read/write	Writing a „1“ enables clock output on external clock output connector. Writing a „0“ disables the clock output (tristate)
SPC_CLOCKOUTFREQUENCY	20111	read	Allows to read out the frequency of an internally synthesized clock present at the clock output.

Oversampling

All fast instruments have a minimum clock frequency that is limited by either the manufacturer limit of the used data converter (ADC or DAC) or by limiting factors of the clock design.

When using one of the above mentioned internal clock modes the driver allows you to program sampling clocks that lie far beneath this minimum sampling clock. To run the instrument properly we use a special oversampling mode where the A/D or D/A converter in conjunction with the clock section is within its converter specification and only the digital part of the card is running with the slower clock. This is completely handled inside the driver and cannot be modified by the user. The following register allows to read out the oversampling factor for further calculation

Table 63: Spectrum API: clock oversampling readout register

Register	Value	Direction	Description
SPC_OVERSAMPLINGFACTOR	200123	read only	Returns the oversampling factor for further calculations. If oversampling isn't active a 1 is returned.

When using clock output the sampling clock at the output connector is not reflecting the oversampling factor. To get the frequency of the output clock, please just read the SPC_CLOCKOUTFREQUENCY register.



External clock (reference clock)

The external clock input is fed through a PLL to the clock system. Therefore the input will act as a reference clock input thus allowing to either use a copy of the external clock or to generate any sampling clock within the allowed range from the reference clock. Please note the limited setup granularity in comparison to the internal sampling clock generation. Details are found in the technical data section.

Table 64: Spectrum API: clock mode register and external reference clock setup

Register	Value	Direction	Description
SPC_CLOCKMODE	20200	read/write	Defines the used clock mode
SPC_CM_EXTREFCLOCK	32		Enables internal PLL with external reference for sample clock generation

Due to the fact that the driver needs to know the external fed in frequency for an exact calculation of the sampling rate you must set the SPC_REFERENCECLOCK register accordingly as shown in the table below. The driver then automatically sets the PLL to achieve the desired sampling rate. Please be aware that the PLL has some internal limits and not all desired sampling rates may be reached with every reference clock.

Table 65: Spectrum API: reference clock register and available settings

Register	Value	Direction	Description
SPC_REFERENCECLOCK	20140	read/write	Programs the external reference clock in the range stated in the technical data section.
	External sampling rate in Hz as an integer value		You need to set up this register exactly to the frequency of the external fed in clock.

Example of reference clock:

```
spcm_dwSetParam_i32 (hDrv, SPC_CLOCKMODE, SPC_CM_EXTREFCLOCK); // Set to reference clock mode
spcm_dwSetParam_i32 (hDrv, SPC_REFERENCECLOCK, 10000000); // Reference clock that is fed in is 10 MHz
spcm_dwSetParam_i64 (hDrv, SPC_SAMPLERATE, 62500000); // We want to have 62.5 MHz as sampling rate
```

It is recommended that the sampling clock is always an integer multiple of the reference clock. If the sampling clock is a division of the reference clock, the clock starting phase is undetermined and may change between resets or clock configuration changes.



PLL Locking Error

The external clock signal is routed to a PLL to generate any sampling clock from this external clock. Due to the internal structure of the card the PLL is even used if a copy of the clock fed in externally is used for sampling (SPC_REFERENCECLOCK = SPC_SAMPLERATE). The PLL needs a stable and defined external clock with no gaps and no variation in the frequency. The external clock must be present when issuing the start command. It is not possible to start the card with external clock activated and no external clock available.

When starting the card all settings are written to hardware and the PLL is programmed to generate the desired sampling clock. If there has been any change to the clock setting the PLL then tries to lock on the external clock signal to generate the sampling clock. This locking will normally need 10 to 20 ms until the sampling clock is stable. Some clock settings may also need 200 ms to lock the PLL. This waiting time is automatically added at card start.

However if the PLL can not lock on the external clock either because there is no clock available or it hasn't sufficient signal levels or the clock is not stable the driver will return with an error code ERR_CLOCKNOTLOCKED. In that case it is necessary to check the external clock connection. Please see the example below:

```
// settings done to external clock like shown above.
if (spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_CARD_START | M2CMD_CARD_ENABLETRIGGER) == ERR_CLOCKNOTLOCKED)
{
    printf („External clock not locked. Please check connection\n");
    return -1;
}
```

Independent of the used clock source it is possible to enable the clock output. The clock will be available on the external clock output connector and can be used to synchronize external equipment with the board.

Table 66: Spectrum API: clock output and clock output frequency register

Register	Value	Direction	Description
SPC_CLOCKOUT	20110	read/write	Writing a „1“ enables clock output on external clock output connector. Writing a „0“ disables the clock output (tristate)
SPC_CLOCKOUTFREQUENCY	20111	read	Allows to read out the frequency of an internally synthesized clock present at the clock output.

PXI Reference Clock (M4x cards only)

Table 67: Spectrum API: clock mode register and PXI reference clock usage

Register	Value	Direction	Description
SPC_CLOCKMODE	20200	read/write	Defines the used clock mode
SPC_CM_PXIREFCLOCK	64		Enables internal PLL with PXI reference for sample clock generation

The 100 MHz PXIe system reference clock can be used as a reference clock for internal sample rate generation on all M4x PXIe cards from Spectrum. With the above mentioned software command the PXIe reference clock is routed to the internal PLL. Afterwards you only have to program the sample rate register to the desired sampling rate. The remaining internal calculations will be automatically done by the driver.

Example of PXI reference clock:

```
spcm_dwSetParam_i32 (hDrv, SPC_CLOCKMODE, SPC_CM_PXIREFCLOCK); // Set to PXI reference clock mode
spcm_dwSetParam_i64 (hDrv, SPC_SAMPLERATE, 65200000); // We want to have 62.5 MHz as sampling rate
```

PLL Locking Error

The PXI reference signal is routed to a PLL to generate any sampling clock from this external clock. The PLL needs a stable and defined external clock with no gaps and no variation in the frequency. Some backplanes might allow to turn off the reference clock. The PXI clock must be present when issuing the start command. It is not possible to start the card with external clock activated and no external clock available.

When starting the card all settings are written to hardware and the PLL is programmed to generate the desired sampling clock. If there has been any change to the clock setting the PLL then tries to lock on the external clock signal to generate the sampling clock. This locking will normally need 10 to 20 ms until the sampling clock is stable. Some clock settings may also need 200 ms to lock the PLL. This waiting time is automatically added at card start.

However if the PLL can not lock on the PXI clock because there is no clock available (if however disabled on the backplane), the driver will return with an error code `ERR_CLOCKNOTLOCKED`. In that case it is necessary to check the external clock connection. Please see the example below:

```
// settings done to PXI clock like shown above.
if (spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_CARD_START | M2CMD_CARD_ENABLETRIGGER) == ERR_CLOCKNOTLOCKED)
{
    printf („External clock not locked. Please check connection\n");
    return -1;
}
```

Trigger modes and appendant registers

General Description

The trigger modes of the Spectrum M4i/M4x series A/D and D/A cards are very extensive and give you the possibility to detect nearly any trigger event you can think of.

You can choose between more than 10 external trigger modes and up to 20 internal trigger modes (on analog acquisition cards) including software and channel trigger, depending on your type of board. Many of the channel trigger modes can be independently set for each input channel (on A/D boards only) resulting in a even bigger variety of modes. This chapter is about to explain all of the different trigger modes and setting up the card's registers for the desired mode.

Trigger Engine Overview

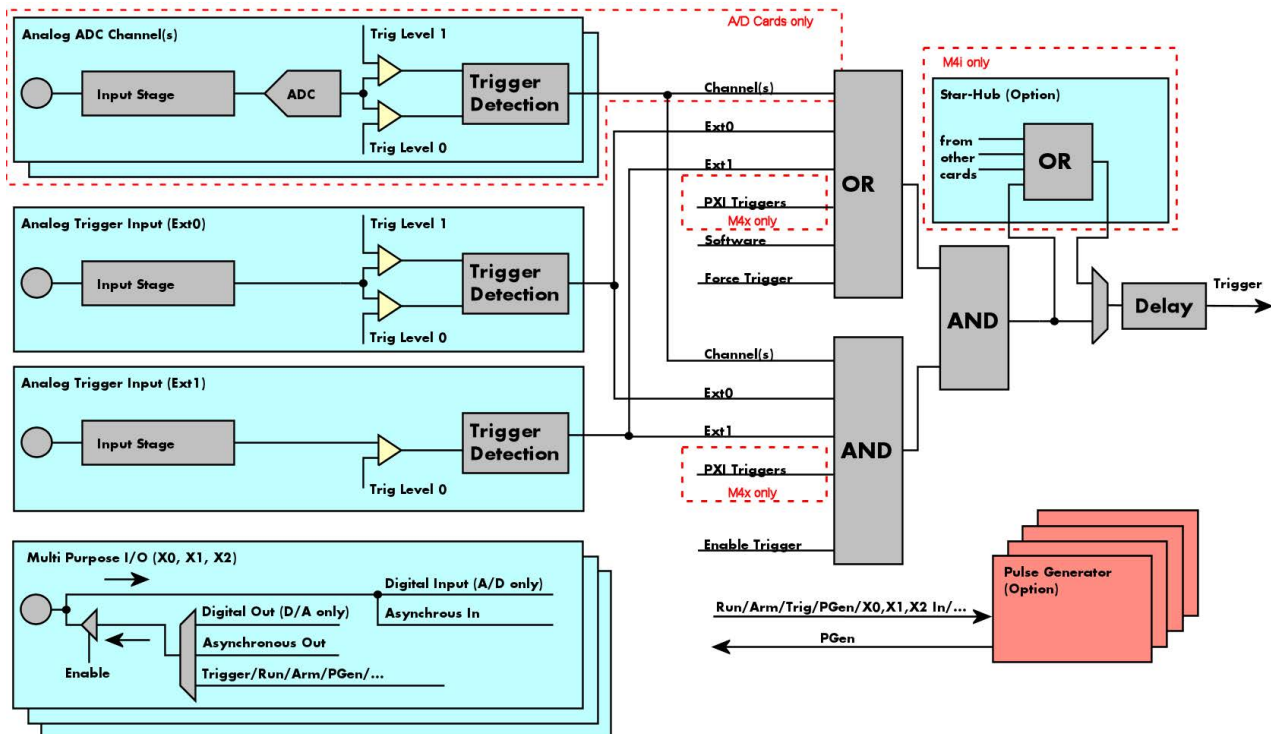


Image 51: Trigger Engine Overview. Red marked parts not available on all card types

The trigger engine of the M4i/M4x card series allows to combine several different trigger sources with OR and AND combination, with a trigger delay or even with an OR combination across several cards when using the Star-Hub option. The above drawing gives a complete overview of the trigger engine and shows all possible features that are available.

On A/D cards each analog input channel has two trigger level comparators to detect edges as well as windowed triggers. All card types have a total of two different additional external trigger sources. One main trigger source (Ext0, labelled Trg0 on front panel) which also has two analog level comparators also allowing to use edge and windowed trigger detection and one secondary analog trigger (Ext1, labelled Trg1 on front panel) with one analog level comparator. Additionally three multi purpose in/outputs that can be software programmed to either inputs or outputs some extended status signals.

The Enable trigger allows the user to enable or disable all trigger sources (including channel trigger on A/D cards and external trigger) with a single software command. The enable trigger command will not work on force trigger.

When the card is waiting for a trigger event, either a channel trigger or an external trigger the force trigger command allows to force a trigger event with a single software command. The force trigger overrides the enable trigger command.

Before the trigger event is finally generated, it is wired through a programmable trigger delay. This trigger delay will also work when used in a synchronized system thus allowing each card to individually delay its trigger recognition.

Trigger masks

Trigger OR mask

The purpose of this passage is to explain the trigger OR mask (see left figure) and all the appendant software registers in detail.

The OR mask shown in the overview before as one object, is separated into two parts: a general OR mask for main external trigger (external analog window trigger), the secondary external trigger (external analog comparator trigger, the various PXI triggers (available on M4x PXIe cards only) and software trigger and a channel OR mask.

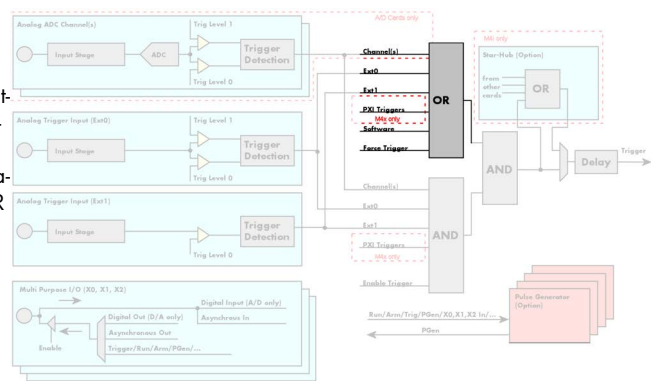


Image 52: trigger engine overview with trigger OR mask shown

Every trigger source of the M4i/M4x series cards is wired to one of the above mentioned OR masks. The user then can program which trigger source will be recognized, and which one won't.

This selection for the general mask is realized with the SPC_TRIG_ORMASK register in combination with constants for every possible trigger source.

This selection for the channel mask (A/D cards only) is realized with the SPC_TRIG_CH_ORMASK0 register in combination with constants for every possible channel trigger source.

In either case the sources are coded as a bitfield, so that they can be combined by one access to the driver with the help of a bitwise OR.

If no input is enabled, the output will be a logic "true", to not block the following static AND mask.

The table below shows the relating register for the general OR mask and the possible constants that can be written to it.

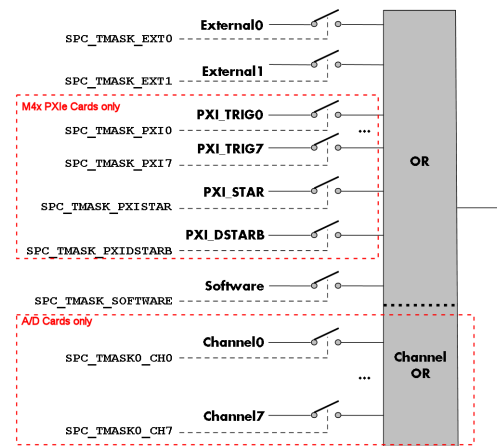


Image 53: trigger engine OR mask details

Table 68: Spectrum API: general trigger OR mask register and available settings

Register	Value	Direction	Description
SPC_TRIG_AVAILORMASK	40400	read	Bitmask, in which all bits of the below mentioned sources for the OR mask are set, if available.
SPC_TRIG_ORMASK	40410	read/write	Defines the events included within the trigger OR mask of the card.
SPC_TMASK_NONE	0		No trigger source selected
SPC_TMASK_SOFTWARE	1h		Enables the software trigger for the OR mask. The card will trigger immediately after start.
SPC_TMASK_EXT0	2h		Enables the external (analog window) trigger 0 (labelled Trg0 on front panel) for the OR mask. The card will trigger when the programmed condition for this input is valid.
SPC_TMASK_EXT1	4h		Enables the external (analog comparator) trigger 1 (labelled Trg1 on front panel) for the OR mask. The card will trigger when the programmed condition for this input is valid.
SPC_TMASK_PXI0	100000h		Enables the PXI_TRIG0 for the OR mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI1	200000h		Enables the PXI_TRIG1 for the OR mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI2	400000h		Enables the PXI_TRIG2 for the OR mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI3	800000h		Enables the PXI_TRIG3 for the OR mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI4	1000000h		Enables the PXI_TRIG4 for the OR mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI5	2000000h		Enables the PXI_TRIG5 for the OR mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI6	4000000h		Enables the PXI_TRIG6 for the OR mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI7	8000000h		Enables the PXI_TRIG7 for the OR mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI STAR	10000000h		Enables the PXI STAR line for the OR mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI DSTARB	20000000h		Enables the PXI DSTARB for the OR mask. The card will trigger when the signal on this input is HIGH.



Please note that as default the SPC_TRIG_ORMASK is set to SPC_TMASK_SOFTWARE. When not using any trigger mode requiring values in the SPC_TRIG_ORMASK register, this mask should explicitly be cleared, as otherwise the software trigger will override other modes.

The following example shows, how to setup the OR mask, for the two external trigger inputs, ORing them together. When using just a single trigger, only this particular trigger must be used in the OR mask register, respectively. As an example a simple edge detection has been

chosen for Ext1 input and a window edge detection has been chosen for Ext0 input. The explanation and a detailed description of the different trigger modes for the external trigger inputs will be shown in the dedicated passage within this chapter.

```

spcm_dwSetParam_i32 (hDrv, SPC_TRIG_EXT0_LEVEL0, 1800); // lower Window Trigger level set to 1.8 V
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_EXT0_LEVEL1, 2000); // upper Window Trigger level set to 2.0 V
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_EXT0_MODE, SPC_TM_WINENTER); // Setting up main window trigger for entering

spcm_dwSetParam_i32 (hDrv, SPC_TRIG_EXT1_LEVEL0, 2500); // Trigger level set to 2.5 V
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_EXT1_MODE, SPC_TM_POS); // Setting up secondary trigger for rising edges

// Enable both external triggers within the OR mask, hence ORing them together
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_ORMASK, SPC_TMASK_EXT1 | SPC_TMASK_EXT0);

```

The table below is showing the registers for the channel OR mask (A/D cards only) and the possible constants that can be written to it.

Table 69: Spectrum API: channel trigger OR mask registers and available settings

Register	Value	Direction	Description
SPC_TRIG_CH_AVAILORMASK0	40450	read	Bitmask, in which all bits of the below mentioned sources/channels (0...7) for the channel OR mask are set, if available.
SPC_TRIG_CH_ORMASK0	40460	read/write	Includes the analog channels (0...7) within the channel trigger OR mask of the card.
SPC_TMASK0_CH0	00000001h		Enables channel0 for recognition within the channel OR mask.
SPC_TMASK0_CH1	00000002h		Enables channel1 for recognition within the channel OR mask.
SPC_TMASK0_CH2	00000004h		Enables channel2 for recognition within the channel OR mask.
SPC_TMASK0_CH3	00000008h		Enables channel3 for recognition within the channel OR mask.

The following example shows, how to setup the OR mask for channel trigger. As an example a simple edge detection has been chosen. The explanation and a detailed description of the different trigger modes for the channel trigger modes will be shown in the dedicated passage within this chapter.

```

spcm_dwSetParam_i32 (hDrv, SPC_TRIG_ORMASK, SPC_TMASK_NONE); // disable default software trigger
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_CH_ORMASK0, SPC_TMASK_CH0); // Enable channel0 trigger within the OR mask
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_CH0_LEVEL0, 0); // Trigger level is zero crossing
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_CH0_MODE, SPC_TM_POS); // Setting up channel trigger for rising edges

```

Trigger AND mask

The purpose of this passage is to explain the trigger AND mask (see left figure) and all the additional software registers in detail.

The AND mask shown in the overview before as one object, is separated into two parts: a general AND mask for external trigger and software trigger and a channel AND mask.

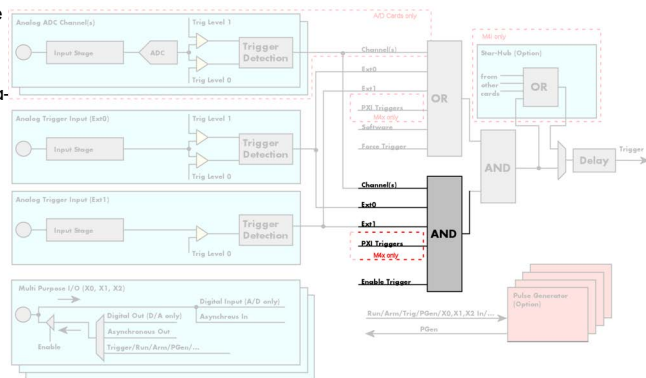


Image 54: trigger engine overview with trigger AND mask shown

Every trigger source of the M4i/M4x series cards except the software trigger is wired to one of the above mentioned AND masks. The user then can program which trigger source will be recognized, and which one won't.

This selection for the general mask is realized with the SPC_TRIG_ANDMASK register in combination with constants for every possible trigger source.

This selection for the channel mask (A/D cards only) is realized with the SPC_TRIG_CH_ANDMASK0 register in combination with constants for every possible channel trigger trigger source.

In either case the sources are coded as a bit-field, so that they can be combined by one access to the driver with the help of a bitwise OR.

If no input is enabled, the output will be a logic "true", to not block the following static AND mask.

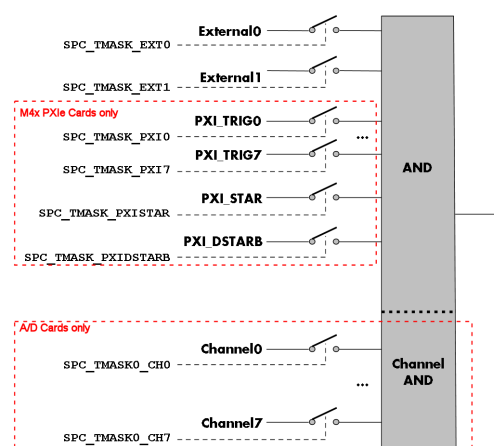


Image 55: trigger engine AND mask details

The table below shows the relating register for the general AND mask and the possible constants that can be written to it.

Table 70: Spectrum API: general trigger AND mask registers and available settings

Register	Value	Direction	Description
SPC_TRIG_AVAILANDMASK	40420	read	Bit mask, in which all bits of the below mentioned sources for the AND mask are set, if available.
SPC_TRIG_ANDMASK	40430	read/write	Defines the events included within the trigger AND mask of the card.
SPC_TMASK_NONE	0		No trigger source selected
SPC_TMASK_EXT0	2h		Enables the external (analog window) trigger 0 (labelled Trg0 on front panel) for the AND mask. The card will trigger when the programmed condition for this input is valid.
SPC_TMASK_EXT1	4h		Enables the external (analog comparator) trigger 1 (labelled Trg1 on front panel) for the AND mask. The card will trigger when the programmed condition for this input is valid.
SPC_TMASK_PXI0	100000h		Enables the PXI_TRIG0 for the AND mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI1	200000h		Enables the PXI_TRIG1 for the AND mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI2	400000h		Enables the PXI_TRIG2 for the AND mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI3	800000h		Enables the PXI_TRIG3 for the AND mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI4	1000000h		Enables the PXI_TRIG4 for the AND mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI5	2000000h		Enables the PXI_TRIG5 for the AND mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI6	4000000h		Enables the PXI_TRIG6 for the AND mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI7	8000000h		Enables the PXI_TRIG7 for the AND mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXISTAR	10000000h		Enables the PXISTAR line for the AND mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXIDSTARB	20000000h		Enables the PXI_DSTARB for the AND mask. The card will trigger when the signal on this input is HIGH.

The following example shows, how to setup the AND mask, for an external trigger. As an example a simple high level detection has been chosen. When multiple external triggers shall be combined by AND, both of the external sources must be included in the AND mask register, similar to the OR mask example shown before. The explanation and a detailed description of the different trigger modes for the external trigger inputs will be shown in the dedicated passage within this chapter.

```

spcm_dwSetParam_i32 (hDrv, SPC_TRIG_ORMASK, SPC_TMASK_NONE); // disable default software trigger
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_ANDMASK, SPC_TMASK_EXT0); // Enable external trigger within the AND mask
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_EXT0_LEVEL0, 2000); // Trigger level is 2.0 V (2000 mV)
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_EXT0_MODE, SPC_TM_HIGH); // Setting up external trigger for HIGH level

```

The table below is showing the constants for the channel AND mask (A/D cards only) and all the constants for the different channels.

Table 71: Spectrum API: channel trigger AND mask registers and available settings

Register	Value	Direction	Description
SPC_TRIG_CH_AVAILANDMASK0	40470	read	Bitmask, in which all bits of the below mentioned sources/channels (0...7) for the channel AND mask are set, if available.
SPC_TRIG_CH_ANDMASK0	40480	read/write	Includes the analog or digital channels (0...7) within the channel trigger AND mask of the card.
SPC_TMASK0_CH0	00000001h		Enables channel0 for recognition within the channel OR mask.
SPC_TMASK0_CH1	00000002h		Enables channel1 for recognition within the channel OR mask.
SPC_TMASK0_CH2	00000004h		Enables channel2 for recognition within the channel OR mask.
SPC_TMASK0_CH3	00000008h		Enables channel3 for recognition within the channel OR mask.

The following example shows, how to setup the AND mask for a channel trigger. As an example a simple level detection has been chosen. The explanation and a detailed description of the different trigger modes for the channel trigger modes will be shown in the dedicated passage within this chapter.

```

spcm_dwSetParam_i32 (hDrv, SPC_TRIG_ORMASK, SPC_TMASK_NONE); // disable default software trigger
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_CH_ANDMASK0, SPC_TMASK_CH0); // Enable channel0 trigger within AND mask
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_CH0_LEVEL0, 0); // channel level to detect is zero level
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_CH0_MODE, SPC_TM_HIGH); // Setting up ch0 trigger for HIGH levels

```

Combining multiple trigger sources by OR/AND masks

When combining multiple trigger sources with different trigger modes, it is recommended to add all trigger sources with modes generating

- “edge-events” (TM_POS, TM_NEG, TM_BOTH, etc.) to add to the OR-mask
- sources with modes generating “level-events” (TM_HIGH, TM_LOW, etc.) to add to the AND-mask

Example for setting up a trigger combination where Ch0 acts as a “Gate/Enable” signal for edges to be detected on EXT0:

```

spcm_dwSetParam_i32 (hCard, SPC_TRIG_EXT0_MODE, SPC_TM_POS); // setup EXT0 to use rising edge
spcm_dwSetParam_i32 (hCard, SPC_TRIG_CH0_MODE, SPC_TM_HIGH); // setup Ch0 to use high level

// put EXT0 into OR mask and Ch0 into AND mask
spcm_dwSetParam_i32 (hCard, SPC_TRIG_ORMASK, SPC_TMASK_EXT0); // also disables default software trigger
spcm_dwSetParam_i32 (hCard, SPC_TRIG_CH_ANDMASK0, SPC_TMASK0_CH0);

```


Example for setting up a trigger combination where EXT0 acts as a “Gate/Enable” signal for edges to be detected on either Ch0 or Ch1 or Ch2:

```
spcm_dwSetParam_i32 (hCard, SPC_TRIG_EXT0_MODE, SPC_TM_HIGH); // setup EXT0 to use high level
spcm_dwSetParam_i32 (hCard, SPC_TRIG_CH0_MODE, SPC_TM_POS); // setup Ch0 to use rising edge
spcm_dwSetParam_i32 (hCard, SPC_TRIG_CH1_MODE, SPC_TM_NEG); // setup Ch1 to use falling edge
spcm_dwSetParam_i32 (hCard, SPC_TRIG_CH2_MODE, SPC_TM_BOTH); // setup Ch2 to use both edges

spcm_dwSetParam_i32 (hDrv, SPC_TRIG_ORMASK, SPC_TMASK_NONE); // disable default software trigger

// put EXT0 into AND mask and Ch0, Ch1 and Ch2 into OR mask
spcm_dwSetParam_i32 (hCard, SPC_TRIG_CH_ORMASK0, SPC_TMASK0_CH0 | SPC_TMASK0_CH1 | SPC_TMASK0_CH2);
spcm_dwSetParam_i32 (hCard, SPC_TRIG_ANDMASK, SPC_TMASK_EXT0);
```

Software trigger

The software trigger is the easiest way of triggering any Spectrum board. The acquisition or replay of data will start immediately after the card is started and the trigger engine is armed. The resulting delay upon start includes the time the board needs for its setup and the time for recording the pre-trigger area (for acquisition cards).

For enabling the software trigger one simply has to include the software event within the trigger OR mask, as the following table is showing:



Table 72: Spectrum API: software register and register setting for software trigger

Register	Value	Direction	Description
SPC_TRIG_ORMASK	40410	read/write	Defines the events included within the trigger OR mask of the card.
SPC_TMASK_SOFTWARE	1h		Sets the trigger mode to software, so that the recording/replay starts immediately.

Example for setting up the software trigger:

```
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_ORMASK, SPC_TMASK_SOFTWARE); // Internal software trigger mode is used
```

Force- and Enable trigger

In addition to the software trigger (free run) it is also possible to force a trigger event by software while the board is waiting for a real physical trigger event. The forcetrigger command will only have any effect, when the board is waiting for a trigger event. The command for forcing a trigger event is shown in the table below.

Issuing the forcetrigger command will every time only generate one trigger event. If for example using Multiple Recording that will result in only one segment being acquired by forcetrigger. After execution of the forcetrigger command the trigger engine will fall back to the trigger mode that was originally programmed and will again wait for a trigger event.

Table 73: Spectrum API: command register and force trigger command

Register	Value	Direction	Description
SPC_M2CMD	100	write	Command register of the M2i/M3i/M4i/M4x/M2p/M5i series cards.
M2CMD_CARD_FORCETRIGGER	10h		Forces a trigger event if the hardware is still waiting for a trigger event.

The example shows, how to use the forcetrigger command:

```
spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_CARD_FORCETRIGGER); // Force trigger is used.
```

It is also possible to enable (arm) or disable (disarm) the card's whole triggerengine by software. By default the trigger engine is disabled.

Table 74: Spectrum API: command register and trigger enable/disable command

Register	Value	Direction	Description
SPC_M2CMD	100	write	Command register of the M2i/M3i/M4i/M4x/M2p/M5i series cards.
M2CMD_CARD_ENABLETRIGGER	8h		Enables the trigger engine. Any trigger event will now be recognized.
M2CMD_CARD_DISABLETRIGGER	20h		Disables the trigger engine. No trigger events will be recognized, except force trigger.

The example shows, how to arm and disarm the card's trigger engine properly:

```
spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_CARD_ENABLETRIGGER); // Trigger engine is armed.
...
spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_CARD_DISABLETRIGGER); // Trigger engine is disarmed.
```

Trigger delay

All of the Spectrum M4i/M4x series cards allow the user to program an additional trigger delay. As shown in the trigger overview section, this delay is the last element in the trigger chain. Therefore the user does not have to care for the sources when programming the trigger delay.

As shown in the overview the trigger delay is located after the star-hub connection meaning that every M4i card being synchronized can still have its own trigger delay programmed. The Star-Hub will combine the original trigger events before the result is being delayed.

The delay is programmed in samples. The resulting time delay will therefore be $\text{[Programmed Delay]} / \text{[Sampling Rate]}$.

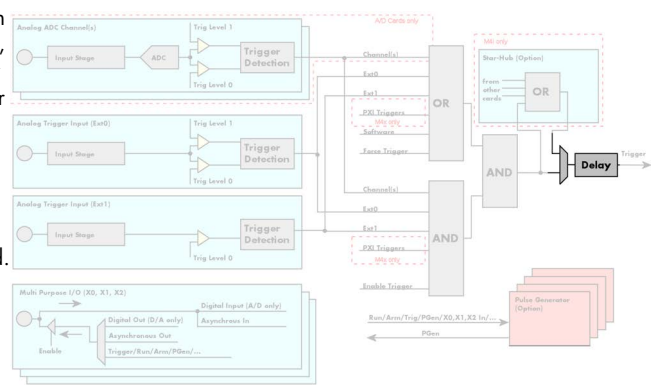


Image 56: trigger engine overview with marked trigger delay stage

The following table shows the related register and the possible values. A value of 0 disables the trigger delay.

Table 75: Spectrum API: trigger delay registers and available settings

Register	Value	Direction	Description
SPC_TRIG_AVAIDELAY	40800	read	Contains the maximum available delay as a decimal integer value.
SPC_TRIG_AVAIDELAY_STEP	40801	read	Returns the step size of the trigger delay register in sample clocks.
SPC_TRIG_DELAY	40810	read/write	Defines the delay for the detected trigger events.
0			No additional delay will be added. The resulting internal delay is mentioned in the technical data section.
16...[8Gi - 8]			Defines the additional trigger delay in number of sample clocks. The trigger delay can be programmed up to $(8\text{Gi} - 16) = 8589934576$. Step size is 16 samples for 12, 14, 16 bit cards.
32...[8Gi - 32]			Defines the additional trigger delay in number of sample clocks. The trigger delay can be programmed up to $(8\text{Gi} - 32) = 8589934560$. Step size is 32 samples for 8 bit cards.

The example shows, how to use the trigger delay command:

```
spcm_dwSetParam_i64 (hDrv, SPC_TRIG_DELAY, 1984); // A detected trigger event will be
// delayed for 1984 sample clocks.
```

Using the delay trigger does not affect the ratio between pre trigger and post trigger recorded number of samples, but only shifts the trigger event itself. For changing these values, please take a look in the relating chapter about „Acquisition Modes“.



Trigger Counter

The number of acquired trigger events is counted in hardware and can be read out while the acquisition is running or after the acquisition has finished. The trigger events are counted both in standard mode as well as in FIFO mode.

Table 76: Spectrum API: trigger counter register and register return values

Register	Value	Direction	Description
SPC_TRIGGERCOUNTER	200905	read	Returns the number of trigger events that has been acquired since the acquisition start. The internal trigger counter has 48 bits. It is therefore necessary to read out the trigger counter value with 64 bit access or 2 x 32 bit access if the number of trigger events exceed the 32 bit range.

The trigger counter feature needs at least driver version V2.17 and firmware version V20 (M2i series), V10 (M3i series), V6 (M4i/M4x series) or V1 (M2p and M5i series). Please update the driver and the card firmware to these versions to use this feature. Trying to use this feature without the proper firmware version will issue a driver error.



On M2i and M3i cards, using the trigger counter information allows to determine how many Multiple Recording segments have been acquired and can perform a memory flush by issuing Force trigger commands to read out all data. This is helpful if the number of trigger events is not known at the start of the acquisition. In that case one will do the following steps:



- Program the maximum number of segments that one expects or use the FIFO mode with unlimited segments
- Set a timeout to be sure that there are no more trigger events acquired. Alternatively one can manually proceed as soon as it is clear from the application that all trigger events have been acquired
- Read out the number of acquired trigger segments
- Issue a number of Force Trigger commands to fill the complete memory (standard mode) or to transfer the last FIFO block that contains valid data segments
- Use the trigger counter value to split the acquired data into valid data with a real trigger event and invalid data with a force trigger event.

Main external window trigger (Ext0/Trg0)

The M4i/M4x series has one main external trigger input consisting of an input stage with programmable termination and programmable AC/DC coupling and two comparators that can be programmed in the range of +/- 10000 mV. Using two comparators offers a wide range of different trigger modes that are support like edge, level, re-arm and window trigger.

The main external analog trigger can be easily combined with channel trigger or with the secondary external trigger being programmed as an additional external trigger input. The programming of the masks is shown in the chapters above.

The external trigger Ext0 is labelled Trg0 on the front-panel

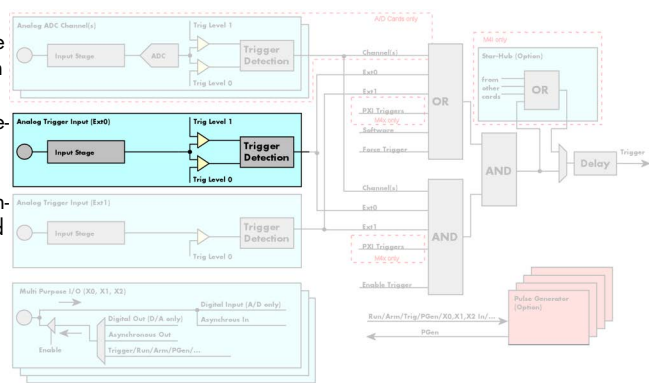


Image 57: trigger engine overview with marked main external trigger Ext0/Trg0

Trigger Mode

Please find the main external (analog) trigger input modes below. A detailed description of the modes follows in the next chapters..

Table 77: Spectrum API: external trigger Ext0 registers and register settings

Register	Value	Direction	Description
SPC_TRIG_EXT0_AVAILMODES	40500	read	Bitmask showing all available trigger modes for external 0 (Ext0) = main analog trigger input
SPC_TRIG_EXT0_MODE	40510	read/write	Defines the external trigger mode for the external SMA connector trigger input. The trigger need to be added to either OR or AND mask input to be activated.
SPC_TM_NONE	00000000h		Channel is not used for trigger detection. This is as with the trigger masks another possibility for disabling channels.
SPC_TM_POS	00000001h		Trigger detection for positive edges (crossing level 0 from below to above)
SPC_TM_NEG	00000002h		Trigger detection for negative edges (crossing level 0 from above to below)
SPC_TM_POS SPC_TM_REARM	01000001h		Trigger detection for positive edges on level 0. Trigger is armed when crossing level 1 to avoid false trigger on noise
SPC_TM_NEG SPC_TM_REARM	01000002h		Trigger detection for negative edges on level 1. Trigger is armed when crossing level 0 to avoid false trigger on noise
SPC_TM_BOTH	00000004h		Trigger detection for positive and negative edges (any crossing of level 0)
SPC_TM_HIGH	00000008h		Trigger detection for HIGH levels (signal above level 0)
SPC_TM_LOW	00000010h		Trigger detection for LOW levels (signal below level 0)
SPC_TM_WINENTER	00000020h		Window trigger for entering area between level 0 and level 1
SPC_TM_WINLEAVE	00000040h		Window trigger for leaving area between level 0 and level 1
SPC_TM_INWIN	00000080h		Window trigger for signal inside window between level 0 and level 1
SPC_TM_OUTSIDEWIN	00000100h		Window trigger for signal outside window between level 0 and level 1

For all external edge and level trigger modes, the OR mask must contain the corresponding input, as the following table shows:

Table 78: Spectrum API: external trigger Ext0 OR mask settings

Register	Value	Direction	Description
SPC_TRIG_ORMASK	40410	read/write	Defines the OR mask for the different trigger sources.
SPC_TMASK_EXT0	2h		Enable main external trigger input for the OR mask

Trigger Input Termination

The external trigger input is a high impedance input with 1kOhm termination against GND. It is possible to program a 50 Ohm termination by software to terminate fast trigger signals correctly. If you enable the termination, please make sure, that your trigger source is capable to deliver the needed current. Please check carefully whether the source is able to fulfil the trigger input specification given in the technical data section.

Table 79: Spectrum API: external trigger Ext0 input termination

Register	Value	Direction	Description
SPC_TRIG_TERM	40110	read/write	A „1“ sets the 50 Ohm termination for external trigger signals. A „0“ sets the high impedance termination

Please note that the signal levels will drop by 50% if using the 50 ohm termination and your source also has 50 ohm output impedance (both terminators will then work as a 1:2 divider). In that case it will be necessary to reprogram the trigger levels to match the new signal levels. In case of problems receiving a trigger please check the signal level of your source while connected to the terminated input.

Trigger Input Coupling

The external trigger input can be switched by software between AC and DC coupling. Please see the technical data section for details on the AC bandwidth.

Table 80: Spectrum API: external trigger Ext0 input coupling

Register	Value	Direction	Description
SPC_TRIG_EXT0_ACDC	40120	read/write	COUPLING_DC enables DC coupling, COUPLING_AC enables AC coupling for the external trigger input (AC coupling is the default).

Secondary external level trigger (Ext1/Trg1)

The M4i/M4x series has one secondary external trigger input consisting of an input stage with fixed 10 kOhm termination and one comparator that can be programmed in the range of +/- 10000 mV. Using one comparators offers a wide range of different logic levels for the available trigger modes that are support like edge, level.

The secondary external analog trigger can be easily combined with channel trigger or with the main external trigger being programmed as an additional external trigger input. The programming of the masks is shown in the chapters above.

The secondary trigger input Ext1 is labelled Trg1 on the front-panel.

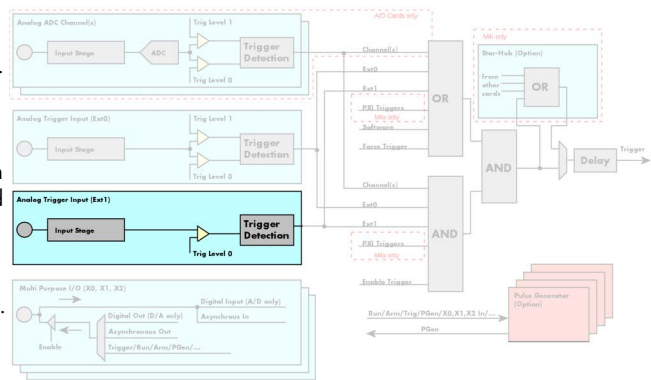


Image 58: trigger engine overview with external trigger Ext1 marked

Trigger Mode

Please find the main external (analog) trigger input modes below. A detailed description of the modes follows in the next chapters..

Table 81: Spectrum API: external trigger Ext1 registers and register settings

Register	Value	Direction	Description
SPC_TRIG_EXT1_AVAILMODES	40501	read	Bit mask showing all available trigger modes for Ext1 (Trg1) = secondary analog trigger input
SPC_TRIG_EXT1_MODE	40511	read/write	Defines the external trigger mode for the external MMCX connector trigger input. The trigger need to be added to either OR or AND mask input to be activated.
SPC_TM_NONE	00000000h		Channel is not used for trigger detection. This is as with the trigger masks another possibility for disabling channels.
SPC_TM_POS	00000001h		Trigger detection for positive edges (crossing level 0 from below to above)
SPC_TM_NEG	00000002h		Trigger detection for negative edges (crossing level 0 from above to below)
SPC_TM_BOTH	00000004h		Trigger detection for positive and negative edges (any crossing of level 0)
SPC_TM_HIGH	00000008h		Trigger detection for HIGH levels (signal above level 0)
SPC_TM_LOW	00000010h		Trigger detection for LOW levels (signal below level 0)

For all external edge and level trigger modes, the OR mask must contain the corresponding input, as the following table shows:

Table 82: Spectrum API: external trigger Ext1 OR mask settings

Register	Value	Direction	Description
SPC_TRIG_ORMASK	40410	read/write	Defines the OR mask for the different trigger sources.
SPC_TMASK_EXT1	4h		Enable secondary external trigger input for the OR mask

Trigger level

All of the external (analog) trigger modes listed above require at least one trigger level to be set (except SPC_TM_NONE of course). Some like the window or the re-arm triggers require even two levels (upper and lower level) to be set. The meaning of the trigger levels is depending on the selected mode and can be found in the detailed trigger mode description that follows.

Trigger levels for the external (analog) trigger to be programmed in mV:

Table 83: Spectrum API: external trigger available settings for trigger levels

Register	Value	Direction	Description	Range
SPC_TRIG_EXT_AVAIL0_MIN	42340	read	returns the minimum trigger level for Ext0 to be programmed in mV	
SPC_TRIG_EXT_AVAIL0_MAX	42341	read	returns the maximum trigger level for Ext0 to be programmed in mV	
SPC_TRIG_EXT_AVAIL0_STEP	42342	read	returns the step size of trigger level for Ext0 to be programmed in mV	
SPC_TRIG_EXT_AVAIL1_MIN	42345	read	returns the minimum trigger level for Ext1 to be programmed in mV	
SPC_TRIG_EXT_AVAIL1_MAX	42346	read	returns the maximum trigger level for Ext1 to be programmed in mV	
SPC_TRIG_EXT_AVAIL1_STEP	42347	read	returns the step size of trigger level for Ext1 to be programmed in mV	
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Trigger level 0 for external trigger Ext0	-10000 mV to +10000 mV

Table 83: Spectrum API: external trigger available settings for trigger levels

Register	Value	Direction	Description	Range
SPC_TRIG_EXT0_LEVEL1	42330	read/write	Trigger level 1 for external trigger Ext0	-10000 mV to +10000 mV
SPC_TRIG_EXT1_LEVEL0	42321	read/write	Trigger level 0 for external trigger Ext1	-10000 mV to +10000 mV

Detailed description of the external analog trigger modes

For all external analog trigger modes shown below, either the OR mask or the AND must contain the external trigger to activate the external input as trigger source:.

Table 84: Spectrum API: external trigger OR mask and AND mask register and settings

Register	Value	Direction	Description
SPC_TRIG_ORMASK	40410	read/write	Defines the events included within the trigger OR mask of the card.
SPC_TRIG_ANDMASK	40430	read/write	Defines the events included within the trigger AND mask of the card.
SPC_TMASK_EXT0	2h		Enables the main external (analog) trigger 0 (labelled Trg0 on front panel) for the mask.
SPC_TMASK_EXT1	4h		Enables the secondary external (analog) trigger 1 (labelled Trg1 on front panel) for the mask.

The following pages explain the available modes in detail. All modes that only require one single trigger level are available for both external trigger inputs. All modes that require two trigger levels are only available for the main external trigger input Ext0 (Trg0).

Trigger on positive edge

The trigger input is continuously sampled with the selected sample rate. If the programmed trigger level is crossed by the trigger signal from lower values to higher values (rising edge) then the trigger event will be detected.

This edge triggered external trigger mode correspond to the trigger possibilities of usual oscilloscopes.

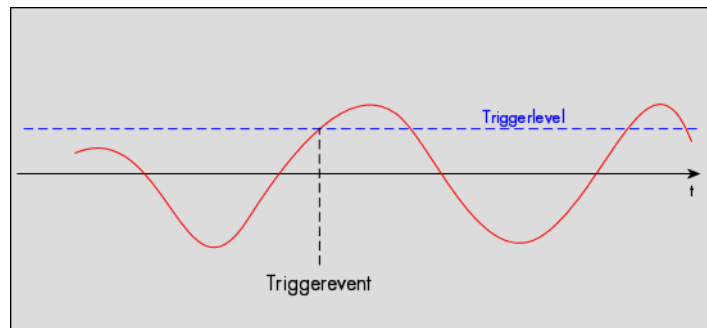


Table 85: Spectrum API: external register mode setup for trigger on positive edge

Register	Value	Direction	set to	Value
SPC_TRIG_EXT0_MODE	40510	read/write	SPC_TM_POS	1h
SPC_TRIG_EXT1_MODE	40511	read/write	SPC_TM_POS	1h
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Set it to the desired trigger level in mV	mV

Trigger on negative edge

The trigger input is continuously sampled with the selected sample rate. If the programmed trigger level is crossed by the trigger signal from higher values to lower values (falling edge) then the trigger event will be detected.

This edge triggered external trigger mode correspond to the trigger possibilities of usual oscilloscopes.

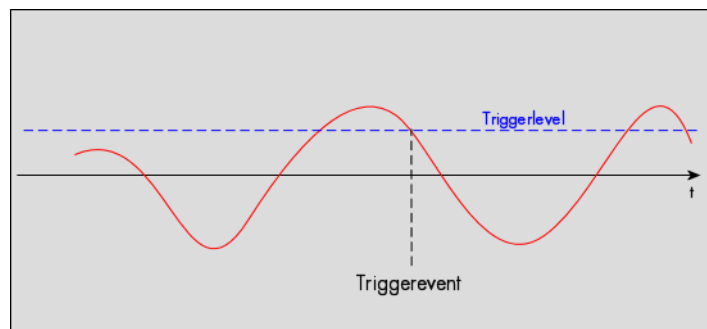


Table 86: Spectrum API: external register mode setup for trigger on negative edge

Register	Value	Direction	set to	Value
SPC_TRIG_EXT0_MODE	40510	read/write	SPC_TM_NEG	2h
SPC_TRIG_EXT1_MODE	40511	read/write	SPC_TM_NEG	2h
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Set it to the desired trigger level in mV	mV

Trigger on positive and negative edge

The trigger input is continuously sampled with the selected sample rate. If the programmed trigger level is crossed by the trigger signal (either rising or falling edge) the trigger event will be detected.

This edge triggered external trigger mode correspond to the trigger possibilities of usual oscilloscopes.

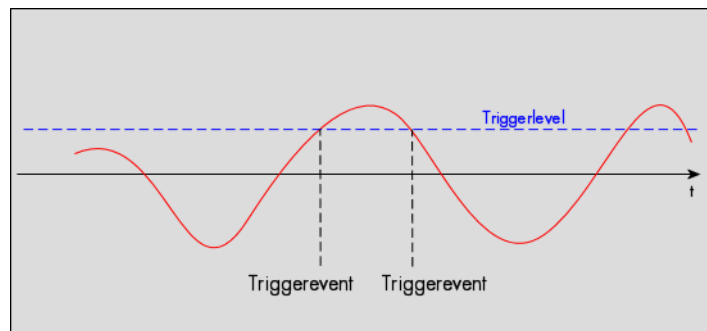


Table 87: Spectrum API: external trigger register mode setup for trigger on positive and negative edge

Register	Value	Direction	set to	Value
SPC_TRIG_EXT0_MODE	40510	read/write	SPC_TM_BOTH	4h
SPC_TRIG_EXT1_MODE	40511	read/write	SPC_TM_BOTH	4h
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Set it to the desired trigger level in mV	mV

Re-arm trigger on positive edge

The trigger input is continuously sampled with the selected sample rate. If the programmed re-arm level is crossed from lower to higher values, the trigger engine is armed and waiting for trigger. If the programmed trigger level is crossed by the trigger signal from lower values to higher values (rising edge) then the trigger event will be detected and the trigger engine will be disarmed. A new trigger event is only detected if the trigger engine is armed again.

The re-arm trigger modes can be used to prevent the board from triggering on wrong edges in noisy signals.

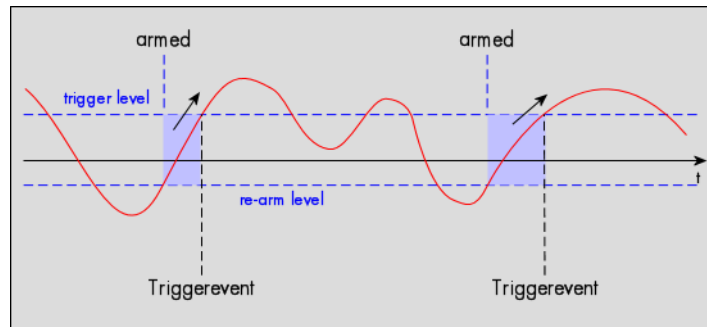


Table 88: Spectrum API: external trigger register mode setup for trigger re-arm on positive edge

Register	Value	Direction	set to	Value
SPC_TRIG_EXT0_MODE	40510	read/write	SPC_TM_POS SPC_TM_REARM	01000001h
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Set it to the desired trigger level in mV	mV
SPC_TRIG_EXT0_LEVEL1	42330	read/write	Defines the re-arm level in mV	mV

Re-arm trigger on negative edge

The trigger input is continuously sampled with the selected sample rate. If the programmed re-arm level is crossed from higher to lower values, the trigger engine is armed and waiting for trigger. If the programmed trigger level is crossed by the trigger signal from higher values to lower values (falling edge) then the trigger event will be detected and the trigger engine will be disarmed. A new trigger event is only detected, if the trigger engine is armed again.

The re-arm trigger modes can be used to prevent the board from triggering on wrong edges in noisy signals.

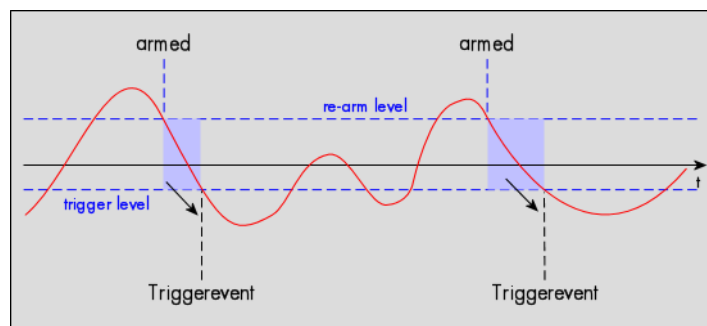


Table 89: Spectrum API: external trigger register mode setup for trigger re-arm on negative edge

Register	Value	Direction	set to	Value
SPC_TRIG_EXT0_MODE	40510	read/write	SPC_TM_NEG SPC_TM_REARM	01000002h
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Defines the re-arm level in mV	mV
SPC_TRIG_EXT0_LEVEL1	42330	read/write	Set it to the desired trigger level in mV	mV

Window trigger for entering signals

The trigger input is continuously sampled with the selected sample rate. The upper and the lower level define a window. Every time the signal enters the window from the outside, a trigger event will be detected.

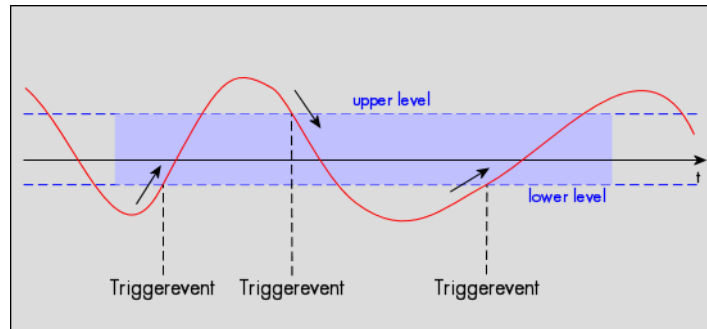


Table 90: Spectrum API: external trigger register mode setup for window trigger for entering signals

Register	Value	Direction	set to	Value
SPC_TRIG_EXT0_MODE	40510	read/write	SPC_TM_WINENTER	00000020h
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Set it to the upper trigger level in mV	mV
SPC_TRIG_EXT0_LEVEL1	42330	read/write	Set it to the lower trigger level in mV	mV

Window trigger for leaving signals

The trigger input is continuously sampled with the selected sample rate. The upper and the lower level define a window. Every time the signal leaves the window from the inside, a trigger event will be detected.

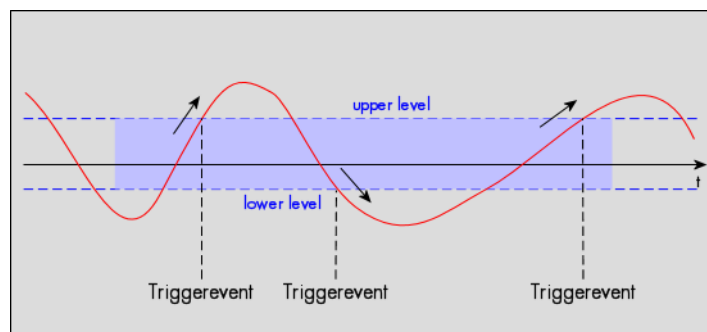


Table 91: Spectrum API: external trigger register mode setup for window trigger for leaving signals

Register	Value	Direction	set to	Value
SPC_TRIG_EXT0_MODE	40510	read/write	SPC_TM_WINLEAVE	00000040h
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Set it to the upper trigger level in mV	mV
SPC_TRIG_EXT0_LEVEL1	42330	read/write	Set it to the lower trigger level in mV	mV

High level trigger

This trigger mode will generate an internal gate signal that can be useful in conjunction with a second trigger mode to gate that second trigger. If using this mode as a single trigger source the card will detect a trigger event at the time when entering the high level (acting like positive edge trigger) or if the trigger signal is already above the programmed level at the start it will immediately detect a trigger event.

The trigger input is continuously sampled with the selected sample rate. The trigger event will be detected if the trigger input is above the programmed trigger level.

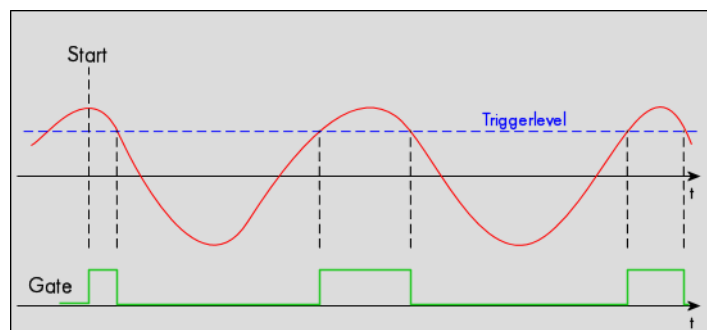


Table 92: Spectrum API: external trigger register mode setup for high level trigger

Register	Value	Direction	set to	Value
SPC_TRIG_EXT0_MODE	40510	read/write	SPC_TM_HIGH	00000008h
SPC_TRIG_EXT1_MODE	40511	read/write	SPC_TM_HIGH	00000008h
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Set it to the upper trigger level in mV	mV

Low level trigger

This trigger mode will generate an internal gate signal that can be useful in conjunction with a second trigger mode to gate that second trigger. If using this mode as a single trigger source the card will detect a trigger event at the time when entering the low level (acting like negative edge trigger) or if the trigger signal is already above the programmed level at the start it will immediately detect a trigger event.

The trigger input is continuously sampled with the selected sample rate. The trigger event will be detected if the trigger input is below the programmed trigger level.

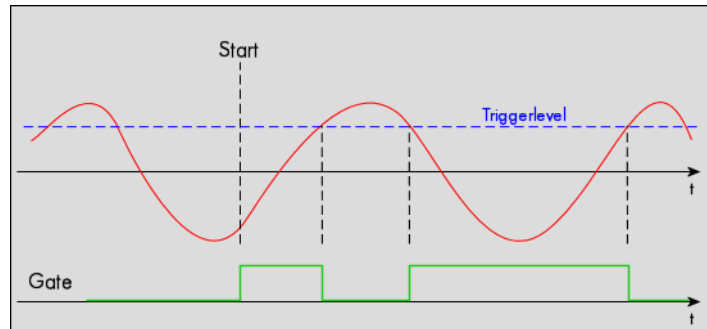


Table 93: Spectrum API: external trigger register mode setup for low level trigger

Register	Value	Direction	set to	Value
SPC_TRIG_EXT0_MODE	40510	read/write	SPC_TM_LOW	00000010h
SPC_TRIG_EXT1_MODE	40511	read/write	SPC_TM_LOW	00000010h
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Set it to the upper trigger level in mV	mV

In window trigger

This trigger mode will generate an internal gate signal that can be useful in conjunction with a second trigger mode to gate that second trigger. If using this mode as a single trigger source the card will detect a trigger event at the time when entering the window defined by the two trigger levels (acting like window enter trigger) or if the trigger signal is already inside the programmed window at the start it will immediately detect a trigger event.

The trigger input is continuously sampled with the selected sample rate. The trigger event will be detected if the trigger input is inside the programmed trigger window.

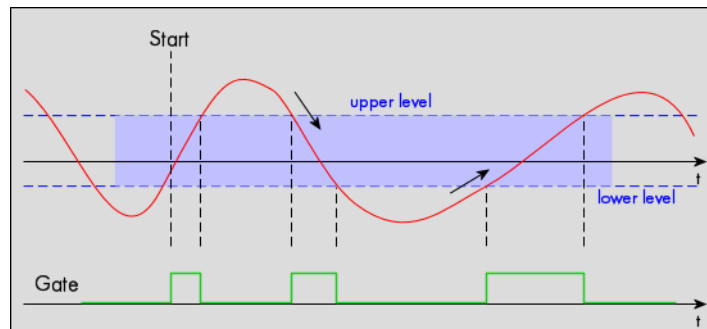


Table 94: Spectrum API: external trigger register mode setup for in window trigger

Register	Value	Direction	set to	Value
SPC_TRIG_EXT0_MODE	40510	read/write	SPC_TM_INWIN	00000080h
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Set it to the upper trigger level in mV	mV
SPC_TRIG_EXT0_LEVEL1	42330	read/write	Set it to the lower trigger level in mV	mV

Outside window trigger

This trigger mode will generate an internal gate signal that can be useful in conjunction with a second trigger mode to gate that second trigger. If using this mode as a single trigger source the card will detect a trigger event at the time when leaving the window defined by the two trigger levels (acting like leaving window trigger) or if the trigger signal is already outside the programmed window at the start it will immediately detect a trigger event.

The trigger input is continuously sampled with the selected sample rate. The trigger event will be detected if the trigger input is outside the programmed trigger window.

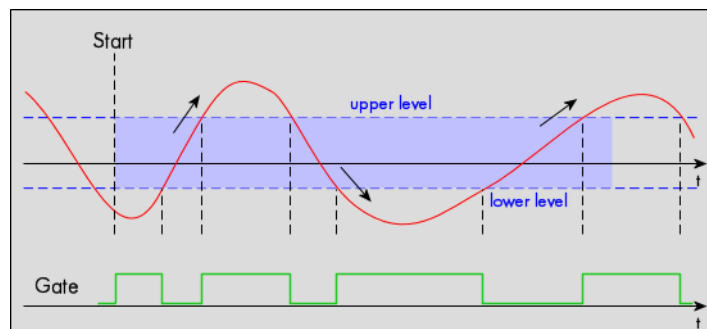


Table 95: Spectrum API: external trigger register mode setup for outside window trigger

Register	Value	Direction	set to	Value
SPC_TRIG_EXT0_MODE	40510	read/write	SPC_TM_OUTSIDEWIN	00000100h
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Set it to the upper trigger level in mV	mV
SPC_TRIG_EXT0_LEVEL1	42330	read/write	Set it to the lower trigger level in mV	mV

Channel Trigger

Overview of the channel trigger registers

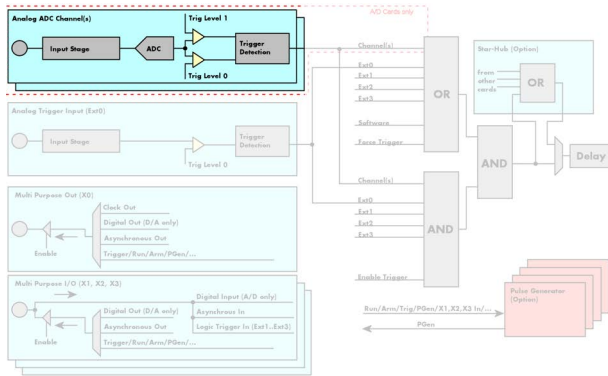


Image 59: trigger engine overview with channel trigger section marked

The channel trigger modes are the most common modes, compared to external equipment like oscilloscopes. The huge variety of different channel trigger modes enables you to observe nearly any part of the analog signal. This chapter is about to explain the different modes in detail. To enable the channel trigger, you have to set the channel triggermode register accordingly. Therefore you have to choose, if you either want only one channel to be the trigger source, or if you want to combine two or more channels to a logical OR or a logical AND trigger.

For all channel trigger modes, the OR mask must contain the corresponding input channels (channel 0 taken as example here):

Table 96: Spectrum API: channel trigger OR mask register

Register	Value	Direction	Description
SPC_TRIG_CH_ORMASK0	40460	read/write	Defines the OR mask for the channel trigger sources.
SPC_TMASK0_CH0	1h		Enables channel0 input for the channel OR mask

The following table shows the according registers for the two general channel trigger modes. It lists the maximum of the available channel mode registers for your card's series. So it can be that you have less channels installed on your specific card and therefore have less valid channel mode registers. If you try to set a channel that is not installed on your specific card, an error message will be returned.

Table 97: Spectrum API: channel trigger mode registers and available mode settings

Register	Value	Direction	Description
SPC_TRIG_CH_AVAILMODES	40600	read	Bitmask, in which all bits of the below mentioned modes for the channel trigger are set, if available.
SPC_TRIG_CH0_MODE	40610	read/write	Sets the trigger mode for channel 0. Channel 0 must be enabled in the channel OR/AND mask.
SPC_TRIG_CH1_MODE	40611	read/write	Sets the trigger mode for channel 1. Channel 1 must be enabled in the channel OR/AND mask.
SPC_TRIG_CH2_MODE	40612	read/write	Sets the trigger mode for channel 2. Channel 2 must be enabled in the channel OR/AND mask.
SPC_TRIG_CH3_MODE	40613	read/write	Sets the trigger mode for channel 3. Channel 3 must be enabled in the channel OR/AND mask.
SPC_TM_NONE	0000000h		Channel is not used for trigger detection. This is as with the trigger masks another possibility for disabling channels.
SPC_TM_POS	00000001h		Enables the trigger detection for positive edges
SPC_TM_NEG	00000002h		Enables the trigger detection for negative edges
SPC_TM_BOTH	00000004h		Enables the trigger detection for positive and negative edges
SPC_TM_POS SPC_TM_REARM	01000001h		Trigger detection for positive edges on level 0. Trigger is armed when crossing level 1 to avoid false trigger on noise
SPC_TM_NEG SPC_TM_REARM	01000002h		Trigger detection for negative edges on level 1. Trigger is armed when crossing level 0 to avoid false trigger on noise
SPC_TM_LOW	00000010h		Enables the trigger detection for LOW levels
SPC_TM_HIGH	00000008h		Enables the trigger detection for HIGH levels
SPC_TM_WINENTER	00000020h		Enables the window trigger for entering signals
SPC_TM_WINLEAVE	00000040h		Enables the window trigger for leaving signals
SPC_TM_INWIN	00000080h		Enables the window trigger for inner signals
SPC_TM_OUTSIDEWIN	00000100h		Enables the window trigger for outer signals
SPC_TM_POS SPC_TM_HYSTERESIS	20000001h		Enables the trigger detection for positive edges with hysteresis
SPC_TM_NEG SPC_TM_HYSTERESIS	20000002h		Enables the trigger detection for negative edges with hysteresis
SPC_TM_POS SPC_TM_REARM SPC_TM_HYSTERESIS	21000001h		Trigger detection for positive edges with hysteresis on level 0. Trigger is armed when crossing level 1 to avoid false trigger on noise
SPC_TM_NEG SPC_TM_REARM SPC_TM_HYSTERESIS	21000002h		Trigger detection for negative edges with hysteresis on level 1. Trigger is armed when crossing level 0 to avoid false trigger on noise
SPC_TM_LOW SPC_TM_HYSTERESIS	20000010h		Enables the trigger detection for LOW levels with hysteresis
SPC_TM_HIGH SPC_TM_HYSTERESIS	20000008h		Enables the trigger detection for HIGH levels with hysteresis

If you want to set up a two channel board to detect only a positive edge on channel 0, you would have to setup the board like the following example. Both of the examples either for the single trigger source and the OR trigger mode do not include the necessary settings for the trigger levels. These settings are detailed described in the following paragraphs.

```

spcm_dwSetParam_i32 (hDrv, SPC_TRIG_ORMASK, SPC_TMASK_NONE); // disable software trigger
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_CH_ORMASK0, SPC_TMASK0_CH0); // Enable channel 0 in the OR mask
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_CH0_MODE, SPC_TM_POS ); // Set triggermode of Ch 0 to positive edge

```

If you want to set up a two channel board to detect a trigger event on either a positive edge on channel 0 or a negative edge on channel 1 you would have to set up your board as the following example shows.

```
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_ORMASK, SPC_TMASK_NONE); // disable software trigger
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_CH_ORMASK0, SPC_TMASK0_CH0 | SPC_TMASK0_CH1); // Enable Ch 0 & Ch 1
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_CH0_MODE, SPC_TM_POS ); // Set triggermode of Ch 0 to positive edge
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_CH1_MODE, SPC_TM_NEG ); // Set triggermode of Ch 1 to negative edge
```

Channel trigger level

All of the channel trigger modes listed above require at least one trigger level to be set (except SPC_TM_NONE of course). Some modes like the window triggers require even two levels (upper and lower level) to be set.

After the data has been sampled, the upper N data bits are compared with the N bits of the trigger levels. The following table shows the level registers and the possible values they can be set to for your specific card.

As the trigger levels are compared to the digitized data, the trigger levels depend on the channels input range. For every input range available to your board there is a corresponding range of trigger levels. On the different input ranges the possible stepsize for the trigger levels differs as well as the maximum and minimum values. The table further below gives you the absolute trigger levels for your specific card series.

7 bit resolution for the trigger levels:

Register	Value	Direction	Description	Range
SPC_TRIG_CH0_LEVEL0	42200	read/write	Trigger level 0 channel 0: main trigger level / upper level if 2 levels used	-63 to +63
SPC_TRIG_CH1_LEVEL0	42201	read/write	Trigger level 0 channel 1: main trigger level / upper level if 2 levels used	-63 to +63
SPC_TRIG_CH2_LEVEL0	42202	read/write	Trigger level 0 channel 2: main trigger level / upper level if 2 levels used	-63 to +63
SPC_TRIG_CH3_LEVEL0	42203	read/write	Trigger level 0 channel 3: main trigger level / upper level if 2 levels used	-63 to +63
SPC_TRIG_CH0_LEVEL1	42300	read/write	Trigger level 1 channel 0: auxiliary trigger level / lower level if 2 levels used	-63 to +63
SPC_TRIG_CH1_LEVEL1	42301	read/write	Trigger level 1 channel 1: auxiliary trigger level / lower level if 2 levels used	-63 to +63
SPC_TRIG_CH2_LEVEL1	42302	read/write	Trigger level 1 channel 2: auxiliary trigger level / lower level if 2 levels used	-63 to +63
SPC_TRIG_CH3_LEVEL1	42303	read/write	Trigger level 1 channel 3: auxiliary trigger level / lower level if 2 levels used	-63 to +63

Trigger level representation depending on selected input range

Triggerlevel	Input ranges			
	±200 mV	±500 mV	±1 V	±2.5 V
63	196.9 mV	492.2 mV	984.4 mV	+2460.9 mV
62	193.8 mV	484.4 mV	968.8 mV	+2421.9 mV
...				
32	100.0 mV	250.0 mV	500.0 mV	+1250.0 mV
...				
2	6.3 mV	15.6 mV	31.3 mV	+78.1 mV
1	3.1 mV	7.8 mV	15.6 mV	+39.1 mV
0	0.0 mV	0.0 mV	0.0 mV	0 V
-1	-3.1 mV	-7.8 mV	-15.6 mV	-39.1 mV
-2	-6.3 mV	-15.6 mV	-31.3 mV	-78.1 mV
...				
-32	-100.0 mV	-250.0 mV	-500.0 mV	-1250.0 mV
...				
-62	-193.8 mV	-484.4 mV	-968.8 mV	-2421.9 mV
-63	-196.9 mV	-492.2 mV	-984.4 mV	-2460.9 mV
Step size	3.1 mV	7.8 mV	15.6 mV	39.1 mV

The following example shows, how to set up a one channel board to trigger on channel 0 with rising edge. It is assumed, that the input range of channel 0 is set to the the ±200 mV range. The decimal value for SPC_TRIG_CH0_LEVEL0 corresponds then with 150 mV, which is the resulting trigger level.

```
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_ORMASK, SPC_TMASK_NONE); // disable default software trigger
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_CH0_MODE, SPC_TM_POS); // Setting up channel trig (rising edge)
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_CH0_LEVEL0, 48); // Sets triggerlevel to 150 mV
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_CH_ORMASK0, SPC_TMASK0_CH0); // and enable it within the OR mask
```

Reading out the number of possible trigger levels

The Spectrum driver also contains a register that holds the value of the maximum possible different trigger levels considering the above mentioned exclusion of the most negative possible value. This is useful, as new drivers can also be used with older hardware versions, because you can check the trigger resolution during run time. The register is shown in the following table:

Table 98: Spectrum API: trigger level count register

Register	Value	Direction	Description
SPC_READTRIGLVLCOUNT	2500	r	Contains the number of different possible trigger levels meaning $\pm$ of the value.

In case of a board that uses 8 bits for trigger detection the returned value would be 127, as either the zero and 127 positive and negative values are possible. The resulting trigger step width in mV can easily be calculated from the returned value. It is assumed that you know the actually selected input range.

$$\text{Trigger step width} = \frac{\text{Input Range}_{\max}}{\text{Number of trigger levels} + 1}$$

To give you an example on how to use this formula we assume, that the ± 1.0 V input range is selected and the board uses 8 bits for trigger detection. The result would be 7.81 mV, which is the step width for your type of board within the actually chosen input range.

$$\text{Trigger step width} = \frac{+1000 \text{ mV}}{127 + 1}$$

Detailed description of the channel trigger modes

For all channel trigger modes, the OR mask must contain the corresponding input channels (channel 0 taken as example here):

Table 99: Spectrum API: channel trigger OR mask register

Register	Value	Direction	Description
SPC_TRIG_CH_ORMASK0	40460	read/write	Defines the OR mask for the channel trigger sources.
SPC_TMASK0_CH0	1h		Enables channel0 input for the channel OR mask

Channel trigger on positive edge

The analog input is continuously sampled with the selected sample rate. If the programmed trigger level is crossed by the channel's signal from lower values to higher values (rising edge) then the trigger event will be detected.

These edge triggered channel trigger modes correspond to the trigger possibilities of usual oscilloscopes.

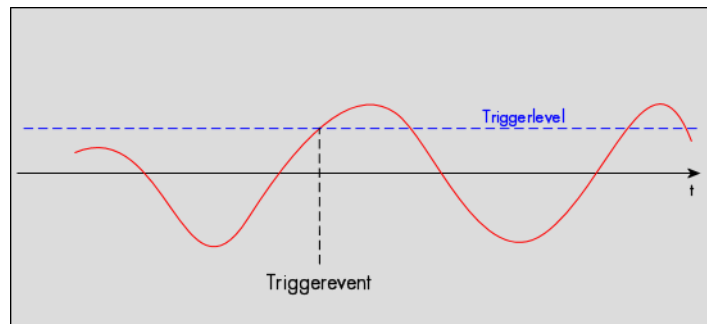


Table 100: Spectrum API: channel trigger register settings for positive edge trigger

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_POS	1h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the desired trigger level relatively to the channel's input range.	board dependent

Channel trigger on negative edge

The analog input is continuously sampled with the selected sample rate. If the programmed trigger level is crossed by the channel's signal from higher values to lower values (falling edge) then the trigger event will be detected.

These edge triggered channel trigger modes correspond to the trigger possibilities of usual oscilloscopes.

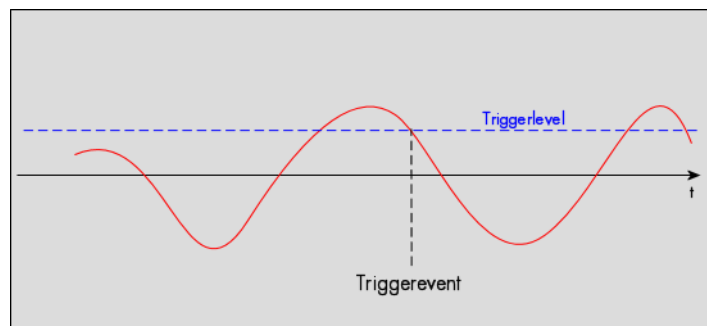


Table 101: Spectrum API: channel trigger register settings for negative edge trigger

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_NEG	2h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the desired trigger level relatively to the channel's input range.	board dependent

Channel trigger on positive and negative edge

The analog input is continuously sampled with the selected sample rate. If the programmed trigger level is crossed by the channel's signal (either rising or falling edge) the trigger event will be detected.

These edge triggered channel trigger modes correspond to the trigger possibilities of usual oscilloscopes.

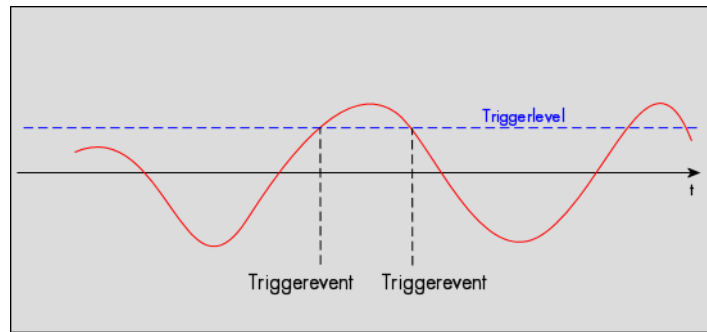


Table 102: Spectrum API: channel trigger register settings for positive and negative edge trigger

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_BOTH	4h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the desired trigger level relatively to the channel's input range.	board dependent

Channel re-arm trigger on positive edge

The analog input is continuously sampled with the selected sample rate. If the programmed re-arm level is crossed from lower to higher values, the trigger engine is armed and waiting for trigger. If the programmed trigger level is crossed by the channel's signal from lower values to higher values (rising edge) then the trigger event will be detected and the trigger engine will be disarmed. A new trigger event is only detected if the trigger engine is armed again.

The re-arm trigger modes can be used to prevent the board from triggering on wrong edges in noisy signals.

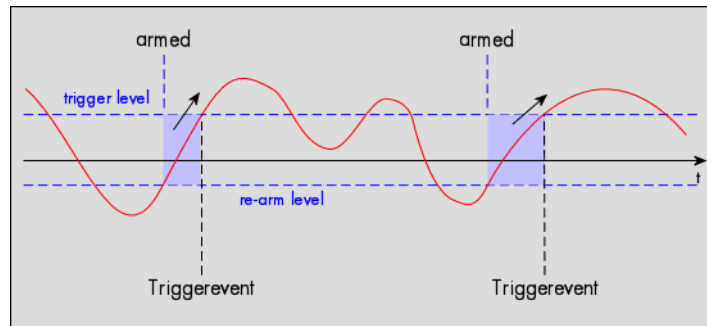


Table 103: Spectrum API: channel trigger register settings for re-arm trigger on positive edge

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_POS SPC_TM_REARM	01000001h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the desired trigger level relatively to the channel's input range.	board dependent
SPC_TRIG_CH0_LEVEL1	42300	read/write	Defines the re-arm level relatively to the channel's input range	board dependent

Channel re-arm trigger on negative edge

The analog input is continuously sampled with the selected sample rate. If the programmed re-arm level is crossed from higher to lower values, the trigger engine is armed and waiting for trigger. If the programmed trigger level is crossed by the channel's signal from higher values to lower values (falling edge) then the trigger event will be detected and the trigger engine will be disarmed. A new trigger event is only detected, if the trigger engine is armed again.

The re-arm trigger modes can be used to prevent the board from triggering on wrong edges in noisy signals.

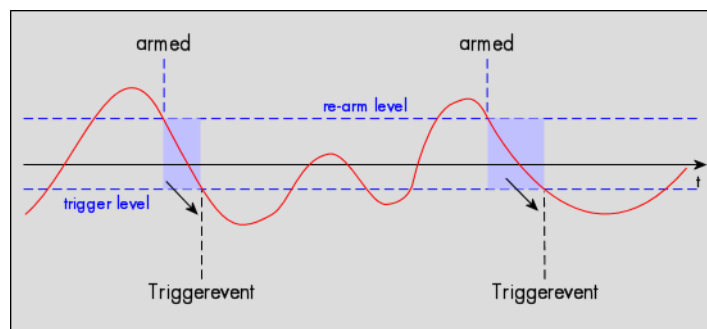


Table 104: Spectrum API: channel trigger register settings for re-arm trigger on negative edge

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_NEG SPC_TM_REARM	01000002h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Defines the re-arm level relatively to the channel's input range	board dependent
SPC_TRIG_CH0_LEVEL1	42300	read/write	Set it to the desired trigger level relatively to the channel's input range.	board dependent

Channel window trigger for entering signals

The analog input is continuously sampled with the selected sample rate. The upper and the lower level define a window. Every time the signal enters the window from the outside, a trigger event will be detected.

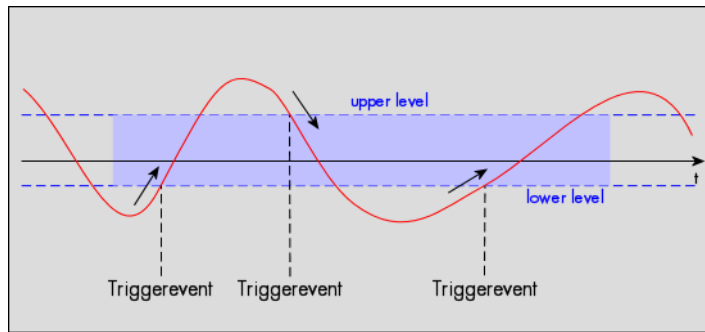


Table 105: Spectrum API: channel trigger register settings for window trigger for entering signals

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_WINENTER	00000020h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the upper trigger level relatively to the channel's input range.	board dependent
SPC_TRIG_CH0_LEVEL1	42300	read/write	Set it to the lower trigger level relatively to the channel's input range.	board dependent

Channel window trigger for leaving signals

The analog input is continuously sampled with the selected sample rate. The upper and the lower level define a window. Every time the signal leaves the window from the inside, a trigger event will be detected.

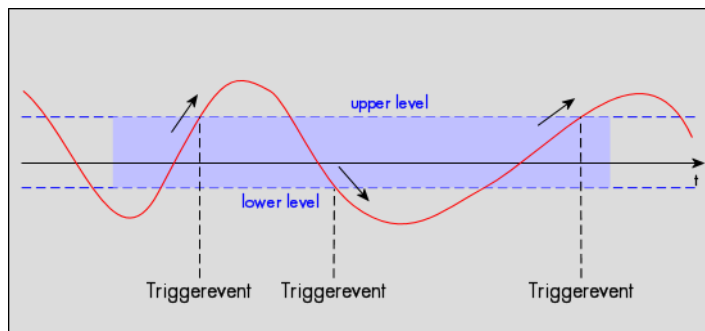


Table 106: Spectrum API: channel trigger register settings for window trigger for leaving signals

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_WINLEAVE	00000040h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the upper trigger level relatively to the channel's input range.	board dependent
SPC_TRIG_CH0_LEVEL1	42300	read/write	Set it to the lower trigger level relatively to the channel's input range.	board dependent

High level trigger

This trigger mode will generate an internal gate signal that can be useful for masking a second trigger event generated by a different mode. If using this mode as a single trigger source the card will detect a trigger event at the time when entering the high level (acting like positive edge trigger) or if the analog signal is already above the programmed level at the start it will immediately detect a trigger event.

The channel is continuously sampled with the selected sample rate. The trigger event will be detected if the analog signal is above the programmed trigger level.

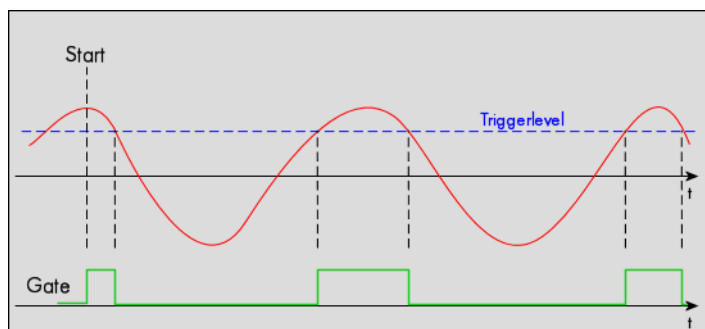


Table 107: Spectrum API: channel trigger register settings for high level trigger

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_HIGH	00000008h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the upper trigger level relatively to the channel's input range.	board dependent

Low level trigger

This trigger mode will generate an internal gate signal that can be useful for masking a second trigger event generated by a different mode. If using this mode as a single trigger source the card will detect a trigger event at the time when entering the low level (acting like negative edge trigger) or if the signal is already above the programmed level at the start it will immediately detect a trigger event.

The channel is continuously sampled with the selected sample rate. The trigger event will be detected if the analog signal is below the programmed trigger level.

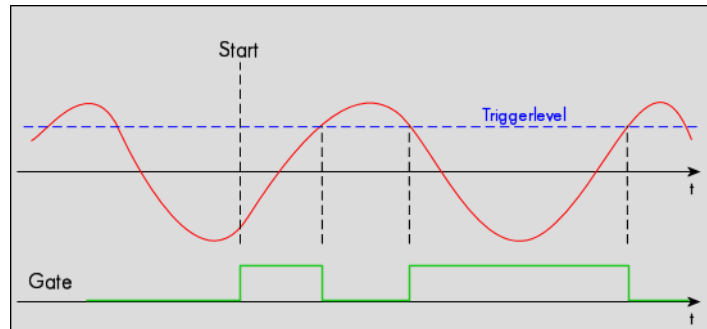


Table 108: Spectrum API: channel trigger register settings for low level trigger

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_LOW	00000010h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the upper trigger level relatively to the channel's input range.	board dependent

In window trigger

This trigger mode will generate an internal gate signal that can be useful for masking a second trigger event generated by a different mode. If using this mode as a single trigger source the card will detect a trigger event at the time when entering the window defined by the two trigger levels (acting like window enter trigger) or if the signal is already inside the programmed window at the start it will immediately detect a trigger event.

The channel is continuously sampled with the selected sample rate. The trigger event will be detected if the analog signal is inside the programmed trigger window.

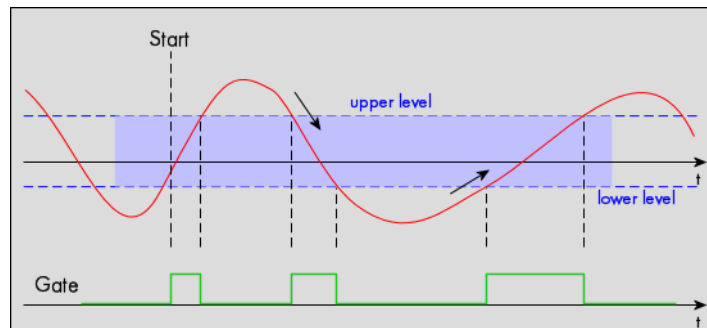


Table 109: Spectrum API: channel trigger register settings for in-window trigger

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_INWIN	00000080h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the upper trigger level relatively to the channel's input range.	board dependent
SPC_TRIG_CH0_LEVEL1	42300	read/write	Set it to the lower trigger level relatively to the channel's input range.	board dependent

Outside window trigger

This trigger mode will generate an internal gate signal that can be useful for masking a second trigger event generated by a different mode. If using this mode as a single trigger source the card will detect a trigger event at the time when leaving the window defined by the two trigger levels (acting like leaving window trigger) or if the signal is already outside the programmed window at the start it will immediately detect a trigger event.

The channel is continuously sampled with the selected sample rate. The trigger event will be detected if the analog signal is outside the programmed trigger window.

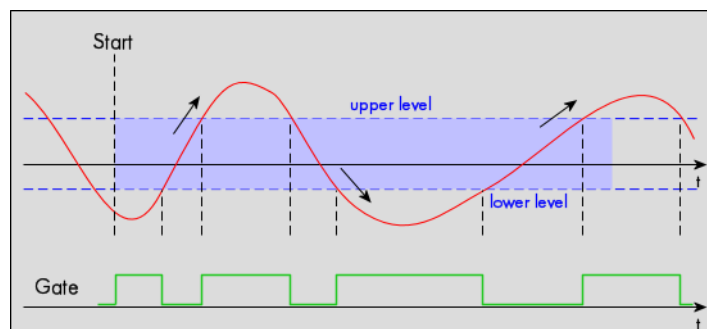


Table 110: Spectrum API: channel trigger register settings for outside-window trigger

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_OUTSIDEWIN	00000100h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the upper trigger level relatively to the channel's input range.	board dependent
SPC_TRIG_CH0_LEVEL1	42300	read/write	Set it to the lower trigger level relatively to the channel's input range.	board dependent

Channel hysteresis trigger on positive edge

This trigger mode will generate an internal gate signal that can be useful for masking a second trigger event generated by a different mode. The analog input is continuously sampled with the selected sample rate.

If the programmed trigger level is crossed by the channel's signal from lower values to higher values (rising edge) the gate starts.

When the signal crosses the programmed hysteresis level from higher values to lower values (falling edge) then the gate will stop.

As this mode is purely edge-triggered, the high level at the cards start time does not trigger the board.

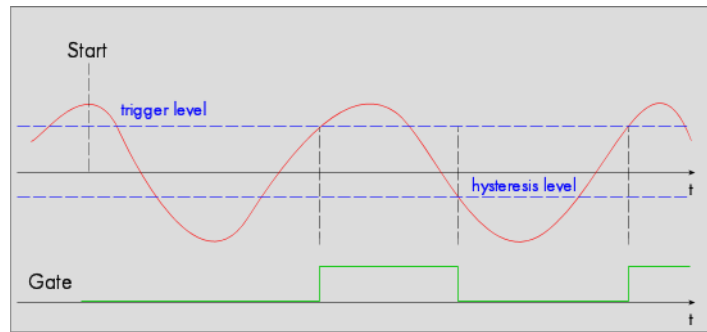


Table 111: Spectrum API: register settings for channel hysteresis trigger on positive edge

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_POS SPC_TM_HYSTERESIS	20000001h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the desired trigger level relatively to the channel's input range.	board dependant
SPC_TRIG_CH0_LEVEL1	42300	read/write	Defines the hysteresis level relatively to the channel's input range	board dependant

Channel hysteresis trigger on negative edge

This trigger mode will generate an internal gate signal that can be useful for masking a second trigger event generated by a different mode. The analog input is continuously sampled with the selected sample rate.

If the programmed trigger level is crossed by the channel's signal higher values to lower values (falling edge) the gate starts.

When the signal crosses the programmed hysteresis level from lower values to higher values (rising edge) then the gate will stop.

As this mode is purely edge-triggered, the low level at the cards start time does not trigger the board.

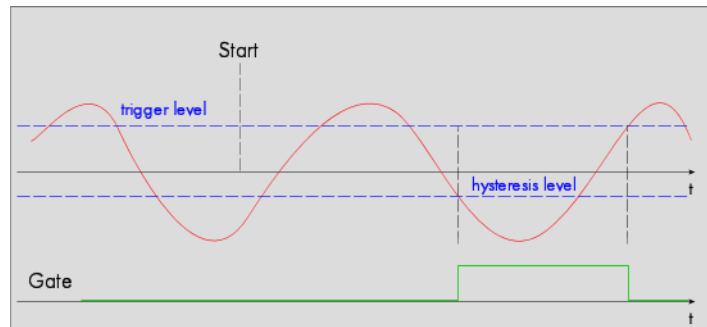



Table 112: Spectrum API: register settings for channel hysteresis trigger on negative edge

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_NEG SPC_TM_HYSTERESIS	20000002h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the desired trigger level relatively to the channel's input range.	board dependant
SPC_TRIG_CH0_LEVEL1	42300	read/write	Defines the hysteresis level relatively to the channel's input range	board dependant

Channel re-arm hysteresis trigger on positive edge

This trigger mode will generate an internal gate signal that can be useful for masking a second trigger event generated by a different mode. The analog input is continuously sampled with the selected sample rate.

If the programmed re-arm/hysteresis level is crossed from lower to higher values, the trigger engine is armed and waiting for trigger. If the programmed trigger level is crossed by the channel's signal from lower values to higher values (rising edge) then the gate starts and the trigger engine will be disarmed. If the programmed re-arm/hysteresis level is crossed by the channel's signal from higher values to lower values (falling edge) the gate stops.

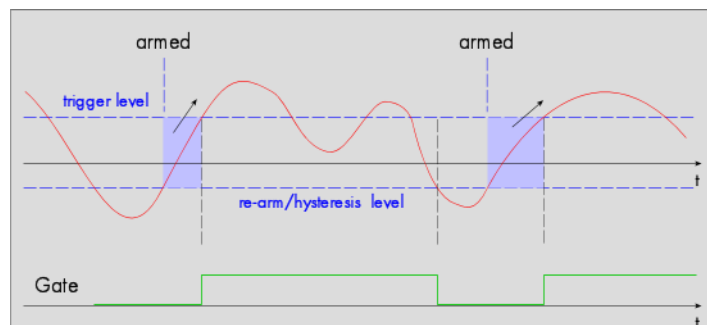

A new trigger event is only detected, if the trigger engine is armed again. The re-arm trigger modes can be used to prevent the board from triggering on wrong edges in noisy signals.


Table 113: Spectrum API: register settings for channel hysteresis re-arm trigger on positive edge

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_POS SPC_TM_REARM SPC_TM_HYSTERESIS	21000001h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the desired trigger level relatively to the channel's input range.	board dependant
SPC_TRIG_CH0_LEVEL1	42300	read/write	Defines the re-arm and hysteresis level relatively to the channel's input range	board dependant

Channel re-arm hysteresis trigger on negative edge

This trigger mode will generate an internal gate signal that can be useful for masking a second trigger event generated by a different mode. The analog input is continuously sampled with the selected sample rate.

If the programmed re-arm/hysteresis level is crossed from higher to lower values, the trigger engine is armed and waiting for trigger. If the programmed trigger level is crossed by the channel's signal from higher values to lower values (falling edge) then the gate starts and the trigger engine will be disarmed. If the programmed re-arm/hysteresis level is crossed by the channel's signal from lower values to higher values (rising edge) the gate stops.

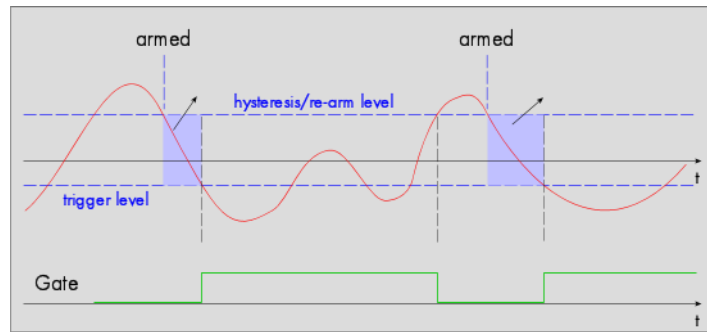

A new trigger event is only detected, if the trigger engine is armed again. The re-arm trigger modes can be used to prevent the board from triggering on wrong edges in noisy signals.

Table 114: Spectrum API: register settings for channel hysteresis re-arm trigger on negative edge

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_NEG SPC_TM_REARM SPC_TM_HYSTERESIS	21000002h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Defines the trigger level relatively to the channel's input range	board dependant
SPC_TRIG_CH0_LEVEL1	42300	read/write	Defines the re-arm and hysteresis level relatively to the channel's input range	board dependant

High level hysteresis trigger

This trigger mode will generate an internal gate signal that can be useful for masking a second trigger event generated by a different mode. The analog input is continuously sampled with the selected sample rate.

If the signal is equal or higher than the programmed trigger level the gate starts.

When the signal is lower than the programmed hysteresis level the gate will stop.

As this mode is level-triggered, the high level at the cards start time does trigger the board.

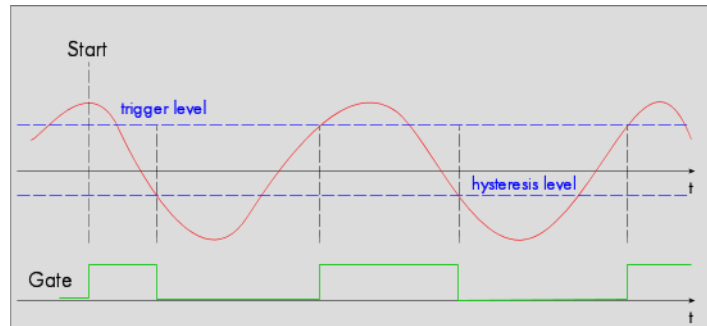


Table 115: Spectrum API: register settings for high-level channel hysteresis trigger

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_HIGH SPC_TM_HYSTERESIS	20000008h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the desired trigger level relatively to the channel's input range.	board dependant
SPC_TRIG_CH0_LEVEL1	42300	read/write	Defines the hysteresis level relatively to the channel's input range	board dependant

Low level hysteresis trigger

This trigger mode will generate an internal gate signal that can be useful for masking a second trigger event generated by a different mode. The analog input is continuously sampled with the selected sample rate.

If the signal is equal or lower than the programmed trigger level the gate starts.

When the signal is higher than the programmed hysteresis level the gate will stop.

As this mode is level-triggered, the high level at the cards start time does trigger the board.

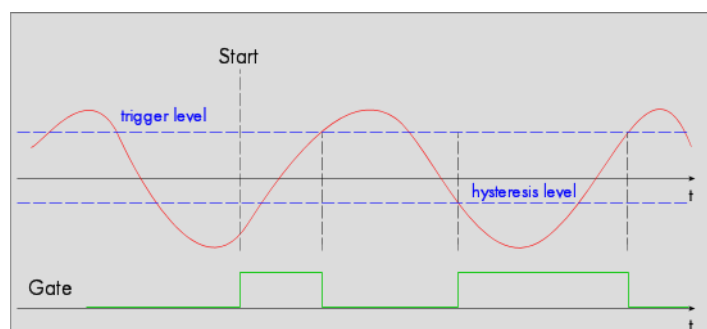


Table 116: Spectrum API: register settings for low-level channel hysteresis trigger

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_LOW SPC_TM_HYSTERESIS	20000010h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the desired trigger level relatively to the channel's input range.	board dependant
SPC_TRIG_CH0_LEVEL1	42300	read/write	Defines the hysteresis level relatively to the channel's input range	board dependant

PXI Trigger (M4x PXIe cards only)

The M4x PXIe cards can use the various PXI trigger sources for trigger detection and/or trigger and status distribution.

This includes the eight lines from the PXI trigger bus (PXI_TRIG[7] to PXI_TRIG[0]), as well as the „older“ single-ended PXI Star-Trigger line (PXI_STAR) and the „newer“ differential PXI_DSTARC (dedicated output) and PXI_DSTARB (dedicated input) lines, that have been introduced with the PXI Express standard.

All these lines can be included within the programmable masks on the cards, either within the OR mask as well within the AND mask, to form rather complex trigger conditions required to properly synchronize multiple M4x.xxxx cards to a single trigger event.

The following passage shows, how to program these lines for either input or output and how to properly use them for trigger synchronization between multiple M4x.xxxx cards inside a PXI or PXIe chassis.

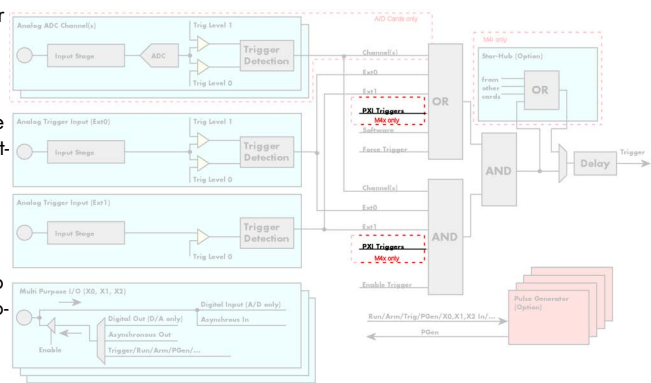


Table 117: trigger overview with PXI trigger lines marked

To set up PXI trigger conditions, the mode registers have to be set up properly, to define the direction of one or multiple PXI lines, as well as the trigger masks registers for including one or multiple PXI lines to generate a trigger event from.

PXI Trigger Mode Registers

Please find the list of the various modes the different PXI trigger lines can be used for below. The modes available for driving the PXI lines are very similar to those of the Multi Purpose I/O lines described earlier in this manual.

Table 118: Spectrum API: PXI trigger register and available register settings

Register	Value	Direction	Description
SPC_PXITRG0_AVAILMODES	47310	read	Bitmask showing all available PXI trigger modes usable with PXI_TRIG0 line.
SPC_PXITRG1_AVAILMODES	47311	read	Bitmask showing all available PXI trigger modes usable with PXI_TRIG1 line.
SPC_PXITRG2_AVAILMODES	47312	read	Bitmask showing all available PXI trigger modes usable with PXI_TRIG2 line.
SPC_PXITRG3_AVAILMODES	47313	read	Bitmask showing all available PXI trigger modes usable with PXI_TRIG3 line.
SPC_PXITRG4_AVAILMODES	47314	read	Bitmask showing all available PXI trigger modes usable with PXI_TRIG4 line.
SPC_PXITRG5_AVAILMODES	47315	read	Bitmask showing all available PXI trigger modes usable with PXI_TRIG5 line.
SPC_PXITRG6_AVAILMODES	47316	read	Bitmask showing all available PXI trigger modes usable with PXI_TRIG6 line.
SPC_PXITRG7_AVAILMODES	47317	read	Bitmask showing all available PXI trigger modes usable with PXI_TRIG7 line.
SPC_PXISTAR_AVAILMODES	47318	read	Bitmask showing all available PXI trigger modes usable with PXI_STAR line.
SPC_PXIDSTARC_AVAILMODES	47310	read	Bitmask showing all available PXI trigger modes usable with PXI_DSTARC line, to send information to a Startrigger card, installed in the System Timing Slot. The corresponding returned signal (from the System Timing Slot to the card) will be available on the DSTARB line, which then has to be properly included into the trigger source masks, as described later.
SPC_PXITRG0_MODE	47300	read/write	Defines the output mode for the PXI_TRIG0 line.
SPC_PXITRG1_MODE	47301	read/write	Defines the output mode for the PXI_TRIG1 line.
SPC_PXITRG2_MODE	47302	read/write	Defines the output mode for the PXI_TRIG2 line.
SPC_PXITRG3_MODE	47303	read/write	Defines the output mode for the PXI_TRIG3 line.
SPC_PXITRG4_MODE	47304	read/write	Defines the output mode for the PXI_TRIG4 line.
SPC_PXITRG5_MODE	47305	read/write	Defines the output mode for the PXI_TRIG5 line.
SPC_PXITRG6_MODE	47306	read/write	Defines the output mode for the PXI_TRIG6 line.
SPC_PXITRG7_MODE	47307	read/write	Defines the output mode for the PXI_TRIG7 line.
SPC_PXISTAR_MODE	47308	read/write	Defines the trigger mode for the PXI_STAR line, to send information to a Startrigger card, installed in the System Timing Slot.
SPC_PXIDSTARC_MODE	47309	read/write	Defines the trigger mode for the PXI_DSTARC line, to send information to a possible Startrigger card, installed in the System Timing Slot. The corresponding returned signal (from the System Timing Slot to the card) will be available on the DSTARB line, which then has to be properly included into the trigger source masks, as described later.
SPCM_PXITRGMODE_DISABLE	00000000h		The PXI line is neither used as input or output and is in high-impedance mode (tristate).
SPCM_PXITRGMODE_IN	00000001h		The PXI line is used as an input and can now be included in the trigger masks, as described below.
SPCM_PXITRGMODE_ASYNCOUT	00000002h		The PXI line is programmed for asynchronous output. Use SPC_PXITRG_ASYNCIO to write data asynchronously.
SPCM_PXITRGMODE_RUNSTATE	00000004h		The PXI line outputs the current run state of the card. If acquisition/output is running the signal is HIGH. If card has stopped the signal is LOW.
SPCM_PXITRGMODE_ARMSTATE	00000008h		The PXI line outputs the current ARM state of the card. If the card is armed and ready to receive a trigger the signal is HIGH. If the card isn't running or the card is either still acquiring pretrigger data or the trigger has already been detected the signal is LOW.
SPCM_PXITRGMODE_TRIGOUT	00000010h		The PXI line outputs a detected trigger and hence shows the trigger detection. The trigger output goes HIGH as soon as the trigger is recognized. After end of acquisition it is LOW again. In Multiple Recording/Gated Sampling/ABA mode it goes LOW after the acquisition of the current segment stops. In standard FIFO mode the trigger output is HIGH until FIFO mode is stopped.

SPCM_PXITRGMODE_REFLCKOUT	00000020h	The PXI line reflects the internal generated 10 MHz reference clock signal generated from the PXI_CLK100 clock signal in conjunction with the PXI_SYNC100 signal. Can be used to provide other equipment with an additional clock signal via one of the trigger lines.
SPCM_PXITRGMODE_CONTOUTMARK	00000040h	Generator Cards only: the PXI line outputs a HIGH pulse as continuous marker signal for continuous replay mode. The marker signal length is ½ of the programmed memory size.

Depending on the used PXI/PXIe backplane, the PXI trigger bus (PXI_TRIG[7..0]) might be segmented and needs to be setup separately, to allow routing of trigger signals between different segments an even within one segment. Please consult your PXI chassis/backplane manual for details on the routing capabilities of these lines and the relating software interface.



Be aware not to enable outputs on the same PXI trigger line on multiple cards, or to enable a segmented backplane driver and a card's output on the same line within the same segment. If two or more outputs are working against each other the result is unpredictable and may even harm the hardware parts.



The PXI trigger lines cannot be used to phase-synchronize multiple PXIe cards. The PXIe trigger lines are asynchronous to the used sampling rate and thus may result in a phase difference of more than one sample between multiple cards.



PXI Trigger Sources within the Trigger Masks

To include PXI lines, whose mode has been set to „SPCM_PXITRGMODE_IN“, as shown above, the desired masks must contain the corresponding input, as the following table shows:

Table 119: Spectrum API: PXI trigger mask register and available register settings

Register	Value	Direction	Description
SPC_TRIG_ORMASK	40410	read/write	Defines the events included within the trigger OR mask of the card.
SPC_TRIG_ANDMASK	40430	read/write	Defines the events included within the trigger AND mask of the card.
SPC_TMASK_PXI0	100000h		Enables the PXI_TRIG0 for the mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI1	200000h		Enables the PXI_TRIG1 for the mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI2	400000h		Enables the PXI_TRIG2 for the mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI3	800000h		Enables the PXI_TRIG3 for the mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI4	1000000h		Enables the PXI_TRIG4 for the mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI5	2000000h		Enables the PXI_TRIG5 for the mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI6	4000000h		Enables the PXI_TRIG6 for the mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXI7	8000000h		Enables the PXI_TRIG7 for the mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXISTAR	10000000h		Enables the PXISTAR line for the mask. The card will trigger when the signal on this input is HIGH.
SPC_TMASK_PXIDSTARB	20000000h		Enables the PXI_DSTARB for the mask. The card will trigger when the signal on this input is HIGH.

The use of multiple PXI_TRIG lines in either mask to combine status and trigger information is shown in the following example for clarification.

PXI Trigger Setup Example

Example of connecting three M4x.xxxx cards, card 0 is triggering all three cards:

```
drv_handle hDrv[3];

for (i = 0; i < 3; i++)
{
    sprintf (s, "/dev/spcm%d", i);
    hDrv[i] = spcm_hOpen (s); // open all three cards

    spcm_dwSetParam_i32 (hDrv[i], SPC_CLOCKMODE, SPC_CM_PXIREFCLOCK); // Use PXI reference clock on all cards
    spcm_dwGetParam_i64 (hDrv[i], SPC_SAMPLERATE, 100000000); // Use 100 MS/s as sample clock
}

// Slave card1 trigger setup
spcm_dwSetParam_i32 (hDrv[1], SPC_PXITRG0_MODE, SPCM_PXITRGMODE_IN); // set PXI_TRIG0 as input
spcm_dwSetParam_i32 (hDrv[1], SPC_PXITRG1_MODE, SPCM_PXITRGMODE_ARMSTATE); // Output my ARM state on PXI_TRIG1
spcm_dwSetParam_i32 (hDrv[1], SPC_TRIG_ORMASK, SPC_TMASK_PXI0); // trigger source: PXI_TRIG0

// Slave card2 trigger setup
spcm_dwSetParam_i32 (hDrv[2], SPC_PXITRG0_MODE, SPCM_PXITRGMODE_IN); // set PXI_TRIG0 as input
spcm_dwSetParam_i32 (hDrv[2], SPC_PXITRG2_MODE, SPCM_PXITRGMODE_ARMSTATE); // Output my ARM state on PXI_TRIG2
spcm_dwSetParam_i32 (hDrv[2], SPC_TRIG_ORMASK, SPC_TMASK_PXI0); // trigger source: PXI_TRIG0

// Master card0: Acts as a trigger master distributing External trigger 0 trigger
spcm_dwSetParam_i32 (hDrv[0], SPC_TRIG_ORMASK, SPC_TMASK_EXT0);

// Setting Ext0 trigger for rising edges (for AD/DA cards trigger levels might need to be adjusted)
spcm_dwSetParam_i32 (hDrv[0], SPC_TRIG_EXT0_MODE, SPC_TM_POS);

spcm_dwSetParam_i32 (hDrv[0], SPC_PXITRG0_MODE, SPCM_PXITRGMODE_TRIGOUT); // Output trigger on PXI_TRIG0
spcm_dwSetParam_i32 (hDrv[0], SPC_PXITRG1_MODE, SPCM_PXITRGMODE_IN); // Set PXI_TRIG1 as input
spcm_dwSetParam_i32 (hDrv[0], SPC_PXITRG2_MODE, SPCM_PXITRGMODE_IN); // Set PXI_TRIG2 as input

// Synchronize Pre-Trigger area of all cards to prevent unintended trigger detection, while the
// other card(s) are not ready yet. Therefore include PXI_TRIG1 and PXI_TRIG2 inputs in the AND mask,
// so that these lines both must be HIGH, to enable trigger detection on card0 and hence
// trigger distribution to the other cards.
spcm_dwSetParam_i32 (hDrv[0], SPC_TRIG_ANDMASK, SPC_TMASK_PXI2 | SPC_TMASK_PXI1);

// transfer setup to all cards to allow PXI lines to be activated (leave a possible high-impedance mode)
for (i = 0; i < 3; i++)
    spcm_dwSetParam_i32 (hCard[i], SPC_M2CMD, M2CMD_CARD_WRITESETUP);

// Start the cards now in any order, as any triggering is now prevented as long no all the cards are armed.

// Wait for all cards to finish recording and then get data from all cards and do processing.
```

The above example assumes, that a possible PXI trigger bus segmentation of the used backplane has been properly set up, so that each card's output can reach the other card's inputs properly and that no two drivers on one segment are driving against each other.



Multi Purpose I/O Lines

On-board I/O lines (X0, X1, X2)

The M4i/M4x series cards and the based upon digitizerNETBOX, generatorNETBOX and hybridNETBOX products have three multi purpose I/O lines that can be used for a wide variety of functions to help the interconnection with external equipment. The functionality of these multi purpose I/O lines can be software programmed and each of these lines can either be used for input or output.

The multi purpose I/O lines may be used as status outputs such as trigger output or internal arm/run as well as for asynchronous I/O to control external equipment as well as additional digital input lines that are sampled synchronously with the analog data.

The multi purpose I/O lines are available on the front plate and labeled with X0 (line 0), X1 (line 1) and X2 (line 2). As default these lines are switched off.

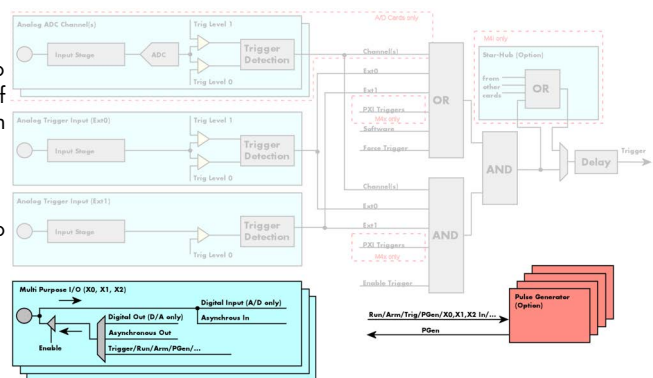


Image 60: trigger overview with multi-purpose lines marked



As default (power-on and after reset command) the I/O capable lines are switched off and hence are not actively driven. Hence the on-board 10 kOhm pull-up resistors are pulling these lines to logic HIGH. If a logic LOW is required, external lower-value (1 kOhm) pull-down resistors might be used.



Please be careful when programming these lines as an output whilst maybe still being connected with an external signal source, as that may damage components either on the external equipment or on the card itself.

Programming the behavior

Each multi purpose I/O line can be individually programmed. Please check the available modes by reading the SPCM_X0_AVAILMODES, SPCM_X1_AVAILMODES and SPCM_X2_AVAILMODES register first. The available modes may differ from card to card and may be enhanced with new driver/firmware versions to come.

Table 120: Spectrum API: multi-purpose I/O lines registers and available register settings

Register	Value	Direction	Description
SPCM_X0_AVAILMODES	47210	read	Bitmask with all bits of the below mentioned modes showing the available modes for (X0)
SPCM_X1_AVAILMODES	47211	read	Bitmask with all bits of the below mentioned modes showing the available modes for (X1)
SPCM_X2_AVAILMODES	47212	read	Bitmask with all bits of the below mentioned modes showing the available modes for (X2)
SPCM_X0_MODE	47200	read/write	Defines the mode for (X0). Only one mode selection is possible to be set at a time
SPCM_X1_MODE	47201	read/write	Defines the mode for (X1). Only one mode selection is possible to be set at a time
SPCM_X2_MODE	47202	read/write	Defines the mode for (X2). Only one mode selection is possible to be set at a time
SPCM_XMODE_DISABLE	0000000h		No mode selected. Output is tristate (default setup)
SPCM_XMODE_ASYNCIN	00000001h		Connector is programmed for asynchronous input. Use SPCM_XX_ASYNCIO to read data asynchronous as shown in next chapter.
SPCM_XMODE_ASYNCOUT	00000002h		Connector is programmed for asynchronous output. Use SPCM_XX_ASYNCIO to write data asynchronous as shown in next chapter.
SPCM_XMODE_DIGIN	00000004h		A/D cards only: Connector is programmed for synchronous digital input. For each analog channel, one digital channel X0/X1/X2 is integrated into the ADC data stream. Depending on the ADC resolution of your card the resulting merged samples can have different formats. Please check the „Sample format“ chapter for more details. Please note that automatic sign extension of analog data is ineffective as soon as one digital input line is activated and the software must properly mask out the digital bits.
SPCM_XMODE_DIGOUT	00000008h		D/A cards only: Connector is programmed for synchronous digital output. Digital channels can be „included“ within the analog samples and synchronously replayed along. Requires additional MODE bits to be set along with this flag, as explained later on.
SPCM_XMODE_TRIGOUT	00000020h		Connector is programmed as trigger output and shows the trigger detection. The trigger output goes HIGH as soon as the trigger is recognized. After end of acquisition it is LOW again. In Multiple Recording/Gated Sampling/ABA mode it goes LOW after the acquisition of the current segment stops. In FIFO single mode the trigger output is HIGH until FIFO mode is stopped.
SPCM_XMODE_DIGIN2BIT	00000080h		Connector is programmed for digital input. For each analog channel, two digital channels X0/X1/X2 are integrated into the ADC data stream. Depending on the ADC resolution of your card the resulting merged samples can have different formats. Please check the data format chapter to see more details. Please note that automatic sign extension of analog data is ineffective as soon as one digital input line is activated and the software must properly mask out the digital bits.
SPCM_XMODE_RUNSTATE	00000100h		Connector shows the current run state of the card. If acquisition/output is running the signal is HIGH. If card has stopped the signal is LOW.
SPCM_XMODE_ARMSTATE	00000200h		Connector shows the current ARM state of the card. If the card is armed and ready to receive a trigger the signal is HIGH. If the card isn't running or the card is still acquiring pretrigger data or the trigger has been detected the signal is LOW.
SPCM_XMODE_REFCLKOUT	00001000h		Connector reflects the internally generated PLL reference clock in the range of 10 to 62.5 MHz.
SPCM_XMODE_CONTOUTMARK	00002000h		Generator Cards only: outputs a HIGH pulse as continuous marker signal for continuous replay mode. The marker signal length is 1/2 of the programmed memory size.

SPCM_XMODE_SYSCLOCKOUT	00004000h	Connector reflects the internally generated system clock in the range of 2.5 up to 156.25 MHz.
SPCM_XMODE_PULSEGEN	00080000h	A/D and D/A cards only (optional): Connector reflects the output of the same index pulse generator (X0 output from pulse generator 0, X1 from pulse generator 1 etc.). For details on the pulse generator option please consult the "Pulse Generator (Option)" chapter.



Please note that a change to the SPCM_X0_MODE, SPCM_X1_MODE or SPCM_X2_MODE will only be updated with the next call to either the M2CMD_CARD_START or M2CMD_CARD_WRITESETUP register. For further details please see the relating chapter on the M2CMD_CARD registers.

Using asynchronous I/O

To use asynchronous I/O on the multi purpose I/O lines it is first necessary to switch these lines to the desired asynchronous mode by programming the above explained mode registers. As a special feature asynchronous input can also be read if the mode is set to trigger input or digital input.

Table 121: Spectrum API: asynchronous I/O register settings of the multi-purpose I/O registers

Register	Value	Direction	Description
SPCM_XX_ASYNCIO	47220	read/write	Connector X0 is linked to bit 0 of the register, connector X1 is linked to bit 1 while connector X2 is linked to bit 2 of this register. Data is written/read immediately without any relation to the currently used sampling rate or mode. If a line is programmed to output, reading this line asynchronously will return the current output level.

Example of asynchronous write and read. We write a high pulse on output X1 and wait for a high level answer on input X0:

```

spcm_dwSetParam_i32 (hDrv, SPCM_X0_MODE, SPCM_XMODE_ASYNCIN); // X0 set to asynchronous input
spcm_dwSetParam_i32 (hDrv, SPCM_X1_MODE, SPCM_XMODE_ASYNCOUT); // X1 set to asynchronous output
spcm_dwSetParam_i32 (hDrv, SPCM_X2_MODE, SPCM_XMODE_TRIGOUT); // X2 set to trigger output

spcm_dwSetParam_i32 (hDrv, SPCM_XX_ASYNCIO, 0); // programming a high pulse on output
spcm_dwSetParam_i32 (hDrv, SPCM_XX_ASYNCIO, 2);
spcm_dwSetParam_i32 (hDrv, SPCM_XX_ASYNCIO, 0);

do {
    spcm_dwGetParam_i32 (hDrv, SPCM_XX_ASYNCIO, &lAsyncIn); // read input in a loop
} while ((lAsyncIn & 1) == 0); // until X0 is going to high level

```

Special behavior of trigger output

As the driver of the M4i/M4x series is the same as the driver for the M2i/M3i series and some old software may rely on register structure of the M2i/M3i card series, there is a special compatible trigger output register that will work according to the M2i/M3i series style. It is not recommended to use this register unless you're writing software for multiple card series:

Table 122: Spectrum API: additional trigger output register for compatibility with older hardware

Register	Value	Direction	Description
SPC_TRIG_OUTPUT	40100	read/write	M2i style trigger output programming. Write a „1“ to enable: - X2 trigger output (SPCM_X2_MODE = SPCM_XMODE_TRIGOUT) - X1 arm state (SPCM_X1_MODE = SPCM_XMODE_ARMSTATE). - X0 run state (SPCM_X0_MODE = SPCM_XMODE_RUNSTATE). Write a „0“ to disable all three outputs: - SPCM_X0_MODE = SPCM_X1_MODE = SPCM_X2_MODE = SPCM_XMODE_DISABLE



The SPC_TRIG_OUTPUT register overrides the multi purpose I/O settings done by SPCM_X0_MODE, SPCM_X1_MODE and SPCM_X2_MODE and vice versa. Do not use both methods together from within one program.

Synchronous digital inputs

The cards of the M4i.23xx series allow to optionally record synchronous digital channels along with analog acquisition. The table below shows the related registers and the values that correspond with the different possibilities. This mode, when set, changes the sample format for all active channels according to the table further below:

Register	Value	Direction	Description
SPCM_X0_AVAILMODES	47210	read	Bitmask with all bits of the below mentioned modes showing the available modes for (X0)
SPCM_X1_AVAILMODES	47211	read	Bitmask with all bits of the below mentioned modes showing the available modes for (X1)
SPCM_X2_AVAILMODES	47212	read	Bitmask with all bits of the below mentioned modes showing the available modes for (X2)
SPCM_X0_MODE	47200	read/write	Defines the mode for (X0). Only one mode selection is possible to be set at a time
SPCM_X1_MODE	47201	read/write	Defines the mode for (X1). Only one mode selection is possible to be set at a time
SPCM_X2_MODE	47202	read/write	Defines the mode for (X2). Only one mode selection is possible to be set at a time
SPCM_XMODE_DISABLE	00000000h		No mode selected. Output is tristate (default setup)
SPCM_XMODE_DIGIN	00000004h		A/D cards only: Connector is programmed for synchronous digital input. For each analog channel, one digital channel X0/X1/X2 is integrated into the ADC data stream. Depending on the ADC resolution of your card the resulting merged samples can have different formats. Please check the „Sample format“ chapter for more details. Please note that automatic sign extension of analog data is ineffective as soon as one digital input line is activated and the software must properly mask out the digital bits.

The driver will automatically scale the analog samples prior to inserting the digital channels to keep the channel at the maximum possible resolution.

Sample Format

The card is using 7 bit A/D samples, that are stored in two's complement in one 8 bit data byte. 7 bit resolution means that data is ranging from -64...to...+63:

	Standard Mode M4i.23xx 8 bit ADC resolution	Digital inputs enabled SPCM_XMODE_DIGIN M4i.23xx 7 bit ADC resolution
D7	ADx Bit 6 (sign extension)	Ch3: Digital bit 0 (X0) Ch2: Digital bit 2 (X2) Ch1: Digital bit 1 (X1) Ch0: Digital bit 0 (X0)
D6	ADx Bit 6 (MSB)	ADx Bit 6 (MSB)
D5	ADx Bit 5	ADx Bit 5
D4	ADx Bit 4	ADx Bit 4
D3	ADx Bit 3	ADx Bit 3
D2	ADx Bit 2	ADx Bit 2
D1	ADx Bit 1	ADx Bit 1
D0	ADx Bit 0 (LSB)	ADx Bit 0 (LSB)



Please note that automatic sign extension of analog data is ineffective as soon as one digital input line is activated and the software must properly mask out all the digital bits from the samples.

The following example shows how to enable a single digital channels for all analog channels (four in this example)

```
// enable all four analog channels
spcm_dwSetParam_i32 (hDrv, SPC_CHENABLE, CHANNEL0 | CHANNEL1 | CHANNEL2 | CHANNEL3);

// enable acquisition of one digital bit per analog channel
spcm_dwSetParam_i32 (hDrv, SPCM_X0_MODE, SPCM_XMODE_DIGIN); // X0 set to synchronous input
spcm_dwSetParam_i32 (hDrv, SPCM_X1_MODE, SPCM_XMODE_DIGIN); // X1 set to synchronous input
spcm_dwSetParam_i32 (hDrv, SPCM_X2_MODE, SPCM_XMODE_DIGIN); // X2 set to synchronous input
```

Mode Multiple Recording

The Multiple Recording mode allows the acquisition of data blocks with multiple trigger events without restarting the hardware.

The on-board memory will be divided into several segments of the same size. Each segment will be filled with data when a trigger event occurs (acquisition mode).

As this mode is totally controlled in hardware there is a very small re-arm time from end of one segment until the trigger detection is enabled again. You'll find that re-arm time in the technical data section of this manual.

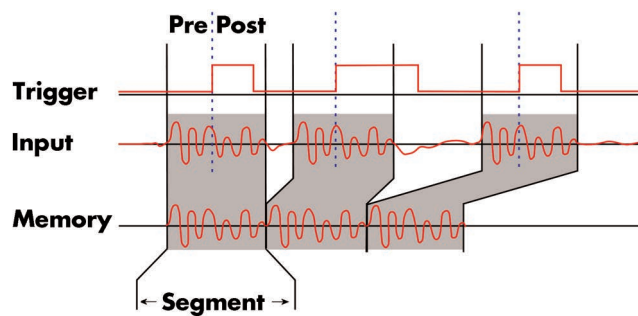


Image 61: Drawing of Multiple Recording acquisition

The following table shows the register for defining the structure of the segments to be recorded with each trigger event.

Table 123: Spectrum API: software registers for Multiple Recording mode setup

Register	Value	Direction	Description
SPC_POSTTRIGGER	10100	read/write	Acquisition only: defines the number of samples to be recorded per channel after the trigger event.
SPC_SEGMENTSIZE	10010	read/write	Size of one Multiple Recording segment: the total number of samples to be recorded per channel after detection of one trigger event including the time recorded before the trigger (pre trigger).

Each segment in acquisition mode can consist of pretrigger and/or posttrigger samples. The user always has to set the total segment size and the posttrigger, while the pretrigger is calculated within the driver with the formula: $[\text{pretrigger}] = [\text{segment size}] - [\text{posttrigger}]$.

When using Multiple Recording the maximum pretrigger is limited depending on the number of active channels. When the calculated value exceeds that limit, the driver will return the error ERR_PRETRIGGERLEN. Please have a look at the table further below to see the maximum pretrigger length that is possible.



Recording modes

Standard Mode

With every detected trigger event one data block is filled with data. The length of one multiple recording segment is set by the value of the segment size register SPC_SEGMENTSIZE. The total amount of samples to be recorded is defined by the memsize register. Memsize must be set to a multiple of the segment size. The table below shows the register for enabling Multiple Recording. For detailed information on how to setup and start the standard acquisition mode please refer to the according chapter earlier in this manual.

Table 124: Spectrum API: card mode register and multiple recording settings

Register	Value	Direction	Description
SPC_CARDMODE	9500	read/write	Defines the used operating mode
SPC_REC_STD_MULTI	2		Enables Multiple Recording for standard acquisition.

The total number of samples to be recorded to the on-board memory in Standard Mode is defined by the SPC_MEMSIZE register.

Table 125: Spectrum API: memory and loop registers with related multiple recording settings

Register	Value	Direction	Description
SPC_MEMSIZE	10000	read/write	Defines the total number of samples to be recorded per channel.

FIFO Mode

The Multiple Recording in FIFO Mode is similar to the Multiple Recording in Standard Mode. In contrast to the standard mode it is not necessary to program the number of samples to be recorded. The acquisition is running until the user stops it. The data is read block by block by the driver as described under FIFO single mode example earlier in this manual. These blocks are online available for further data processing by the user program. This mode significantly reduces the amount of data to be transferred on the PCI bus as gaps of no interest do not have to be transferred. This enables you to use faster sample rates than you would be able to in FIFO mode without Multiple Recording. The advantage of Multiple Recording in FIFO mode is that you can stream data online to the host system. You can make real-time data processing or store a huge amount of data to the hard disk. The table below shows the dedicated register for enabling Multiple Recording. For detailed information how to setup and start the board in FIFO mode please refer to the according chapter earlier in this manual.

Table 126: Spectrum API: card mode register and multiple replay FIFO mode settings

Register	Value	Direction	Description
SPC_CARDMODE	9500	read/write	Defines the used operating mode
SPC_REC_FIFO_MULTI	32		Enables Multiple Recording for FIFO acquisition.

The number of segments to be recorded must be set separately with the register shown in the following table:

Table 127: Spectrum API: loops register settings when using Multiple Replay FIFO mode

Register	Value	Direction	Description
SPC_LOOPS	10020	read/write	Defines the number of segments to be recorded
0			Recording will be infinite until the user stops it.
1 ... [4G - 1]			Defines the total segments to be recorded.

Limits of pre trigger, post trigger, memory size

The maximum memory size parameter is only limited by the number of activated channels and by the amount of installed memory. Please keep in mind that each sample needs 1 bytes of memory to be stored. Minimum memory size as well as minimum and maximum post trigger limits are independent of the activated channels or the installed memory.

Due to the internal organization of the card memory there is a certain stepsize when setting these values that has to be taken into account. The following table gives you an overview of all limits concerning pre trigger, post trigger, memory size, segment size and loops. The table shows all values in relation to the installed memory size in samples. If more memory is installed the maximum memory size figures will increase according to the complete installed memory

Table 128: Spectrum API: Limits of pre trigger, post trigger and memory size

Activated Channels	Used Mode	Memory size SPC_MEMSIZE			Pre trigger SPC_PRETRIGGER			Post trigger SPC_POSTTRIGGER			Segment size SPC_SEGMENTSIZE			Loops SPC_LOOPS		
		Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step
1 Ch	Standard Single	64	Mem	32	32	Mem - 32 (defined by mem and post)	32	32	8Gi - 32	32	not used			not used		
	Standard Multi/ABA	64	Mem	32	32	8Ki (defined by segment and post)	32	32	Mem/2-32 (Limited by max pretrigger)	32	64	Mem/2	32	not used		
	Standard Gate	64	Mem	32	32	8Ki	32	32	Mem-32	32	not used			not used		
	Standard Average	For the limits in this mode please refer to the dedicated chapter in this manual.														
	FIFO Single	not used			32	8Ki	32	not used			64	8Gi - 32	32	0 (x)	4Gi - 1	1
	FIFO Multi/ABA	not used			32	8Ki (defined by segment and post)	32	32	8Gi-32 (Limited by max pretrigger)	32	64	pre+post	32	0 (x)	4Gi - 1	1
	FIFO Gate	not used			32	8Ki	32	32	8Gi - 32	32	not used			0 (x)	4Gi - 1	1
	FIFO Average	For the limits in this mode please refer to the dedicated chapter in this manual.														
2 Ch	Standard Single	64	Mem/2	32	32	Mem/2 - 32 (defined by mem and post)	32	32	8Gi - 32	32	not used			not used		
	Standard Multi/ABA	64	Mem/2	32	32	8Ki (defined by segment and post)	32	32	Mem/4-32 (Limited by max pretrigger)	32	64	Mem/4	32	not used		
	Standard Gate	64	Mem/2	32	32	8Ki	32	32	Mem/2-32	32	not used			not used		
	Standard Average	For the limits in this mode please refer to the dedicated chapter in this manual.														
	FIFO Single	not used			32	8Ki	32	not used			64	8Gi - 32	32	0 (x)	4Gi - 1	1
	FIFO Multi/ABA	not used			32	8Ki (defined by segment and post)	32	32	8Gi-32 (Limited by max pretrigger)	32	64	pre+post	32	0 (x)	4Gi - 1	1
	FIFO Gate	not used			32	8Ki	32	32	8Gi - 32	32	not used			0 (x)	4Gi - 1	1
	FIFO Average	For the limits in this mode please refer to the dedicated chapter in this manual.														
4 Ch	Standard Single	64	Mem/4	32	32	Mem/4 - 32 (defined by mem and post)	32	32	8Gi - 16	32	not used			not used		
	Standard Multi/ABA	64	Mem/4	32	32	8Ki (defined by segment and post)	32	32	Mem/4-32 (Limited by max pretrigger)	32	64	Mem/8	32	not used		
	Standard Gate	64	Mem/4	32	32	8Ki	32	32	Mem/4-16	32	not used			not used		
	Standard Average	For the limits in this mode please refer to the dedicated chapter in this manual.														
	FIFO Single	not used			32	8Ki	32	not used			64	8Gi - 32	32	0 (x)	4Gi - 1	1
	FIFO Multi/ABA	not used			32	8Ki (defined by segment and post)	32	32	8Gi-32 (Limited by max pretrigger)	32	64	pre+post	32	0 (x)	4Gi - 1	1
	FIFO Gate	not used			32	8Ki	32	32	8Gi - 32	32	not used			0 (x)	4Gi - 1	1
	FIFO Average	For the limits in this mode please refer to the dedicated chapter in this manual.														

All figures listed here are given in samples. An entry of [8Gi - 32] means [8 GiB Samples - 32] = 8,589,934,560 samples.

The given memory and memory / divider figures depend on the installed on-board memory as listed below:

	Installed Memory	
	2 GiSample	8 GiSample (Option: M5i.xxx-MEM8G5)
Mem	2 GiSample	8 GiSample
Mem / 2	1 GiSample	4 GiSample
Mem / 4	512 MiSample	2 GiSample
Mem / 8	256 MiSample	1 GiSample

Please keep in mind that this table shows all values at once. Only the absolute maximum and minimum values are shown. There might be additional limitations. Which of these values is programmed depends on the used mode. Please read the detailed documentation of the mode.

Multiple Recording and Timestamps

Multiple Recording is well matching with the timestamp option. If timestamp recording is activated each trigger event and therefore each Multiple Recording segment will get timestamped as shown in the drawing on the right.

Please keep in mind that the trigger events are timestamped, not the beginning of the acquisition. The first sample that is available is at the time position of [Timestamp - Pretrigger].

The programming details of the timestamp option is explained in an extra chapter.

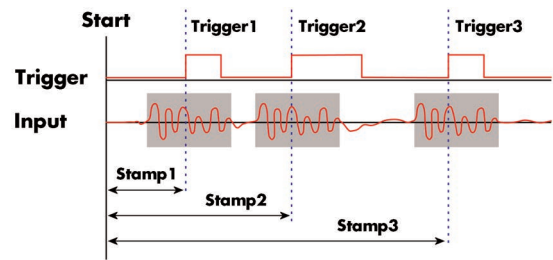


Image 62: drawing of Multiple Recording Acquisition with Timestamps

Trigger Modes

When using Multiple Recording all of the card's trigger modes can be used including the software trigger. For detailed information on the available trigger modes, please take a look at the relating chapter earlier in this manual.

Programming examples

The following example shows how to set up the card for Multiple Recording in standard mode.

```
spcm_dwSetParam_i32 (hDrv, SPC_CARDMODE, SPC_REC_STD_MULTI); // Enables Standard Multiple Recording

spcm_dwSetParam_i64 (hDrv, SPC_SEGMENTSIZE, 1024); // Set the segment size to 1024 samples
spcm_dwSetParam_i64 (hDrv, SPC_POSTTRIGGER, 768); // Set the posttrigger to 768 samples and therefore
// the pretrigger will be 256 samples
spcm_dwSetParam_i64 (hDrv, SPC_MEMSIZE, 4096); // Set the total memsize for recording to 4096 samples
// so that actually four segments will be recorded

spcm_dwSetParam_i32 (hDrv, SPC_TRIG_EXT0_MODE, SPC_TM_POS); // Set trigmode to ext. TTL mode (rising edge)
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_ORMASK, SPC_TMASK_EXT0); // and enable it within the trigger OR-mask
```

The following example shows how to set up the card for Multiple Recording in FIFO mode.

```
spcm_dwSetParam_i32 (hDrv, SPC_CARDMODE, SPC_REC_FIFO_MULTI); // Enables FIFO Multiple Recording

spcm_dwSetParam_i64 (hDrv, SPC_SEGMENTSIZE, 2048); // Set the segment size to 2048 samples
spcm_dwSetParam_i64 (hDrv, SPC_POSTTRIGGER, 1920); // Set the posttrigger to 1920 samples and therefore
// the pretrigger will be 128 samples
spcm_dwSetParam_i64 (hDrv, SPC_LOOPS, 256); // 256 segments will be recorded

spcm_dwSetParam_i32 (hDrv, SPC_TRIG_EXT0_MODE, SPC_TM_NEG); // Set trigmode to ext. TTL mode (falling edge)
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_ORMASK, SPC_TMASK_EXT0); // and enable it within the trigger OR-mask
```

Mode Gated Sampling

The Gated Sampling mode allows the data acquisition controlled by an external or an internal gate signal. Data will only be recorded if the programmed gate condition is true. When using the Gated Sampling acquisition mode it is in addition also possible to program a pre- and/or posttrigger for recording samples prior to and/or after the valid gate.

This chapter will explain all the necessary software register to set up the card for Gated Sampling properly.

The section on the allowed trigger modes deals with detailed description on the different trigger events and the resulting gates.

When using Gated Sampling the maximum pretrigger is limited as shown in the technical data section. When the programmed value exceeds that limit, the driver will return the error ERR_PRETRIGGERLEN.

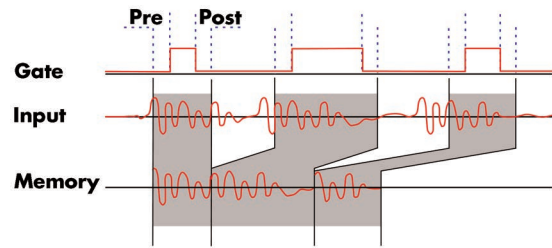


Image 63: Drawing of Gated Sampling mode

Table 129: Spectrum API: registers and settings for Gated Sampling mode

Register	Value	Direction	Description
SPC_PRETRIGGER	10030	read/write	Defines the number of samples to be recorded per channel prior to the gate start.
SPC_POSTTRIGGER	10100	read/write	Defines the number of samples to be recorded per channel after the gate end.

Acquisition modes

Standard Mode

Data will be recorded as long as the gate signal fulfils the programmed gate condition. At the end of the gate interval the recording will be stopped and the card will pause until another gates signal appears. If the total amount of data to acquire has been reached, the card stops immediately. For that reason the last gate segment is ended by the expiring memory size counter and not by the gate end signal. The total amount of samples to be recorded can be defined by the memsize register. The table below shows the register for enabling Gated Sampling. For detailed information on how to setup and start the standard acquisition mode please refer to the according chapter earlier in this manual.

Table 130: Spectrum API: card mode register and settings for Gated Sampling standard mode

Register	Value	Direction	Description
SPC_CARDMODE	9500	read/write	Defines the used operating mode
SPC_REC_STD_GATE	4		Enables Gated Sampling for standard acquisition.

The total number of samples to be recorded to the on-board memory in Standard Mode is defined by the SPC_MEMSIZE register.

Table 131: Spectrum API: memsize and loops register and register settings for Gated Replay mode

Register	Value	Direction	Description
SPC_MEMSIZE	10000	read/write	Defines the total number of samples to be recorded per channel.

FIFO Mode

The Gated Sampling in FIFO Mode is similar to the Gated Sampling in Standard Mode. In contrast to the Standard Mode you cannot program a certain total amount of samples to be recorded, but two other end conditions can be set instead. The acquisition can either run until the user stops it by software (infinite recording), or until a programmed number of gates has been recorded. The data is read continuously by the driver. This data is online available for further data processing by the user program. The advantage of Gated Sampling in FIFO mode is that you can stream data online to the host system with a lower average data rate than in conventional FIFO mode without Gated Sampling. You can make real-time data processing or store a huge amount of data to the hard disk. The table below shows the dedicated register for enabling Gated Sampling in FIFO mode. For detailed information how to setup and start the card in FIFO mode please refer to the according chapter earlier in this manual.

Table 132: Spectrum API: card mode register and Gated Sampling FIFO mode settings

Register	Value	Direction	Description
SPC_CARDMODE	9500	read/write	Defines the used operating mode
SPC_REC_FIFO_GATE	64		Enables Gated Sampling for FIFO acquisition.

The number of gates to be recorded must be set separately with the register shown in the following table:

Table 133: Spectrum API: Gated Sampling FIFO mode loops register settings

Register	Value	Direction	Description
SPC_LOOPS	10020	read/write	Defines the number of gates to be recorded
0			Recording will be infinite until the user stops it.
1 ... [4Gi - 1]			Defines the total number of gates to be recorded.

Limits of pre trigger, post trigger, memory size

The maximum memory size parameter is only limited by the number of activated channels and by the amount of installed memory. Please keep in mind that each sample needs 1 bytes of memory to be stored. Minimum memory size as well as minimum and maximum post trigger limits are independent of the activated channels or the installed memory.

Due to the internal organization of the card memory there is a certain stepsize when setting these values that has to be taken into account. The following table gives you an overview of all limits concerning pre trigger, post trigger, memory size, segment size and loops. The table shows all values in relation to the installed memory size in samples. If more memory is installed the maximum memory size figures will increase according to the complete installed memory

Table 134: Spectrum API: Limits of pre trigger, post trigger and memory size

Activated Channels	Used Mode	Memory size SPC_MEMSIZE			Pre trigger SPC_PRETRIGGER			Post trigger SPC_POSTTRIGGER			Segment size SPC_SEGMENTSIZE			Loops SPC_LOOPS		
		Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step
1 Ch	Standard Single	64	Mem	32	32	Mem - 32 (defined by mem and post)	32	32	8Gi - 32	32	not used			not used		
	Standard Multi/ABA	64	Mem	32	32	8Ki (defined by segment and post)	32	32	Mem/2-32 (Limited by max pretrigger)	32	64	Mem/2	32	not used		
	Standard Gate	64	Mem	32	32	8Ki	32	32	Mem-32	32	not used			not used		
	Standard Average	For the limits in this mode please refer to the dedicated chapter in this manual.														
	FIFO Single	not used			32	8Ki	32	not used			64	8Gi - 32	32	0 (x)	4Gi - 1	1
	FIFO Multi/ABA	not used			32	8Ki (defined by segment and post)	32	32	8Gi-32 (Limited by max pretrigger)	32	64	pre+post	32	0 (x)	4Gi - 1	1
	FIFO Gate	not used			32	8Ki	32	32	8Gi - 32	32	not used			0 (x)	4Gi - 1	1
	FIFO Average	For the limits in this mode please refer to the dedicated chapter in this manual.														
2 Ch	Standard Single	64	Mem/2	32	32	Mem/2 - 32 (defined by mem and post)	32	32	8Gi - 32	32	not used			not used		
	Standard Multi/ABA	64	Mem/2	32	32	8Ki (defined by segment and post)	32	32	Mem/4-32 (Limited by max pretrigger)	32	64	Mem/4	32	not used		
	Standard Gate	64	Mem/2	32	32	8Ki	32	32	Mem/2-32	32	not used			not used		
	Standard Average	For the limits in this mode please refer to the dedicated chapter in this manual.														
	FIFO Single	not used			32	8Ki	32	not used			64	8Gi - 32	32	0 (x)	4Gi - 1	1
	FIFO Multi/ABA	not used			32	8Ki (defined by segment and post)	32	32	8Gi-32 (Limited by max pretrigger)	32	64	pre+post	32	0 (x)	4Gi - 1	1
	FIFO Gate	not used			32	8Ki	32	32	8Gi - 32	32	not used			0 (x)	4Gi - 1	1
	FIFO Average	For the limits in this mode please refer to the dedicated chapter in this manual.														
4 Ch	Standard Single	64	Mem/4	32	32	Mem/4 - 32 (defined by mem and post)	32	32	8Gi - 16	32	not used			not used		
	Standard Multi/ABA	64	Mem/4	32	32	8Ki (defined by segment and post)	32	32	Mem/4-32 (Limited by max pretrigger)	32	64	Mem/8	32	not used		
	Standard Gate	64	Mem/4	32	32	8Ki	32	32	Mem/4-16	32	not used			not used		
	Standard Average	For the limits in this mode please refer to the dedicated chapter in this manual.														
	FIFO Single	not used			32	8Ki	32	not used			64	8Gi - 32	32	0 (x)	4Gi - 1	1
	FIFO Multi/ABA	not used			32	8Ki (defined by segment and post)	32	32	8Gi-32 (Limited by max pretrigger)	32	64	pre+post	32	0 (x)	4Gi - 1	1
	FIFO Gate	not used			32	8Ki	32	32	8Gi - 32	32	not used			0 (x)	4Gi - 1	1
	FIFO Average	For the limits in this mode please refer to the dedicated chapter in this manual.														

All figures listed here are given in samples. An entry of [8Gi - 32] means [8 GiB Samples - 32] = 8,589,934,560 samples.

The given memory and memory / divider figures depend on the installed on-board memory as listed below:

	Installed Memory	
	2 GiSample	8 GiSample (Option: M5i.xxx-MEM8GS)
Mem	2 GiSample	8 GiSample
Mem / 2	1 GiSample	4 GiSample
Mem / 4	512 MiSample	2 GiSample
Mem / 8	256 MiSample	1 GiSample

Please keep in mind that this table shows all values at once. Only the absolute maximum and minimum values are shown. There might be additional limitations. Which of these values is programmed depends on the used mode. Please read the detailed documentation of the mode.

Gate-End Alignment

Due to the structure of the on-board memory, the length of a gate will be rounded up until the next card specific alignment:

Table 135: Spectrum API: gate end alignment in Gated Sampling mode

Active Channels	M2i + M2i-exp		M4i + M4x		M2p	
	8bit	12/14/16 bit	8bit	14/16 bit	A/D and D/A 16bit	DIO
1 channel	4 Samples	2 Samples	32 Samples	16 Samples	8 Samples	—
2 channels	2 Samples	1 Samples	16 Samples	8 Samples	4 Samples	—
4 channels	1 Sample	1 Samples	8 Samples	4 Samples	2 Samples	—
8 channels	—	1 Samples	—	—	1 Samples	—
16 channels	—	1 Samples	—	—	—	8 Samples
32 channels	—	—	—	—	—	4 Samples

So in case of a M4i.22xx card with 8bit samples and one active channel, the gate-end can only stop at 32 Sample boundaries, so that up to 31 more samples can be recorded until the posttrigger starts. The timestamps themselves are not affected by this alignment.

The above listed alignment can also read out from the driver:

Table 136: Spectrum API: reading out the Gated Sampling or Gated Replay gate-end alignment value

Register	Value	Direction	Description
SPC_GATE_LEN_ALIGNMENT	200401	read only	Read out the gate-end alignment.

Gated Sampling and Timestamps

Gated Sampling and the timestamp mode fit very good together. If timestamp recording is activated each gate will get timestamped as shown in the drawing on the right. Both, beginning and end of the gate interval, are timestamped. Each gate segment will therefore produce two timestamps (Timestamp1 and Timestamp2) showing start of the gate interval and end of the gate interval. By taking both timestamps into account one can read out the time position of each gate as well as the length in samples. There is no other way to examine the length of each gate segment than reading out the timestamps.

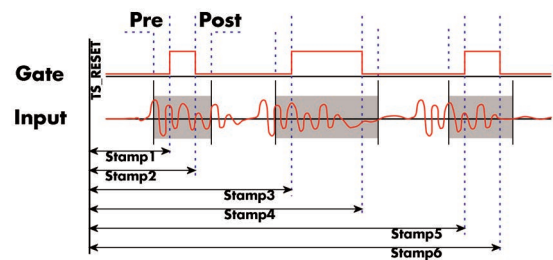


Image 64: Drawing of Gated Sampling mode and Timestamp positions

Please keep in mind that the gate signals are timestamped, not the beginning and end of the acquisition. The first sample that is available is at the time position of [Timestamp1 - Pretrigger]. The length of the gate segment is [Timestamp2 - Timestamp1 + Alignment + Pretrigger + Posttrigger]. The last sample of the gate segment is at the position [Timestamp2 + Alignment + Posttrigger]. When using the standard gate mode the end of recording is defined by the expiring memsize counter. In standard gate mode there will be an additional timestamp for the last gate segment, when the maximum memsize is reached!

The programming details of the timestamp mode are explained in an extra chapter.

Trigger

Detailed description of the external analog trigger modes

For all external analog trigger modes shown below, either the OR mask or the AND must contain the external trigger to activate the external input as trigger source:.

Table 137: Spectrum API: trigger mask registers and available register settings

Register	Value	Direction	Description
SPC_TRIG_ORMASK	40410	read/write	Defines the events included within the trigger OR mask of the card.
SPC_TRIG_ANDMASK	40430	read/write	Defines the events included within the trigger AND mask of the card.
SPC_TMASK_EXT0	2h		Enables the main external (analog) trigger 0 for the mask.
SPC_TMASK_EXT1	4h		Enables the secondary external (analog) trigger 0 for the mask.

The following pages explain the available modes in detail. All modes that only require one single trigger level are available for both external trigger inputs. All modes that require two trigger levels are only available for the main external trigger input (Ext0).

Trigger on positive edge

The trigger input is continuously sampled with the selected sample rate. If the programmed trigger level is crossed by the trigger signal from lower values to higher values (rising edge) then the gate starts.

When the signal crosses the programmed trigger level from higher values to lower values (falling edge) then the gate will stop.

As this mode is purely edge-triggered, the high level at the cards start time does not trigger the board.

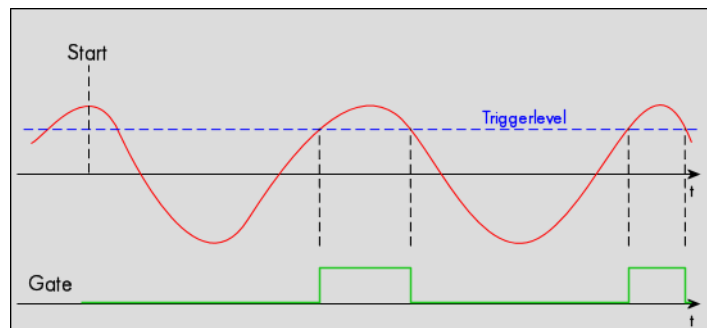


Table 138: Spectrum API: trigger register settings for trigger on positive edge

Register	Value	Direction	set to	Value
SPC_TRIG_EXT0_MODE	40510	read/write	SPC_TM_POS	1h
SPC_TRIG_EXT1_MODE	40511	read/write	SPC_TM_POS	1h
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Set it to the desired trigger level in mV	mV

Trigger on negative edge

The trigger input is continuously sampled with the selected sample rate. If the programmed trigger level is crossed by the trigger signal from higher values to lower values (falling edge) then the gate starts.

When the signal crosses the programmed trigger from lower values to higher values (rising edge) then the gate will stop.

As this mode is purely edge-triggered, the low level at the cards start time does not trigger the board.

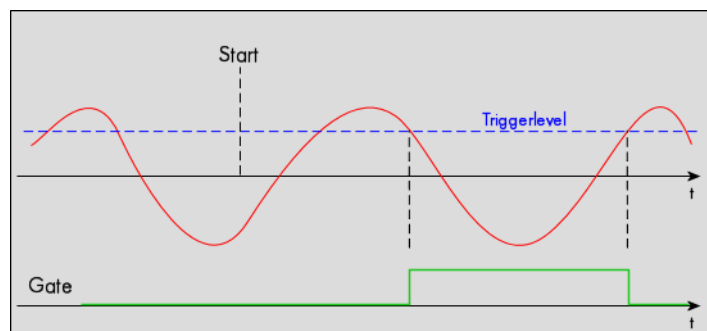



Table 139: Spectrum API: trigger register settings for trigger on negative edge

Register	Value	Direction	set to	Value
SPC_TRIG_EXT0_MODE	40510	read/write	SPC_TM_NEG	2h
SPC_TRIG_EXT1_MODE	40511	read/write	SPC_TM_NEG	2h
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Set it to the desired trigger level in mV	mV

Re-arm trigger on positive edge

The trigger input is continuously sampled with the selected sample rate. If the programmed re-arm level is crossed from lower to higher values, the trigger engine is armed and waiting for trigger. If the programmed trigger level is crossed by the trigger signal from lower values to higher values (rising edge) then the gate starts will be detected and the trigger engine will be disarmed. A new trigger event is only detected if the trigger engine is armed again.

If the programmed trigger level is crossed by the external signal from higher values to lower values (falling edge) the gate stops.

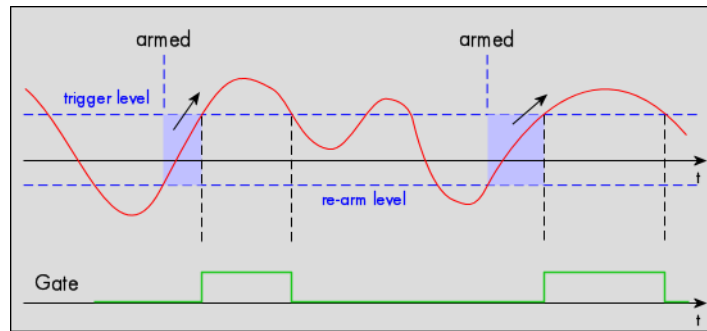

The re-arm trigger modes can be used to prevent the board from triggering on wrong edges in noisy signals.


Table 140: Spectrum API: trigger register settings for re-arm trigger on positive edge

Register	Value	Direction	set to	Value
SPC_TRIG_EXT0_MODE	40510	read/write	SPC_TM_POS SPC_TM_REARM	01000001h
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Set it to the desired trigger level in mV	mV
SPC_TRIG_EXT0_LEVEL1	42330	read/write	Defines the re-arm level in mV	mV

Re-arm trigger on negative edge

The trigger input is continuously sampled with the selected sample rate. If the programmed re-arm level is crossed from higher to lower values, the trigger engine is armed and waiting for trigger. If the programmed trigger level is crossed by the trigger signal from higher values to lower values (falling edge) then the gate starts and the trigger engine will be disarmed. A new trigger event is only detected, if the trigger engine is armed again.

If the programmed trigger level is crossed by the external signal from lower values to higher values (rising edge) the gate stops.

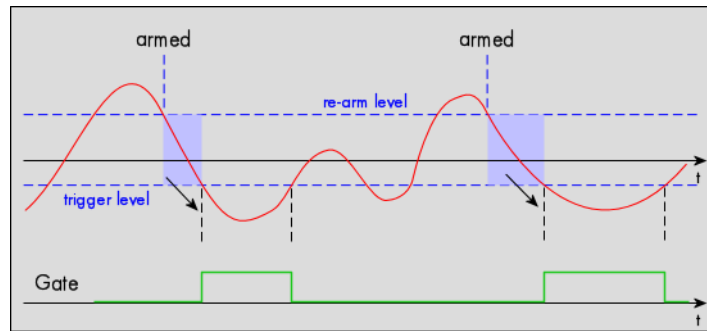

The re-arm trigger modes can be used to prevent the board from triggering on wrong edges in noisy signals.

Table 141: Spectrum API: trigger register settings for re-arm trigger on negative edge

Register	Value	Direction	set to	Value
SPC_TRIG_EXT0_MODE	40510	read/write	SPC_TM_NEG SPC_TM_REARM	01000002h
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Defines the re-arm level in mV	mV
SPC_TRIG_EXT0_LEVEL1	42330	read/write	Set it to the desired trigger level in mV	mV

Window trigger for entering signals

The trigger input is continuously sampled with the selected sample rate. The upper and the lower level define a window.

When the signal enters the window from the outside to the inside, the gate will start. When the signal leaves the window from the inside to the outside, the gate will stop.

As this mode is purely edge-triggered, the signal outside the window at the cards start time does not trigger the board.

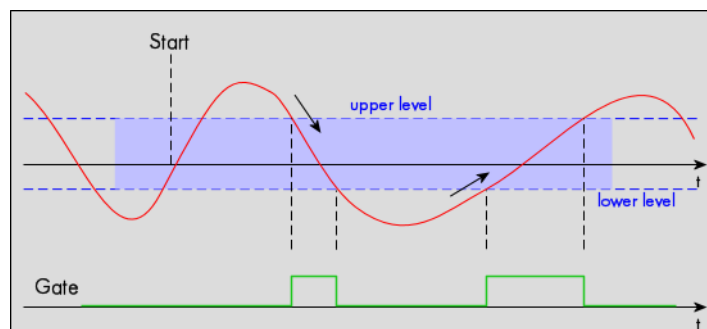


Table 142: Spectrum API: trigger register settings for window trigger on entering signals

Register	Value	Direction	set to	Value
SPC_TRIG_EXT0_MODE	40510	read/write	SPC_TM_WINENTER	00000020h
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Set it to the upper trigger level in mV	mV
SPC_TRIG_EXT0_LEVEL1	42330	read/write	Set it to the lower trigger level in mV	mV

Window trigger for leaving signals

The trigger input is continuously sampled with the selected sample rate. The upper and the lower level define a window. Every time the signal leaves the window from the inside, a trigger event will be detected.

When the signal leaves the window from the inside to the outside, the gate will start. When the signal enters the window from the outside to the inside, the gate will stop.

As this mode is purely edge-triggered, the signal within the window at the cards start time does not trigger the board.

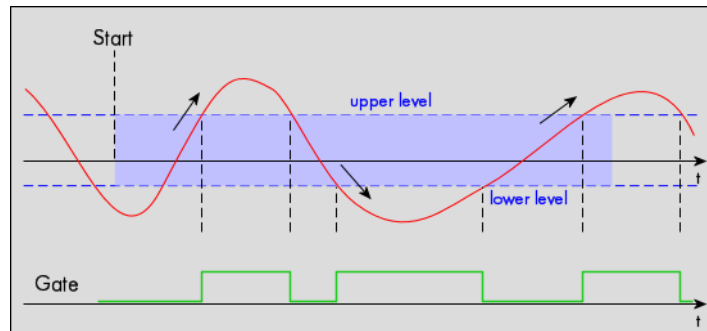


Table 143: Spectrum API: trigger register settings for window trigger on leaving signals

Register	Value	Direction	set to	Value
SPC_TRIG_EXT0_MODE	40510	read/write	SPC_TM_WINLEAVE	00000040h
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Set it to the upper trigger level in mV	mV
SPC_TRIG_EXT0_LEVEL1	42330	read/write	Set it to the lower trigger level in mV	mV

High level trigger

The external input is continuously sampled with the selected sample rate. If the signal is equal or higher than the programmed trigger level the gate starts.

When the signal is lower than the programmed trigger level the gate will stop.

As this mode is level-triggered, the high level at the cards start time does trigger the board.

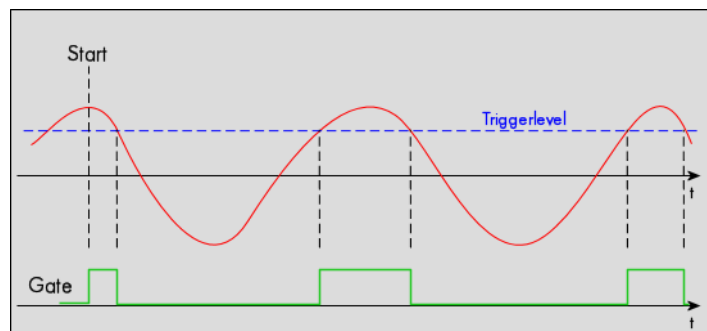


Table 144: Spectrum API: trigger register settings for high-level trigger

Register	Value	Direction	set to	Value
SPC_TRIG_EXT0_MODE	40510	read/write	SPC_TM_HIGH	00000008h
SPC_TRIG_EXT1_MODE	40511	read/write	SPC_TM_HIGH	00000008h
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Set it to the upper trigger level in mV	mV

Low level trigger

The external input is continuously sampled with the selected sample rate. If the signal is equal or lower than the programmed trigger level the gate starts.

When the signal is higher than the programmed trigger level the gate will stop.

As this mode is level-triggered, the high level at the cards start time does trigger the board.

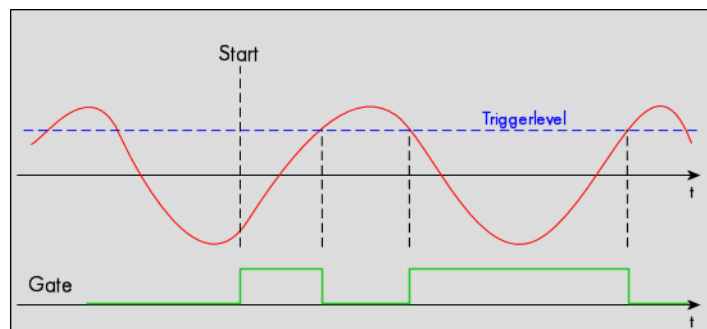


Table 145: Spectrum API: trigger register settings for low-level trigger

Register	Value	Direction	set to	Value
SPC_TRIG_EXT0_MODE	40510	read/write	SPC_TM_LOW	00000010h
SPC_TRIG_EXT1_MODE	40511	read/write	SPC_TM_LOW	00000010h
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Set it to the upper trigger level in mV	mV

In window trigger

The external input is continuously sampled with the selected sample rate. The upper and the lower level define a window.

When the signal enters the window from the outside to the inside, the gate will start.

When the signal leaves the window from the inside to the outside, the gate will stop.

As this mode is level-triggered, the signal inside the window at the cards start time does trigger the board.

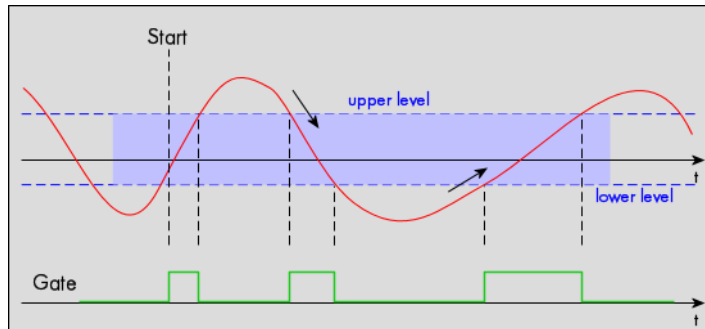


Table 146: Spectrum API: trigger register settings for in-window trigger

Register	Value	Direction	set to	Value
SPC_TRIG_EXT0_MODE	40510	read/write	SPC_TM_INWIN	00000080h
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Set it to the upper trigger level in mV	mV
SPC_TRIG_EXT0_LEVEL1	42330	read/write	Set it to the lower trigger level in mV	mV

Outside window trigger

The external input is continuously sampled with the selected sample rate. The upper and the lower level define a window.

When the signal leaves the window from the inside to the outside, the gate will start.

When the signal enters the window from the outside to the inside, the gate will stop.

As this mode is level-triggered, the signal outside the window at the cards start time does trigger the board.

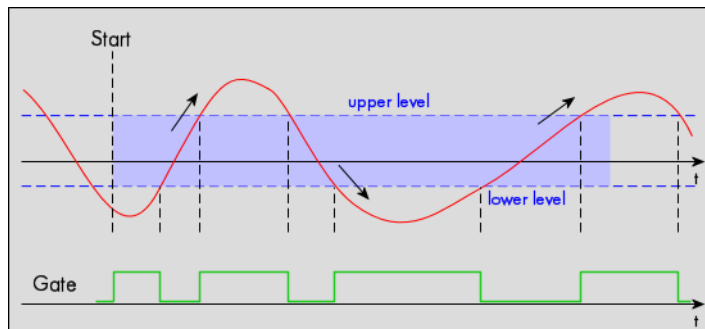


Table 147: Spectrum API: trigger register settings for outside-window trigger

Register	Value	Direction	set to	Value
SPC_TRIG_EXT0_MODE	40510	read/write	SPC_TM_OUTSIDEWIN	00000100h
SPC_TRIG_EXT0_LEVEL0	42320	read/write	Set it to the upper trigger level in mV	mV
SPC_TRIG_EXT0_LEVEL1	42330	read/write	Set it to the lower trigger level in mV	mV

Channel triggers modes

For all channel trigger modes, the OR mask must contain the corresponding input channels (channel 0 taken as example here):.

Table 148: Spectrum API: channel trigger OR mask register

Register	Value	Direction	Description
SPC_TRIG_CH_ORMASK0	40460	read/write	Defines the OR mask for the channel trigger sources.
SPC_TMASK0_CH0	1h		Enables channel0 input for the channel OR mask

Channel trigger on positive edge

The analog input is continuously sampled with the selected sample rate. If the programmed trigger level is crossed by the channel's signal from lower values to higher values (rising edge) the gate starts.

When the signal crosses the programmed trigger level from higher values to lower values (falling edge) then the gate will stop.

As this mode is purely edge-triggered, the high level at the cards start time does not trigger the board.

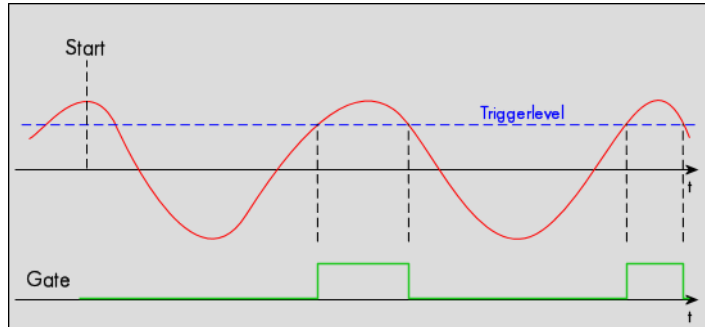


Table 149: Spectrum API: trigger register mode and level setup for trigger on positive edge

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_POS	1h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the desired trigger level relatively to the channel's input range.	board dependent

Channel trigger HIGH level

The analog input is continuously sampled with the selected sample rate. If the signal is equal or higher than the programmed trigger level the gate starts.

When the signal is lower than the programmed trigger level the gate will stop.

As this mode is level-triggered, the high level at the cards start time does trigger the board.

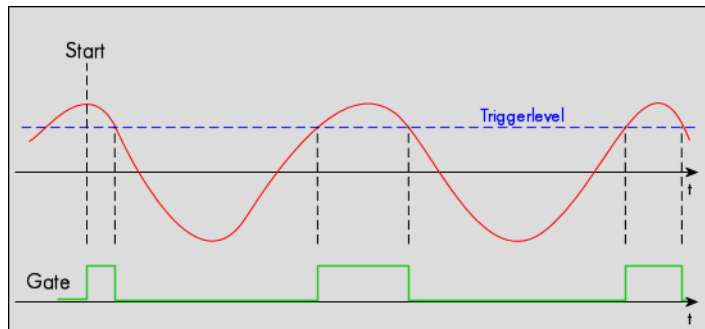


Table 150: Spectrum API: trigger register mode and level setup for trigger on high level

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_HIGH	8h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the desired trigger level relatively to the channel's input range.	board dependent

Channel trigger on negative edge

The analog input is continuously sampled with the selected sample rate. If the programmed trigger level is crossed by the channel's signal higher values to lower values (falling edge) the gate starts.

When the signal crosses the programmed trigger level from lower values to higher values (rising edge) then the gate will stop.

As this mode is purely edge-triggered, the low level at the cards start time does not trigger the board.

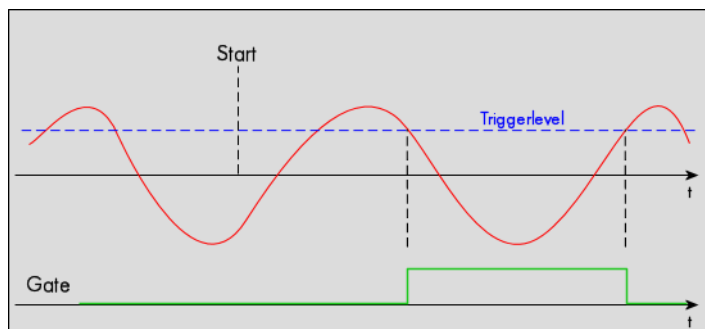


Table 151: Spectrum API: trigger register mode and level setup for trigger on negative edge

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_NEG	2h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the desired trigger level relatively to the channel's input range.	board dependent

Channel trigger LOW level

The analog input is continuously sampled with the selected sample rate. If the signal is equal or lower than the programmed trigger level the gate starts.

When the signal is higher than the programmed trigger level the gate will stop.

As this mode is level-triggered, the high level at the cards start time does trigger the board.

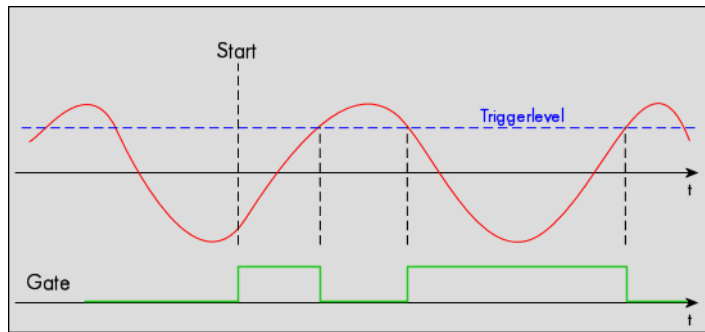


Table 152: Spectrum API: trigger register mode and level setup for trigger on low level


Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_LOW	10h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the desired trigger level relatively to the channel's input range.	board dependent

Channel re-arm trigger on positive edge

The analog input is continuously sampled with the selected sample rate. If the programmed re-arm level is crossed from lower to higher values, the trigger engine is armed and waiting for trigger.

If the programmed trigger level is crossed by the channel's signal from lower values to higher values (rising edge) then the gate starts and the trigger engine will be disarmed.

If the programmed trigger level is crossed by the channel's signal from higher values to lower values (falling edge) the gate stops.

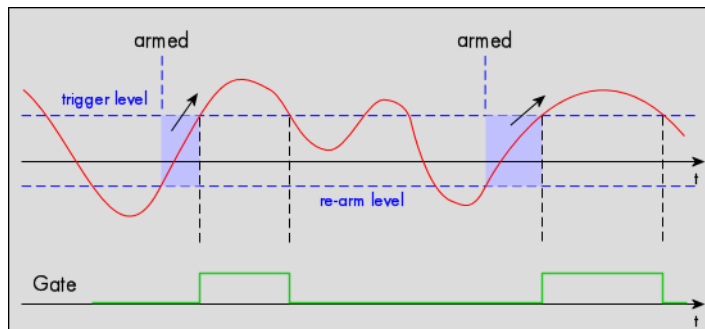

A new trigger event is only detected, if the trigger engine is armed again. The re-arm trigger modes can be used to prevent the board from triggering on wrong edges in noisy signals.

Table 153: Spectrum API: trigger register mode and level setup for trigger on positive edge with re-arm level


Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_POS SPC_TM_REARM	01000001h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the desired trigger level relatively to the channel's input range.	board dependent
SPC_TRIG_CH0_LEVEL1	42300	read/write	Defines the re-arm level relatively to the channel's input range	board dependent

Channel re-arm trigger on negative edge

The analog input is continuously sampled with the selected sample rate. If the programmed re-arm level is crossed from higher to lower values, the trigger engine is armed and waiting for trigger.

If the programmed trigger level is crossed by the channel's signal from higher values to lower values (falling edge) then the gate starts and the trigger engine will be disarmed.

If the programmed trigger level is crossed by the channel's signal from lower values to higher values (rising edge) the gate stops.

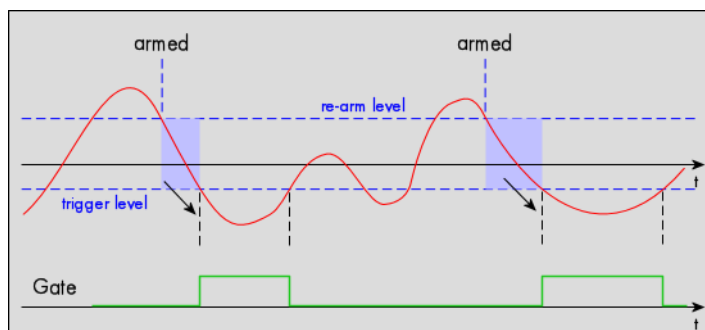

A new trigger event is only detected, if the trigger engine is armed again. The re-arm trigger modes can be used to prevent the board from triggering on wrong edges in noisy signals.

Table 154: Spectrum API: trigger register mode and level setup for trigger on negative edge with re-arm level

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_NEG SPC_TM_REARM	01000002h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Defines the re-arm level relatively to the channel's input range	board dependent
SPC_TRIG_CH0_LEVEL1	42300	read/write	Defines the re-arm level relatively to the channel's input range	board dependent

Channel window trigger for entering signals

The analog input is continuously sampled with the selected sample rate. The upper and the lower level define a window.

When the signal enters the window from the outside to the inside, the gate will start.

When the signal leaves the window from the inside to the outside, the gate will stop.

As this mode is purely edge-triggered, the signal outside the window at the cards start time does not trigger the board.

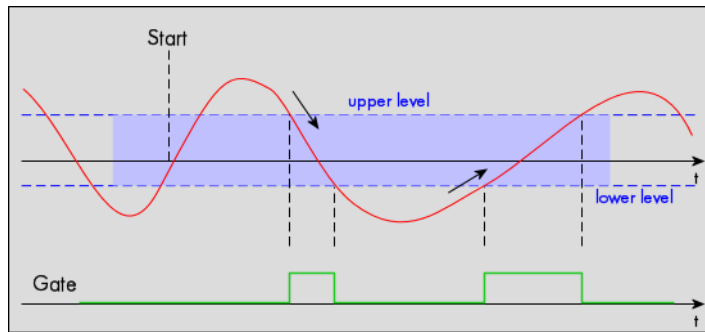


Table 155: Spectrum API: trigger register mode and level setup for trigger on signal entering window

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_WINENTER	00000020h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the upper trigger level relatively to the channel's input range.	board dependent
SPC_TRIG_CH0_LEVEL1	42300	read/write	Set it to the lower trigger level relatively to the channel's input range.	board dependent

Channel window trigger for leaving signals

The analog input is continuously sampled with the selected sample rate. The upper and the lower level define a window.

When the signal leaves the window from the inside to the outside, the gate will start.

When the signal enters the window from the outside to the inside, the gate will stop.

As this mode is purely edge-triggered, the signal within the window at the cards start time does not trigger the board.

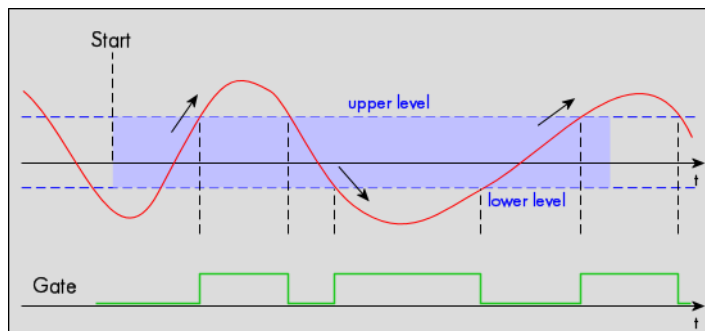


Table 156: Spectrum API: trigger register mode and level setup for trigger on signal leaving window

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_WINLEAVE	00000040h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the upper trigger level relatively to the channel's input range.	board dependent
SPC_TRIG_CH0_LEVEL1	42300	read/write	Set it to the lower trigger level relatively to the channel's input range.	board dependent

Channel window trigger for inner signals

The analog input is continuously sampled with the selected sample rate. The upper and the lower level define a window.

When the signal enters the window from the outside to the inside, the gate will start.

When the signal leaves the window from the inside to the outside, the gate will stop.

As this mode is level-triggered, the signal inside the window at the cards start time does trigger the board.

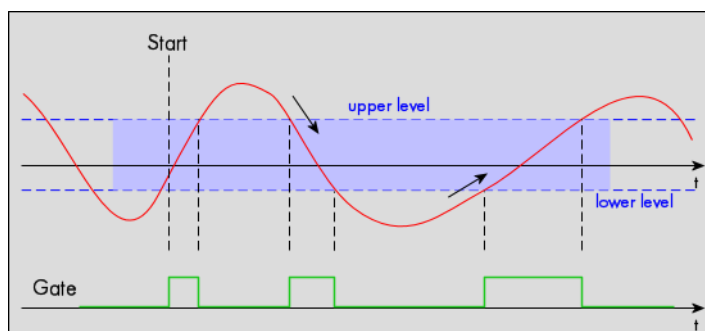


Table 157: Spectrum API: trigger register mode and level setup for trigger on signal inside window

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_INWIN	00000080h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the upper trigger level relatively to the channel's input range.	board dependent
SPC_TRIG_CH0_LEVEL1	42300	read/write	Set it to the lower trigger level relatively to the channel's input range.	board dependent

Channel window trigger for outer signals

The analog input is continuously sampled with the selected sample rate. The upper and the lower level define a window.

When the signal leaves the window from the inside to the outside, the gate will start.

When the signal enters the window from the outside to the inside, the gate will stop.

As this mode is level-triggered, the signal outside the window at the cards start time does trigger the board.

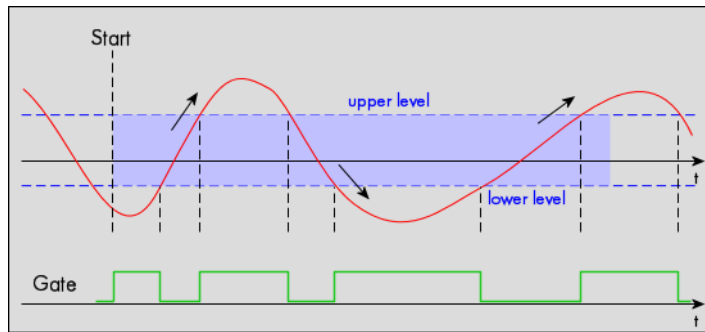


Table 158: Spectrum API: trigger register mode and level setup for trigger on signal outside window

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_OUTSIDEWIN	00000100h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the upper trigger level relatively to the channel's input range.	board dependent
SPC_TRIG_CH0_LEVEL1	42300	read/write	Set it to the lower trigger level relatively to the channel's input range.	board dependent

Channel hysteresis trigger on positive edge

The analog input is continuously sampled with the selected sample rate. If the programmed trigger level is crossed by the channel's signal from lower values to higher values (rising edge) the gate starts.

When the signal crosses the programmed hysteresis level from higher values to lower values (falling edge) then the gate will stop.

As this mode is purely edge-triggered, the high level at the cards start time does not trigger the board.

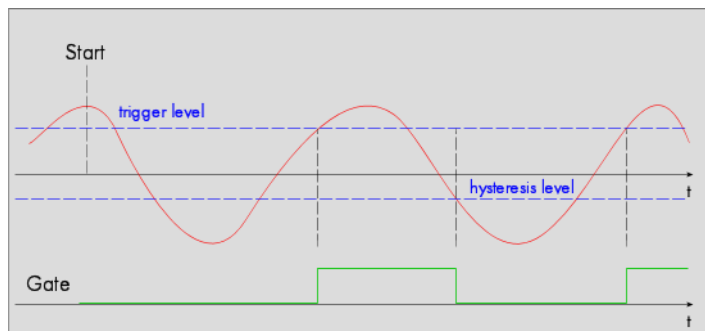


Table 159: Spectrum API: trigger register mode and level setup for trigger on positive edge with hysteresis

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_POS SPC_TM_HYSTERESIS	20000001h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the desired trigger level relatively to the channel's input range.	board dependent
SPC_TRIG_CH0_LEVEL1	42300	read/write	Defines the hysteresis level relatively to the channel's input range	board dependent

Channel hysteresis trigger HIGH level

The analog input is continuously sampled with the selected sample rate. If the signal is equal or higher than the programmed trigger level the gate starts.

When the signal is lower than the programmed hysteresis level the gate will stop.

As this mode is level-triggered, the high level at the cards start time does trigger the board.

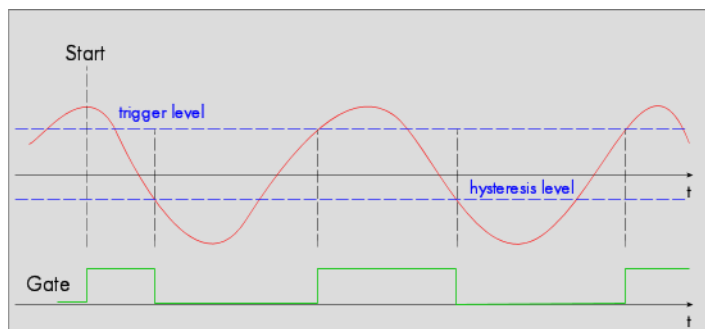


Table 160: Spectrum API: trigger register mode and level setup for trigger on high level with hysteresis

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_HIGH SPC_TM_HYSTERESIS	20000008h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the desired trigger level relatively to the channel's input range.	board dependent
SPC_TRIG_CH0_LEVEL1	42300	read/write	Defines the hysteresis level relatively to the channel's input range	board dependent

Channel hysteresis trigger on negative edge

The analog input is continuously sampled with the selected sample rate. If the programmed trigger level is crossed by the channel's signal higher values to lower values (falling edge) the gate starts.

When the signal crosses the programmed hysteresis level from lower values to higher values (rising edge) then the gate will stop.

As this mode is purely edge-triggered, the low level at the cards start time does not trigger the board.

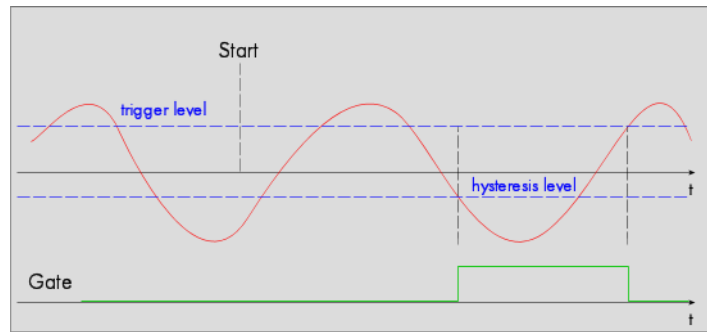


Table 161: Spectrum API: trigger register mode and level setup for trigger on negative edge with hysteresis

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_NEG SPC_TM_HYSTERESIS	2000002h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the desired trigger level relatively to the channel's input range.	board dependent
SPC_TRIG_CH0_LEVEL1	42300	read/write	Defines the hysteresis level relatively to the channel's input range	board dependent

Channel hysteresis trigger LOW level

The analog input is continuously sampled with the selected sample rate. If the signal is equal or lower than the programmed trigger level the gate starts.

When the signal is higher than the programmed hysteresis level the gate will stop.

As this mode is level-triggered, the high level at the cards start time does trigger the board.

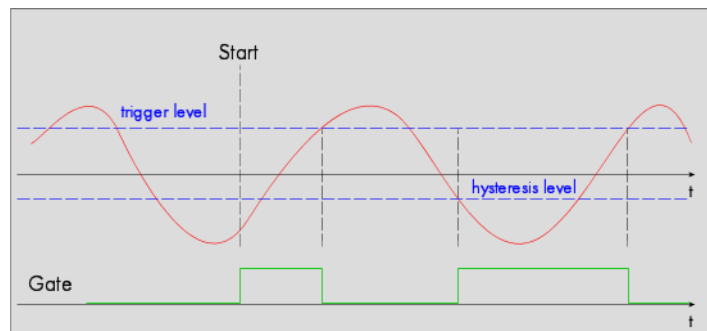


Table 162: Spectrum API: trigger register mode and level setup for trigger on low level with hysteresis


Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_LOW SPC_TM_HYSTERESIS	20000010h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the desired trigger level relatively to the channel's input range.	board dependent
SPC_TRIG_CH0_LEVEL1	42300	read/write	Defines the hysteresis level relatively to the channel's input range	board dependent

Channel re-arm hysteresis trigger on positive edge

The analog input is continuously sampled with the selected sample rate. If the programmed re-arm/hysteresis level is crossed from lower to higher values, the trigger engine is armed and waiting for trigger.

If the programmed trigger level is crossed by the channel's signal from lower values to higher values (rising edge) then the gate starts and the trigger engine will be disarmed.

If the programmed re-arm/hysteresis level is crossed by the channel's signal from higher values to lower values (falling edge) the gate stops.

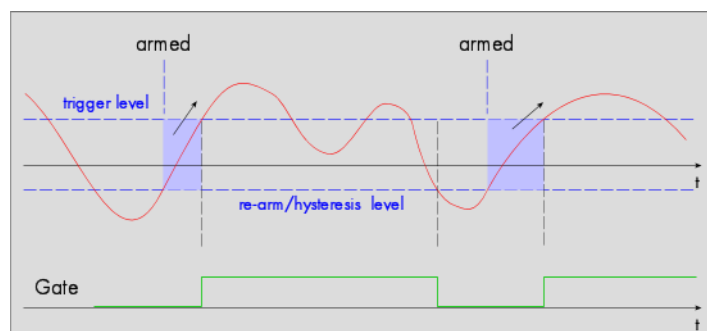

A new trigger event is only detected, if the trigger engine is armed again. The re-arm trigger modes can be used to prevent the board from triggering on wrong edges in noisy signals.

Table 163: Spectrum API: trigger register mode and level setup for trigger on positive edge with re-arm level and hysteresis


Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_POS SPC_TM_REARM SPC_TM_HYSTERESIS	21000001h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Set it to the desired trigger level relatively to the channel's input range.	board dependent
SPC_TRIG_CH0_LEVEL1	42300	read/write	Defines the re-arm and hysteresis level relatively to the channel's input range	board dependent

Channel re-arm hysteresis trigger on negative edge

The analog input is continuously sampled with the selected sample rate. If the programmed re-arm/hysteresis level is crossed from higher to lower values, the trigger engine is armed and waiting for trigger.

If the programmed trigger level is crossed by the channel's signal from higher values to lower values (falling edge) then the gate starts and the trigger engine will be disarmed.

If the programmed re-arm/hysteresis level is crossed by the channel's signal from lower values to higher values (rising edge) the gate stops.

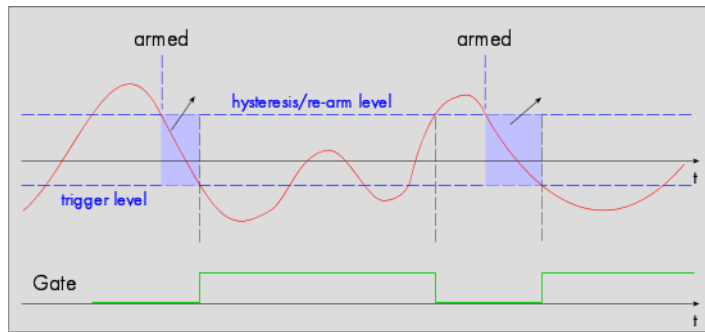

A new trigger event is only detected, if the trigger engine is armed again. The re-arm trigger modes can be used to prevent the board from triggering on wrong edges in noisy signals.

Table 164: Spectrum API: trigger register mode and level setup for trigger on negative edge with re-arm level and hysteresis

Register	Value	Direction	set to	Value
SPC_TRIG_CH0_MODE	40610	read/write	SPC_TM_NEG SPC_TM_REARM SPC_TM_HYSTERESIS	21000002h
SPC_TRIG_CH0_LEVEL0	42200	read/write	Defines the re-arm level relatively to the channel's input range	board dependent
SPC_TRIG_CH0_LEVEL1	42300	read/write	Defines the re-arm and hysteresis level relatively to the channel's input range	board dependent

Programming examples

The following examples shows how to set up the card for Gated Sampling in standard mode for Gated Sampling in FIFO mode.

```

spcm_dwSetParam_i32 (hDrv, SPC_CARDMODE, SPC_REC_STD_GATE); // Enables Standard Gated Sampling

spcm_dwSetParam_i64 (hDrv, PRETRIGGER, 256);                // Set the pretrigger to 256 samples
spcm_dwSetParam_i64 (hDrv, POSTTRIGGER, 2048);              // Set the posttrigger to 2048 samples
spcm_dwSetParam_i64 (hDrv, SPC_MEMSIZE, 8192);              // Set the total memsize for recording to 8192 samples

spcm_dwSetParam_i32 (hDrv, SPC_TRIG_EXT0_MODE, SPC_TM_POS); // Set triggermode to ext. TTL mode (rising edge)
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_EXT0_LEVEL0, 1500);    // Set trigger level to +1500 mV
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_ORMASK, SPC_TMASK_EXT0); // and enable it within the trigger OR-mask

```

```

spcm_dwSetParam_i32 (hDrv, SPC_CARDMODE, SPC_REC_FIFO_GATE); // Enables FIFO Gated Sampling

spcm_dwSetParam_i64 (hDrv, PRETRIGGER, 128);                // Set the pretrigger to 128 samples
spcm_dwSetParam_i64 (hDrv, POSTTRIGGER, 512);              // Set the posttrigger to 512 samples
spcm_dwSetParam_i64 (hDrv, SPC_LOOP, 1024);                // 1024 gates will be recorded

spcm_dwSetParam_i32 (hDrv, SPC_TRIG_EXT0_MODE, SPC_TM_NEG); // Set triggermode to ext. TTL mode (falling edge)
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_EXT0_LEVEL0, -1500);   // Set trigger level to -1500 mV
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_ORMASK, SPC_TMASK_EXT0); // and enable it within the trigger OR-mask

```


Timestamps

General information

The timestamp function is used to record trigger events relative to the beginning of the measurement, relative to a fixed time-zero point or synchronized to an external reset clock. The reset clock can come from a radio clock, a GPS signal or from any other external machine.

The timestamp is internally realized as a very wide counter that is running with the currently used sampling rate. The counter is reset either by explicit software command or depending on the mode by the start of the card. On receiving the trigger event the current counter value is stored in an extra FIFO memory.

This function is designed as an enhancement to the Multiple Recording mode and is also used together with the Gated Sampling and ABA mode, but can also be used with plain single acquisitions.

Each recorded timestamp consists of the number of samples that has been counted since the last counter reset has been done. The actual time in relation to the reset command can be easily calculated by the formula on the right. Please note that the timestamp recalculation depends on the currently used sampling rate. Please have a look at the clock chapter to see how to read out the sampling rate.

$$t = \frac{\text{Timestamp}}{\text{Sampling rate}}$$

If you want to know the time between two timestamps, you can simply calculate this by the formula on the right.

$$\Delta t = \frac{\text{Timestamp}_{n+1} - \text{Timestamp}_n}{\text{Sampling rate}}$$

The following registers can be used for the timestamp function:

Table 165: Spectrum API: timestamp related register and available timestamp commands

Register	Value	Direction	Description
SPC_TIMESTAMP_STARTTIME	47030	read/write	Return the reset time when using reference clock mode. Hours are placed in bit 16 to 23, minutes are placed in bit 8 to 15, seconds are placed in bit 0 to 7. Returned value is expressed as a UTC time.
SPC_TIMESTAMP_STARTDATE	47031	read/write	Return the reset date when using reference clock mode. The year is placed in bit 16 to 31, the month is placed in bit 8 to 15 and the day of month is placed in bit 0 to 7
SPC_TIMESTAMP_TIMEOUT	47045	read/write	Set's a timeout in milliseconds for waiting of an reference clock edge. Writing a zero disables the timeout. Default value is zero. Allowed values are 10 ms up to 10000 ms.
SPC_TIMESTAMP_AVALIABLEMODES	47001	read	Returns all available modes as a bitmap. Modes are listed below
SPC_TIMESTAMP_CMD	47000	read/write	Programs a timestamp mode and performs commands as listed below
SPC_TSMODE_DISABLE	0		Timestamp is disabled.
SPC_TS_RESET	1h		The counters are reset and the local PC time is stored for read out by SPC_TIMESTAMP_STARTTIME and SPC_TIMESTAMP_STARTDATE registers. Only usable with mode TSMODE_STANDARD
SPC_TSMODE_STANDARD	2h		Standard mode, counter is reset by explicit reset command SPC_TS_RESET or SPC_TS_RESET_WAITREFCLOCK.
SPC_TSMODE_STARTRESET	4h		Counter is reset on every card start, all timestamps are in relation to card start.
SPC_TS_RESET_WAITREFCLK	8h		Similar as SPC_TS_RESET, but aimed at SPC_TSCNT_REFLOCKxxx modes: The counters are reset then the driver waits for the reference edge as long as defined by the timestamp timeout time. After detecting the edge, the local PC time is stored for read out by SPC_TIMESTAMP_STARTTIME and SPC_TIMESTAMP_STARTDATE registers. Only usable with mode TSMODE_STANDARD
SPC_TSCNT_INTERNAL	100h		Counter is running with complete width on sampling clock
SPC_TSCNT_REFLOCKPOS	200h		Counter is split, upper part is running with external reference clock positive edge, lower part is running with sampling clock
SPC_TSCNT_REFLOCKNEG	400h		Counter is split, upper part is running with external reference clock negative edge, lower part is running with sampling clock
SPC_TSIOACQ_ENABLE	1000h		Enables the trigger synchronous acquisition of the multi-purpose inputs with every stored timestamp in the upper 64 bit. See Multi-purpose I/O chapter for details on these inputs.
SPC_TSFEAT_NONE	0		No additional timestamp is created. The total number of stamps is only trigger related.
SPC_TSFEAT_STORE1STABA	10000h		Enables the creation of one additional timestamp for the first A area sample when using the optional ABA (dual-time-base) mode.
SPC_TSFEAT_TRGSRC	80000h		Reding this flag from the SPC_TIMESTAMP_AVALIABLEMODES indicates that the card is capable of encoding the trigger source into the timestamp. Writing this flag to the SPC_TIMESTAMP_CMD register enables the storage of the trigger source in the upper 64 bit of the timestamp value.

Writing of SPC_TS_RESET and SPC_TS_RESET_WAITREFCLK to the command register can only have an effect on the counters, if the cards clock generation is already active and the timestamp mode has been written to the hardware. This is the case when the card either has already done an acquisition with enabled timestamps after the last reset or if the clock setup and timestamp mode has already been actively transferred to the card by issuing the M2CMD_CARD_WRITESETUP command.



Example for setting timestamp mode:

The timestamp mode must consist of one of the mode constants, one of the counter and one of the feature constants:

```
// setting timestamp mode to standard using internal clocking
spcm_dwSetParam_i32 (hDrv, SPC_TIMESTAMP_CMD, SPC_TSMODE_STANDARD | SPC_TSCNT_INTERNAL | SPC_TSFEAT_NONE);

// setting timestamp mode to start reset mode using internal clocking
spcm_dwSetParam_i32 (hDrv, SPC_TIMESTAMP_CMD, SPC_TSMODE_STARTRESET | SPC_TSCNT_INTERNAL | SPC_TSFEAT_NONE);

// setting timestamp mode to standard using external reference clock with positive edge
spcm_dwSetParam_i32 (hDrv, SPC_TIMESTAMP_CMD, SPC_TSMODE_STANDARD | SPC_TSCNT_REFCLOCKPOS | SPC_TSFEAT_NONE);
```

Timestamp modes

Standard mode

In standard mode the timestamp counter is set to zero once by writing the TS_RESET command to the command register. After that command the counter counts continuously independent of start and stop of acquisition. The timestamps of all recorded trigger events are referenced to this common zero time. With this mode you can calculate the exact time difference between different recordings and also within one acquisition (if using for example Multiple Recording).

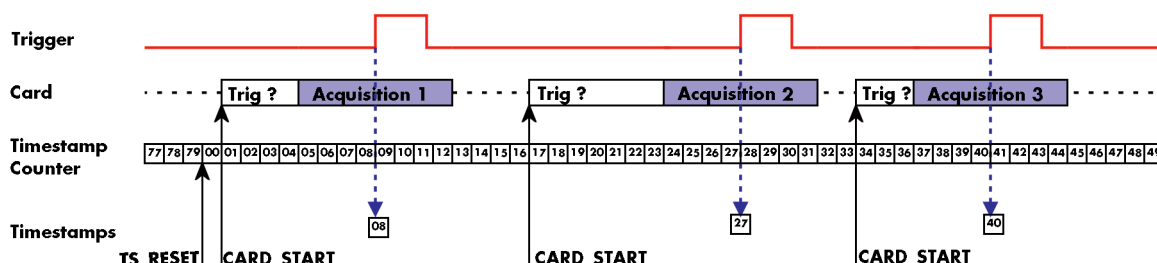


Image 65: drawing of timestamp acquisition in standard mode in relation to card start and trigger detection

The following table shows the valid values that can be written to the timestamp command register for this mode:

Table 166: Spectrum API: timestamp commands for standard mode

Register	Value	Direction	Description
SPC_TIMESTAMP_CMD	47000	read/write	Programs a timestamp mode and performs commands as listed below
SPC_TSMODE_DISABLE	0		Timestamp is disabled.
SPC_TS_RESET	1h		The timestamp counter is set to zero
SPC_TSMODE_STANDARD	2h		Standard mode, counter is reset by explicit reset command.
SPC_TSCNT_INTERNAL	100h		Counter is running with complete width on sampling clock

Please keep in mind that this mode only work sufficiently as long as you don't change the sampling rate between two acquisitions that you want to compare.



StartReset mode

In StartReset mode the timestamp counter is set to zero on every start of the card. After starting the card the counter counts continuously. The timestamps of one recording are referenced to the start of the recording. This mode is very useful for Multiple Recording and Gated Sampling (see according chapters for detailed information on these two optional modes).

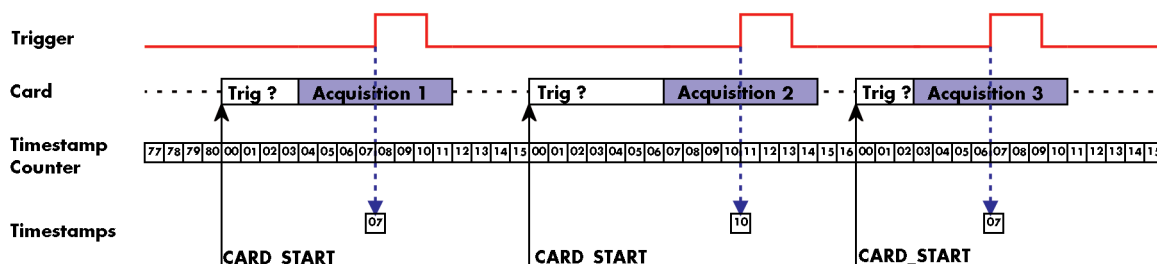


Image 66: drawing of timestamp acquisition in start-reset mode in relation to card start and trigger detection

The following table shows the valid values that can be written to the timestamp command register.

Table 167: Spectrum API: timestamp commands for star-reset mode

Register	Value	Direction	Description
SPC_TIMESTAMP_CMD	47000	read/write	Programs a timestamp mode and performs commands as listed below
SPC_TSMODE_DISABLE	0		Timestamp is disabled.
SPC_TSMODE_STARTRESET	4h		Counter is reset on every card start, all timestamps are in relation to card start.
SPC_TSCNT_INTERNAL	100h		Counter is running with complete width on sampling clock

Refclock mode

In addition to the counter counting the samples a second separate counter is utilized. An additional external signal is used, which affects both counters and needs to be fed in externally. This external reference clock signal will reset the sample counter and also increase the second counter. The second counter holds the number of the clock edges that have occurred on the external reference clock signal and the sample counter holds the position within the current reference clock period with the resolution of the sampling rate.

This mode can be used to obtain an absolute time reference when using an external radio clock or a GPS receiver. In that case the higher part is counting the seconds since the last reset and the lower part is counting the position inside the second using the current sampling rate.

Please keep in mind that as this mode uses an additional external signal and can therefore only be used when connecting an reference clock signal on the related connector on the card:



- X0 on M4i/M4x/M5i and related digitizerNETBOX products
- X1 on M2p and related digitizerNETBOX products

The counting is initialized with the timestamp reset command. Both counters will then be set to zero.

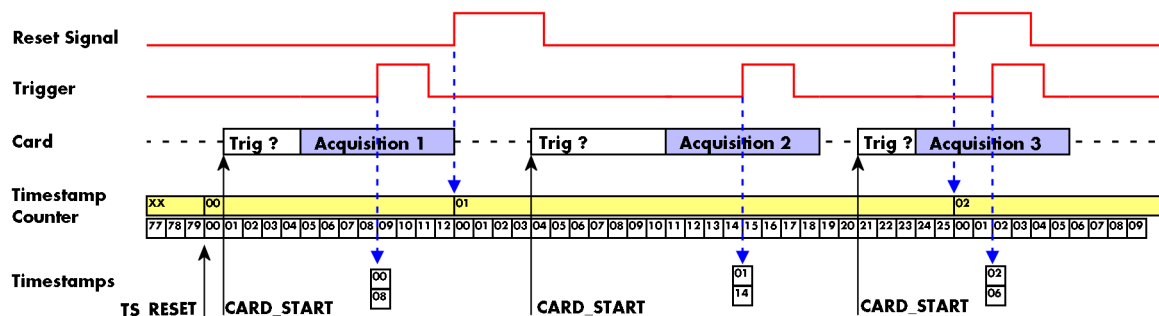


Image 67: drawing of timestamp acquisition in refclock mode in relation to card start and trigger detection

The following table shows the valid values that can be written to the timestamp command register for this mode:

Table 168: Spectrum API: timestamp commands for refclock mode

Register	Value	Direction	Description
SPC_TIMESTAMP_STARTTIME	47030	read/write	Return the reset time when using reference clock mode. Hours are placed in bit 16 to 23, minutes are placed in bit 8 to 15, seconds are placed in bit 0 to 7
SPC_TIMESTAMP_STARTDATE	47031	read/write	Return the reset date when using reference clock mode. The year is placed in bit 16 to 31, the month is placed in bit 8 to 15 and the day of month is placed in bit 0 to 7
SPC_TIMESTAMP_TIMEOUT	47045	read/write	Sets a timeout in milliseconds for waiting for a reference clock edge. Allowed values are 10ms up to 10000ms.
SPC_TIMESTAMP_CMD	47000	read/write	Programs a timestamp mode and performs commands as listed below
SPC_TSMODE_DISABLE	0		Timestamp is disabled.
SPC_TS_RESET	1h		The counters are reset and the local PC time is stored for read out by SPC_TIMESTAMP_STARTTIME and SPC_TIMESTAMP_STARTDATE registers.
SPC_TS_RESET_WAITREFCLK	8h		Similar as SPC_TS_RESET, but aimed at SPC_TSCNT_REFCLOCKxxx modes: The counters are reset then the driver waits for the reference edge as long as defined by the timeout time. After detecting the edge, the local PC time is stored for read out by SPC_TIMESTAMP_STARTTIME and SPC_TIMESTAMP_STARTDATE registers.
SPC_TSMODE_STANDARD	2h		Standard mode, counter is reset by explicit reset command.
SPC_TSMODE_STARTRESET	4h		Counter is reset on every card start, all timestamps are in relation to card start.
SPC_TSCNT_REFCLOCKPOS	200h		Counter is split, upper part is running with external reference clock positive edge, lower part is running with sampling clock
SPC_TSCNT_REFCLOCKNEG	400h		Counter is split, upper part is running with external reference clock negative edge, lower part is running with sampling clock

To synchronize the external reference clock signal with the PC clock it is possible to perform a timestamp reset command which waits a specified time for the occurrence of the external clock edge. As soon as the clock edge is found the function stores the current PC time and date which can be used to get the absolute time. As the timestamp reference clock can also be used with other clocks that don't need to be synchronized with the PC clock the waiting time can be programmed using the SPC_TIMESTAMP_TIMEOUT register.

Example for initialization of timestamp reference clock and synchronization of a seconds signal with the PC clock:

```

spcm_dwSetParam_i32 (hDrv, SPC_TIMESTAMP_CMD, SPC_TSMODE_STANDARD | SPC_TSCNT_REFCLOCKPOS);
spcm_dwSetParam_i32 (hDrv, SPC_TIMESTAMP_TIMEOUT, 1500);
if (ERR_TIMESTAMP_SYNC == spcm_dwSetParam_i32 (hDrv, SPC_TIMESTAMP_CMD, SPC_TS_RESET_WAITREFCLK))
    printf ("Synchronization with external clock signal failed\n");

// now we read out the stored synchronization clock and date
int32 lSyncDate, lSyncTime;
spcm_dwGetParam_i32 (hDrv, SPC_TIMESTAMP_STARTDATE, &lSyncDate);
spcm_dwGetParam_i32 (hDrv, SPC_TIMESTAMP_STARTTIME, &lSyncTime); // expressed as UTC time

// and print the start date and time information (European format: day.month.year hour:minutes:seconds)
printf ("Start date: %02d.%02d.%04d\n", lSyncDate & 0xff, (lSyncDate >> 8) & 0xff, (lSyncDate >> 16) & 0xffff);
printf ("Start time: %02d:%02d:%02d\n", (lSyncTime >> 16) & 0xff, (lSyncTime >> 8) & 0xff, lSyncTime & 0xff);

```

Reading out the timestamps

General

The timestamps are stored in an extra FIFO that is located in hardware on the card. This extra FIFO can read out timestamps using DMA transfer similar to the DMA transfer of the main sample data DMA transfer. The card has three completely independent busmaster DMA engines in hardware allowing the simultaneous transfer of both timestamp and sample data.

As seen in the picture there are separate FIFOs holding ABA (if available) and timestamp data.

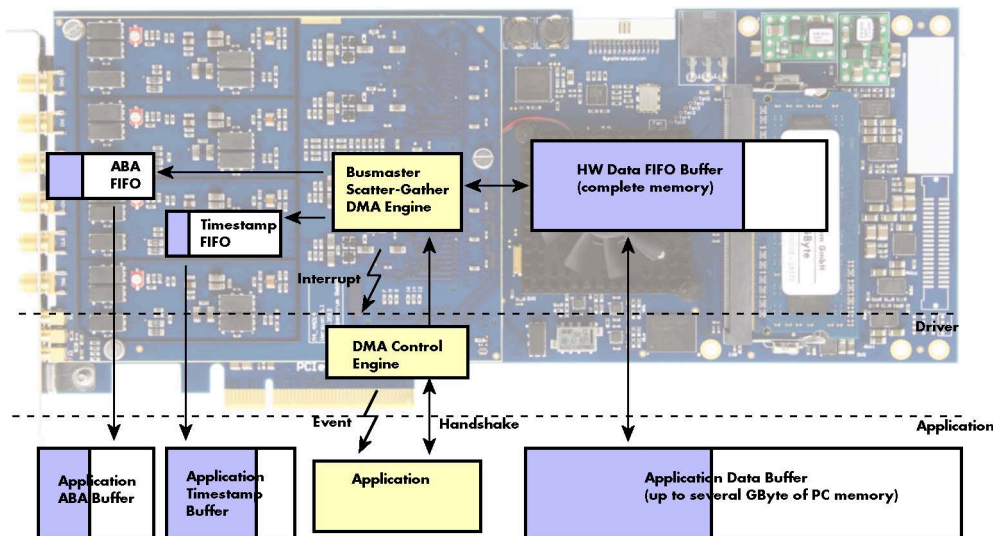


Image 68: Overview of acquisition data, ABA data and timestamp data DMA transfer

Although an M4i is shown here, this applies to M4x and M2p cards as well. M5i cards are similar, but don't have the ABA path. Each FIFO has its own DMA channel, the way data is handled by the DMA engine is similar for both kinds of extra FIFOs and is also very similar to the main sample data transfer engine. Therefore additional information can be found in the chapter explaining the main data transfer.

Commands and Status information for extra transfer buffers.

As explained above the data transfer is performed with the same command and status registers like the card control and sample data transfer. It is possible to send commands for card control, data transfer and extra FIFO data transfer at the same time

Table 169: Spectrum API: extra DMA commands (ABA and Timestamp)

Register	Value	Direction	Description
SPC_M2CMD	100	write only	Executes a command for the card or data transfer
M2CMD_EXTRA_STARTDMA	100000h		Starts the DMA transfer for an already defined buffer.
M2CMD_EXTRA_WAITDMA	200000h		Waits until the data transfer has ended or until at least the amount of bytes defined by notify size are available. This wait function also takes the timeout parameter into account.
M2CMD_EXTRA_STOPDMA	400000h		Stops a running DMA transfer. Data is invalid afterwards.
M2CMD_EXTRA_POLL	800000h		Polls data without using DMA. As DMA has some overhead and has been implemented for fast data transfer of large amounts of data it is in some cases more simple to poll for available data. Please see the detailed examples for this mode. It is not possible to mix DMA and polling mode.

The extra FIFO data transfer can generate one of the following status information:

Table 170: Spectrum API: extra DMA status (ABA and Timestamp)

Register	Value	Direction	Description
SPC_M2STATUS	110	read only	Reads out the current status information
M2STAT_EXTRA_BLOCKREADY	1000h		The next data block as defined in the notify size is available. It is at least the amount of data available but it also can be more data.
M2STAT_EXTRA_END	2000h		The data transfer has completed. This status information will only occur if the notify size is set to zero.
M2STAT_EXTRA_OVERRUN	4000h		The data transfer had on overrun (acquisition) or underrun (replay) while doing FIFO transfer.
M2STAT_EXTRA_ERROR	8000h		An internal error occurred while doing data transfer.

Data Transfer using DMA

Data transfer consists of two parts: the buffer definition and the commands/status information that controls the transfer itself. Extra data transfer shares the command and status register with the card control, data transfer commands and status information.

The DMA based data transfer mode is activated as soon as the M2CMD_EXTRA_STARTDMA is given. Please see next chapter to see how the polling mode works.

Definition of the transfer buffer

Before any data transfer can start it is necessary to define the transfer buffer with all its details. The definition of the buffer is done with the `spcm_dwDefTransfer` function as explained in an earlier chapter. The following example will show the definition of a transfer buffer for timestamp data, definition for ABA data is similar:

```
spcm_dwDefTransfer_i64 (hDrv, SPCM_BUF_TIMESTAMP, SPCM_DIR_CARDTOPC, 0, pvBuffer, 0, lLenOfBufferInBytes);
```

In this example the notify size is set to zero, meaning that we don't want to be notified until all extra data has been transferred. Please have a look at the sample data transfer in an earlier chapter to see more details on the notify size.

Please note that extra data transfer is only possible from card to PC and there's no programmable offset available for this transfer.

M5i cards only:

On M5i cards the `lLenOfBufferInBytes` parameter needs to be an integer multiple of 64 bytes.



Buffer handling

A data buffer handshake is implemented in the driver which allows to run the card in different data transfer modes. The software transfer buffer is handled as one large buffer for each kind of data (timestamp and ABA) which is on the one side controlled by the driver and filled automatically by busmaster DMA from the hardware extra FIFO buffer and on the other hand it is handled by the user who set's parts of this software buffer available for the driver for further transfer. The handshake is fulfilled with the following 3 software registers:

Table 171: Spectrum API: ABA and Timestamp DMA buffer handling registers

Register	Value	Direction	Description
SPC_ABA_AVAIL_USER_LEN	210	read	This register contains the currently available number of bytes that are filled with newly transferred slow ABA data. The user can now use this ABA data for own purposes, copy it, write it to disk or start calculations with this data.
SPC_ABA_AVAIL_USER_POS	211	read	The register holds the current byte index position where the available ABA bytes start. The register is just intended to help you and to avoid own position calculation
SPC_ABA_AVAIL_CARD_LEN	212	write	After finishing the job with the new available ABA data the user needs to tell the driver that this amount of bytes is again free for new data to be transferred.
SPC_TS_AVAIL_USER_LEN	220	read	This register contains the currently available number of bytes that are filled with newly transferred timestamp data. The user can now use these timestamps for own purposes, copy it, write it to disk or start calculations with the timestamps.
SPC_TS_AVAIL_USER_POS	221	read	The register holds the current byte index position where the available timestamp bytes start. The register is just intended to help you and to avoid own position calculation
SPC_TS_AVAIL_CARD_LEN	222	write	After finishing the job with the new available timestamp data the user needs to tell the driver that this amount of bytes is again free for new data to be transferred.

Directly after start of transfer the `SPC_XXX_AVAIL_USER_LEN` is every time zero as no data is available for the user and the `SPC_XXX_AVAIL_CARD_LEN` is every time identical to the length of the defined buffer as the complete buffer is available for the card for transfer.

The counter that is holding the user buffer available bytes (`SPC_XXX_AVAIL_USER_LEN`) is sticking to the defined notify size at the `DefTransfer` call. Even when less bytes already have been transferred you won't get notice of it if the notify size is programmed to a higher value.



Remarks

- The transfer between hardware FIFO buffer and application buffer is done with scatter-gather DMA using a busmaster DMA controller located on the card. Even if the PC is busy with other jobs data is still transferred until the application buffer is completely used.
- As shown in the drawing above the DMA control will announce new data to the application by sending an event. Waiting for an event is done internally inside the driver if the application calls one of the wait functions. Waiting for an event does not consume any CPU time and is therefore highly requested if other threads do lot of calculation work. However it is not necessary to use the wait functions and one can simply request the current status whenever the program has time to do so. When using this polling mode the announced available

bytes still stick to the defined notify size!

- If the on-board FIFO buffer has an overrun data transfer is stopped immediately.

Buffer handling example for DMA timestamp transfer (ABA transfer is similar, just using other registers)

```
int8* pcData = (int8*) pvAllocMemPageAligned (lBufSizeInBytes);

// we now define the transfer buffer with the minimum notify size of one page = 4 KiByte
spcm_dwDefTransfer_i64 (hDrv, SPCM_BUF_TIMESTAMP, SPCM_DIR_CARDTOPC, 4096, (void*) pcData, 0, lBufSizeInBytes);

do
{
    // we wait for the next data to be available. After this call we get at least 4KiByte of data to proceed
    dwError = spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_EXTRA_STARTDMA | M2CMD_EXTRA_WAITDMA);

    if (!dwError)
    {
        // if there was no error we can proceed and read out the current amount of available data
        spcm_dwGetParam_i32 (hDrv, SPC_TS_AVAIL_USER_LEN, &lAvailBytes);
        spcm_dwGetParam_i32 (hDrv, SPC_TS_AVAIL_USER_POS, &lBytePos);

        printf ("We now have %d new bytes available\n", lAvailBytes);
        printf ("The available data starts at position %d\n", lBytePos);

        // we take care not to go across the end of the buffer
        if ((lBytePos + lAvailBytes) >= lBufSizeInBytes)
            lAvailBytes = lBufSizeInBytes - lBytePos;

        // our do function gets a pointer to the start of the available data section and the length
        vProcessTimestamps (&pcData[lBytePos], lAvailBytes);

        // the buffer section is now immediately set available for the card
        spcm_dwSetParam_i32 (hDrv, SPC_TS_AVAIL_CARD_LEN, lAvailBytes);
    }
}
while (!dwError); // we loop forever if no error occurs
```

The extra FIFO has a quite small size compared to the main data buffer. As the transfer is done initiated by the hardware using busmaster DMA this is not critical as long as the application data buffers are large enough and as long as the extra transfer is started BEFORE starting the card.



Data Transfer using Polling

If the extra data is quite slow and the delay caused by the notify size on DMA transfers is unacceptable for your application it is possible to use the polling mode. Please be aware that the polling mode uses CPU processing power to get the data and that there might be an overrun if your CPU is otherwise busy. You should only use polling mode in special cases and if the amount of data to transfer is not too high.

Most of the functionality is similar to the DMA based transfer mode as explained above.

The polling data transfer mode is activated as soon as the M2CMD_EXTRA_POLL is executed.

Definition of the transfer buffer

This is similar to the above explained DMA buffer transfer. The value „notify size“ is ignored and should be set to 4Ki (4096).

Buffer handling

The buffer handling is also similar to the DMA transfer. As soon as one of the registers SPC_TS_AVAIL_USER_LEN or SPC_ABA_AVAIL_USER_LEN is read the driver will read out all available data from the hardware and will return the number of bytes that has been read. In minimum this will be one DWORD = 4 bytes.

Buffer handling example for polling timestamp transfer (ABA transfer is similar, just using other registers)

```
int8* pcData = (int8*) pvAllocMemPageAligned (lBufSizeInBytes);

// we now define the transfer buffer with the minimum notify size of one page = 4 KiByte
spcm_dwDefTransfer_i64 (hDrv, SPCM_BUF_TIMESTAMP, SPCM_DIR_CARDTOPC, 4096, (void*) pcData, 0, lBufSizeInBytes);

// we start the polling mode
dwError = spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_EXTRA_POLL);

// this is our polling loop
do
{
    spcm_dwGetParam_i32 (hDrv, SPC_TS_AVAIL_USER_LEN, &lAvailBytes);
    spcm_dwGetParam_i32 (hDrv, SPC_TS_AVAIL_USER_POS, &lBytePos);

    if (lAvailBytes > 0)
    {
        printf ("We now have %d new bytes available\n", lAvailBytes);
        printf ("The available data starts at position %d\n", lBytePos);

        // we take care not to go across the end of the buffer
        if ((lBytePos + lAvailBytes) >= lBufSizeInBytes)
            lAvailBytes = lBufSizeInBytes - lBytePos;

        // our do function get's a pointer to the start of the available data section and the length
        vProcessTimestamps (&pcData[lBytePos], lAvailBytes);

        // the buffer section is now immediately set available for the card
        spcm_dwSetParam_i32 (hDrv, SPC_TS_AVAIL_CARD_LEN, lAvailBytes);
    }
}
while (!dwError); // we loop forever if no error occurs
```

Comparison of DMA and polling commands

This chapter shows you how small the difference in programming is between the DMA and the polling mode:

	DMA mode	Polling mode
Define the buffer	spcm_dwDefTransfer_i64 (hDrv, SPCM_BUF_TIMESTAMP, SPCM_DIR...);	spcm_dwDefTransfer_i64 (hDrv, SPCM_BUF_TIMESTAMP, SPCM_DIR...);
Start the transfer	spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_EXTRA_STARTDMA)	spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_EXTRA_POLL)
Wait for data	spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_EXTRA_WAITDMA)	not in polling mode
Available bytes?	spcm_dwGetParam_i32 (hDrv, SPC_TS_AVAIL_USER_LEN, &lBytes);	spcm_dwGetParam_i32 (hDrv, SPC_TS_AVAIL_USER_LEN, &lBytes);
Min available bytes	programmed notify size	4 bytes
Current position?	spcm_dwGetParam_i32 (hDrv, SPC_TS_AVAIL_USER_LEN, &lBytes);	spcm_dwGetParam_i32 (hDrv, SPC_TS_AVAIL_USER_LEN, &lBytes);
Free buffer for card	spcm_dwSetParam_i32 (hDrv, SPC_TS_AVAIL_CARD_LEN, lBytes);	spcm_dwSetParam_i32 (hDrv, SPC_TS_AVAIL_CARD_LEN, lBytes);

Data format

Each timestamp is 128 bit long and internally mapped to two consecutive 64 bit (8 bytes) values. The lower 64 bit (counter value) contains the number of clocks that have been recorded with the currently used sampling rate since the last counter-reset has been done. The matching time can easily be calculated as described in the general information section at the beginning of this chapter.

The values the counter is counting and that are stored in the timestamp FIFO represent the moments the trigger event occurs internally. Compared to the real external trigger event, these values are delayed. This delay is fix and therefore can be ignored, as it will be identical for all recordings with the same setup.

Standard data format

When internally mapping the timestamp from 128 bit to two 64 bit values, the unused upper 64 bits are filled up with zeros.

Table 172: Spectrum API: timestamp sample format for standard mode

Timestamp Mode	16 th byte	...	11 th byte	10 th byte	9 th byte	8 th byte	7 th byte	6 th byte	5 th byte	4 th byte	3 rd byte	2 nd byte	1 st byte
Standard/StartReset	0h					64 bit wide Timestamp							
Refclock mode	0h					24 bit wide Refclock edge counter (seconds counter)				40 bit wide Timestamp			

Extended timestamp data format

Sometimes it is useful to store the level of additional external static signals together with a recording, such as e.g. control inputs of an external input multiplexer or settings of other external equipment. When programming a special flag the upper 64 bit of every 128 bit timestamp

value is not (as in standard data mode) filled up with leading zeros, but with the values of either the digital inputs (X3, X2, X1) or optionally also (X10 ..X3). The following table shows the resulting 128 bit timestamps.

Table 173: Spectrum API: timestamp sample format for extended mode

Timestamp Mode	16 th byte	...	14 th byte	13 th byte	...	9 th byte	8 th byte	7 th byte	6 th byte	5 th byte	4 th byte	3 rd byte	2 nd byte	1 st byte
Standard/StartReset	0h			Extra Data Word			64 bit wide Timestamp							
Refclock mode	0h			Extra Data Word			24 bit wide Refclock edge counter (seconds counter)				40 bit wide Timestamp			

The above mentioned „Extra Data Word“ contains the following 40bit wide data, depending on the selected timestamp data format:

Table 174: Spectrum API: timestamp extra data word format

Timestamp Data Format	Bit 39	...	Bit 32	Bit 31	Bit ...	Bit 26	Bit 25	...	Bit 16	Bit 15	...	Bit 13	Bit 12	Bit 11	Bit 10	...	Bit 0
no special data format is set	0h																
SPC_TSXIOACQ_ENABLE	X10 .. X3 (option)			0h						X2 .. X0			0h				
SPC_TSFEAT_TRGSRC	0h						Trigger source bit-mask PXI sources (see table below)			0h			Trigger source bit-mask (Ch0 .. Force) (see table below)				
SPC_TSXIOACQ_ENABLE SPC_TSFEAT_TRGSRC	X10 .. X3 (option)			0h			Trigger source bit-mask PXI sources (see table below)			X2 .. X0			0h		Trigger source bit-mask (Ch0 .. Force) (see table below)		

The multi-purpose lines X10...X3 are only available when the additional digital I/O option (DigSMA) is installed. For cards where this option is not installed, Bits 39 down to 32 are always zero. Depending on the chosen mode for acquiring digital data (see Multi-Purpose I/O chapter for details) either group (X2..X0) or (X10..X3) are active as digital input lines, whilst the inactive group is always zero.



The trigger sources are encoded as follows:

SPC_TRGSRC_MASK_CH0	1h	Set when a trigger event occurring on channel 0 was leading to final trigger event.
SPC_TRGSRC_MASK_CH1	2h	Set when a trigger event occurring on channel 1 was leading to final trigger event.
SPC_TRGSRC_MASK_CH2	4h	Set when a trigger event occurring on channel 2 was leading to final trigger event.
SPC_TRGSRC_MASK_CH3	8h	Set when a trigger event occurring on channel 3 was leading to final trigger event.
SPC_TRGSRC_MASK_EXT0	100h	Set when a trigger event occurring on external trigger(Ext0) was leading to final trigger event.
SPC_TRGSRC_MASK_EXT1	200h	Set when a trigger event occurring on external trigger(Ext1) was leading to final trigger event.
SPC_TRGSRC_MASK_FORCE	400h	Set when a trigger event occurring by using the force trigger command is leading to final trigger event.
SPC_TRGSRC_MASK_PXI0	10000h	M4x only: Set when a trigger event occurring on PXI trigger 0 was leading to final trigger event.
SPC_TRGSRC_MASK_PXI1	20000h	M4x only: Set when a trigger event occurring on PXI trigger 1 was leading to final trigger event.
SPC_TRGSRC_MASK_PXI2	40000h	M4x only: Set when a trigger event occurring on PXI trigger 2 was leading to final trigger event.
SPC_TRGSRC_MASK_PXI3	80000h	M4x only: Set when a trigger event occurring on PXI trigger 3 was leading to final trigger event.
SPC_TRGSRC_MASK_PXI4	100000h	M4x only: Set when a trigger event occurring on PXI trigger 4 was leading to final trigger event.
SPC_TRGSRC_MASK_PXI5	200000h	M4x only: Set when a trigger event occurring on PXI trigger 5 was leading to final trigger event.
SPC_TRGSRC_MASK_PXI6	400000h	M4x only: Set when a trigger event occurring on PXI trigger 6 was leading to final trigger event.
SPC_TRGSRC_MASK_PXI7	800000h	M4x only: Set when a trigger event occurring on PXI trigger 7 was leading to final trigger event.
SPC_TRGSRC_MASK_PXISTAR	1000000h	M4x only: Set when a trigger event occurring on PXI star-trigger was leading to final trigger event.
SPC_TRGSRC_MASK_PXIDSTARB	2000000h	M4x only: Set when a trigger event occurring on PXI DStarB was leading to final trigger event.

Selecting the timestamp data format

Table 175: Spectrum API: timestamp data format register

Register	Value	Direction	Description
SPC_TIMESTAMP_CMD	47000	read/write	Programs a timestamp mode and performs commands as listed below
SPC_TSXIOACQ_ENABLE	1000h		Enables the trigger synchronous acquisition of the X0...X2 or X3...X10 inputs with every stored timestamp in the upper 64 bit.
SPC_TSFEAT_TRGSRC	80000h		Enables the storage of the trigger source in the upper 64 bit of the timestamp value.

The selection between the different data format for the timestamps is done with a flag that is written to the timestamp command register. As this register is organized as a bitfield, the data format selection is available for all possible timestamp modes and different data modes can be combined.

Combination of Memory Segmentation Options with Timestamps

This topic should give you a brief overview how the timestamp option interacts with the options Multiple Recording and ABA mode for which the timestamps option has been made.

Multiple Recording and Timestamps

Multiple Recording is well matching with the timestamp option. If timestamp recording is activated each trigger event and therefore each Multiple Recording segment will get timestamped as shown in the drawing on the right.

Please keep in mind that the trigger events are timestamped, not the beginning of the acquisition. The first sample that is available is at the time position of [Timestamp - Pretrigger].

The programming details of the timestamp option is explained in an extra chapter.

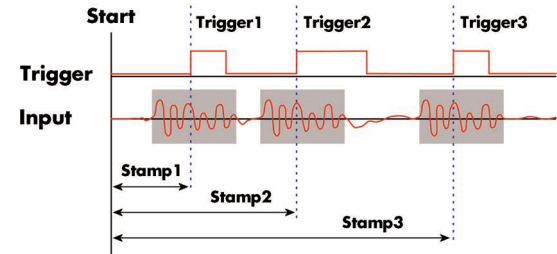


Image 69: drawing of Multiple Recording Acquisition with Timestamps

The following example shows the setup of the Multiple Recording mode together with activated timestamps recording and a short display of the acquired timestamps. The example doesn't care for the acquired data itself and doesn't check for error:

```
// setup of the Multiple Recording mode
spcm_dwSetParam_i32 (hDrv, SPC_CARDMODE, SPC_REC_STD_MULTI); // Enable Standard Multiple Recording
spcm_dwSetParam_i64 (hDrv, SPC_SEGMENTSIZE, 1024); // Segment size is 1 KiSamples, Posttrigger is 768
spcm_dwSetParam_i64 (hDrv, SPC_POSTTRIGGER, 768); // samples and pretrigger therefore 256 samples.
spcm_dwSetParam_i64 (hDrv, SPC_MEMSIZE, 4096); // 4 KiSamples in total acquired -> 4 segments

// setup the Timestamp mode and make a reset of the timestamp counter
spcm_dwSetParam_i32 (hDrv, SPC_TIMESTAMP_CMD, SPC_TSMODE_STANDARD | SPC_TSCNT_INTERNAL);
spcm_dwSetParam_i32 (hDrv, SPC_TIMESTAMP_CMD, SPC_TSMODE_RESET);

// now we define a buffer for timestamp data and start the acquisition. Each timestamp is 128 bit = 16 bytes.
int64* pllStamps = (int64*) pvAllocMemPageAligned (16 * 4);
spcm_dwDefTransfer_i64 (hDrv, SPCM_BUF_TIMESTAMP, SPCM_DIR_CARDTOPC, 0, (void*) pllStamps, 0, 4 * 16);
spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_CARD_START | M2CMD_CARD_ENABLETRIGGER | M2CMD_EXTRA_STARTDMA);

// we wait for the end timestamps transfer which will be received if all segments have been recorded
spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_EXTRA_WAITDMA);

// as we now have the timestamps we just print them and calculate the time in milli seconds
// for simplicity only the lower 64 bit part of the 128 bit stamp is used, hence only every
// second array element of pllStamps is used here.
int64 llSamplerate;
double dTime_ms;
spcm_dwGetParam_i64 (hDrv, SPC_SAMPLERATE, &llSamplerate);

for (int i = 0; i < 4; i++)
{
    dTime_ms = 1000.0 * pllStamps[2 * i] / llSamplerate;

    printf ("%d: %I64d samples = %.3f ms\n", i, pllStamps[2 * i], dTime_ms);
}
```

Gate-End Alignment

Due to the structure of the on-board memory, the length of a gate will be rounded up until the next card specific alignment:

Table 176: Spectrum API: gate end alignment in Gated Sampling mode

Active Channels	M2i + M2i-exp		M4i + M4x		M2p	
	8bit	12/14/16 bit	8bit	14/16 bit	A/D and D/A 16bit	DIO
1 channel	4 Samples	2 Samples	32 Samples	16 Samples	8 Samples	—
2 channels	2 Samples	1 Samples	16 Samples	8 Samples	4 Samples	—
4 channels	1 Sample	1 Samples	8 Samples	4 Samples	2 Samples	—
8 channels	—	1 Samples	—	—	1 Samples	—
16 channels	—	1 Samples	—	—	—	8 Samples
32 channels	—	—	—	—	—	4 Samples

So in case of a M4i.22xx card with 8bit samples and one active channel, the gate-end can only stop at 32 Sample boundaries, so that up to 31 more samples can be recorded until the posttrigger starts. The timestamps themselves are not affected by this alignment.

The above listed alignment can also read out from the driver:

Table 177: Spectrum API: reading out the Gated Sampling or Gated Replay gate-end alignment value

Register	Value	Direction	Description
SPC_GATE_LEN_ALIGNMENT	200401	read only	Read out the gate-end alignment.

Gated Sampling and Timestamps

Gated Sampling and the timestamp mode fit very good together. If timestamp recording is activated each gate will get timestamped as shown in the drawing on the right. Both, beginning and end of the gate interval, are timestamped. Each gate segment will therefore produce two timestamps (Timestamp1 and Timestamp2) showing start of the gate interval and end of the gate interval. By taking both timestamps into account one can read out the time position of each gate as well as the length in samples. There is no other way to examine the length of each gate segment than reading out the timestamps.

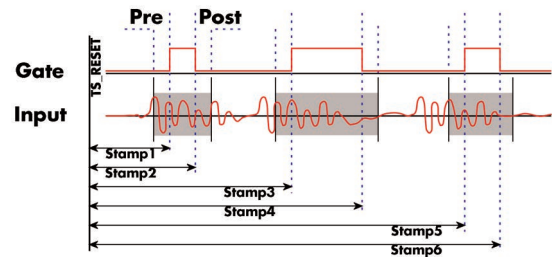


Image 70: Drawing of Gated Sampling mode and Timestamp positions

Please keep in mind that the gate signals are timestamped, not the beginning and end of the acquisition. The first sample that is available is at the time position of [Timestamp1 - Pretrigger]. The length of the gate segment is [Timestamp2 - Timestamp1 + Alignment + Pretrigger + Posttrigger]. The last sample of the gate segment is at the position [Timestamp2 + Alignment + Posttrigger]. When using the standard gate mode the end of recording is defined by the expiring memsize counter. In standard gate mode there will be an additional timestamp for the last gate segment, when the maximum memsize is reached!

The programming details of the timestamp mode are explained in an extra chapter.

The following example shows the setup of the Gated Sampling mode together with activated timestamps recording and a short display of the acquired timestamps. The example doesn't care for the acquired data itself and doesn't check for error:

```
// setup of the Gated Sampling mode
spcm_dwSetParam_i32 (hDrv, SPC_CARDMODE, SPC_REC_STD_GATE); // Enables Standard Gated Sampling
spcm_dwSetParam_i64 (hDrv, SPC_PRETRIGGER, 32); // 32 samples to acquire before gate start
spcm_dwSetParam_i64 (hDrv, SPC_POSTTRIGGER, 32); // 32 samples to acquire before gate end
spcm_dwSetParam_i64 (hDrv, SPC_MEMSIZE, 4096); // 4 KiSamples in total acquired

// setup the Timestamp mode and make a reset of the timestamp counter
spcm_dwSetParam_i32 (hDrv, SPC_TIMESTAMP_CMD, SPC_TSMODE_STANDARD | SPC_TSCNT_INTERNAL);
spcm_dwSetParam_i32 (hDrv, SPC_TIMESTAMP_CMD, SPC_TS_RESET);

// now we define a buffer for timestamp data and start acquisition, each timestamp is 128 bit = 16 bytes
// as we don't know the number of gate intervals we define the buffer quite large
int64* pllStamps = (int64*) pvAllocMemPageAligned (16 * 1000);
spcm_dwDefTransfer_i64 (hDrv, SPC_BUF_TIMESTAMP, SPCM_DIR_CARDTOPC, 0, (void*) pllStamps, 0, 1000 * 16);
spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_CARD_START | M2CMD_CARD_ENABLETRIGGER | M2CMD_EXTRA_STARTDMA);

// we wait for the end of timestamps transfer and read out the number of timestamps that have been acquired
int32 lAvailTimestampBytes;
spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_EXTRA_WAITDMA);
spcm_dwSetParam_i32 (hDrv, SPC_TS_AVAIL_USER_LEN, &lAvailTimestampBytes);

// as we now have the timestamps we just print them and calculate the time in milli seconds
// for simplicity only the lower 64 bit part of the 128 bit stamp is used, hence only every
// second array element of pllStamps is used here.
int64 llSamplerate, llLen, llAlign;
double dTime_ms;
spcm_dwGetParam_i64 (hDrv, SPC_SAMPLERATE, &llSamplerate);
spcm_dwGetParam_i64 (hDrv, SPC_GATE_LEN_ALIGNMENT, &llAlign);

// each even 128 bit timestamp is the start position of a gate segment each odd stamp is the end position
for (int i = 0; (i < (lAvailTimestampBytes / 16)) && (i < 1000); i++)
{
    dTime_ms = 1000.0 * pllStamps[4 * i] / llSamplerate;
    llLen = pllStamps[4 * i + 2] - pllStamps[4 * i] + 32 + 32; // (stop - start) + pre + post

    if ((llLen % llAlign) != 0)
        llLen = (llLen + llAlign) - (llLen % llAlign); // correct for alignment

    printf ("%d: Start %I64d samples = %.3f ms", i, pllStamps[4 * i], dTime_ms);
    printf ("(Len = %I64d samples)\n", llLen);
}
```

ABA Mode and Timestamps

The ABA mode is well matching with the timestamp option. If timestamp recording is activated, each trigger event and therefore each B time base segment will get time stamped as shown in the drawing on the right.

Please keep in mind that the trigger events - located in the B area - are time stamped, not the beginning of the acquisition. The first B sample that is available is at the time position of [Timestamp - Pretrigger].

The first A area sample is related to the card start and therefore in a fixed but various settings dependent relation to the timestamped B sample. To bring exact relation between the first A area sample (and therefore all area A samples) and the B area samples it is possible to let the card stamp the first A area sample automatically after the card start. The following table shows the register to enable this mode:

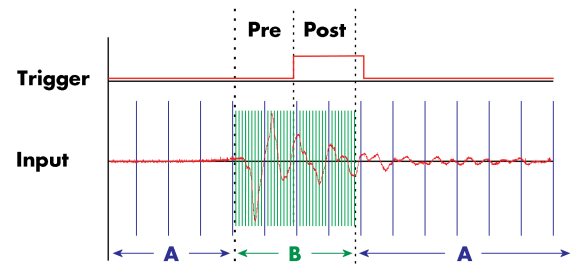


Image 71: Drawing of ABA mode

Table 178: Spectrum API: timestamp command register and ABA mode settings

Register	Value	Direction	Description
SPC_TIMESTAMP_CMD	47000	read/write	Programs a timestamp setup including mode and additional features
SPC_TSFEAT_MASK	F0000h		Mask for the feature relating bits of the SPC_TIMESTAMP_CMD bitmask.
SPC_TSFEAT_STORE1STABA	10000h		Enables storage of one additional timestamp for the first A area sample (B time base related) in addition to the trigger related timestamps.
SPC_TSFEAT_NONE	0h		No additional timestamp is created. The total number of stamps is only trigger related.

This mode is compatible with all existing timestamp modes. Please keep in mind that the timestamp counter is running with the B area time-base.

```
// normal timestamp setup (e.g. setting timestamp mode to standard using internal clocking)
uint32 dwTimestampMode = (SPC_TSMODE_STANDARD | SPC_TSMODE_DISABLE);

// additionally enable index of the first A area sample
dwTimestampMode |= SPC_TSFEAT_STORE1STABA;

spcm_dwSetParam_i32 (hDrv, SPC_TIMESTAMP_CMD, dwTimestampMode);
```

The programming details of the ABA mode and timestamp modes are each explained in a dedicated chapter in this manual.

ABA mode (dual timebase)

General information

The ABA mode allows the acquisition of data with a dual timebase. In case of trigger event the inputs are sampled very fast with the programmed sampling rate. This part is similar to the Multiple Recording option. But instead of having no data in between the segments one has the opportunity to continuously sample the inputs with a slower sampling rate the whole time. Combining this with the recording of the timestamps gives you a complete acquisition with a dual timebase as shown in the drawing.

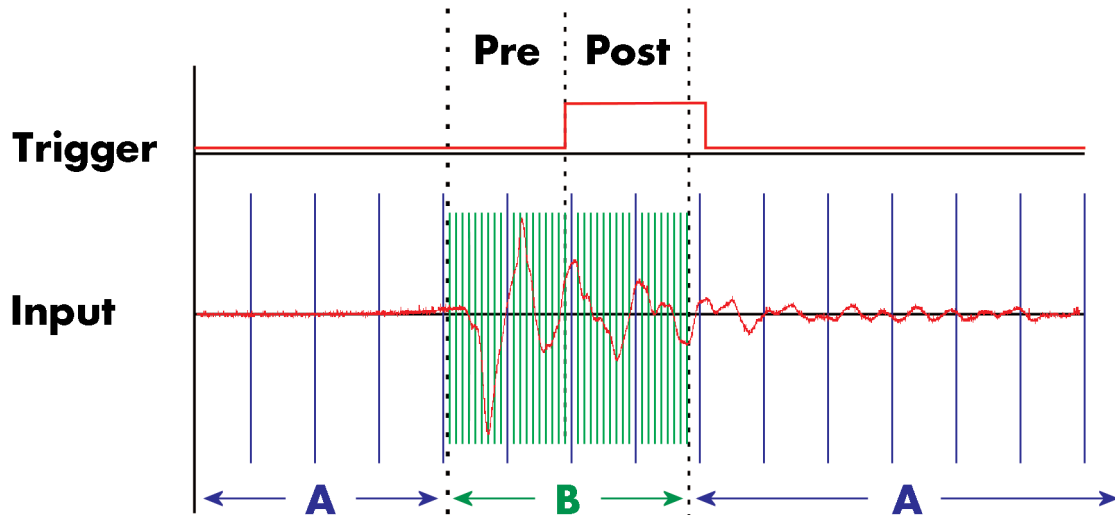


Image 72: overview of ABA mode data acquisition with slow A-data and fast B-data

As seen in the drawing the area around the trigger event is sampled between pretrigger and posttrigger with full sampling speed (area B of the acquisition). Outside of this area B the input is sampled with the slower ABA clock (area A of the acquisition). As changing sampling clock on the fly is not possible there is no real change in the sampling speed but area A runs continuously with a slow sampling speed without stopping when the fast sampling takes place. As a result one gets a continuous slow sampled acquisition (area A) with some fast sampled parts (area B)

The ABA mode is available for standard recording as well as for FIFO recording. In case of FIFO recording ABA and the acquisition of the fast sampled segments will run continuously until it is stopped by the user.

A second possible application for the ABA mode is the use of the ABA data for slow monitoring of the inputs while waiting for an acquisition. In that case one wouldn't record the timestamps but simply monitor the current values by acquiring ABA data.

The ABA mode needs a second clock base. As explained above the acquisition is not changing the sampling clock but runs the slower acquisition with a divided clock. The ABA memory setup including the divider value can be programmed with the following registers

Table 179: Spectrum API: ABA mode relevant registers and register settings

Register	Value	Direction	Description
SPC_SEGMENTSIZE	10010	read/write	Size of one Multiple Recording segment: the number of samples to be record after each trigger event.
SPC_POSTTRIGGER	10030	read/write	Defines the number of samples to be recorded after each trigger event.
SPC_ABADIVIDER	10040	read/write	Programs the divider which is used to sample slow ABA data: For 12 bit, 14 bit and 16 bit cards : between 16 and 131056 in steps of 16 For 8 bit cards : between 32 and 262112 in steps of 32

The resulting ABA clock is then calculated by sampling rate / ABA divider.

Each segment can consist of pretrigger and/or posttrigger samples. The user always has to set the total segment size and the posttrigger, while the pretrigger is calculated within the driver with the formula: [pretrigger] = [segment size] - [posttrigger].

When using ABA mode or Multiple Recording the maximum pretrigger is limited depending on the number of active channels. When the calculated value exceeds that limit, the driver will return the error ERR_PRETRIGGERLEN.



Standard Mode

With every detected trigger event one data block is filled with data. The length of one ABA segment is set by the value of the segmentsize register. The total amount of samples to be recorded is defined by the memsize register.

Memsize must be set to a multiple of the segment size. The table below shows the register for enabling standard ABA mode. For detailed information on how to setup and start the standard acquisition mode please refer to the according chapter earlier in this manual.

Table 180: Spectrum API: card mode programming register and setup for ABA mode

Register	Value	Direction	Description
SPC_CARDMODE	9500	read/write	Defines the used operating mode
SPC_REC_STD_ABA	8h		Data acquisition to on-board memory for multiple trigger events. While the multiple trigger events are stored with programmed sampling rate the inputs are sampled continuously with a slower sampling speed.

The total number of samples to be recorded to the on-board memory in standard mode is defined by the SPC_MEMSIZE register.

Table 181: Spectrum API: memory size register and available register settings

Register	Value	Direction	Description
SPC_MEMSIZE	10000	read/write	Defines the total number of samples to be recorded.

FIFO Mode

The ABA FIFO Mode is similar to the Multiple Recording FIFO mode. In contrast to the standard mode it is not necessary to program the number of samples to be recorded. The acquisition is running until the user stops it. The data is read block by block by the driver as described under Single FIFO mode example earlier in this manual. These blocks are online available for further data processing by the user program. This mode significantly reduces the average data transfer rate on the PCI bus. This enables you to use faster sample rates then you would be able to in FIFO mode without ABA.

Table 182: Spectrum API: card mode programming register and setup for ABA FIFO mode

Register	Value	Direction	Description
SPC_CARDMODE	9500	read/write	Defines the used operating mode
SPC_REC_FIFO_ABA	80h		Continuous data acquisition for multiple trigger events together with continuous data acquisition with a slower sampling clock.
SPC_REC_FIFO_SINGLE_MONITOR	80h		Continuous data acquisition with just one trigger event together with continuous data acquisition with a slower sampling clock. Combination of SPC_REC_FIFO_SINGLE mode with additional slower sampling clock data stream for monitoring purposes (same as A-data of SPC_REC_FIFO_ABA mode).

The number of segments to be recorded must be set separately with the register shown in the following table:

Table 183: Spectrum API: loops programming register and available register settings

Register	Value	Direction	Description
SPC_LOOPS	10020	read/write	Defines the number of segments to be recorded
0			Recording will be infinite until the user stops it.
1 ... [4Gi - 1]			Defines the total segments to be recorded.

Limits of pre trigger, post trigger, memory size

The maximum memory size parameter is only limited by the number of activated channels and by the amount of installed memory. Please keep in mind that each sample needs 1 bytes of memory to be stored. Minimum memory size as well as minimum and maximum post trigger limits are independent of the activated channels or the installed memory.

Due to the internal organization of the card memory there is a certain stepsize when setting these values that has to be taken into account. The following table gives you an overview of all limits concerning pre trigger, post trigger, memory size, segment size and loops. The table shows all values in relation to the installed memory size in samples. If more memory is installed the maximum memory size figures will increase according to the complete installed memory

Table 184: Spectrum API: Limits of pre trigger, post trigger and memory size

Activated Channels	Used Mode	Memory size SPC_MEMSIZE			Pre trigger SPC_PRETRIGGER			Post trigger SPC_POSTTRIGGER			Segment size SPC_SEGMENTSIZE			Loops SPC_LOOPS		
		Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step
1 Ch	Standard Single	64	Mem	32	32	Mem - 32 (defined by mem and post)	32	32	8Gi - 32	32	not used			not used		
	Standard Multi/ABA	64	Mem	32	32	8Ki (defined by segment and post)	32	32	Mem/2-32 (Limited by max pretrigger)	32	64	Mem/2	32	not used		
	Standard Gate	64	Mem	32	32	8Ki	32	32	Mem-32	32	not used			not used		
	Standard Average	For the limits in this mode please refer to the dedicated chapter in this manual.														
	FIFO Single	not used			32	8Ki	32	not used			64	8Gi - 32	32	0 (∞)	4Gi - 1	1
	FIFO Multi/ABA	not used			32	8Ki (defined by segment and post)	32	32	8Gi-32 (Limited by max pretrigger)	32	64	pre+post	32	0 (∞)	4Gi - 1	1
	FIFO Gate	not used			32	8Ki	32	32	8Gi - 32	32	not used			0 (∞)	4Gi - 1	1
	FIFO Average	For the limits in this mode please refer to the dedicated chapter in this manual.														
2 Ch	Standard Single	64	Mem/2	32	32	Mem/2 - 32 (defined by mem and post)	32	32	8Gi - 32	32	not used			not used		
	Standard Multi/ABA	64	Mem/2	32	32	8Ki (defined by segment and post)	32	32	Mem/4-32 (Limited by max pretrigger)	32	64	Mem/4	32	not used		

Table 184: Spectrum API: Limits of pre trigger, post trigger and memory size

Activated Channels	Used Mode	Memory size SPC_MEMSIZE			Pre trigger SPC_PRETRIGGER			Post trigger SPC_POSTTRIGGER			Segment size SPC_SEGMENTSIZE			Loops SPC_LOOPS		
		Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step
	Standard Gate	64	Mem/2	32	32	8Ki	32	32	Mem/2-32	32	not used			not used		
	Standard Average	For the limits in this mode please refer to the dedicated chapter in this manual.														
	FIFO Single	not used			32	8Ki	32	not used			64	8Gi - 32	32	0 (x)	4Gi - 1	1
	FIFO Multi/ABA	not used			32	8Ki (defined by segment and post)	32	32	8Gi-32	32	64	pre+post	32	0 (x)	4Gi - 1	1
	FIFO Gate	not used			32	8Ki	32	32	8Gi - 32	32	not used			0 (x)	4Gi - 1	1
	FIFO Average	For the limits in this mode please refer to the dedicated chapter in this manual.														
4 Ch	Standard Single	64	Mem/4	32	32	Mem/4 - 32	32	32	8Gi - 16	32	not used			not used		
					(defined by mem and post)											
	Standard Multi/ABA	64	Mem/4	32	32	8Ki (defined by segment and post)	32	32	Mem/4-32	32	64	Mem/8	32	not used		
								(Limited by max pretrigger)								
	Standard Gate	64	Mem/4	32	32	8Ki	32	32	Mem/4-16	32	not used			not used		
	Standard Average	For the limits in this mode please refer to the dedicated chapter in this manual.														
	FIFO Single	not used			32	8Ki	32	not used			64	8Gi - 32	32	0 (x)	4Gi - 1	1
	FIFO Multi/ABA	not used			32	8Ki (defined by segment and post)	32	32	8Gi-32	32	64	pre+post	32	0 (x)	4Gi - 1	1
								(Limited by max pretrigger)								
	FIFO Gate	not used			32	8Ki	32	32	8Gi - 32	32	not used			0 (x)	4Gi - 1	1
FIFO Average	For the limits in this mode please refer to the dedicated chapter in this manual.															

All figures listed here are given in samples. An entry of [8Gi - 32] means [8 GiSamples - 32] = 8,589,934,560 samples.

The given memory and memory / divider figures depend on the installed on-board memory as listed below:

	Installed Memory	
	2 GiSample	8 GiSample (Option: M5i.xxx-MEM8GS)
Mem	2 GiSample	8 GiSample
Mem / 2	1 GiSample	4 GiSample
Mem / 4	512 MiSample	2 GiSample
Mem / 8	256 MiSample	1 GiSample

Please keep in mind that this table shows all values at once. Only the absolute maximum and minimum values are shown. There might be additional limitations. Which of these values is programmed depends on the used mode. Please read the detailed documentation of the mode.

Example for setting ABA mode:

The following example will program the standard ABA mode, will set the fast sampling rate to 100 MHz and acquire 2Ki segments with 1Ki pretrigger and 1Ki posttrigger on every rising edge of the trigger input. Meanwhile the inputs are sampled continuously with the ABA mode with a ABA divider set to 5000 resulting in a slow sampling clock for the A area of 100 MHz / 5000 = 20 kHz:

```
// setting the fast sampling clock as internal 100 MHz
spcm_dwSetParam_i32 (hDrv, SPC_CLOCKMODE, SPC_CM_INTPLL);
spcm_dwSetParam_i64 (hDrv, SPC_SAMPLERATE, 100000000);

// enable the ABA mode and set the ABA divider to 5000 -> 100 MHz / 5000 = 20 kHz
spcm_dwSetParam_i32 (hDrv, SPC_CARDMODE, SPC_REC_STD_ABA);
spcm_dwSetParam_i32 (hDrv, SPC_ABADIVIDER, 5000);

// define the segmentsize, pre and posttrigger and the total amount of data to acquire
spcm_dwSetParam_i64 (hDrv, SPC_MEMSIZE, 16384);
spcm_dwSetParam_i64 (hDrv, SPC_SEGMENTSIZE, 2048);
spcm_dwSetParam_i64 (hDrv, SPC_POSTTRIGGER, 1024);

// set the trigger mode to external with positive edge
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_ORMASK, SPC_TMASK_EXT0);
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_EXT0_MODE, SPC_TM_POS);
```

Reading out ABA data

General

The slow „A“ data is stored in an additional FIFO that is located in hardware on the card. This additional FIFO can read out slow „A“ data using DMA transfer similar to the DMA transfer of the main sample data DMA transfer. The card has three completely independent busmaster DMA engines in hardware allowing the simultaneous transfer of both „A“ and sample data, as well as optionally timestamp data. The sample data itself is read out as explained before using the standard DMA routine.

As seen in the picture there are separate FIFOs holding ABA (if available) and timestamp data.

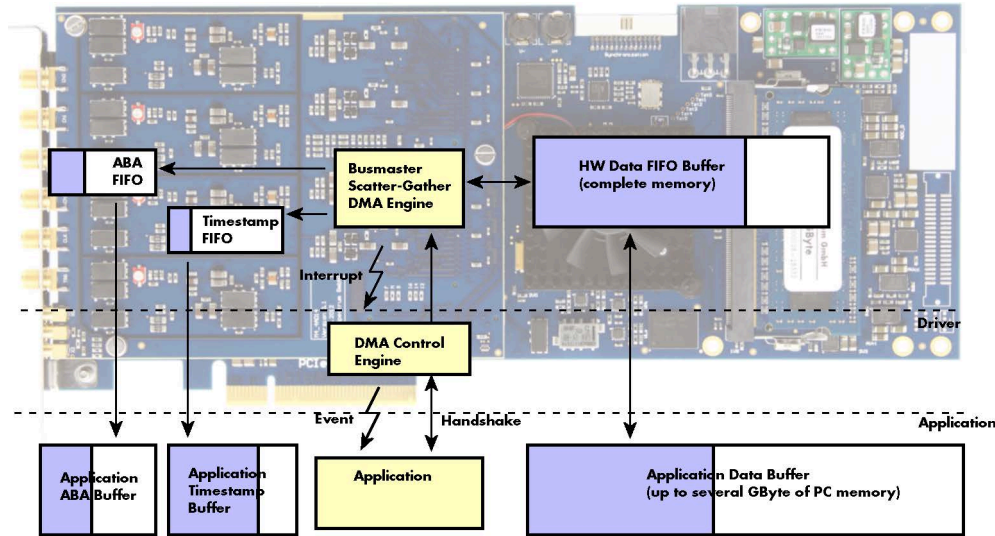


Image 73: Overview of acquisition data, ABA data and timestamp data DMA transfer

Although an M4i is shown here, this applies to M4x and M2p cards as well. M5i cards are similar, but don't have the ABA path. Each FIFO has its own DMA channel, the way data is handled by the DMA engine is similar for both kinds of extra FIFOs and is also very similar to the main sample data transfer engine. Therefore additional information can be found in the chapter explaining the main data transfer.

Commands and Status information for extra transfer buffers.

As explained above the data transfer is performed with the same command and status registers like the card control and sample data transfer. It is possible to send commands for card control, data transfer and extra FIFO data transfer at the same time

Table 185: Spectrum API: extra DMA commands (ABA and Timestamp)

Register	Value	Direction	Description
SPC_M2CMD	100	write only	Executes a command for the card or data transfer
M2CMD_EXTRA_STARTDMA	100000h		Starts the DMA transfer for an already defined buffer.
M2CMD_EXTRA_WAITDMA	200000h		Waits until the data transfer has ended or until at least the amount of bytes defined by notify size are available. This wait function also takes the timeout parameter into account.
M2CMD_EXTRA_STOPDMA	400000h		Stops a running DMA transfer. Data is invalid afterwards.
M2CMD_EXTRA_POLL	800000h		Polls data without using DMA. As DMA has some overhead and has been implemented for fast data transfer of large amounts of data it is in some cases more simple to poll for available data. Please see the detailed examples for this mode. It is not possible to mix DMA and polling mode.

The extra FIFO data transfer can generate one of the following status information:

Table 186: Spectrum API: extra DMA status (ABA and Timestamp)

Register	Value	Direction	Description
SPC_M2STATUS	110	read only	Reads out the current status information
M2STAT_EXTRA_BLOCKREADY	1000h		The next data block as defined in the notify size is available. It is at least the amount of data available but it also can be more data.
M2STAT_EXTRA_END	2000h		The data transfer has completed. This status information will only occur if the notify size is set to zero.
M2STAT_EXTRA_OVERRUN	4000h		The data transfer had on overrun (acquisition) or underrun (replay) while doing FIFO transfer.
M2STAT_EXTRA_ERROR	8000h		An internal error occurred while doing data transfer.

Data Transfer using DMA

Data transfer consists of two parts: the buffer definition and the commands/status information that controls the transfer itself. Extra data transfer shares the command and status register with the card control, data transfer commands and status information.

The DMA based data transfer mode is activated as soon as the M2CMD_EXTRA_STARTDMA is given. Please see next chapter to see how the polling mode works.

Definition of the transfer buffer

Before any data transfer can start it is necessary to define the transfer buffer with all its details. The definition of the buffer is done with the `spcm_dwDefTransfer` function as explained in an earlier chapter. The following example will show the definition of a transfer buffer for timestamp data, definition for ABA data is similar:

```
spcm_dwDefTransfer_i64 (hDrv, SPCM_BUF_TIMESTAMP, SPCM_DIR_CARDTOPC, 0, pvBuffer, 0, 1LenOfBufferInBytes);
```


In this example the notify size is set to zero, meaning that we don't want to be notified until all extra data has been transferred. Please have a look at the sample data transfer in an earlier chapter to see more details on the notify size.

Please note that extra data transfer is only possible from card to PC and there's no programmable offset available for this transfer.

M5i cards only:

On M5i cards the `ILenOfBufferInBytes` parameter needs to be an integer multiple of 64 bytes.



Buffer handling

A data buffer handshake is implemented in the driver which allows to run the card in different data transfer modes. The software transfer buffer is handled as one large buffer for each kind of data (timestamp and ABA) which is on the one side controlled by the driver and filled automatically by busmaster DMA from the hardware extra FIFO buffer and on the other hand it is handled by the user who set's parts of this software buffer available for the driver for further transfer. The handshake is fulfilled with the following 3 software registers:

Table 187: Spectrum API: ABA and Timestamp DMA buffer handling registers

Register	Value	Direction	Description
SPC_ABA_AVAIL_USER_LEN	210	read	This register contains the currently available number of bytes that are filled with newly transferred slow ABA data. The user can now use this ABA data for own purposes, copy it, write it to disk or start calculations with this data.
SPC_ABA_AVAIL_USER_POS	211	read	The register holds the current byte index position where the available ABA bytes start. The register is just intended to help you and to avoid own position calculation
SPC_ABA_AVAIL_CARD_LEN	212	write	After finishing the job with the new available ABA data the user needs to tell the driver that this amount of bytes is again free for new data to be transferred.
SPC_TS_AVAIL_USER_LEN	220	read	This register contains the currently available number of bytes that are filled with newly transferred timestamp data. The user can now use these timestamps for own purposes, copy it, write it to disk or start calculations with the timestamps.
SPC_TS_AVAIL_USER_POS	221	read	The register holds the current byte index position where the available timestamp bytes start. The register is just intended to help you and to avoid own position calculation
SPC_TS_AVAIL_CARD_LEN	222	write	After finishing the job with the new available timestamp data the user needs to tell the driver that this amount of bytes is again free for new data to be transferred.

Directly after start of transfer the `SPC_XXX_AVAIL_USER_LEN` is every time zero as no data is available for the user and the `SPC_XXX_AVAIL_CARD_LEN` is every time identical to the length of the defined buffer as the complete buffer is available for the card for transfer.

The counter that is holding the user buffer available bytes (`SPC_XXX_AVAIL_USER_LEN`) is sticking to the defined notify size at the `DefTransfer` call. Even when less bytes already have been transferred you won't get notice of it if the notify size is programmed to a higher value.



Remarks

- The transfer between hardware FIFO buffer and application buffer is done with scatter-gather DMA using a busmaster DMA controller located on the card. Even if the PC is busy with other jobs data is still transferred until the application buffer is completely used.
- As shown in the drawing above the DMA control will announce new data to the application by sending an event. Waiting for an event is done internally inside the driver if the application calls one of the wait functions. Waiting for an event does not consume any CPU time and is therefore highly requested if other threads do lot of calculation work. However it is not necessary to use the wait functions and one can simply request the current status whenever the program has time to do so. When using this polling mode the announced available

bytes still stick to the defined notify size!

- If the on-board FIFO buffer has an overrun data transfer is stopped immediately.

Buffer handling example for DMA timestamp transfer (ABA transfer is similar, just using other registers)

```
int8* pcData = (int8*) pvAllocMemPageAligned (lBufSizeInBytes);

// we now define the transfer buffer with the minimum notify size of one page = 4 KiByte
spcm_dwDefTransfer_i64 (hDrv, SPCM_BUF_TIMESTAMP, SPCM_DIR_CARDTOPC, 4096, (void*) pcData, 0, lBufSizeInBytes);

do
{
    // we wait for the next data to be available. After this call we get at least 4KiByte of data to proceed
    dwError = spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_EXTRA_STARTDMA | M2CMD_EXTRA_WAITDMA);

    if (!dwError)
    {
        // if there was no error we can proceed and read out the current amount of available data
        spcm_dwGetParam_i32 (hDrv, SPC_TS_AVAIL_USER_LEN, &lAvailBytes);
        spcm_dwGetParam_i32 (hDrv, SPC_TS_AVAIL_USER_POS, &lBytePos);

        printf ("We now have %d new bytes available\n", lAvailBytes);
        printf ("The available data starts at position %d\n", lBytePos);

        // we take care not to go across the end of the buffer
        if ((lBytePos + lAvailBytes) >= lBufSizeInBytes)
            lAvailBytes = lBufSizeInBytes - lBytePos;

        // our do function gets a pointer to the start of the available data section and the length
        vProcessTimestamps (&pcData[lBytePos], lAvailBytes);

        // the buffer section is now immediately set available for the card
        spcm_dwSetParam_i32 (hDrv, SPC_TS_AVAIL_CARD_LEN, lAvailBytes);
    }
}
while (!dwError); // we loop forever if no error occurs
```

The extra FIFO has a quite small size compared to the main data buffer. As the transfer is done initiated by the hardware using busmaster DMA this is not critical as long as the application data buffers are large enough and as long as the extra transfer is started BEFORE starting the card.



Data Transfer using Polling

If the extra data is quite slow and the delay caused by the notify size on DMA transfers is unacceptable for your application it is possible to use the polling mode. Please be aware that the polling mode uses CPU processing power to get the data and that there might be an overrun if your CPU is otherwise busy. You should only use polling mode in special cases and if the amount of data to transfer is not too high.

Most of the functionality is similar to the DMA based transfer mode as explained above.

The polling data transfer mode is activated as soon as the M2CMD_EXTRA_POLL is executed.

Definition of the transfer buffer

This is similar to the above explained DMA buffer transfer. The value „notify size“ is ignored and should be set to 4Ki (4096).

Buffer handling

The buffer handling is also similar to the DMA transfer. As soon as one of the registers SPC_TS_AVAIL_USER_LEN or SPC_ABA_AVAIL_USER_LEN is read the driver will read out all available data from the hardware and will return the number of bytes that has been read. In minimum this will be one DWORD = 4 bytes.

Buffer handling example for polling timestamp transfer (ABA transfer is similar, just using other registers)

```

int8* pcData = (int8*) pvAllocMemPageAligned (lBufSizeInBytes);

// we now define the transfer buffer with the minimum notify size of one page = 4 KiByte
spcm_dwDefTransfer_i64 (hDrv, SPCM_BUF_TIMESTAMP, SPCM_DIR_CARDTOPC, 4096, (void*) pcData, 0, lBufSizeInBytes);

// we start the polling mode
dwError = spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_EXTRA_POLL);

// this is our polling loop
do
{
    spcm_dwGetParam_i32 (hDrv, SPC_TS_AVAIL_USER_LEN, &lAvailBytes);
    spcm_dwGetParam_i32 (hDrv, SPC_TS_AVAIL_USER_POS, &lBytePos);

    if (lAvailBytes > 0)
    {
        printf ("We now have %d new bytes available\n", lAvailBytes);
        printf ("The available data starts at position %d\n", lBytePos);

        // we take care not to go across the end of the buffer
        if ((lBytePos + lAvailBytes) >= lBufSizeInBytes)
            lAvailBytes = lBufSizeInBytes - lBytePos;

        // our do function get's a pointer to the start of the available data section and the length
        vProcessTimestamps (&pcData[lBytePos], lAvailBytes);

        // the buffer section is now immediately set available for the card
        spcm_dwSetParam_i32 (hDrv, SPC_TS_AVAIL_CARD_LEN, lAvailBytes);
    }
}
while (!dwError); // we loop forever if no error occurs

```

Comparison of DMA and polling commands

This chapter shows you how small the difference in programming is between the DMA and the polling mode:

	DMA mode	Polling mode
Define the buffer	spcm_dwDefTransfer_i64 (hDrv, SPCM_BUF_TIMESTAMP, SPCM_DIR...);	spcm_dwDefTransfer_i64 (hDrv, SPCM_BUF_TIMESTAMP, SPCM_DIR...);
Start the transfer	spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_EXTRA_STARTDMA)	spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_EXTRA_POLL)
Wait for data	spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_EXTRA_WAITDMA)	not in polling mode
Available bytes?	spcm_dwGetParam_i32 (hDrv, SPC_TS_AVAIL_USER_LEN, &lBytes);	spcm_dwGetParam_i32 (hDrv, SPC_TS_AVAIL_USER_LEN, &lBytes);
Min available bytes	programmed notify size	4 bytes
Current position?	spcm_dwGetParam_i32 (hDrv, SPC_TS_AVAIL_USER_LEN, &lBytes);	spcm_dwGetParam_i32 (hDrv, SPC_TS_AVAIL_USER_LEN, &lBytes);
Free buffer for card	spcm_dwSetParam_i32 (hDrv, SPC_TS_AVAIL_CARD_LEN, lBytes);	spcm_dwSetParam_i32 (hDrv, SPC_TS_AVAIL_CARD_LEN, lBytes);

ABA Mode and Timestamps

The ABA mode is well matching with the timestamp option. If timestamp recording is activated, each trigger event and therefore each B time base segment will get time stamped as shown in the drawing on the right.

Please keep in mind that the trigger events - located in the B area - are time stamped, not the beginning of the acquisition. The first B sample that is available is at the time position of [Timestamp - Pretrigger].

The first A area sample is related to the card start and therefore in a fixed but various settings dependent relation to the timestamped B sample. To bring exact relation between the first A area sample (and therefore all area A samples) and the B area samples it is possible to let the card stamp the first A area sample automatically after the card start. The following table shows the register to enable this mode:

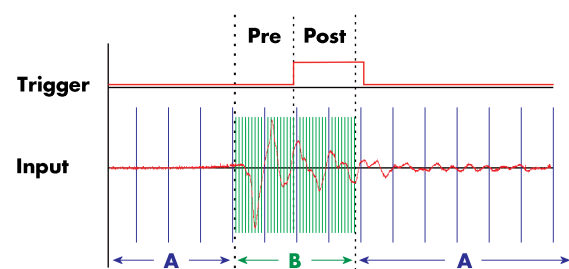


Image 74: Drawing of ABA mode

Table 188: Spectrum API: timestamp command register and ABA mode settings

Register	Value	Direction	Description
SPC_TIMESTAMP_CMD	47000	read/write	Programs a timestamp setup including mode and additional features
SPC_TSFEAT_MASK	F0000h		Mask for the feature relating bits of the SPC_TIMESTAMP_CMD bitmask.
SPC_TSFEAT_STORE1STABA	10000h		Enables storage of one additional timestamp for the first A area sample (B time base related) in addition to the trigger related timestamps.
SPC_TSFEAT_NONE	0h		No additional timestamp is created. The total number of stamps is only trigger related.

This mode is compatible with all existing timestamp modes. Please keep in mind that the timestamp counter is running with the B area timebase.

```
// normal timestamp setup (e.g. setting timestamp mode to standard using internal clocking)
uint32 dwTimestampMode = (SPC_TSMODE_STANDARD | SPC_TSMODE_DISABLE);

// additionally enable index of the first A area sample
dwTimestampMode |= SPC_TSFEAT_STORE1STABA;

spcm_dwSetParam_i32 (hDrv, SPC_TIMESTAMP_CMD, dwTimestampMode);
```

The programming details of the ABA mode and timestamp modes are each explained in an dedicated chapter in this manual.

Option Remote Server

Introduction

Using the Spectrum Remote Server (order code -SPc-RServer) it is possible to access the M2i/M3i/M4i/M4x/M2p/M5i card(s) installed in one PC (server) from another PC (client) via local area network (LAN), similar to using a digitizerNETBOX, generatorNETBOX or hybridNETBOX.

It is possible to use different operating systems on both server and client. For example the Remote Server is running on a Linux system and the client is accessing them from a Windows system.

The Remote Server software requires, that the option „SPc-RServer“ is installed on at least one card installed within the server side PC. You can either check this with the Control Center in the "Installed Card features" node or by reading out the feature register, as described in the „Installed features and options“ passage, earlier in this manual.

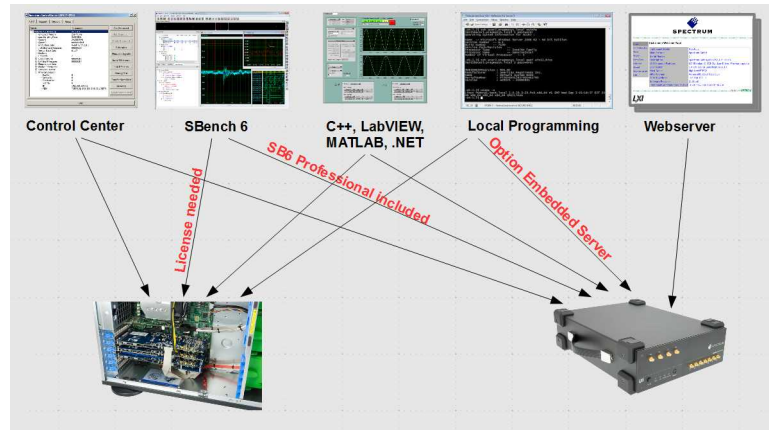


Image 75: Overview of remote server option interaction in comparison to NETBOX devices

To run the Remote Server software, it is required to have least version 3.18 of the Spectrum SPCM driver installed. Additionally at least on one card in the server PC the feature flag SPCM_FEAT_REMOTESERVER must be set.



Installing and starting the Remote Server

Windows

Windows users find the Control Center installer on the USB-Stick under „Install\win\spcm_remote_install.exe“. After the installation has finished there will be a new start menu entry in the Folder "Spectrum GmbH" to start the Remote Server. To start the Remote Server automatically after login, just copy this shortcut to the Autostart directory.

Linux

Linux users find the versions of the installer for the different StdC libraries under under /Install/linux/spcm_control_center/ as RPM packages.

To start the Remote Server type "spcm_remote_server" (without quotation marks). To start the Remote Server automatically after login, add the following line to the .bashrc or .profile file (depending on the used Linux distribution) in the user's home directory:

```
spcm_remote_server&
```

```
Spectrum Remote Server (32-bit)
SPCM Remote Server 1.3.17767
Providing access to the following cards:
M2p.5968-x4 sn13573
Listening on the following IPs:
192.168.56.1
192.168.169.42
Remote Server started successfully.
Press q + Enter to stop the Remote Server and close the program.
```

Detecting the digitizerNETBOX/generatorNETBOX/hybridNETBOX

Before accessing the digitizerNETBOX/generatorNETBOX/hybridNETBOX one has to determine the IP address of the device. Normally that can be done using one of the two methods described below:

Discovery Function

The digitizerNETBOX/generatorNETBOX/hybridNETBOX responds to the VISA described Discovery function. The next chapter will show how to install and use the Spectrum control center to execute the discovery function and to find the Spectrum hardware. As the discovery function is a standard feature of all LXI devices there are other software packages that can find the device using the discovery function:

- Spectrum control center (limited to Spectrum remote products)
- free LXI System Discovery Tool from the LXI consortium (www.lxi-standard.org)
- Measurement and Automation Explorer from National Instruments (NI MAX)
- Keysight Connection Expert from Keysight Technologies

Additionally the discovery procedure can be started from your own application, as shown below:

```
#define TIMEOUT_DISCOVERY 5000 // timeout value in ms

const uint32 dwMaxNumRemoteCards = 50;

char* pszVisa[dwMaxNumRemoteCards] = { NULL };
char* pszIdn[dwMaxNumRemoteCards] = { NULL };

const uint32 dwMaxIdnStringLen = 256;
const uint32 dwMaxVisaStringLen = 50;

// allocate memory for string list
for (uint32 i = 0; i < dwMaxNumRemoteCards; i++)
{
    pszVisa[i] = new char [dwMaxVisaStringLen];
    pszIdn[i] = new char [dwMaxIdnStringLen];
    memset (pszVisa[i], 0, dwMaxVisaStringLen);
    memset (pszIdn[i], 0, dwMaxIdnStringLen);
}

// first make discovery - check if there are any LXI compatible remote devices
dwError = spcm_dwDiscovery ((char**)pszVisa, dwMaxNumRemoteCards, dwMaxVisaStringLen, TIMEOUT_DISCOVERY);

// second: check from which manufacturer the devices are
spcm_dwSendIDNRequest ((char**)pszIdn, dwMaxNumRemoteCards, dwMaxIdnStringLen);

// Use the VISA strings of these devices with Spectrum as manufacturer
// for accessing remote devices without previous knowledge of their IP address
```

Finding the digitizerNETBOX/generatorNETBOX/hybridNETBOX in the network

As the digitizerNETBOX/generatorNETBOX/hybridNETBOX is a standard network device, it has its own IP address and host name and can therefore be found on the computer network by other devices. The standard host name consist of the model type and the serial number of the device. The serial number is also found on the type plate on the back of the digitizerNETBOX/generatorNETBOX/hybridNETBOX chassis.

As default DHCP (IPv4) will be used and an IP address will be automatically set. In case no DHCP server is found, an IP will be obtained using the AutoIP feature. This will lead to an IPv4 address of 169.254.x.y (with x and y being assigned to a free IP in the network) using a subnet mask of 255.255.0.0.

The default IP setup can also be restored, by using the „LAN Reset“ button on the device.

If a fixed IP address should be used instead, the parameters need to be set according to the current LAN requirements.

Windows 7, Windows 8, Windows 10 and Windows 11

Under Windows 7, Windows 8, Windows 10 and Windows 11 the digitizerNETBOX, generatorNETBOX and hybridNETBOX devices are listed under the „other devices“ tree with their given host name.

A right click on the digitizerNETBOX or generatorNETBOX device opens the properties window where you find further information on the device including the IP address.

From here it is possible to go the website of the device where all necessary information are found to access the device from software.

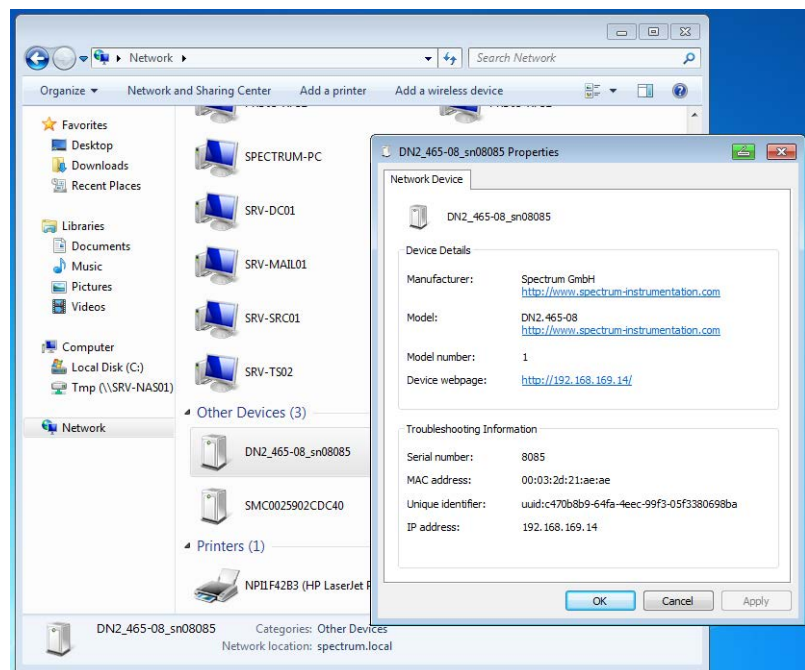


Image 76: Windows screenshot: finding a remote Spectrum device like digitizerNETBOX

Troubleshooting

If the above methods do not work please try one of the following steps:

- Ask your network administrator for the IP address of the digitizerNETBOX/generatorNETBOX and access it directly over the IP address.
- Check your local firewall whether it allows access to the device and whether it allows to access the ports listed in the technical data section.
- Check with your network administrator whether the subnet, the device and the ports that are listed in the technical data section are accessible from your system due to company security settings.

Accessing remote cards

To detect remote card(s) from the client PC, start the Spectrum Control Center on the client and click "Netbox Discovery". All discovered cards will be listed under the "Remote" node.

Using remote cards instead of using local ones is as easy as using a digitizerNETBOX and only requires a few lines of code to be changed compared to using local cards.

Instead of opening two locally installed cards like this:

```
hDrv0 = spcm_hOpen ("/dev/spcm0"); // open local card spcm0
hDrv1 = spcm_hOpen ("/dev/spcm1"); // open local card spcm1
```

one would call `spcm_hOpen()` with a VISA string as a parameter instead:

```
hDrv0 = spcm_hOpen ("TCPIP::192.168.1.2::inst0::INSTR"); // open card spcm0 on a Remote Server PC
hDrv1 = spcm_hOpen ("TCPIP::192.168.1.2::inst1::INSTR"); // open card spcm1 on a Remote Server PC
```

to open cards on the Remote Server PC with the IP address 192.168.1.2. The driver will take care of all the network communication.

Pulse Generator (Firmware Option)

General Information

The pulse generator module provides a versatile timing synchronization interface between the acquisition/replay functionality of the card and external equipment.

The module consists of four pulse generators, where each generator allows for (in)dependent generation of individual pulses, pulse trains or a continuous stream of pulses that can be output on a Multi-Purpose I/O Line, greatly enhancing the versatility of the XIO lines.

The versatile trigger capabilities allow for external or internal triggering. Moreover, the pulse generators can trigger each other, hence allowing for cascading of up to four pulse repetition time scales.

The outputs of the pulse generators are intrinsically synchronized to the card acquisition/replay functionality and its sampling clock, hence allowing for reproducible enabling or switching of external signals (e.g., for signal actuating). Other use cases might be pulse broadening, pulse delaying, or just pulse generation.

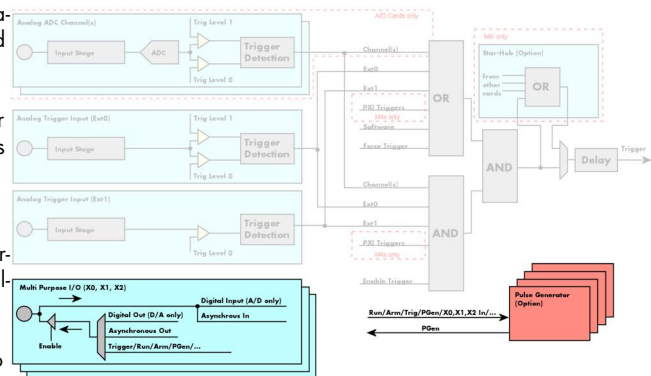


Image 77: overview block diagram of multi-purpose I/O lines and pulse generators

The generation of the pulse trains and timing signals is performed inside the FPGA of the card and is working in parallel to any other functionality of the card (such as data acquisition or replay), and hence not reducing the performance.

Feature Overview

- Four pulse generators are available
- Single-shot, multiple repetitions or continuous/infinite repetition of pulses
- Individual control of pulse length/duty cycle
- External or internal triggering/starting individually for each pulse generator
- Individual trigger delay per pulse generator allowing for phase shifting
- Internal cascading of pulse generators possible allowing up to four repetition time scales.

The “standard” modes of the multi purpose I/O lines are still available, as described in the “Multi Purpose I/O Lines” section. This chapter focuses on the additional functionality, available with the pulse generator firmware option installed.

The multi purpose I/O lines are available on the front plate and labelled with X0 (line 0), X1 (line 1), and X2 (line 2). As default these lines are switched off.



As default (power-on and after reset command) the I/O capable lines are switched off and hence are not actively driven. Hence the on-board 10 kOhm pull-up resistors are pulling these lines to logic HIGH. If a logic LOW is required, external lower-value (1 kOhm) pull-down resistors might be used.



Please be careful when programming these lines as an output whilst maybe still being connected with an external signal source, as that may damage components either on the external equipment or on the card itself.

Principle of Operation

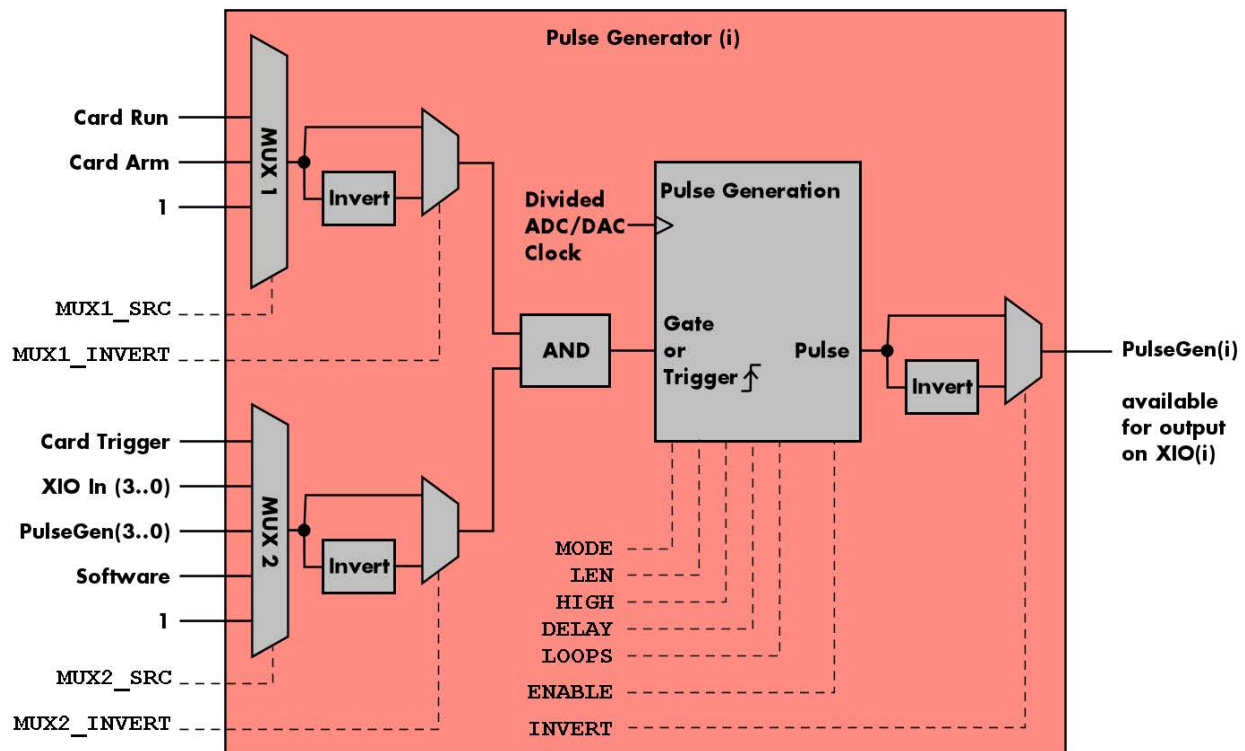


Image 78: overview block diagram of the pulse generator

All of the four available pulse generator units are identical in their feature set and individually programmable.

As shown above, each unit consists of:

- A dedicated trigger setup consisting of two multiplexers MUX1 and MUX2 combining various signals
- A programmable inverter on the output of each multiplexer
- A static logic AND gate combining the outputs of both multiplexers to form a trigger/gate for the pulse generating unit
- The pulse generating unit itself with its trigger signal driven by the AND gate
- A final programmable output inverter

The pulse generator unit is clocked with an FPGA internal clock, which is a divided version derived from the acquisition or generation sampling rate. Since the division ratio is depending on the used card type, the number of active channels and the sampling rate, an dedicated read only register allows to read out the frequency value by the following register:

Table 189: Spectrum API: pulse generator clock frequency read register

Register	Value	Direction	Description
SPC_XIO_PULSEGEN_CLOCK	602000	read	Returns the clock driving the pulse generator in Hz.

The following short excerpt shows which parameters need to be defined first and how to read out the clock rate at which the pulse generator units then are clocked:

```
...
// first set up the parameters, that influence the pulse generator's clock rate
spcm_dwSetParam_i32 (hCard, SPC_CHENABLE, CHANNEL0); // channel enable
spcm_dwSetParam_i64 (hCard, SPC_SAMPLERATE, MEGA(1)); // desired acquisition/generation sampling rate
...
// afterwards read out the divided clock rate, clocking the pulse generator units
int64 llPulseGenClock_Hz = 0;
spcm_dwGetParam_i64 (hCard, SPC_XIO_PULSEGEN_CLOCK, &llPulseGenClock_Hz);
```

See the end of this chapter for a more complete example setup of a pulse generator unit.



Changing the card settings while pulse generators are active will cause a stop and restart of the pulse generators automatically issued by the driver to the pulse generators.

Setting up the Pulse Generator

Enabling, disabling and resetting a pulse generator

Each pulse generator unit can be enabled and disabled separately:

Table 190: Spectrum API: pulse generator enable registers

Register	Value	Direction	Description
SPC_XIO_PULSEGEN_ENABLE	601500	read/write	Bitmask to enable any combination of the four different pulse generators.
SPCM_PULSEGEN_ENABLE0	1h		Enable pulse generator 0. When disabled, the output (prior to the output inverter) is set to logic LOW.
SPCM_PULSEGEN_ENABLE1	2h		Enable pulse generator 1. When disabled, the output (prior to the output inverter) is set to logic LOW.
SPCM_PULSEGEN_ENABLE2	4h		Enable pulse generator 2. When disabled, the output (prior to the output inverter) is set to logic LOW.
SPCM_PULSEGEN_ENABLE3	8h		Enable pulse generator 3. When disabled, the output (prior to the output inverter) is set to logic LOW.

Disabling a unit will act as a reset dedicated to this single unit. A disabled pulse generator will output a logic LOW prior to the programmable output inverter, hence with an active output inverter the final output of a disabled pulse generator will be logically HIGH.

Defining the basic pulse parameters

The two basic properties for generating a (repetitive) pulsed output is to define the length (or period) and define how much of the waveform should the output be HIGH:

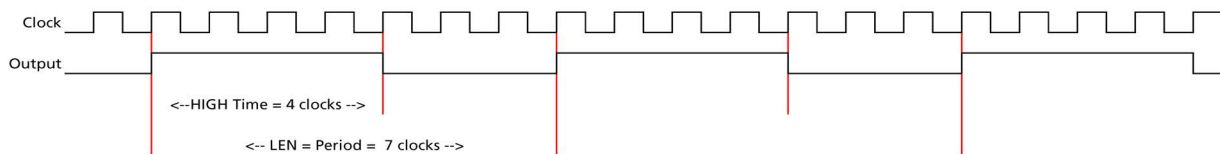


Image 79: timing diagram illustrating the basic pulse parameters

The pulse generator will upon start (trigger) first set the output HIGH for the programmed amount of time. Afterwards it will set the waveform LOW for the remaining time until the programmed length (period) has been reached. As a result, the number of clock cycles during which the output is LOW calculates to: $LOW = LEN - HIGH$. In the example above with $LEN = 7$ and $HIGH = 4$, the signal will be LOW for the remaining 3 clock cycles.

The following table shows the registers required to set the total length of the pulse to be generated. The length is defined in clock cycles:

Table 191: Spectrum API: pulse generator length/period register

Register	Value	Direction	Description
SPC_XIO_PULSEGEN_AVAILLEN_MIN	602001	read	Returns the minimum length (period) of the pulse generator's output pulses in clock cycles.
SPC_XIO_PULSEGEN_AVAILLEN_MAX	602002	read	Returns the maximum length (period) of the pulse generator's output pulses in clock cycles.
SPC_XIO_PULSEGEN_AVAILLEN_STEP	602003	read	Returns the step size the pulse generator's output pulses in clock cycles.
SPC_XIO_PULSEGEN0_LEN	601001	read/write	Define the length of the pulse period generated by pulse generator 0 in clock cycles.
SPC_XIO_PULSEGEN1_LEN	601101	read/write	Define the length of the pulse period generated by pulse generator 1 in clock cycles.
SPC_XIO_PULSEGEN2_LEN	601201	read/write	Define the length of the pulse period generated by pulse generator 2 in clock cycles.
SPC_XIO_PULSEGEN3_LEN	601301	read/write	Define the length of the pulse period generated by pulse generator 3 in clock cycles.

The second parameter that needs to be defined is the amount of clock pulses that force the output to a logic HIGH. The following table shows the registers required to set the total length of the pulse to be generated:

Table 192: Spectrum API: pulse generator HIGH time registers

Register	Value	Direction	Description
SPC_XIO_PULSEGEN_AVAILHIGH_MIN	602004	read	Returns the minimum HIGH time of the pulse generator's output pulses in clock cycles.
SPC_XIO_PULSEGEN_AVAILHIGH_MAX	602005	read	Returns the maximum HIGH time of the pulse generator's output pulses in clock cycles.
SPC_XIO_PULSEGEN_AVAILHIGH_STEP	602006	read	Returns the step size the pulse generator's HIGH time in clock cycles.
SPC_XIO_PULSEGEN0_HIGH	601002	read/write	Define the HIGH time for the pulse generated by pulse generator 0 in clock cycles.
SPC_XIO_PULSEGEN1_HIGH	601102	read/write	Define the HIGH time for the pulse generated by pulse generator 1 in clock cycles.
SPC_XIO_PULSEGEN2_HIGH	601202	read/write	Define the HIGH time for the pulse generated by pulse generator 2 in clock cycles.
SPC_XIO_PULSEGEN3_HIGH	601302	read/write	Define the HIGH time for the pulse generated by pulse generator 3 in clock cycles.

These two settings alone allow for the creation of periodic signals with the freely programmable duty cycle. Setting the HIGH time to half the LEN will result in a clock-like signal with half the time being HIGH and half the time being LOW, hence having a 50% duty-cycle signal.

Since the output of the pulse generator can only change with every edge of its clock input, the speed of this clock ultimately defines the granularity at which the pulses can be configured. The lower the period of the generated pulse signal the finer this granularity becomes with regards to the output signal frequency.

For example, when creating an output with the maximum output frequency of $Clk/2$ (with $LEN = 2$ and $HIGH = 1$), the only possible remaining configuration is a duty-cycle of 50%. And with a output at frequency with $Clk/3$ (with $LEN=3$ and $HIGH$ either 1 or 2) the duty-cycle is either 33% or 66%, but cannot be 50%.

In addition to defining the length/period of a single pulse, one can also define how often a pulse should be replayed repeatedly. The choice can be made between repeating the pulses infinitely (until being explicitly stopped) or to pre-define a number of repetitions:

Table 193: Spectrum API: pulse generator loops/pulse repetition registers

Register	Value	Direction	Description
SPC_XIO_PULSEGEN_AVAILLOOPS_MIN	602010	read	Returns the minimum number of times, the output of a pulse generator can be repeated.
SPC_XIO_PULSEGEN_AVAILLOOPS_MAX	602011	read	Returns the maximum number of times, the output of a pulse generator can be repeated.
SPC_XIO_PULSEGEN_AVAILLOOPS_STEP	602012	read	Returns the step size when defining the repetition of pulse generator's output.
SPC_XIO_PULSEGEN0_LOOPS	601004	read/write	Define the number of repetitions of the output period when triggered for pulse generator 0.
SPC_XIO_PULSEGEN1_LOOPS	601104	read/write	Define the number of repetitions of the output period when triggered for pulse generator 1.
SPC_XIO_PULSEGEN2_LOOPS	601204	read/write	Define the number of repetitions of the output period when triggered for pulse generator 2.
SPC_XIO_PULSEGEN3_LOOPS	601304	read/write	Define the number of repetitions of the output period when triggered for pulse generator 3.
0			Upon a trigger event the output of the pulse generator will run infinitely until being disabled or reset.
1 ... [4Gi - 2]			Upon a trigger event the output period will be replayed the defined number of times.

Delaying (phase shifting) the Outputs

As mentioned above the pulse generator will always start with the first portion of the period to be HIGH and then will set the output LOW for the remaining number of cycles within the chosen length.

When using the delay, it is possible to delay the initial HIGH portion of the pulse generator(s) by a defined amount of clock cycles. This in combination with a common starting point (start/trigger) allows for the generation of phase shifted signals as shown below for two of the pulse generators. Both are set up with identical LEN and HIGH parameters, but the additional delay for pulse generator 0 (PGen0) is kept at the default of zero clock cycles, whilst PGen1 is delayed by 5 clock cycles:

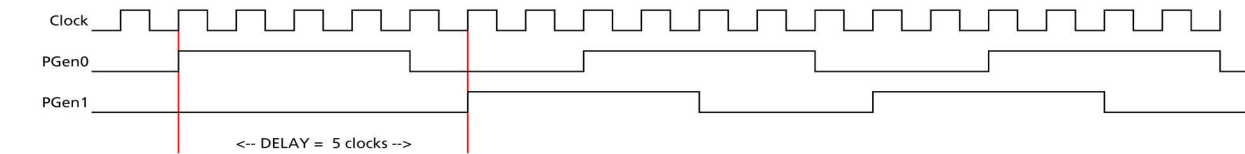


Image 80: timing diagram illustrating delaying a pulse generator output

The amount of additional delay can be set individually for each pulse generator, by using the following registers:

Table 194: Spectrum API: pulse generator delay/phase shift registers

Register	Value	Direction	Description
SPC_XIO_PULSEGEN_AVAILDELAY_MIN	602007	read	Returns the minimum delay of the pulse generator's output in clock cycles.
SPC_XIO_PULSEGEN_AVAILDELAY_MAX	602008	read	Returns the maximum delay of the pulse generator's output in clock cycles.
SPC_XIO_PULSEGEN_AVAILDELAY_STEP	602009	read	Returns the step size of the pulse generator's output delay in clock cycles.
SPC_XIO_PULSEGEN0_DELAY	601003	read/write	Define how much the output of pulse generator 0 is delayed after trigger in clock cycles.
SPC_XIO_PULSEGEN1_DELAY	601103	read/write	Define how much the output of pulse generator 1 is delayed after trigger in clock cycles.
SPC_XIO_PULSEGEN2_DELAY	601203	read/write	Define how much the output of pulse generator 2 is delayed after trigger in clock cycles.
SPC_XIO_PULSEGEN3_DELAY	601303	read/write	Define how much the output of pulse generator 3 is delayed after trigger in clock cycles.

Defining the trigger behavior

Each pulse generator can be set up to react on its trigger input in three different ways, depending on the application's need:

Table 195: Spectrum API: pulse generator mode registers with their available settings

Register	Value	Direction	Description
SPC_XIO_PULSEGEN0_MODE	601000	read/write	Defines the behavior of pulse generator 0 on how to react on its trigger event.
SPC_XIO_PULSEGEN1_MODE	601100	read/write	Defines the behavior of pulse generator 1 on how to react on its trigger event.
SPC_XIO_PULSEGEN2_MODE	601200	read/write	Defines the behavior of pulse generator 2 on how to react on its trigger event.
SPC_XIO_PULSEGEN3_MODE	601300	read/write	Defines the behavior of pulse generator 3 on how to react on its trigger event.
SPCM_PULSEGEN_MODE_GATED	1		Pulse generator will start if the trigger condition or "gate" is met and will stop, if either the gate becomes inactive or the defined number of LOOPS have been generated. Will reset its loop counter, when the gate becomes LOW.
SPCM_PULSEGEN_MODE_TRIGGERED	2		The pulse generator will start if the trigger condition is met and will replay the defined number of loops before re-arming itself and waiting for another trigger event. Changes in the trigger signal while replaying will be ignored.
SPCM_PULSEGEN_MODE_SINGLESOT	3		The pulse generator will start if the trigger condition is met and will replay the defined number of loops once.

For simplicity, the waveforms below will show the modes principle, without any additionally programmed delay, and also omitting the intrinsic pipeline delay from the trigger event to the output's reaction.

Continuously triggered output

After enabling the pulse generator, it will detect trigger events. Upon each trigger, the programmed number of pulses are generated, as defined by the LEN, HIGH, DELAY and LOOPS parameters explained above. After finishing the programmed number of triggers, it will automatically arm itself again and wait for the next trigger.

In contrast to the Gated mode (see below), once a trigger has been detected the trigger input is ignored and the pulse train will finish independent from any activity on the trigger input. Only when it has finished the current generation, a new trigger will be detected:

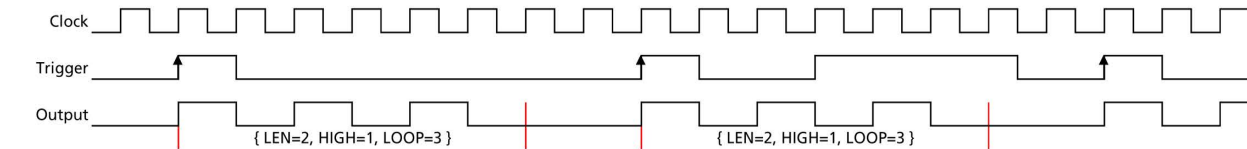


Image 81: timing diagram illustrating the pulse generator triggered output mode

Single Shot triggering

This mode is similar to the triggered mode, but after enabling the pulse generator it will only detect one single trigger. Upon that trigger, the programmed number of pulses are generated, as defined by the LEN, HIGH, DELAY and LOOPS parameters explained above:

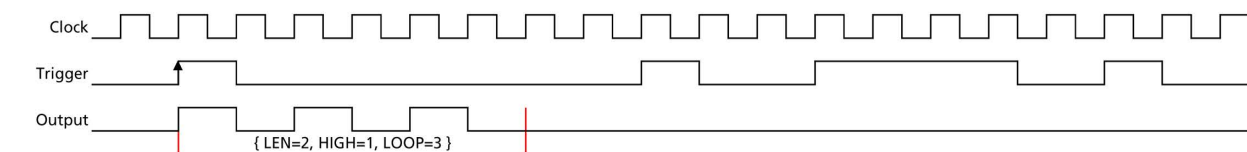


Image 82: timing diagram illustrating the pulse generator single-shot triggered output mode

Afterwards the pulse generator will not detect any further triggers, until being reset by re-enabling:

Continuously gated Output

After enabling the pulse generator, it will detect trigger events. Upon each trigger, the programmed number of pulses are generated, as defined by the LEN, HIGH, DELAY and LOOPS parameters explained above and as long as the trigger condition or gate is still valid (HIGH). If the gate ends, this will stop the output and reset all internal counters back to start. So, each time the gate turns HIGH, the sequence (number of pulses as defined by the LEN, HIGH, DELAY and LOOPS) starts again from its beginning:

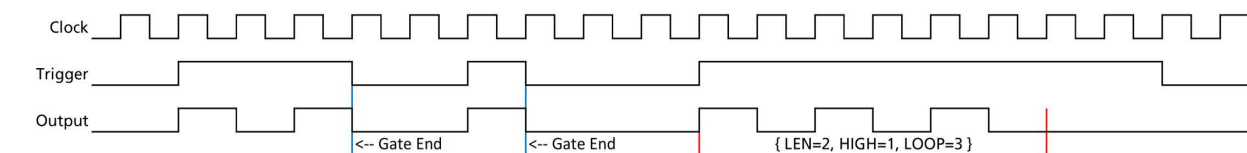


Image 83: timing diagram illustrating the pulse generator gated output mode

Configuring the pulse generator's trigger source

The various possible signals that can logically be combined to form a trigger event for a pulse generator are split up into two portions each consisting of a multiplexer (MUX).

Multiplexer 1

The first multiplexer, MUX1, selects between two different sources and also allows to be completely unused by utilizing a logical '1' or HIGH level, being transparent to the following AND condition combining the two multiplexers:

Table 196: Spectrum API: pulse generator trigger MUX1 registers with their available settings

Register	Value	Direction	Description
SPC_XIO_PULSEGEN0_MUX1_SRC	601005	read/write	Selects the input source for MUX1 for pulse generator 0.
SPC_XIO_PULSEGEN1_MUX1_SRC	601105	read/write	Selects the input source for MUX1 for pulse generator 1.
SPC_XIO_PULSEGEN2_MUX1_SRC	601205	read/write	Selects the input source for MUX1 for pulse generator 2.
SPC_XIO_PULSEGEN3_MUX1_SRC	601305	read/write	Selects the input source for MUX1 for pulse generator 3.
SPCM_PULSEGEN_MUX1_SRC_UNUSED	0		Inputs of MUX1 are not used in creating the trigger condition and instead a static logic HIGH is used for MUX1.
SPCM_PULSEGEN_MUX1_SRC_RUN	1		This input of MUX1 reflects the current run state of the card. If acquisition/output is running the signal is HIGH. If card has stopped the signal is LOW. The signal is identical to XIO output using SPCM_XMODE_RUNSTATE.
SPCM_PULSEGEN_MUX1_SRC_ARM	2		This input of MUX1 reflects the current ARM state of the card. If the card is armed and ready to receive a trigger the signal is HIGH. If the card isn't running or the card is still acquiring pretrigger data or the trigger has already been detected, the signal is LOW. The signal is identical to XIO output using SPCM_XMODE_ARMSTATE.

By having the two status lines ARM and RUN available as input, it is either possible to generate pulses depending only on the card's RUN or ARM state (e.g., currently running or currently *not* running enabling the inverter of MUX1 output) or to mask other trigger conditions from MUX2 to only be passed upon the card's acquisition/replay RUN or ARM state.

Multiplexer 2

The second multiplexer can be transparent and hence unused or allows to select various sources for starting the pulse creation:

- Allowing a start command issued by the application software by issuing a force trigger command
- Any one of the other pulse generator unit outputs to create pulses or pulse trains with up to four repetition time scales
- The card's acquisition or replay trigger output
- An external logic signal coming in from any of the multi-purpose XIO input capable lines

Table 197: Spectrum API: pulse generator trigger MUX2 registers with their available settings

Register	Value	Direction	Description
SPC_XIO_PULSEGEN0_MUX2_SRC	601006	read/write	Selects the input source for MUX2 for pulse generator 0.
SPC_XIO_PULSEGEN1_MUX2_SRC	601106	read/write	Selects the input source for MUX2 for pulse generator 1.
SPC_XIO_PULSEGEN2_MUX2_SRC	601206	read/write	Selects the input source for MUX2 for pulse generator 2.
SPC_XIO_PULSEGEN3_MUX2_SRC	601306	read/write	Selects the input source for MUX2 for pulse generator 3.
SPCM_PULSEGEN_MUX2_SRC_UNUSED	0		No input of MUX2 is used in creating the trigger condition for the pulse generator. A static logic HIGH is used, so that the MUX output is transparent for the following AND gate.
SPCM_PULSEGEN_MUX2_SRC_SOFTWARE	1		This input reflects the positive edge generated by issuing the SPCM_PULSEGEN_CMD_FORCE command.
SPCM_PULSEGEN_MUX2_SRC_CARDTRIGGER	2		This input of MUX2 reflects the trigger detection of the acquisition/replay. The trigger output goes HIGH as soon as the card's main trigger is recognized. After end of acquisition/replay it is LOW again. In Multiple Recording/Gated Sampling/ABA mode it goes LOW after the acquisition of the current segment stops. In FIFO single mode the trigger output is HIGH until FIFO mode is stopped. The signal is identical to what a XIO output is providing when using SPCM_XMODE_TRIGOUT.
SPCM_PULSEGEN_MUX2_SRC_PULSEGEN0	3		Input to MUX2 is set to output of pulse generator 0/1/2 or 3.
SPCM_PULSEGEN_MUX2_SRC_PULSEGEN1	4		This can be used to cascade pulse generators for creating up to four pulse repetition time scales.
SPCM_PULSEGEN_MUX2_SRC_PULSEGEN2	5		Each pulse generator can select to be triggered by any of the other pulse generator's output.
SPCM_PULSEGEN_MUX2_SRC_PULSEGEN3	6		Selecting its own pulse generator's output as a trigger (loopback) is not allowed and will lead to a driver error.
SPCM_PULSEGEN_MUX2_SRC_XIO0	7		Input to MUX2 is set to the input signal coming in from multi-purpose line of X0. <i>M2p:</i> Since X0 is an output only, it therefore is not allowed to be used as an input.
SPCM_PULSEGEN_MUX2_SRC_XIO1	8		Input to MUX2 is set to the input signal coming in from multi-purpose line of X1.
SPCM_PULSEGEN_MUX2_SRC_XIO2	9		Input to MUX2 is set to the input signal coming in from multi-purpose line of X2.
SPCM_PULSEGEN_MUX2_SRC_XIO3	10		Input to MUX2 is set to the input signal coming in from multi-purpose line of X3. <i>M4i/M4x:</i> Since X3 is not available, it therefore is not allowed to be used as an input.

The output of the following command register is connected to all pulse generator units in parallel in a synchronous fashion:

Table 198: Spectrum API: pulse generator command register for trigger forcing by software

Register	Value	Direction	Description
SPC_XIO_PULSEGEN_COMMAND	601501	write only	Executes a command for the pulse generator option.
SPCM_PULSEGEN_CMD_FORCE	1h		Generate a single rising edge, that is common for all pulse generator engines. This allows to start/trigger the output of all enabled pulse generators synchronously by issuing a software command.

This allows to start any number of pulse generators set to MUX2_SRC_SOFTWARE to be started at the same instant even from software, useful when requiring pulses with a known and static phase relation.

Additional trigger configuration (changing the active edge or level)



Please note that the Trigger/Gate input to the "Pulse Generation" portion is always HIGH-active. Depending on the selected pulse generator configuration it is triggering on the rising edge or the logic HIGH state. The two programmable inverters at the multiplexer outputs can be used to trigger on the falling edge or a logical LOW instead.

To access the three programmable inverters and to optionally change whether triggering on a rising edge (the trigger signal changing its state from LOW to HIGH) or on the valid level (the trigger being logically HIGH), following registers can be used:

Table 199: Spectrum API: pulse generator additional configuration registers with the available settings

Register	Value	Direction	Description
SPC_XIO_PULSEGEN0_CONFIG	601007	read/write	Bitmask with additional configuration for pulse generator 0.
SPC_XIO_PULSEGEN1_CONFIG	601107	read/write	Bitmask with additional configuration for pulse generator 1.
SPC_XIO_PULSEGEN2_CONFIG	601207	read/write	Bitmask with additional configuration for pulse generator 2.
SPC_XIO_PULSEGEN3_CONFIG	601307	read/write	Bitmask with additional configuration for pulse generator 3.
SPCM_PULSEGEN_CONFIG_MUX1_INVERT	1h		When bit is set, the output of MUX1 is logically inverted.
SPCM_PULSEGEN_CONFIG_MUX2_INVERT	2h		When bit is set, the output of MUX2 is logically inverted.
SPCM_PULSEGEN_CONFIG_INVERT	4h		When bit is set, the output of the pulse generator is logically inverted.
SPCM_PULSEGEN_CONFIG_HIGH	8h		As default the pulse generator's trigger input is sensitive only to a rising edge. When using this configuration, the input will not look for an active edge, but rather detect a HIGH level. This is similar to the distinction of the card's main trigger modes, when choosing between SPC_TM_POS and SPC_TM_HIGH.

Since the register is implemented as a bitmask, any combination of the above configuration flags is possible.

```
// enable the inverters on MUX1 and MUX2 outputs for pulse generator 2
int32 lPulseGenConfig = (SPCM_PULSEGEN_CONFIG_MUX1_INVERT | SPCM_PULSEGEN_CONFIG_MUX2_INVERT);

spcm_dwSetParam_i32 (hCard, SPC_XIO_PULSEGEN2_CONFIG, lPulseGenConfig);
```

Configuring Multi Purpose lines to output generated pulses

Each of the up to four on-board multi purpose I/O lines can be programmed to output the pulses generated by its corresponding pulse generator unit, making it available for any external devices.

Please check the available modes by reading the SPCM_X0_AVAILMODES, SPCM_X1_AVAILMODES, SPCM_X2_AVAILMODES and SPCM_X3_AVAILMODES register first. The available modes may differ from card to card and may be enhanced with new driver/firmware versions to come.

Table 200: Spectrum API: XIO lines and mode software registers with their reduced to the settings required for outputting pulses

Register	Value	Direction	Description
SPCM_X0_AVAILMODES	600300	read	Bitmask with all bits of the below mentioned modes showing the available modes for (X0)
SPCM_X1_AVAILMODES	600301	read	Bitmask with all bits of the below mentioned modes showing the available modes for (X1)
SPCM_X2_AVAILMODES	600302	read	Bitmask with all bits of the below mentioned modes showing the available modes for (X2)
SPCM_X3_AVAILMODES	600303	read	Bitmask with all bits of the below mentioned modes showing the available modes for (X3)
SPCM_X0_MODE	600200	read/write	Defines the mode for (X0). Only one mode selection is possible to be set at a time
SPCM_X1_MODE	600201	read/write	Defines the mode for (X1). Only one mode selection is possible to be set at a time
SPCM_X2_MODE	600202	read/write	Defines the mode for (X2). Only one mode selection is possible to be set at a time
SPCM_X3_MODE	600203	read/write	Defines the mode for (X3). Only one mode selection is possible to be set at a time
SPCM_XMODE_DISABLE	00000000h		No mode selected. Output is tristate (default setup)
...	...		For all other modes please see chapter "Multi Purpose I/O Lines".
SPCM_XMODE_PULSEGEN	00080000h		A/D and D/A cards only (optional): Connector reflects the output of the same index pulse generator (X1 can output pulses from pulse generator 1, X2 can output pulses from pulse generator 2, ... etc.). On M4i/M4x cards with three XIO lines (X0, X1, X2) and four pulse generators, pulses from pulse generator 3 cannot be output, but can still be used in cascading configurations to trigger another pulse generator.



Please note that a change to the SPCM_X0_MODE, SPCM_X1_MODE, SPCM_X2_MODE or SPCM_X3_MODE will only be updated with the next call to either the M2CMD_CARD_START or M2CMD_CARD_WRITESETUP register. For further details please see the relating chapter on the M2CMD_CARD registers.

Programming Example

The following example shows in principle, the steps required for generating a single, repetitive pulse with one of the pulse generators and how to output that pulse on the matching multi-purpose I/O line:

```
// First we set up the channel selection and the clock.
// For this example we enable only one channel to be able to use max sampling rate on all card types.
spcm_dwSetParam_i32 (hCard, SPC_CHENABLE, CHANNEL0);

// Read out the max. supported sampling rate ...
int64 llMaxSR = 0;
spcm_dwGetParam_i64 (hCard, SPC_PCISAMPLERATE, &llMaxSR);

// ... and use this as the card's sampling rate
spcm_dwSetParam_i64 (hCard, SPC_SAMPLERATE, llMaxSR);

// Read out the clock, at which the pulse generator will run with the above set sampling rate.
int64 llPulseGenClock_Hz = 0;
spcm_dwGetParam_i64 (hCard, SPC_XIO_PULSEGEN_CLOCK, &llPulseGenClock_Hz);

// Configure X0 to output signal from corresponding pulse generator 0
spcm_dwSetParam_i32 (hCard, SPCM_X0_MODE, SPCM_XMODE_PULSEGEN);

// Setup pulse generator 0 (output on X0)
// to generate a continuous signal with 1 MHz and ~50% duty-cycle
int32 lLenFor1MHz = static_cast < int32 > (llPulseGenClock_Hz / MEGA(1));
spcm_dwSetParam_i32 (hCard, SPC_XIO_PULSEGEN0_MODE, SPCM_PULSEGEN_MODE_TRIGGERED);
spcm_dwSetParam_i32 (hCard, SPC_XIO_PULSEGEN0_LEN, lLenFor1MHz);

// An integer division by 2 will be truncated if lLenFor1MHz is an odd number,
// resulting in a slightly shorter HIGH than LOW time.
spcm_dwSetParam_i32 (hCard, SPC_XIO_PULSEGEN0_HIGH, lLenFor1MHz / 2);

// Set LOOPS to 0: repeat infinitely
spcm_dwSetParam_i32 (hCard, SPC_XIO_PULSEGEN0_LOOPS, 0);

// Configure pulse generator to be triggered/started by software force command
spcm_dwSetParam_i32 (hCard, SPC_XIO_PULSEGEN0_MUX1_SRC, SPCM_PULSEGEN_MUX1_SRC_UNUSED);
spcm_dwSetParam_i32 (hCard, SPC_XIO_PULSEGEN0_MUX2_SRC, SPCM_PULSEGEN_MUX2_SRC_SOFTWARE);

// Enable the selected pulse generator and hence arm its trigger detection
spcm_dwSetParam_i32 (hCard, SPC_XIO_PULSEGEN_ENABLE, SPCM_PULSEGEN_ENABLE0);

// Write the settings to the card:
// This will update the clock section to generate the programmed frequencies
// (SPC_SAMPLERATE) and also write the pulse generator settings to the card.
spcm_dwSetParam_i32 (hCard, SPC_M2CMD, M2CMD_CARD_WRITESETUP);

// Start all armed pulse generators (in this case just one) by a software command
spcm_dwSetParam_i32 (hCard, SPC_XIO_PULSEGEN_COMMAND, SPCM_PULSEGEN_CMD_FORCE);

// Wait until a key is pressed
printf ("\nPress a key to stop the pulse generator(s) ");
cGetch ();

// Stop all running pulse generators
spcm_dwSetParam_i32 (hCard, SPC_XIO_PULSEGEN_ENABLE, 0);
spcm_dwSetParam_i32 (hCard, SPC_M2CMD, M2CMD_CARD_WRITESETUP);
```



Spectrum provides a dedicated programming example for the pulse generator feature as part of the standard example package. This example is showing different and more complex configurations than shown above, e.g., cascading of multiple pulse generators for more complex pulse generation time scales.

Option Star-Hub (M3i and M4i only)

Star-Hub introduction

The purpose of the Star-Hub is to extend the number of channels available for acquisition or generation by interconnecting multiple cards and running them simultaneously.

The Star-Hub option allows to synchronize several cards of the same M3i/M4i series that are mounted within one host system (PC):

- For the M3i series there are the two different versions available: a small version with 4 connectors (option SH4) for synchronizing up to four cards and a big version with 8 connectors (option SH8) for synchronizing up to eight cards.
- For the M4i series there are the two different mechanical versions available, with 8 connectors for synchronizing up to eight cards.

The Star-Hub allows synchronizing cards of the same family only. It is not possible to synchronize cards of different families!



Both versions are implemented as a piggy-back module that is mounted to one of the cards. For details on how to install several cards including the one carrying the Star-Hub module, please refer to the section on hardware installation.

Either which of the two available Star-Hub options is used, there will be no phase delay between the sampling clocks of the synchronized cards and either no delay between the trigger events. The card holding the Star-Hub is automatically also the clock master. Any one of the synchronized cards can be part of the trigger generation.

Star-Hub trigger engine

The trigger bus between an M3i/M4i card and the Star-Hub option consists of several lines. Some of them send the trigger information from the card's trigger engine to the Star-Hub and some receives the resulting trigger from the Star-Hub. All trigger events from the different cards connected are combined with OR on the Star-Hub.

While the returned trigger is identical for all synchronized cards, the sent out trigger of every single card depends on their trigger settings.

Star-Hub clock engine

The card holding the Star-Hub is the clock master for the complete system. If you need to feed in an external clock to a synchronized system the clock has to be connected to the master card. Slave cards cannot generate a Star-Hub system clock. As shown in the drawing on the right the clock master can use either the programmable quartz 1 or the external clock input to be broadcast to all other cards.

All cards including the clock master itself receive the distributed clock with equal phase information. This makes sure that there is no phase delay between the cards.

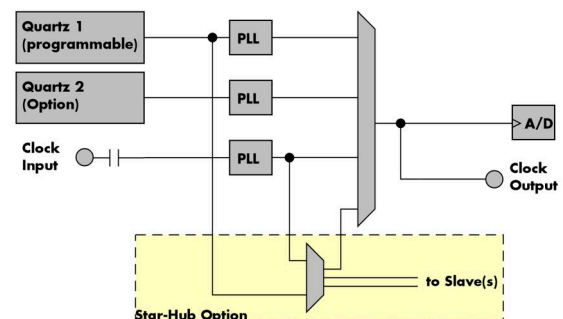


Table 201: star-hub clock overview diagram

Software Interface

The software interface is similar to the card software interface that is explained earlier in this manual. The same functions and some of the registers are used with the Star-Hub. The Star-Hub is accessed using its own handle which has some extra commands for synchronization setup. All card functions are programmed directly on card as before. There are only a few commands that need to be programmed directly to the Star-Hub for synchronization.

The software interface as well as the hardware supports multiple Star-Hubs in one system. Each set of cards connected by a Star-Hub then runs totally independent. It is also possible to mix cards that are connected with the Star-Hub with other cards that run independent in one system.

Star-Hub Initialization

The interconnection between the Star-Hubs is probed at driver load time and does not need to be programmed separately. Instead the cards can be accessed using a logical index. This card index is only based on the ordering of the cards in the system and is not influenced by the current cabling. It is even possible to change the cable connections between two system starts without changing the logical card order that is used for Star-Hub programming.

The Star-Hub initialization must be done AFTER initialization of all cards in the system. Otherwise the inter-connection won't be detected properly.



The Star-Hubs are accessed using a special device name „sync“ followed by the index of the star-hub to access. The Star-Hub is handled completely like a physical card allowing all functions based on the handle like the card itself.

Example with 4 cards and one Star-Hub (no error checking to keep example simple)

```
drv_handle hSync;
drv_handle hCard[4];

for (i = 0; i < 4; i++)
{
    sprintf (s, "/dev/spcm%d", i);
    hCard[i] = spcm_hOpen (s);
}
hSync = spcm_hOpen ("sync0");

...

spcm_vClose (hSync);
for (i = 0; i < 4; i++)
    spcm_vClose (hCard[i]);
```

Example for a digitizerNETBOX or generatorNETBOX with two internal digitizer/generator modules, This example is also suitable for accessing a remote server with two cards installed:

```
drv_handle hSync;
drv_handle hCard[2];

for (i = 0; i < 2; i++)
{
    sprintf (s, "TCPIP::192.168.169.14::INST%d::INSTR", i);
    hCard[i] = spcm_hOpen (s);
}
hSync = spcm_hOpen ("sync0");

...

spcm_vClose (hSync);
for (i = 0; i < 2; i++)
    spcm_vClose (hCard[i]);
```

When opening the Star-Hub the cable interconnection is checked. The Star-Hub may return an error if it sees internal cabling problems or if the connection between Star-Hub and the card that holds the Star-Hub is broken. It can't identify broken connections between Star-Hub and other cards as it doesn't know that there has to be a connection.

The synchronization setup is done using bit masks where one bit stands for one recognized card. All cards that are connected with a Star-Hub are internally numbered beginning with 0. The number of connected cards as well as the connections of the Star-Hub can be read out after initialization. For each card that is connected to the Star-Hub one can read the index of that card:

Table 202: Spectrum API: star-hub related registers for reading detected connections

Register	Value	Direction	Description
SPC_SYNC_READ_NUMCONNECTORS	48991	read	Number of connectors that the Star-Hub offers at max. (available with driver V5.6 or newer)
SPC_SYNC_READ_SYNCCOUNT	48990	read	Number of cards that are connected to this Star-Hub
SPC_SYNC_READ_CARDIDX0	49000	read	Index of card that is connected to star-hub logical index 0 (mask 0x0001)
SPC_SYNC_READ_CARDIDX1	49001	read	Index of card that is connected to Star-Hub logical index 1 (mask 0x0002)
...		read	...
SPC_SYNC_READ_CARDIDX7	49007	read	Index of card that is connected to star-hub logical index 7 (mask 0x0080)
SPC_SYNC_READ_CARDIDX8	49008	read	M2i only: Index of card that is connected to Star-Hub logical index 8 (mask 0x0100)
...		read	...
SPC_SYNC_READ_CARDIDX15	49015	read	M2i only: Index of card that is connected to star-hub logical index 15 (mask 0x8000)
SPC_SYNC_READ_CABLECON0		read	Returns the index of the cable connection that is used for the logical connection 0. The cable connections can be seen printed on the PCB of the star-hub. Use these cable connection information in case that there are hardware failures with the Star-Hub cabling.
...	49100	read	...
SPC_SYNC_READ_CABLECON15	49115	read	Returns the index of the cable connection that is used for the logical connection 15.

In standard systems where all cards are connected to one star-hub reading the Star-Hub logical index will simply return the index of the card again. This results in bit 0 of Star-Hub mask being 1 when doing the setup for card 0, bit 1 in Star-Hub mask being 1 when setting up card

1 and so on. On such systems it is sufficient to read out the SPC_SYNC_READ_SYNCCOUNT register to check whether the Star-Hub has found the expected number of cards to be connected.

```

spcm_dwGetParam_i32 (hSync, SPC_SYNC_READ_SYNCCOUNT, &lSyncCount);
for (i = 0; i < lSyncCount; i++)
{
    spcm_dwGetParam_i32 (hSync, SPC_SYNC_READ_CARDIDX0 + i, &lCardIdx);
    printf ("Star-Hub logical index %d is connected with card %d\n", i, lCardIdx);
}

```

In case of 4 cards in one system and all are connected with the Star-Hub this program excerpt will return:

```

Star-Hub logical index 0 is connected with card 0
Star-Hub logical index 1 is connected with card 1
Star-Hub logical index 2 is connected with card 2
Star-Hub logical index 3 is connected with card 3

```

Let's see a more complex example with two Star-Hubs and one independent card in one system. Star-Hub A connects card 2, card 4 and card 5. Star-Hub B connects card 0 and card 3. Card 1 is running completely independent and is not synchronized at all:

card	Star-Hub connection	card handle	Star-Hub handle	card index in Star-Hub	mask for this card in Star-Hub
card 0	-	/dev/spcm0		0 (of Star-Hub B)	0x0001
card 1	-	/dev/spcm1			-
card 2	Star-Hub A	/dev/spcm2	sync0	0 (of Star-Hub A)	0x0001
card 3	Star-Hub B	/dev/spcm3	sync1	1 (of Star-Hub B)	0x0002
card 4	-	/dev/spcm4		1 (of Star-Hub A)	0x0002
card 5	-	/dev/spcm5		2 (of Star-Hub A)	0x0004

Now the program has to check both Star-Hubs:

```

for (j = 0; j < lStarhubCount; j++)
{
    spcm_dwGetParam_i32 (hSync[j], SPC_SYNC_READ_SYNCCOUNT, &lSyncCount);
    for (i = 0; i < lSyncCount; i++)
    {
        spcm_dwGetParam_i32 (hSync[j], SPC_SYNC_READ_CARDIDX0 + i, &lCardIdx);
        printf ("Star-Hub %c logical index %d is connected with card %d\n", (!j ? 'A' : 'B'), i, lCardIdx);
    }
    printf ("\n");
}

```

In case of the above mentioned cabling this program excerpt will return:

```

Star-Hub A logical index 0 is connected with card 2
Star-Hub A logical index 1 is connected with card 4
Star-Hub A logical index 2 is connected with card 5

Star-Hub B logical index 0 is connected with card 0
Star-Hub B logical index 1 is connected with card 3

```

For the following examples we will assume that 4 cards in one system are all connected to one Star-Hub to keep things easier.

Setup of Synchronization

The synchronization setup only requires one additional register to enable the cards that are synchronized in the next run

Table 203: Spectrum API: synchronization enable mask register

Register	Value	Direction	Description
SPC_SYNC_ENABLEMASK	49200	read/write	Mask of all cards that are enabled for the synchronization

The enable mask is based on the logical index explained above. It is possible to just select a couple of cards for the synchronization. All other cards then will run independently. Please be sure to always enable the card on which the Star-Hub is located as this one is a must for the synchronization.

In our example we synchronize all four cards. The Star-Hub is located on card #2 and is therefore the clock master

```
spcm_dwSetParam_i32 (hSync, SPC_SYNC_ENABLEMASK, 0x000F); // all 4 cards are masked

// set the clock master to 100 MS/s internal clock
spcm_dwSetParam_i32 (hCard[2], SPC_CLOCKMODE, SPC_CM_INTPLL);
spcm_dwSetParam_i32 (hCard[2], SPC_SAMPLERATE, MEGA(100));

// set all the slaves to run synchronously with 100 MS/s
spcm_dwSetParam_i32 (hCard[0], SPC_SAMPLERATE, MEGA(100));
spcm_dwSetParam_i32 (hCard[1], SPC_SAMPLERATE, MEGA(100));
spcm_dwSetParam_i32 (hCard[3], SPC_SAMPLERATE, MEGA(100));
```

Setup of Trigger

Setting up the trigger does not need any further steps of synchronization setup. Simply all trigger settings of all cards that have been enabled for synchronization are connected together. All trigger sources and all trigger modes can be used on synchronization as well.

Having positive edge of external trigger on card 0 to be the trigger source for the complete system needs the following setup:

```
spcm_dwSetParam_i32 (hCard[0], SPC_TRIG_ORMASK, SPC_TMASK_EXT0);
spcm_dwSetParam_i32 (hCard[0], SPC_TRIG_EXT0_MODE, SPC_TM_POS);

spcm_dwSetParam_i32 (hCard[1], SPC_TRIG_ORMASK, SPC_TM_NONE);
spcm_dwSetParam_i32 (hCard[2], SPC_TRIG_ORMASK, SPC_TM_NONE);
spcm_dwSetParam_i32 (hCard[3], SPC_TRIG_ORMASK, SPC_TM_NONE);
```

Assuming that the 4 cards are analog data acquisition cards with 4 channels each we can simply setup a synchronous system with all channels of all cards being trigger source. The following setup will show how to set up all trigger events of all channels to be OR connected. If any of the channels will now have a signal above the programmed trigger level the complete system will do an acquisition:

```
for (i = 0; i < lSyncCount; i++)
{
    int32 lAllChannels = (SPC_TMASK0_CH0 | SPC_TMASK0_CH1 | SPC_TMASK0_CH2 | SPC_TMASK0_CH3);
    spcm_dwSetParam_i32 (hCard[i], SPC_TRIG_CH_ORMASK0, lAllChannels);
    for (j = 0; j < 2; j++)
    {
        // set all channels to trigger on positive edge crossing trigger level 100
        spcm_dwSetParam_i32 (hCard[i], SPC_TRIG_CH0_MODE + j, SPC_TM_POS);
        spcm_dwSetParam_i32 (hCard[i], SPC_TRIG_CH0_LEVEL0 + j, 100);
    }
}
```

Run the synchronized cards

Running of the cards is very simple. The Star-Hub acts as one big card containing all synchronized cards. All card commands have to be omitted directly to the Star-Hub which will check the setup, do the necessary steps for synchronization and distribute the commands in the correct order to all synchronized cards.

The same card commands that are normally send to a single cards are also valid to be send to the Star-Hub:

Table 204: Spectrum API: star-hub synchronization commands

Register	Value	Direction	Description
SPC_M2CMD	100	write only	Executes a command for the card or data transfer
M2CMD_CARD_RESET	1h		Performs a hard and software reset of the card as explained further above
M2CMD_CARD_WRITESSETUP	2h		Writes the current setup to the card without starting the hardware. This command may be useful if changing some internal settings like clock frequency and enabling outputs.
M2CMD_CARD_START	4h		Starts the card with all selected settings. This command automatically writes all settings to the card if any of the settings has been changed since the last one was written. After card has been started none of the settings can be changed while the card is running.
M2CMD_CARD_ENABLETRIGGER	8h		The trigger detection is enabled. This command can be either send together with the start command to enable trigger immediately or in a second call after some external hardware has been started.
M2CMD_CARD_FORCETRIGGER	10h		This command forces a trigger even if none has been detected so far. Sending this command together with the start command is similar to using the software trigger.
M2CMD_CARD_DISABLETRIGGER	20h		The trigger detection is disabled. All further trigger events are ignored until the trigger detection is again enabled. When starting the card the trigger detection is started disabled.
M2CMD_CARD_STOP	40h		Stops the current run of the card. If the card is not running this command has no effect.

All other commands and all other settings should be send directly to the card(s) that they refer to. While sending the wait commands to the Star-Hub handle is allowed, these commands are not distributed to/collected from the synchronized cards but only refer synonymously to the card carrying the Star-Hub.

This example shows the complete setup and synchronization start for our four cards:

```

spcm_dwSetParam_i32 (hSync, SPC_SYNC_ENABLEMASK, 0x000F); // all 4 cards are masked

// to keep it easy we set all card to the same clock and disable trigger
for (i = 0; i < 4; i++)
{
    spcm_dwSetParam_i32 (hCard[i], SPC_CLOCKMODE, SPC_CM_INTPLL);
    spcm_dwSetParam_i32 (hCard[i], SPC_SAMPLERATE, MEGA(100));
    spcm_dwSetParam_i32 (hCard[i], SPC_TRIG_ORMASK, SPC_TM_NONE);
}

// card 0 is trigger master and waits for external positive edge
spcm_dwSetParam_i32 (hCard[0], SPC_TRIG_ORMASK, SPC_TMASK_EXT0);
spcm_dwSetParam_i32 (hCard[0], SPC_TRIG_EXT0_MODE, SPC_TM_POS);

// start the cards and wait for them a maximum of 1 second to be ready
spcm_dwSetParam_i32 (hSync, SPC_TIMEOUT, 1000);
spcm_dwSetParam_i32 (hSync, SPC_M2CMD, M2CMD_CARD_START | M2CMD_CARD_ENABLETRIGGER);
if (spcm_dwSetParam_i32 (hSync, SPC_M2CMD, M2CMD_CARD_WAITREADY) == ERR_TIMEOUT)
    printf ("Timeout occured - no trigger received within time\n");

```

Using one of the wait commands for the Star-Hub will return as soon as the card holding the Star-Hub has reached this state. However when synchronizing cards with different memory sizes there may be other cards that still haven't reached this level.



SH-Direct: using the Star-Hub clock directly without synchronization

Starting with driver version 1.26 it is possible to use the clock from the Star-Hub just like an external clock and running one or more cards totally independent of the synchronized card. The mode is by example useful if one has one or more output cards that run continuously in a loop and are synchronized with Star-Hub and in addition to this one or more acquisition cards should make multiple acquisitions but using the same clock.

For all M2i cards it is also possible to run the „slave“ cards with a divided clock. Therefore please program a desired divided sampling rate in the SPC_SAMPLERATE register (example: running the Star-Hub card with 10 MS/s and the independent cards with 1 MS/s). The sampling rate is automatically adjusted by the driver to the next matching value.

What is necessary?

- All cards need to be connected to the Star-Hub
- The card(s) that should run independently can not hold the Star-Hub
- The card(s) with the Star-Hub must be setup to synchronization even if it's only one card
- The synchronized card(s) have to be started prior to the card(s) that run with the direct Star-Hub clock

Setup

At first all cards that should run synchronized with the Star-Hub are set-up exactly as explained before. The card(s) that should run independently and use the Star-Hub clock need to use the following clock mode:

Table 205: Spectrum API: clock mode register and settings for SH Direct mode

Register	Value	Direction	Description
SPC_CLOCKMODE	20200	read/write	Defines the used clock mode
SPC_CM_SHDIRECT	128		Uses the clock from the Star-Hub as if this was an external clock

When using SH_Direct mode, the register call to SPC_CLOCKMODE enabling this mode must be written before initiating a card start command to any of the connected cards. Also it is not allowed to be modified later in the programming sequence to prevent the driver from calculating wrong sample rates.



Example

In this example we have one generator card with the Star-Hub mounted running in a continuous loop and one acquisition card running independently using the SH-Direct clock.

```
// setup of the generator card
spcm_dwSetParam_i32 (hCard[0], SPC_CARDMODE, SPC_REC_STD_SINGLE);
spcm_dwSetParam_i32 (hCard[0], SPC_LOOPS, 0); // infinite data replay
spcm_dwSetParam_i32 (hCard[0], SPC_CLOCKMODE, SPC_CM_INTPLL);
spcm_dwSetParam_i32 (hCard[0], SPC_SAMPLERATE, MEGA(1));
spcm_dwSetParam_i32 (hCard[0], SPC_TRIG_ORMASK, SPC_TM_SOFTWARE);

spcm_dwSetParam_i32 (hSync, SPC_SYNC_ENABLEMASK, 0x0001); // card 0 is the generator card
spcm_dwSetParam_i32 (hSync, SPC_SYNC_CLKMASK, 0x0001); // only for M2i/M3i cards: set ClkMask

// Setup of the acquisition card (waiting for external trigger)
spcm_dwSetParam_i32 (hCard[1], SPC_CARDMODE, SPC_REC_STD_SINGLE);
spcm_dwSetParam_i32 (hCard[1], SPC_CLOCKMODE, SPC_CM_SHDIRECT);
spcm_dwSetParam_i32 (hCard[1], SPC_SAMPLERATE, MEGA(1));
spcm_dwSetParam_i32 (hCard[1], SPC_TRIG_ORMASK, SPC_TM_MASK_EXT0);
spcm_dwSetParam_i32 (hCard[1], SPC_TRIG_EXT0_MODE, SPC_TM_POS);

// now start the generator card (sync!) first and then the acquisition card
spcm_dwSetParam_i32 (hSync, SPC_TIMEOUT, 1000);
spcm_dwSetParam_i32 (hSync, SPC_M2CMD, M2CMD_CARD_START | M2CMD_CARD_ENABLETRIGGER);

// start first acquisition
spcm_dwSetParam_i32 (hCard[1], SPC_M2CMD, M2CMD_CARD_START | M2CMD_CARD_ENABLETRIGGER | M2CMD_CARD_WAITREADY);

// process data

// start next acquisition
spcm_dwSetParam_i32 (hCard[1], SPC_M2CMD, M2CMD_CARD_START | M2CMD_CARD_ENABLETRIGGER | M2CMD_CARD_WAITREADY);

// process data
```

Error Handling

The Star-Hub error handling is similar to the card error handling and uses the function `spcm_dwGetErrorInfo_i32`. Please see the example in the card error handling chapter to see how the error handling is done.

Mode Block Average (Firmware Option)

Overview

General Information

The Block Average Module improves the fidelity of any repetitive signal by removing its random noise components. The Module allows multiple single acquisitions to be made, accumulated and averaged. The process reduces random noise improving the visibility of the repetitive signal. The averaged signal has an enhanced measurement resolution and increased signal-to-noise (SNR) ratio.

The complete averaging process is performed inside the FPGA of the digitizer and involves no CPU load at all. Averaging also reduces the amount of data that needs to be transferred to the host PC further reducing CPU demand and speeding up measurement times.

The Block Average mode is fully compatible with streaming (FIFO) mode so that the digitizer can accumulate and average signals for hours or days without losing a single event. The Module takes advantage of an advanced trigger circuit, with very fast re-arm time, so that signals can be averaged at ultra-fast rates going as high as 5 million events per second.

The signal processing firmware also includes the standard digitizer firmware so that normal digitizer operation can be performed with no limitations.

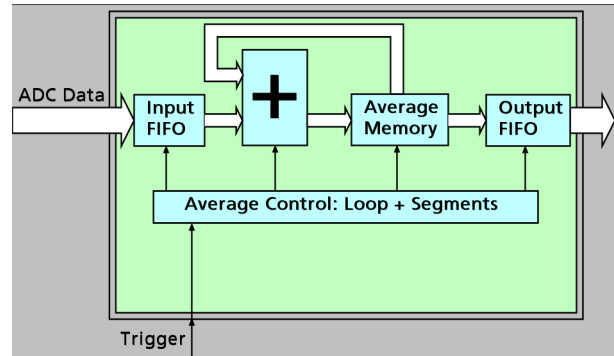


Image 84: block average FPGA option block diagram

Principle of operation

In Block Average mode the acquisition works very similar to the Multiple Recording mode.

The memory is segmented and with each trigger condition a pre-defined number of samples, a segment, is acquired.

The Block Average option now takes a programmable number of these acquired consecutive data segments and averages them sample by sample over one another.

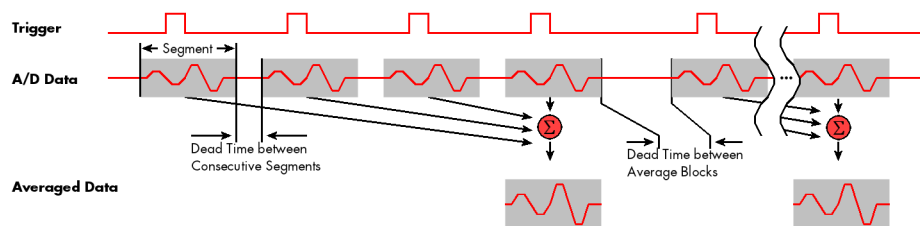


Image 85: block average FPGA option - principle of operation

The result of one averaging operation is a segment with summed values, that has the same length as each original „RAW“ segments, but each sample now consists of the sum of all samples of the averaged segment at the same location in relation to the trigger signal.

In order to get any meaningful results out of the Block Average operation, a repetitive signal is required along with a stable trigger condition.

Simplified Block Diagram

The following block diagram shows the general structure and data flows of the M4i/M4x/M5i based digitizer hardware. When running in the standard digitizer configuration the signal processing block simply consists of a bypass, handing the input data to the memory controller without further calculations.

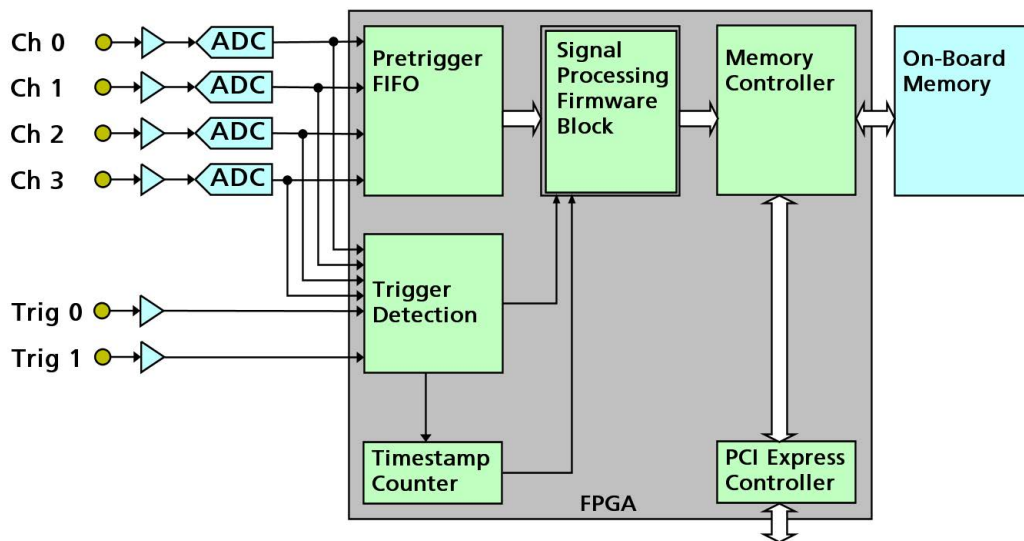


Image 86: simplified block diagram of FPGA structure with signal processing firmware block

Setting up the Acquisition

The Block Average mode allows the acquisition of data blocks with multiple trigger events without restarting the hardware.

With each trigger event, one segment will be acquired (as shown) and the „Segment“ is then processed by the average firmware. The on-board memory will be divided into several segments of the same size to hold the processed data. Each segment will be filled with data from the Averager, if the defined number of triggered segments have been acquired. As this mode is totally controlled in hardware there is a very small re-arm time from end of one segment until the trigger detection is enabled again. You'll find that re-arm time in the technical data section of this manual.

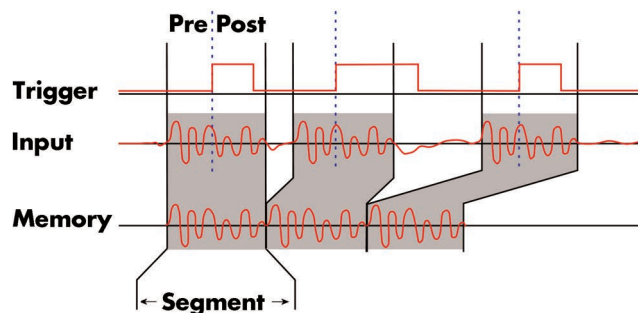


Image 87: timing diagram of block average acquisition

The following table shows the register for defining the structure of the segments to be recorded with each trigger event.

Table 206: Spectrum API: software registers and register settings for programming the block average mode

Register	Value	Direction	Description
SPC_POSTTRIGGER	10100	read/write	Defines the number of samples per channel to be recorded after the trigger event.
SPC_SEGMENTSIZE	10010	read/write	Size of one triggered segment (in RAW samples) as well as the averaged segment (in 32bit samples). The total number of samples to be recorded per channel after detection of one trigger event includes the time recorded before the trigger (pre trigger = segmentsize - posttrigger).
SPC_AVERAGES	10050	read/write	Defines the number of triggered segments that are averaged sample per sample over one another.

Each segment consist of pretrigger and posttrigger samples. The user always has to set the total segment size and the posttrigger, while the pretrigger is calculated within the driver with the formula: [pretrigger] = [segment size] - [posttrigger].

When using Block Averaging the maximum pretrigger is limited depending on the number of active channels. When the calculated value exceeds that limit, the driver will return the error ERR_PRETRIGGERLEN. Please have a look at the table further below to see the maximum pretrigger length that is possible.



Recording modes

Standard Mode

With every detected trigger event one data block is filled with data. The length of one triggered segment is set by the value of the segment size register SPC_SEGMENTSIZE. The total amount of samples to be recorded is defined by the memsize register.

Memsizes must be set to a multiple of the segment size. The table below shows the register for enabling Block Average. For detailed information on how to setup and start the standard acquisition mode please refer to the according chapter earlier in this manual.

Table 207: Spectrum API: card mode registers and register settings for standard lock average mode

Register	Value	Direction	Description
SPC_CARDMODE	9500	read/write	Defines the used operating mode
SPC_REC_STD_AVERAGE	20000h		Enables Block Averaging for standard acquisition with 32 bit wide result data.
SPC_REC_STD_AVERAGE_16BIT	80000h		Enables Block Averaging for standard acquisition with 16 bit wide result data (8 bit cards only).

The total number of samples to be recorded to the on-board memory in Standard Mode is defined by the SPC_MEMSIZE register.

Register	Value	Direction	Description
SPC_MEMSIZE	10000	read/write	Defines the total number of samples to be recorded per channel.

FIFO Mode

The Block Averaging in FIFO Mode is similar to the Block Averaging in Standard Mode. In contrast to the standard mode it is not necessary to program the number of samples to be recorded. The acquisition is running until the user stops it. The data is read block by block by the driver as described under FIFO single mode example earlier in this manual. These blocks are online available for further data processing by the user program. This mode significantly reduces the amount of data to be transferred on the PCI bus as gaps of no interest do not have to be transferred. This enables you to use faster sample rates than you would be able to in FIFO mode without Block Averaging. The advantage of Block Averaging in FIFO mode is that you can stream data online to the host system. You can make real-time data processing or store a huge amount of data to the hard disk. The table below shows the dedicated register for enabling Block Averaging. For detailed information how to setup and start the board in FIFO mode please refer to the according chapter earlier in this manual. The number of seg-

Table 208: Spectrum API: card mode registers and register settings for FIFO block average mode

Register	Value	Direction	Description
SPC_CARDMODE	9500	read/write	Defines the used operating mode
SPC_REC_FIFO_AVERAGE	200000h		Enables Block Averaging for FIFO acquisition with 32 bit wide result data.
SPC_REC_FIFO_AVERAGE_16BIT	400000h		Enables Block Averaging for FIFO acquisition with 16 bit wide result data. (8 bit ADC cards only)

ments to be recorded must be set separately with the register shown in the following table:

Table 209: Spectrum API: block average mode loop register and register settings

Register	Value	Direction	Description
SPC_LOOPS	10020	read/write	Defines the number of segments to be recorded
0			Recording will be infinite until the user stops it.
1 ... [4G - 1]			Defines the total averaged segments to be recorded.

Limits of pre trigger, post trigger, memory size

The maximum memory size parameter is only limited by the number of activated channels and by the amount of installed memory. Please keep in mind, that each averaged sample needs either 2 bytes (16bit) or 4 bytes (32bit) of memory to be stored. The required size in memory depends on the selected average mode. The 16bit modes are available only for cards that have RAW 8bit ADC samples. Minimum memory size as well as minimum and maximum post trigger limits are independent of the activated channels or the installed memory.

Due to the internal organization of the card memory there is a certain stepsize when setting these values that has to be taken into account. The following table gives you an overview of all limits concerning pre trigger, post trigger, memory size, segment size and loops.

For cards with 12bit, 14bit and 16bit ADC resolution (firmware V14 and above):

Activated Channels	Used Mode	Memory size SPC_MEMSIZE			Pre trigger			Post trigger SPC_POSTTRIGGER			Segment size SPC_SEGMENTSIZE			Loops SPC_LOOPS			Number of Averages SPC_AVERAGES		
		Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step
1 Ch	Standard Average FIFO Average	32	1Gi not used	16	16	8Ki	16	16	128Ki-16	16	32	128Ki	16	0 (∞)	not used 4Gi - 1	1	2	64Ki	1
2 Ch	Standard Average FIFO Average	32	512Mi not used	16	16	8Ki	16	16	64Ki-16	16	32	64Ki	16	0 (∞)	not used 4Gi - 1	1	2	64Ki	1
4 Ch	Standard Average FIFO Average	32	256Mi not used	16	16	8Ki	16	16	32Ki-16	16	32	32Ki	16	0 (∞)	not used 4Gi - 1	1	2	64Ki	1

For cards with 8bit ADC resolution, 32 bit data mode (firmware V14 and above):

Activated Channels	Used Mode	Memory size SPC_MEMSIZE			Pre trigger			Post trigger SPC_POSTTRIGGER			Segment size SPC_SEGMENTSIZE			Loops SPC_LOOPS			Number of Averages SPC_AVERAGES		
		Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step
1 Ch	Standard Average FIFO Average	64	not used	32	32	8Ki	32	32	64Ki-32	32	64	64Ki	32	0 (∞)	not used 4Gi - 1	1	4	16Mi	1
2 Ch	Standard Average FIFO Average	64	512Mi not used	32	32	8Ki	32	32	32Ki-32	32	64	32Ki	32	0 (∞)	not used 4Gi - 1	1	4	16Mi	1
4 Ch	Standard Average FIFO Average	64	256Mi not used	32	32	8Ki	32	32	16Ki-32	32	64	16Ki	32	0 (∞)	not used 4Gi - 1	1	4	16Mi	1

For cards with 8bit ADC resolution, 16 bit data mode (firmware V14 and above):

Activated Channels	Used Mode	Memory size SPC_MEMSIZE			Pre trigger			Post trigger SPC_POSTTRIGGER			Segment size SPC_SEGMENTSIZE			Loops SPC_LOOPS			Number of Averages SPC_AVERAGES		
		Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step
1 Ch	Standard Average FIFO Average	64	2Gi not used	32	32	8Ki	32	32	128Ki-32	32	128	128Ki	64	0 (∞)	not used 4Gi - 1	1	4	256	1
2 Ch	Standard Average FIFO Average	64	1Gi not used	32	32	8Ki	32	32	64Ki-32	32	128	64Ki	64	0 (∞)	not used 4Gi - 1	1	4	256	1
4 Ch	Standard Average FIFO Average	64	512Mi not used	32	32	8Ki	32	32	32Ki-32	32	128	32Ki	64	0 (∞)	not used 4Gi - 1	1	4	256	1

All figures listed here are given in samples. An entry of [8Ki - 16] means [8 KibiSamples - 16] = 8176 samples.

Trigger Modes

When using Block Averaging all of the card's trigger modes can be used except the software trigger. For detailed information on the available trigger modes, please take a look at the relating chapter earlier in this manual.

Output Data Format

When using Block Averaging mode the resulting samples will be, depending on the selected average mode, either 16bit signed integer values (8bit ADC cards using AVERAGE_16BIT mode only) or 32bit signed integer values per channel, that each consist of the sum of a particular sample over all averaged segments. The following table illustrates this with the first four of 'S+1' samples of one channel (A0, A1, A2, A3, ..., AS) that are N times averaged (summed):

Table 210: Spectrum API: block average mode output sample format

	Samples of one segment with segment size S over time					
Triggered Segment No. 1	A0(1)	A1(1)	A2(1)	A3(1)	...	AS(1)
Triggered Segment No. 2	A0(2)	A1(2)	A2(2)	A3(2)	...	AS(2)
...	...	...	...	...	...	...
Triggered Segment No. N	A0(N)	A1(N)	A2(N)	A3(N)	...	AS(N)
Resulting averaged Samples	$\sum_{i=1}^N A0(i)$	$\sum_{i=1}^N A1(i)$	$\sum_{i=1}^N A2(i)$	$\sum_{i=1}^N A3(i)$	...	$\sum_{i=1}^N AS(i)$

So the resulting „resolution“ of the samples increases with the number of averages. For example averaging 16 bit RAW samples two times results in a final resolution of 17 bit, averaging it four times results in a sample with 18 bit „resolution“.

By not dividing down the samples by the number of averages in the firmware and providing the user application with the 32 bit/16 bit wide sums, one can take full advantage of the enhanced resolution by using proper data formats in the application software.

Data organization

Data is organized in a multiplexed way in the transfer buffer the same way as the RAW samples would be. If using 2 channels data of first activated channel comes first, then data of second channel:

Table 211: Spectrum API: block average mode data organization

Activated Channels	Ch0	Ch1	Ch2	Ch3	Mode dependent 16bit or 32bit wide averaged samples ordering in buffer memory starting with data offset zero																
1 channel	X				A0	A1	A2	A3	A4	A5	A6	A7	A8	A9	A10	A11	A12	A13	A14	A15	A16
1 channel		X			B0	B1	B2	B3	B4	B5	B6	B7	B8	B9	B10	B11	B12	B13	B14	B15	B16
1 channel			X		C0	C1	C2	C3	C4	C5	C6	C7	C8	C9	C10	C11	C12	C13	C14	C15	C16
1 channel				X	D0	D1	D2	D3	D4	D5	D6	D7	D8	D9	D10	D11	D12	D13	D14	D15	D16
2 channels	X	X			A0	B0	A1	B1	A2	B2	A3	B3	A4	B4	A5	B5	A6	B6	A7	B7	A8
2 channels	X		X		A0	C0	A1	C1	A2	C2	A3	C3	A4	C4	A5	C5	A6	C6	A7	C7	A8
2 channels	X			X	A0	D0	A1	D1	A2	D2	A3	D3	A4	D4	A5	D5	A6	D6	A7	D7	A8
2 channels		X	X		B0	C0	B1	C1	B2	C2	B3	C3	B4	C4	B5	C5	B6	C6	B7	C7	B8
2 channels		X		X	B0	D0	B1	D1	B2	D2	B3	D3	B4	D4	B5	D5	B6	D6	B7	D7	B8
2 channels			X	X	C0	D0	C1	D1	C2	D2	C3	D3	C4	D4	C5	D5	C6	D6	C7	D7	C8
4 channels	X	X	X	X	A0	B0	C0	D0	A1	B1	C1	D1	A2	B2	C2	D2	A3	B3	C3	D3	A4

The samples are re-named for better readability. A0 is sample 0 of channel 0, B4 is sample 4 of channel 1, and so on. The averaged samples now just have a wider format of 32 bit/16 bit independent of the original RAW sample resolution.

Programming examples

The following example shows how to set up the card for Block Average in standard mode with 32 bit wide output data.

```
// define some parameters via variables
uint32 dwNoOfChannels = 2;           // Two active channels
uint64 qwNumberOfSegments = 4;       // four averaged segments will be acquired
uint64 qwSegmentSize = 1024;         // Set the segment size to 1024 samples
uint64 qwPosttrigger = 768;          // Set the posttrigger to 768 samples and therefore
                                      // the pretrigger will be 256 samples

uint64 qwSetMemsize = qwSegmentSize * qwNumberOfSegments; // calculate memsize

// for averaging the number of bytes per sample is fixed to 4 (32 bit samples)
// and memory for all channels is needed
uint64 qwMemInBytes = qwSetMemsize * sizeof(int32) * dwNoOfChannels;
void* pvBuffer = pvAllocMemPageAligned(qwMemInBytes);

// set up DMA transfer with the card
spcm_dwDefTransfer_i64 (stCard.hDrv, SPCM_BUF_DATA, SPCM_DIR_CARDTOPC, 0, pvBuffer, 0, qwMemInBytes);

// configure acquisition
spcm_dwSetParam_i32 (hDrv, SPC_CARDMODE, SPC_REC_STD_AVERAGE); // Enables Standard Averaging
spcm_dwSetParam_i32 (hDrv, SPC_AVERAGES, 100);                  // 100 triggered acquisitions will be
                                                                    // averaged for one output segment

spcm_dwSetParam_i64 (hDrv, SPC_SEGMENTSIZE, qwSegmentSize);
spcm_dwSetParam_i64 (hDrv, SPC_POSTTRIGGER, qwPosttrigger);
spcm_dwSetParam_i64 (hDrv, SPC_MEMSIZE, qwSetMemsize);

spcm_dwSetParam_i32 (hDrv, SPC_TRIG_EXT0_MODE, SPC_TM_POS); // Set triggermode to ext. TTL mode (rising edge)
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_ORMASK, SPC_TMASK_EXT0); // and enable it within the trigger OR-mask
```

The following example shows how to set up the card for Block Average in FIFO mode.

```
// define some parameters via variables
uint64 qwNumberOfSegments = 256;     // 256 averaged segments will be acquired
uint64 qwSegmentSize = 2048;         // Set the segment size to 2048 samples
uint64 qwPosttrigger = 1920;          // Set the posttrigger to 1920 samples and therefore
                                      // the pretrigger will be 128 samples

// FIFO buffer setup not shown here for simplicity. See FIFO buffer setup in according chapter for details.

// configure acquisition
spcm_dwSetParam_i32 (hDrv, SPC_CARDMODE, SPC_REC_FIFO_AVERAGE); // Enables FIFO Averaging
spcm_dwSetParam_i32 (hDrv, SPC_AVERAGES, 100);                  // 100 triggered acquisitions will be
                                                                    // averaged for one output segment

spcm_dwSetParam_i64 (hDrv, SPC_SEGMENTSIZE, qwSegmentSize);
spcm_dwSetParam_i64 (hDrv, SPC_POSTTRIGGER, qwPosttrigger);
spcm_dwSetParam_i64 (hDrv, SPC_MEMSIZE, qwSetMemsize);
spcm_dwSetParam_i64 (hDrv, SPC_LOOPS, qwNumberOfSegments);

spcm_dwSetParam_i32 (hDrv, SPC_TRIG_EXT0_MODE, SPC_TM_POS); // Set triggermode to ext. TTL mode (rising edge)
spcm_dwSetParam_i32 (hDrv, SPC_TRIG_ORMASK, SPC_TMASK_EXT0); // and enable it within the trigger OR-mask
```

Mode Block Statistics (Firmware Option)

Overview

General Information

The Block Statistics and Peak Detection Module implements a widely used data analysis and reduction technology in hardware. Each block is scanned for its minimum and maximum peak and a summary data set that includes the minimum, maximum, average, timestamps and position information is stored in memory.

The complete Block Statistics and Peak Detection process is done inside the FPGA of the digitizer producing no CPU load at all. This data reduction process decreases the amount of data that needs to be transferred to the host PC further reducing CPU demand and speeding up measurement times.

The signal processing firmware also includes the standard digitizer firmware so that normal digitizer operation can be performed with no limitations.

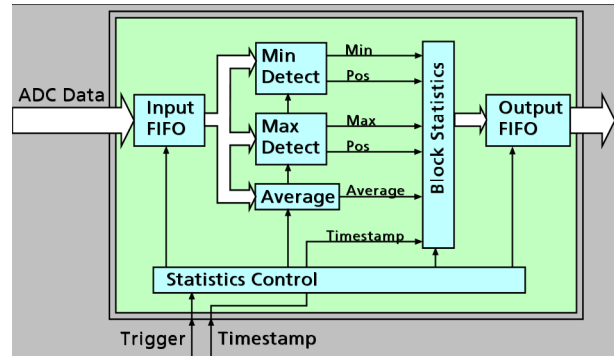


Image 88: block statistics FPGA option block diagram

Waveform Block Statistics

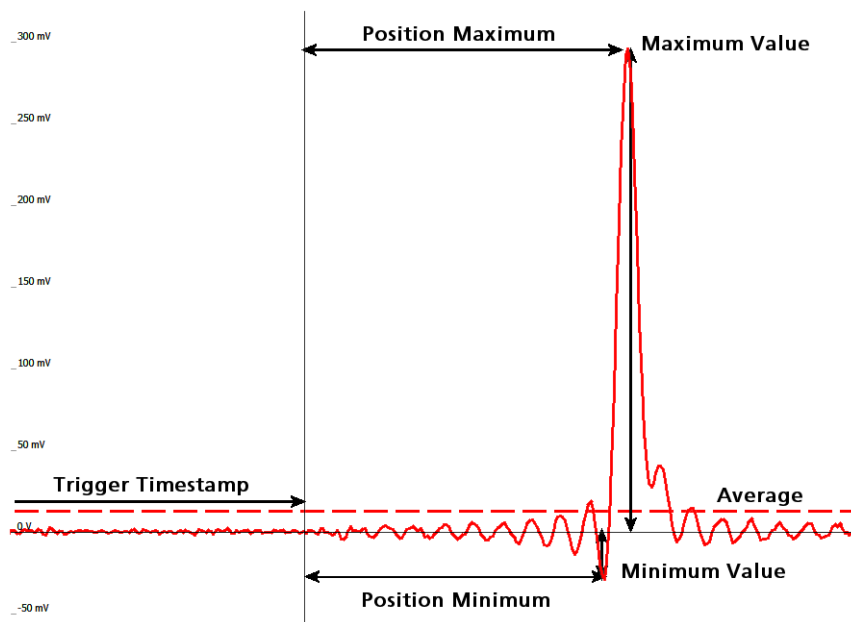


Image 89: Overview of waveform block statistics information results

Information Set

Average Value	64 Bit signed integer
Minimum Value	16 Bit signed integer
Maximum Value	16 Bit signed integer
Minimum Position	32 Bit unsigned integer
Maximum Position	32 Bit unsigned integer
Unused	32 Bit
TriggerTimestamp	64 Bit unsigned integer

The data will be processed per segment by the Block Statistic firmware and reduced to the shown information set. The timestamp data shown here is the lower 64bit of the „normal“ timestamp mentioned in its own chapter in this manual. For convenience this timestamp is included in the information set, so that it is not necessary to set up the EXTRA_DMA channels for separate timestamp transfer as mentioned in the timestamp chapter.

The timestamp value will stamp the trigger position, after the pre-trigger is recorded. The complete segment consisting of pre trigger and post trigger is analyzed by the Block Statistics module afterwards. The positions of the minimum and maximum value shown in the drawing above are counted in samples from the begin of the complete segment - ergo from the begin of the pre trigger.

To combine the timestamp value and the position, the pre trigger value needs to be considered accordingly:

$$[\text{MinPos}(X) \text{ in Segment}(X)] = [\text{Timestamp}(X)] - [\text{Pretrigger}] + [\text{Position Minimum}(X)]$$

$$[\text{MinPos}(X+1) \text{ in Segment}(X+1)] = [\text{Timestamp}(X+1)] - [\text{Pretrigger}] + [\text{Position Minimum}(X+1)]$$

This enables to properly correlate the positions in time and therefore also calculate the time difference between positions:

$$[\text{Delta Minimum Position}] = \text{MinPos}(x+1) - \text{MinPos}(X)$$

Simplified Block Diagram

The following block diagram shows the general structure and data flows of the M4i/M4x/M5i based digitizer hardware. When running in the standard digitizer configuration the signal processing block simply consists of a bypass, handing the input data to the memory controller without further calculations.

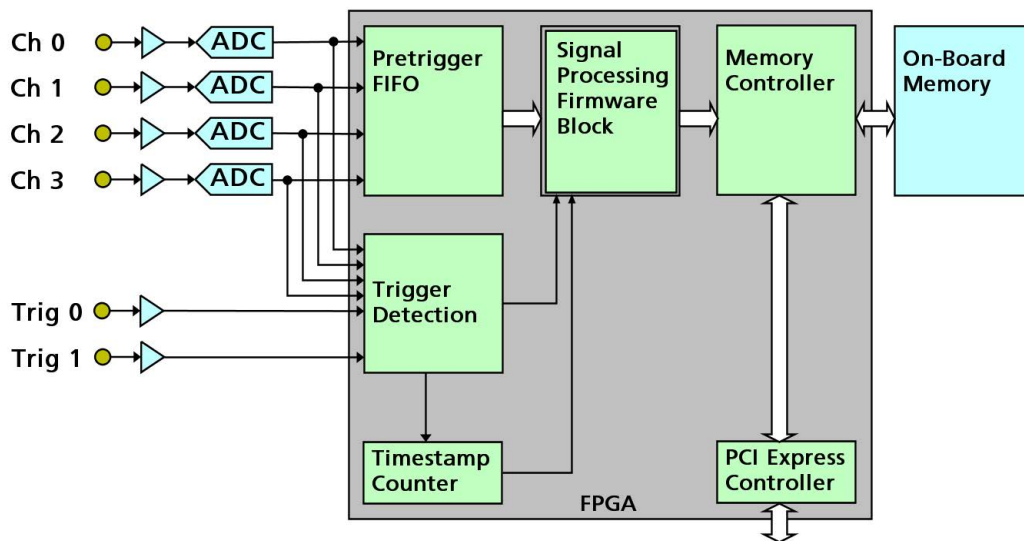


Image 90: simplified block diagram of FPGA structure with signal processing firmware block

Setting up the Acquisition

The Block Statistic mode allows the acquisition of data blocks with multiple trigger events without restarting the hardware.

With each trigger event one segment will be acquired (as shown) and this „Segment“ is then processed by the statistics firmware.

These segments are of pre-defined length very similar to Multiple Recording.

As this mode is totally controlled in hardware there is a very small re-arm time from end of one segment until the trigger detection is enabled again. You'll find that re-arm time in the technical data section of this manual.

The following table shows the register for defining the structure of the segments to be recorded with each trigger event.

Table 212: Spectrum API: software registers and register settings for programming the block statistics mode

Register	Value	Direction	Description
SPC_POSTTRIGGER	10100	read/write	Defines the number of samples to be recorded per channel after the trigger event.
SPC_SEGMENTSIZE	10010	read/write	Size of one segment. The total number of samples to be recorded per channel after detection of one trigger event includes the time recorded before the trigger (pre trigger = segmentsize - posttrigger).

Each segment consist of pretrigger and posttrigger samples. The user always has to set the total segment size and the posttrigger, while the pretrigger is calculated within the driver with the formula: $[\text{pretrigger}] = [\text{segment size}] - [\text{posttrigger}]$.

When using Block Statistics the maximum pretrigger is limited depending on the number of active channels. When the calculated value exceeds that limit, the driver will return the error ERR_PRETRIGGERLEN. Please have a look at the table further below to see the maximum pretrigger length that is possible.



Recording modes

Standard Mode

With every detected trigger event one data block is filled with data. The length of one triggered segment is set by the value of the segment size register SPC_SEGMENTSIZE. The total amount of samples to be recorded is defined by the memsize register.

Memsize must be set to a multiple of the segment size. The table below shows the register for enabling Block Statistic. For detailed information on how to setup and start the standard acquisition mode please refer to the according chapter earlier in this manual.

Table 213: Spectrum API: card mode registers and register settings for standard block statistics mode

Register	Value	Direction	Description
SPC_CARDMODE	9500	read/write	Defines the used operating mode
SPC_REC_STD_SEGSTATS	65536		Enables Block Statistic for standard acquisition.

The total number of samples to be recorded to the on-board memory in Standard Mode is defined by the SPC_MEMSIZE register.

Register	Value	Direction	Description
SPC_MEMSIZE	10000	read/write	Defines the total number of samples to be recorded per channel.

FIFO Mode

The Block Statistic in FIFO Mode is similar to the Block Statistic in Standard Mode. In contrast to the standard mode it is not necessary to program the number of samples to be recorded. The acquisition is running until the user stops it. The data is read block by block by the driver as described under FIFO single mode example earlier in this manual. These blocks are online available for further data processing by the user program. This mode significantly reduces the amount of data to be transferred on the PCI bus as gaps of no interest do not have to be transferred. This enables you to use faster sample rates than you would be able to in FIFO mode without Block Statistic.

The advantage of Block Statistic in FIFO mode is that you can stream data online to the host system. You can make real-time data processing or store a huge amount of data to the hard disk. The table below shows the dedicated register for enabling Block Statistic. For detailed information how to setup and start the board in FIFO mode please refer to the according chapter earlier in this manual.

Table 214: Spectrum API: card mode registers and register settings for FIFO block statistics mode

Register	Value	Direction	Description
SPC_CARDMODE	9500	read/write	Defines the used operating mode
SPC_REC_FIFO_SEGSTATS	1048576		Enables Block Statistic for FIFO acquisition.

The number of segments to be recorded must be set separately with the register shown in the following table:

Table 215: Spectrum API: block statistics mode loop register and register settings

Register	Value	Direction	Description
SPC_LOOPS	10020	read/write	Defines the number of segments to be recorded
0			Recording will be infinite until the user stops it.
1 ... [4Gi - 1]			Defines the total segments to be recorded.

Limits of pre trigger, post trigger, memory size

The maximum memory size parameter is only limited by the number of activated channels and by the amount of installed memory. For each segment and for each channel 32 bytes (256bit) of memory is needed to store the processed data. Minimum memory size as well as minimum and maximum post trigger limits are independent of the activated channels or the installed memory.

Due to the internal organization of the card memory there is a certain stepsize when setting these values that has to be taken into account. The following table gives you an overview of all limits concerning pre trigger, post trigger, memory size, segment size and loops. The table shows all values in relation to the installed memory size in samples. If more memory is installed the maximum memory size figures will increase according to the complete installed memory.

Activated Channels	Used Mode	Memory size			Pre trigger			Post trigger			Segment size			Loops		
		SPC_MEMSIZE						SPC_POSTTRIGGER			SPC_SEGMENTSIZE			SPC_LOOPS		
		Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step
1 Ch	Standard Statistics	32	2Gi	16	16	8Ki	16	16	32Ki-16	16	32	2Gi	16	not used		
	FIFO Statistics		not used		16	8Ki	16				32	2Gi	16	0 [∞]	4Gi - 1	1
2 Ch	Standard Statistics	32	1Gi	16	16	8Ki	16	16	16Ki-16	16	32	1Gi	16	not used		
	FIFO Statistics		not used		16	8Ki	16				32	1Gi	16	0 [∞]	4Gi - 1	1
4 Ch	Standard Statistics	32	512Mi	16	16	8Ki	16	16	8Ki-16	16	32	512Mi	16	not used		
	FIFO Statistics		not used		16	8Ki	16				32	512Mi	16	0 [∞]	4Gi - 1	1

Activated Channels	Used Mode	Memory size SPC_MEMSIZE			Pre trigger			Post trigger SPC_POSTTRIGGER			Segment size SPC_SEGMENTSIZE			Loops SPC_LOOPS		
		Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step	Min	Max	Step
1 Ch	Standard Statistics	32	4Gi	32	32	8Ki	32	32	64Ki-32	32	64	4Gi	32	0 (∞)	not used	4Gi - 1 1
	FIFO Statistics		not used		32	8Ki	32				64	4Gi	32			
2 Ch	Standard Statistics	32	2Gi	32	32	8Ki	32	32	32Ki-32	32	64	2Gi	32	0 (∞)	not used	4Gi - 1 1
	FIFO Statistics		not used		32	8Ki	32				64	2Gi	32			
4 Ch	Standard Statistics	32	1Gi	32	32	8Ki	32	32	16Ki-32	32	64	1Gi	32	0 (∞)	not used	4Gi - 1 1
	FIFO Statistics		not used		32	8Ki	32				64	1Gi	32			

Trigger Modes

Information Set Format

```
// --- define data structure for block statistic mode
typedef struct
{
    int64  llAavg:           64; // 8 bytes
    int16  nMin:             16; // 2 bytes
    int16  nMax:             16; // 2 bytes
    uint32 dwMinPos:         32; // 4 bytes
    uint32 dwMaxPos:         32; // 4 bytes
    uint32 _Unused:          32; // 4 bytes
    uint64 qw Timestamp:     64; // 8 bytes
} SPCM_SEGSTAT_STRUCT_CHx; // 32 bytes in total for one information set of one channel CHx
```



Data organization

Table 216: Spectrum API: block statistics mode data organization

Activated Channels	Ch0	Ch1	Ch2	Ch3	32bytes information set ordering in buffer memory starting with data offset zero																
1 channel	X				A0	A1	A2	A3	A4	A5	A6	A7	A8	A9	A10	A11	A12	A13	A14	A15	A16
1 channel		X			B0	B1	B2	B3	B4	B5	B6	B7	B8	B9	B10	B11	B12	B13	B14	B15	B16
1 channel			X		C0	C1	C2	C3	C4	C5	C6	C7	C8	C9	C10	C11	C12	C13	C14	C15	C16
1 channel				X	D0	D1	D2	D3	D4	D5	D6	D7	D8	D9	D10	D11	D12	D13	D14	D15	D16
2 channels	X	X			A0	B0	A1	B1	A2	B2	A3	B3	A4	B4	A5	B5	A6	B6	A7	B7	A8
2 channels	X		X		A0	C0	A1	C1	A2	C2	A3	C3	A4	C4	A5	C5	A6	C6	A7	C7	A8
2 channels	X			X	A0	D0	A1	D1	A2	D2	A3	D3	A4	D4	A5	D5	A6	D6	A7	D7	A8
2 channels		X	X		B0	C0	B1	C1	B2	C2	B3	C3	B4	C4	B5	C5	B6	C6	B7	C7	B8
2 channels		X		X	B0	D0	B1	D1	B2	D2	B3	D3	B4	D4	B5	D5	B6	D6	B7	D7	B8
2 channels			X	X	C0	D0	C1	D1	C2	D2	C3	D3	C4	D4	C5	D5	C6	D6	C7	D7	C8
4 channels	X	X	X	X	A0	B0	C0	D0	A1	B1	C1	D1	A2	B2	C2	D2	A3	B3	C3	D3	A4

(c) Spectrum Instrumentation GmbH

Programming examples

The following example shows how to set up the card for Block Statistic in standard mode.

```
// define structure for more easy data access to all channels
typedef struct
{
    SPCM_SEGSTAT_STRUCT_CHx pst_Channel[2];
} SPCM_SEGSTAT_STRUCT_2CH;

// define some parameters via variables
uint32 dwNoOfChannels = 2;           // Two active channels
uint64 qwNumberOfSegments = 4;       // four segments will be acquired
uint64 qwSegmentSize = 1024;         // Set the segment size to 1024 samples
uint64 qwPosttrigger = 768;          // Set the posttrigger to 768 samples and therefore
                                     // the pretrigger will be 256 samples

uint64 qwSetMemsize = qwSegmentSize * qwNumberOfSegments; // calculate memsize

// for each information set the number of bytes is fixed to 32bytes
// and memory for all channels and all segments is needed
uint64 qwMemInBytes = qwNumberOfSegments * dwNoOfChannels * sizeof (SPCM_SEGSTAT_STRUCT_CHx);
void* pvBuffer = (void*) pvAllocMemPageAligned (qwMemInBytes);

// configure acquisition
spcm_dwSetParam_i32 (hDrv, SPC_CARDMODE, SPC_REC_STD_SEGSTATS); // Enables Block Statistic

spcm_dwSetParam_i64 (hDrv, SPC_SEGMENTSIZE, qwSegmentSize);
spcm_dwSetParam_i64 (hDrv, SPC_POSTTRIGGER, qwPosttrigger);
spcm_dwSetParam_i64 (hDrv, SPC_MEMSIZE, qwSetMemsize);

// explicitly set timestamp mode to any other value than SPC_TSMODE_DISABLE
spcm_dwSetParam_i32 (hDrv, SPC_TIMESTAMP_CMD, SPC_TSMODE_STARTRESET);

// set up DMA transfer with the card
spcm_dwDefTransfer_i64 (stCard.hDrv, SPCM_BUF_DATA, SPCM_DIR_CARDTOPC, 0, pvBuffer, 0, qwMemInBytes);

// ... Card start and transfer start not shown here for simplicity

// casting the buffer for easy data access
SPCM_SEGSTAT_STRUCT_2CH* ppstData = (SPCM_SEGSTAT_STRUCT_2CH*) pvBuffer;

// read out data of every segment (Min, Max, and Average only to keep things simple)
for (uint64 qwSegment = 0; qwSegment < qwNumberOfSegments; qwSegment++)
    for (uint32 dwChannel = 0, dwChannel < dwNoOfChannels; dwChannel++)
        printf("\nSegment %.2d: Min: %7.4d Max:%7.4d, TS:%16llx, Avrg; %f",
            qwSegment,
            ppstData[qwSegment].pst_Channel[dwChannel].nMin,
            ppstData[qwSegment].pst_Channel[dwChannel].nMax,
            ppstData[qwSegment].pst_Channel[dwChannel].qw_Timestamp,
            ((double) (ppstData[qwSegment].pst_Channel[dwChannel].llAvrg) / (double) qwSegmentSize));
```

Appendix

Error Codes

The following error codes could occur when a driver function has been called. Please check carefully the allowed setup for the register and change the settings to run the program.

Table 217: Spectrum API: driver error codes and error description

error name	value (hex)	value (dec.)	error description
ERR_OK	0h	0	Execution OK, no error.
ERR_INIT	1h	1	An error occurred when initializing the given card. Either the card has already been opened by another process or an hardware error occurred.
ERR_TYP	3h	3	Initialization only: The type of board is unknown. This is a critical error. Please check whether the board is correctly plugged in the slot and whether you have the latest driver version.
ERR_FNCNOTSUPPORTED	4h	4	This function is not supported by the hardware version.
ERR_BRDREMAP	5h	5	The board index re map table in the registry is wrong. Either delete this table or check it carefully for double values.
ERR_KERNELVERSION	6h	6	The version of the kernel driver is not matching the version of the DLL. Please do a complete re-installation of the hardware driver. This error normally only occurs if someone copies the driver library and the kernel driver manually.
ERR_HWDRVVERSION	7h	7	The hardware needs a newer driver version to run properly. Please install the driver that was delivered together with the card.
ERR_ADRRANGE	8h	8	One of the address ranges is disabled (fatal error), can only occur under Linux.
ERR_INVALIDHANDLE	9h	9	The used handle is not valid.
ERR_BOARDNOTFOUND	Ah	10	A card with the given name has not been found.
ERR_BOARDINUSE	Bh	11	A card with given name is already in use by another application.
ERR_EXPHW64BITADR	Ch	12	Express hardware version not able to handle 64 bit addressing -> update needed.
ERR_FWVERSION	Dh	13	Firmware versions of synchronized cards or for this driver do not match -> update needed.
ERR_SYNCPROTOCOL	Eh	14	Synchronization protocol versions of synchronized cards do not match -> update needed.
ERR_KERNEL	Fh	15	Some error occurred in the kernel driver. On Linux check output of dmesg for details.
ERR_LASTERR	10h	16	Old error waiting to be read. Please read the full error information before proceeding. The driver is locked until the error information has been read.
ERR_BOARDINUSE	11h	17	Board is already used by another application. It is not possible to use one hardware from two different programs at the same time.
ERR_ABORT	20h	32	Abort of wait function. This return value just tells that the function has been aborted from another thread. The driver library is not locked if this error occurs.
ERR_BOARDLOCKED	30h	48	The card is already in access and therefore locked by another process. It is not possible to access one card through multiple processes. Only one process can access a specific card at the time.
ERR_DEVICE_MAPPING	32h	50	The device is mapped to an invalid device. The device mapping can be accessed via the Control Center.
ERR_NETWORKSETUP	40h	64	The network setup of a digitizerNETBOX has failed.
ERR_NETWORKTRANSFER	41h	65	The network data transfer from/to a digitizerNETBOX has failed.
ERR_FWPOWERCYCLE	42h	66	Power cycle (PC off/on) is needed to update the card's firmware (a simple OS reboot is not sufficient!).
ERR_NETWORKTIMEOUT	43h	67	A network time out has occurred.
ERR_BUFFERSIZE	44h	68	The buffer size is not sufficient (too small).
ERR_RESTRICTEDACCESS	45h	69	The access to the card has been intentionally restricted.
ERR_INVALIDPARAM	46h	70	An invalid parameter has been used for a certain function.
ERR_TEMPERATURE	47h	71	The temperature of at least one of the card's sensors measures a temperature, that is too high for the hardware.
ERR_REG	100h	256	The register is not valid for this type of board.
ERR_VALUE	101h	257	The value for this register is not in a valid range. The allowed values and ranges are listed in the board specific documentation.
ERR_FEATURE	102h	258	Feature (option) is not installed on this board. It's not possible to access this feature if it's not installed.
ERR_SEQUENCE	103h	259	Command sequence is not allowed. Please check the manual carefully to see which command sequences are possible.
ERR_READABORT	104h	260	Data read is not allowed after aborting the data acquisition.
ERR_NOACCESS	105h	261	Access to this register is denied. This register is not accessible for users.
ERR_TIMEOUT	107h	263	A time out occurred while waiting for an interrupt. This error does not lock the driver.
ERR_CALLTYPE	108h	264	The access to the register is only allowed with one 64 bit access but not with the multiplexed 32 bit (high and low double word) version.
ERR_EXCEEDSINT32	109h	265	The return value is int32 but the software register exceeds the 32 bit integer range. Use double int32 or int64 accesses instead, to get correct return values.
ERR_NOWRITEALLOWED	10Ah	266	The register that should be written is a read-only register. No write accesses are allowed.
ERR_SETUP	10Bh	267	The programmed setup for the card is not valid. The error register will show you which setting generates the error message. This error is returned if the card is started or the setup is written.
ERR_CLOCKNOTLOCKED	10Ch	268	Synchronization to external clock failed: no signal connected or signal not stable. Please check external clock or try to use a different sampling clock to make the PLL locking easier.
ERR_MEMINIT	10Dh	269	On-board memory initialization error. Power cycle the PC and try another PCIe slot (if possible). In case that the error persists, please contact Spectrum support for further assistance.
ERR_POWERSUPPLY	10Eh	270	On-board power supply error. Power cycle the PC and try another PCIe slot (if possible). In case that the error persists, please contact Spectrum support for further assistance.
ERR_ADCCOMMUNICATION	10Fh	271	Communication with ADC failed. Power cycle the PC and try another PCIe slot (if possible). In case that the error persists, please contact Spectrum support for further assistance.

Table 217: Spectrum API: driver error codes and error description

error name	value (hex)	value (dec.)	error description
ERR_CHANNEL	110h	272	The channel number may not be accessed on the board: Either it is not a valid channel number or the channel is not accessible due to the current setup (e.g. Only channel 0 is accessible in interlace mode).
ERR_NOTIFYSIZE	111h	273	The notify size of the last spcm_dwDefTransfer call is not valid. The notify size must be a multiple of the page size of 4096. For data transfer it may also be a fraction of 4Ki in the range of 16, 32, 64, 128, 256, 512, 1Ki or 2Ki. For ABA and timestamp the notify size can be 2Ki as a minimum.
ERR_RUNNING	120h	288	The board is still running, this function is not available now or this register is not accessible now.
ERR_ADJUST	130h	304	Automatic card calibration has reported an error. Please check the card inputs.
ERR_PRETRIGGERLEN	140h	320	The calculated pretrigger size (resulting from the user defined posttrigger values) exceeds the allowed limit.
ERR_DIRMISMATCH	141h	321	The direction of card and memory transfer mismatch. In normal operation mode it is not possible to transfer data from PC memory to card if the card is an acquisition card nor it is possible to transfer data from card to PC memory if the card is a generation card.
ERR_POSTEXCDSEGMENT	142h	322	The posttrigger value exceeds the programmed segment size in multiple recording/ABA mode. A delay of the multiple recording segments is only possible by using the delay trigger!
ERR_SEGMENTINMEM	143h	323	Memsize is not a multiple of segment size when using Multiple Recording/Replay or ABA mode. The programmed segment size must match the programmed memory size.
ERR_MULTIPLEPW	144h	324	Multiple pulsewidth counters used but card only supports one at the time.
ERR_NOCHANNELPWOR	145h	325	The channel pulsewidth on this card can't be used together with the OR conjunction. Please use the AND conjunction of the channel trigger sources.
ERR_ANDORMASKOVLAP	146h	326	Trigger AND mask and OR mask overlap in at least one channel. Each trigger source can only be used either in the AND mask or in the OR mask, no source can be used for both.
ERR_ANDMASKEDGE	147h	327	One channel is activated for trigger detection in the AND mask but has been programmed to a trigger mode using an edge trigger. The AND mask can only work with level trigger modes.
ERR_ORMASKLEVEL	148h	328	One channel is activated for trigger detection in the OR mask but has been programmed to a trigger mode using a level trigger. The OR mask can only work together with edge trigger modes.
ERR_EDGEPERMOD	149h	329	This card is only capable to have one programmed trigger edge for each module that is installed. It is not possible to mix different trigger edges on one module.
ERR_DOLEVELMINDIFF	14Ah	330	The minimum difference between low output level and high output level is not reached.
ERR_STARHUBENABLE	14Bh	331	The card holding the star-hub must be enabled when doing synchronization.
ERR_PATPWSMALEDGE	14Ch	332	Combination of pattern with pulsewidth smaller and edge is not allowed.
ERR_XMODESETUP	14Dh	333	The chosen setup for (SPCM_X0_MODE .. SPCM_X19_MODE) is not valid. See hardware manual for details.
ERR_AVRG_LSA	14Eh	334	Setup for Average LSA Mode not valid. Check Threshold and Replacement values for chosen AVRGMODE.
ERR_PCICHECKSUM	203h	515	The check sum of the card information has failed. This could be a critical hardware failure. Restart the system and check the connection of the card in the slot.
ERR_MEMALLOC	205h	517	Internal memory allocation failed. Please restart the system and be sure that there is enough free memory.
ERR_EEPROMLOAD	206h	518	Time out occurred while loading information from the on-board EEPROM. This could be a critical hardware failure. Please restart the system and check the PCI connector.
ERR_CARDNOSUPPORT	207h	519	The card that has been found in the system seems to be a valid Spectrum card of a type that is supported by the driver but the driver did not find this special type internally. Please get the latest driver from www.spectrum-instrumentation.com and install this one.
ERR_CONFIGACCESS	208h	520	Internal error occurred during config writes or reads. Please contact Spectrum support for further assistance.
ERR_FIFOHWOVERRUN	301h	769	FIFO acquisition: Hardware buffer overrun in FIFO mode. The complete on-board memory has been filled with data and data wasn't transferred fast enough to PC memory. FIFO replay: Hardware buffer underrun in FIFO mode. The complete on-board memory has been replayed and data wasn't transferred fast enough from PC memory. If acquisition or replay throughput is lower than the theoretical bus throughput, check the application buffer setup.
ERR_FIFOFINISHED	302h	770	FIFO transfer has been finished, programmed data length has been transferred completely.
ERR_TIMESTAMP_SYNC	310h	784	Synchronization to timestamp reference clock failed. Please check the connection and the signal levels of the reference clock input.
ERR_STARHUB	320h	800	The auto routing function of the Star-Hub initialization has failed. Please check whether all cables are mounted correctly.
ERR_INTERNAL_ERROR	FFFFh	65535	Internal hardware error detected. Please check for driver and firmware update of the card.

Spectrum Knowledge Base

You will also find additional help and information in our knowledge base available on our website:

<https://spectrum-instrumentation.com/support/knowledgebase/index.php>

Temperature sensors

The M4i/M4x card series has integrated temperature sensors that allow to read out different internal temperatures. These functions are also available for the internal M4i cards inside the digitizerNETBOX, generatorNETBOX or hybridNETBOX series. In here the temperature can be read out for every internal card separately.

Temperature read-out registers

Up to three different temperature sensors can be read-out for each M4i and M4x card. Depending on the specific card type not all of these temperature sensors are used. The temperature can be read in different temperature scales at any time:

Table 218: Spectrum API: temperature read-out registers of internal temperature sensors

Register	Value	Direction	Description
SPC_MON_TK_BASE_CTRL	500022	read	Base card temperature in Kelvin
SPC_MON_TK_MODULE_0	500023	read	Module temperature 0 in Kelvin
SPC_MON_TK_MODULE_1	500024	read	Module temperature 1 in Kelvin
SPC_MON_TC_BASE_CTRL	500025	read	Base card temperature in degrees Celsius
SPC_MON_TC_MODULE_0	500026	read	Module temperature 0 in degrees Celsius
SPC_MON_TC_MODULE_1	500027	read	Module temperature 1 in degrees Celsius
SPC_MON_TF_BASE_CTRL	500028	read	Base card temperature in degrees Fahrenheit
SPC_MON_TF_MODULE_0	500029	read	Module temperature 0 in degrees Fahrenheit
SPC_MON_TF_MODULE_1	500030	read	Module temperature 1 in degrees Fahrenheit

Temperature hints

- Monitoring of the temperature figures is recommended for environments where the operating temperature can reach or even exceed the specified operating temperature. Please see technical data section for specified operating temperatures.
- The temperature sensors can be used to optimize the system cooling.

23xx temperatures and limits

The following description shows the meaning of each temperature figure on the 23xx series and also gives maximum ratings that should not be exceeded. All figures given in degrees Celsius:

Sensor Name	Sensor Location	Typical figure at 25°C environment temperature	Maximum temperature
BASE_CTRL	Inside FPGA	50°C ±5°C	80°C
MODULE_0	Inside ADC	60°C ±5°C	90°C
MODULE_1	Amplifier Front-End	50°C ±5°C	80°C

Details on M4i/M4x cards I/O lines

Multi-Purpose I/O Lines

The MMCX Multi Purpose I/O connectors (X0, X1 and X2) of the M4i/M4x cards from Spectrum are protected against over-voltage conditions. For this purpose clamping diodes of the types CD1005 are used in conjunction with a series resistor. All three I/O lines are internally clamped to signal ground and to 3.3V clamping voltage. This limits the voltage at the buffer to 3.3V plus the diodes intrinsic forward-voltage of 0.6V to 0.7V.

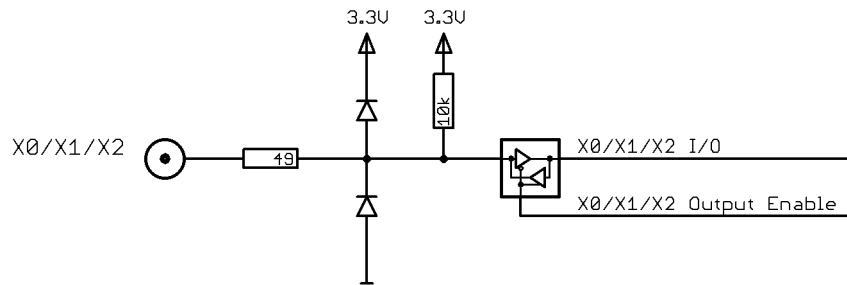


Image 92: electrical structure of multi-purpose I/O lines

The maximum forward current limit for the used CD1005 diodes is 100 mA, which is effectively limited by the used series resistor for logic levels up to 5.0V. To avoid floating levels with unconnected inputs, a pull up resistor of 10 kOhm to 3.3V is used on each line.

Interfacing with clock input

The clock input of the M4i/M4x cards is AC-coupled, single-ended PECL type. Due to the internal biasing and a relatively high maximum input voltage swing, it can be directly connected to various logic standards, without the need for external level converters.

Single-ended LVTTTL sources

All LVTTTL sources, be it 2.5V LVTTTL or 3.3V LVTTTL must be terminated with a 50 Ohm series resistor to avoid reflections and limit the maximum swing for the M4i card.

Differential (LV)PECL sources

Differential drivers require equal load on both the true and the inverting outputs. Therefore the inverting output should be loaded as shown in the drawing. All PECL drivers require a proper DC path to ground, therefore emitter resistors R_e must be used, whose value depends on the supply voltage of the driving PECL buffer:

$V_{CC} - V_{EE}$	2.5 V	3.3 V	5.0 V
R_e	~50 Ohm	~100 Ohm	~200 Ohm

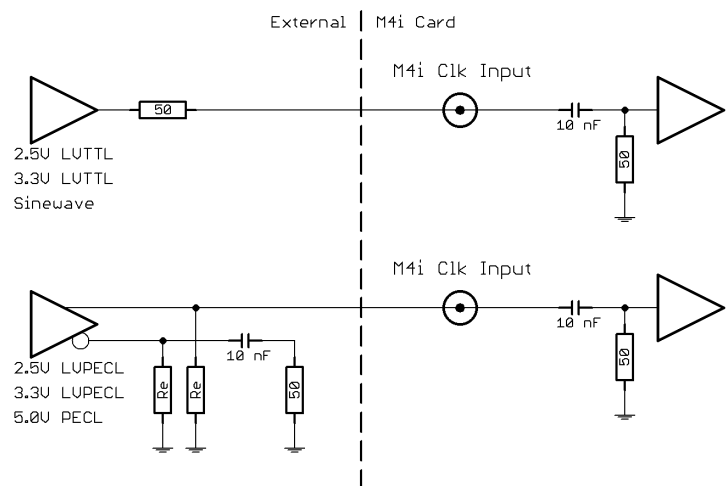


Image 93: electrical structure of clock inputs and potential interfacing circuits

Interfacing with clock output

The clock output of the M4i/M4x cards is AC-coupled, single-ended PECL type. The output swing of the M4i/M4x clock output is approximately 800 mV_{pp}.

Internal biased single-ended receivers

Because of the AC coupling of the M4i/M4x clock output, the signal must be properly re-biased for the receiver. Receivers that provide an internal re-bias only require the signal to be terminated to ground by a 50 Ohm resistor.

Differential (LV)PECL receivers

Differential receivers require proper re-biasing and likely a small minimum difference between the true and the inverting input to avoid ringing with open receiver inputs. Therefore a Thevenin-equivalent can be used, with receiver-type dependent values for R_1 , R_2 , R_1' and R_2' .

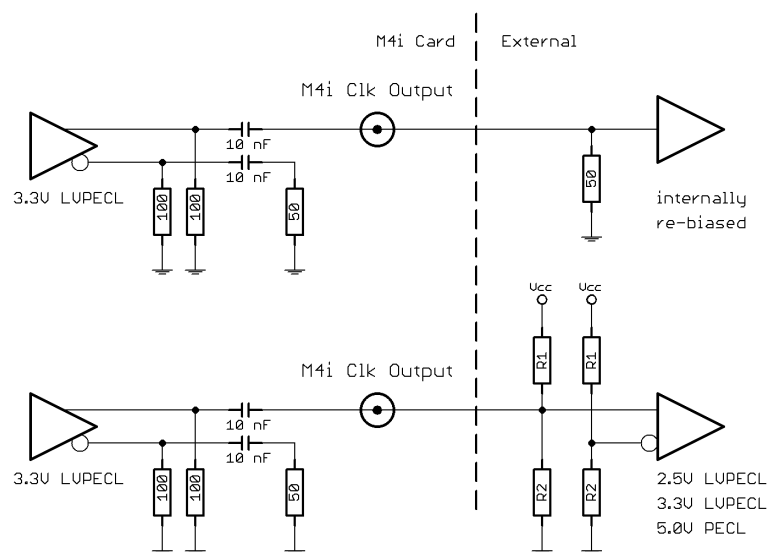


Image 94: electrical structure of clock outputs and potential interfacing circuits

Details on M4i/M4x cards status LED

Every M4i card has a two-color status LED mounted within the multi-purpose I/O connector field on the card bracket.



The same two-color LED is located on the bracket of the M4x cards as well.



This chapter explains the different color codes and offers some possible solutions in case of an error condition.

Table 219: card status LED color and blink coding

Condition	LED color	Status	Solution
Off	Off	Card not powered	Power on the PC.
Error	Static: red	Power supply error	Restart the PC. In case that the error persists, please contact Spectrum support for further assistance.
	Fast blinking (aprox. 4 Hz): red - green - red - green ...	Power supply error	Restart the PC. In case that the error persists, please contact Spectrum support for further assistance.
	Blinking: red - off - red - off ...	Over temperature error	Power down the PC, let the card cool down and restart the system. Please make sure that you have a proper cooling fan installed to supply the M4i card in the PCIe slot with a constant air flow.
	Strobed blinking: long red - short off - short red - short off ...	FPGA boot error	This error code is available with Power Firmware V1.8 or newer. Power down the PC and restart the system. In case that this error is occurring after a firmware update please contact Spectrum support for assistance on how to boot the card's golden recovery image.
	Slow blinking (aprox. 1 Hz): red - green - red - green ...	PCI Express link training has not finished	1) Power down the PC, un-plug and re-plug the card to verify that there is a proper contact between the card and the slot. 2) Try another PCI Express slot, maybe the currently used one is not properly working. In case that the above steps did not help, please contact Spectrum support for assistance.
O.K.	Static: green	Card is ready for operation (at full PCIe speed)	A full speed PCIe link has been established (PCIe x8, Gen 2) and the card is ready for operation.
	Slow blinking (approx. 1 Hz): green - off - green - off ...	Indicator mode on (at full PCIe speed)	To ease the identification of a specific card in a multi-card system without un-installing the card it is possible to activate the card identification status by software. This mode changes the static „Ready for Operation“ green into a blinking state.
	Static: green & red (yellow)	Card is ready for operation (at reduced PCIe speed)	A reduced speed PCIe link has been established either with less than all of the possible 8 lanes and/or the card is installed in a PCIe Gen 1 slot. The card is ready for operation, but the data transfer throughput over the PCI Express bus is reduced. For getting the highest PCIe performance please consult your PC's or motherboard's manual for details on the PCI Express slots of your system.
	Slow blinking (approx. 1 Hz): yellow - off - yellow - off ...	Indicator mode on (at reduced PCIe speed)	To ease the identification of a specific card in a multi-card system without un-installing the card it is possible to activate the card identification status by software. This mode changes the static „Ready for Operation“ yellow into a blinking state.

Turning on card identification LED

To enable/disable the cards LED indicator mode or to read out the current setting, please use the following register:

Table 220: Spectrum API: card identification LED register

Register	Value	Direction	Description
SPC_CARDIDENTIFICATION	201500	read/write	Writing a '1' turns on the LED card indicator mode, writing a '0' turns off the LED indicator mode.

The default for the card identification register is the OFF state.

Continuous memory for increased data transfer rate



The continuous memory buffer has been added to the driver version 1.36. The continuous buffer is not available in older driver versions. Please update to the latest driver if you wish to use this function.

Background

All modern operating systems use a very complex memory management strategy that strictly separates between physical memory, kernel memory and user memory. The memory management is based on memory pages (normally 4 KiByte = 4096 Bytes). All software only sees virtual memory that is translated into physical memory addresses by a memory management unit based on the mentioned pages.

This will lead to the circumstance that although a user program allocated a larger memory block (as an example 1 MiByte) and it sees the whole 1 MiByte as a virtually continuous memory area this memory is physically located as spread 4 KiByte pages all over the physical memory. No problem for the user program as the memory management unit will simply translate the virtual continuous addresses to the physically spread pages totally transparent for the user program.

When using this virtual memory for a DMA transfer things become more complicated. The DMA engine of any hardware can only access physical addresses. As a result the DMA engine has to access each 4 KiByte page separately. This is done through the Scatter-Gather list. This list is simply a linked list of the physical page addresses which represent the user buffer. All translation and set-up of the Scatter-Gather list is done inside the driver without being seen by the user. Although the Scatter-Gather DMA transfer is an advanced and powerful technology it has one disadvantage: For each transferred memory page of data it is necessary to also load one Scatter-Gather entry (which is 16 bytes on 32 bit systems and 32 bytes on 64 bit systems). The little overhead to transfer (16/32 bytes in relation to 4096 bytes, being less than one percent) isn't critical but the fact that the continuous data transfer on the bus is broken up every 4096 bytes and some different addresses have to be accessed slows things down.

The solution is very simple: everything works faster if the user buffer is not only virtually continuous but also physically continuous. Unfortunately it is not possible to get a physically continuous buffer for a user program. Therefore the kernel driver has to do the job and the user program simply has to read out the address and the length of this continuous buffer. This is done with the function `spcm_dwGetContBuf` as already mentioned in the general driver description. The desired length of the continuous buffer has to be programmed to the kernel driver for load time and is done differently on the different operating systems. Please see the following chapters for more details.

Next we'll see some measuring results of the data transfer rate with/without continuous buffer. You will find more results on different motherboards and systems in the application note number 6 „Bus Transfer Speed Details“. Also with newer M5i/M4i/M4x/M2p cards the gain in speed is not as impressive, as it is for older cards, but can be useful in certain applications and settings. As this is also system dependent, your improvements may vary. This can not only depend on the system hardware but also on the used operating system, as in some cases Linux does seem to benefit more than Windows for newer cards.

Bus Transfer Speed Details (M2i/M3i cards in an example system)

Mode	PCI 33 MHz slot		PCI-X 66 MHz slot		PCI Express x1 slot	
	read	write	read	write	read	write
User buffer	109 MB/s	107 MB/s	195 MB/s	190 MB/s	130 MB/s	138 MB/s
Continuous kernel buffer	125 MB/s	122 MB/s	248 MB/s	238 MB/s	160 MB/s	170 MB/s
Speed advantage	15%	14%	27%	25%	24%	23%

Bus Transfer Standard Read/Write Transfer Speed Details (M4i.44xx card in an example system)

Mode	Notifysize 16 KiByte		Notifysize 64 KiByte		Notifysize 512 KiByte		Notifysize 2048 KiByte		Notifysize 4096 KiByte	
	read	write	read	write	read	write	read	write	read	write
User buffer	243 MB/s	132 MB/s	793 MB/s	464 MB/s	2271 MB/s	1352 MB/s	2007 MB/s	1900 MB/s	2687 MB/s	2284 MB/s
Continuous kernel buffer	239 MB/s	133 MB/s	788 MB/s	457 MB/s	2270 MB/s	1470 MB/s	2555 MB/s	2121 MB/s	2989 MB/s	2549 MB/s
Speed advantage	-1.6%	+0.7%	-0.6%	-1.5%	0%	+8.7%	+27.3%	+11.6%	+11.2%	+11.6%

Bus Transfer FIFO Read Transfer Speed Details (M4i.44xx card in an example system)

Mode	Notifysize 4 KiByte	Notifysize 8 KiByte	Notifysize 16 KiByte	Notifysize 32 KiByte	Notifysize 64 KiByte	Notifysize 256 KiByte	Notifysize 1024 KiByte	Notifysize 2048 KiByte	Notifysize 4096 KiByte
	FIFO read	FIFO read	FIFO read	FIFO read	FIFO read	FIFO read	FIFO read	FIFO read	FIFO read
User buffer	455 MB/s	858 MB/s	1794 MB/s	2005 MB/s	3335 MB/s	3386 MB/s	3369 MB/s	3331 MB/s	3335 MB/s
Continuous kernel buffer	540 MB/s	833 MB/s	1767 MB/s	1965 MB/s	3216 MB/s	3386 MB/s	3389 MB/s	3388 MB/s	3389 MB/s
Speed advantage	+18.6%	-2.9%	-1.5%	-2.0%	-3.5%	0%	+0.6%	+1.7%	+1.6%

Bus Transfer FIFO Read Transfer Speed Details (M2p.5942 card in an example system)

Mode	Notifysize 4 KiByte	Notifysize 8 KiByte	Notifysize 16 KiByte	Notifysize 32 KiByte	Notifysize 64 KiByte	Notifysize 256 KiByte	Notifysize 1024 KiByte	Notifysize 2048 KiByte	Notifysize 4096 KiByte
	FIFO read	FIFO read	FIFO read	FIFO read	FIFO read	FIFO read	FIFO read	FIFO read	FIFO read
User buffer	282 MB/s	462 MB/s	597 MB/s	800 MB/s	800 MB/s	799 MB/s	799 MB/s	799 MB/s	797 MB/s
Continuous kernel buffer	279 MB/s	590 MB/s	577 MB/s	800 MB/s	800 MB/s	800 MB/s	800 MB/s	800 MB/s	799 MB/s
Speed advantage	-1.1%	+27.7%	-3.4%	+0.0%	+0.0%	0%	+0.1%	+0.1%	+0.3%

Bus Transfer FIFO Read Transfer Speed Details (M5i.3337 card in an example system)

Mode	Notifysize 1024 KiByte	Notifysize 2048 KiByte	Notifysize 4096 KiByte
	FIFO read	FIFO read	FIFO read
User buffer	12.95 GB/s	13.26 GB/s	13.32 MB/s
Continuous buffer	13.02 GB/s	13.26 GB/s	13.39 GB/s
Windows 128 MiB			

Setup on Linux systems

On Linux systems the continuous buffer setting is done via the command line argument `contmem_mb` when loading the kernel driver module:

```
insmod spcm.ko contmem_mb=4
```

As memory allocation is organized completely different compared to Windows the amount of data that is available for a continuous DMA buffer is unfortunately limited to a maximum of 8 MiByte. On most systems it will even be only 4 MiBytes.

To use a larger continuous buffer you can use the Continuous Memory Allocator (CMA). To allocate continuous memory this way you pass „cma=xyz“ as kernel boot parameter, with xyz being the size of the continuous memory, e.g. „cma=128M“ for 128 MiByte.



Your kernel needs to have CMA support enabled to use this.

You can check this with „grep CONFIG_CMA /boot/config-\$(uname -r)“.

To enable CMA in our `spcm4` kernel driver module edit the Makefile for the kernel driver module and uncomment the line `#EXTRA_CFLAGS += -DSPCM4_USE_CMA` by removing the `#` in front. Then recompile the kernel module and load it as described above, like so as example:

```
insmod spcm4.ko contmem_mb=128
```



Using a continuous buffer of this size will need root privileges for the using program on most systems!

Setup on Windows systems

The continuous buffer settings is done with the Spectrum Control Center using a setup located on the „Support“ page. Please fill in the desired continuous buffer settings as MiByte. After setting up the value the system needs to be restarted as the allocation of the buffer is done during system boot time.

If the system cannot allocate the amount of memory it will divide the desired memory by two and try again. This will continue until the system can allocate a continuous buffer. Please note that this try and error routine will need several seconds for each failed allocation try during boot up procedure. During these tries the system will look like being crashed. It is then recommended to change the buffer settings to a smaller value to avoid the long waiting time during boot up.

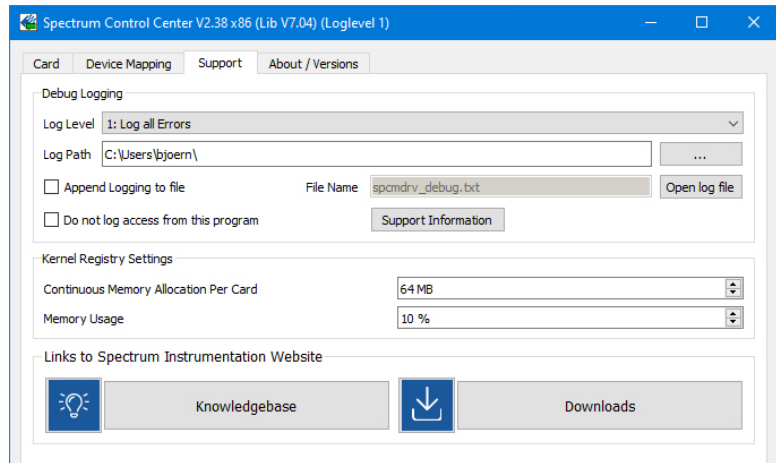


Image 95: setting up continuous memory buffer in Spectrum Control Center

Continuous buffer settings should not exceed 1/4 of system memory. During tests the maximum amount that could be allocated was 384 MiByte of continuous buffer on a system with 4 GiByte memory installed.

Usage of the buffer

The usage of the continuous memory is very simple. It is just necessary to read the start address of the continuous memory from the driver and use this address instead of a self allocated user buffer for data transfer.

Function `spcm_dwGetContBuf`

This function reads out the internal continuous memory buffer (in bytes) if one has been allocated. If no buffer has been allocated the function returns a size of zero and a NULL pointer.

```
uint32 _stdcall spcm_dwGetContBuf_i64 ( // Return value is an error code
    drv_handle hDevice,                // handle to an already opened device
    uint32 dwBufType,                  // type of the buffer to read as listed above under SPCM_BUF_XXXX
    void** ppvDataBuffer,              // address of available data buffer
    uint64* pqwContBufLen);            // length of available continuous buffer

uint32 _stdcall spcm_dwGetContBuf_i64m ( // Return value is an error code
    drv_handle hDevice,                // handle to an already opened device
    uint32 dwBufType,                  // type of the buffer to read as listed above under SPCM_BUF_XXXX
    void** ppvDataBuffer,              // address of available data buffer
    uint32* pdwContBufLenH,            // high part of length of available continuous buffer
    uint32* pdwContBufLenL);           // low part of length of available continuous buffer
```

Please note that it is not possible to free the continuous memory for the user application.

Example

The following example shows a simple standard single mode data acquisition setup (for a card with 12/14/16 bit per resolution one sample equals 2 bytes) with the read out of data afterwards. To keep this example simple there is no error checking implemented.

```
int32 lMemsize = 16384; // recording length is set to 16 KiSamples

spcm_dwSetParam_i64 (hDrv, SPC_CHENABLE, CHANNEL0); // only one channel activated
spcm_dwSetParam_i32 (hDrv, SPC_CARDMODE, SPC_REC_STD_SINGLE); // set the standard single recording mode
spcm_dwSetParam_i64 (hDrv, SPC_MEMSIZE, lMemsize); // recording length in samples
spcm_dwSetParam_i64 (hDrv, SPC_POSTTRIGGER, 8192); // samples to acquire after trigger = 8Ki
// now we start the acquisition and wait for the interrupt that signalizes the end
spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_CARD_START | M2CMD_CARD_ENABLETRIGGER | M2CMD_CARD_WAITREADY);

// we now try to use a continuous buffer for data transfer or allocate our own buffer in case there's none
spcm_dwGetContBuf_i64 (hDrv, SPCM_BUF_DATA, &pvData, &qwContBufLen);
if (qwContBufLen < (2 * lMemsize))
    pvData = pvAllocMemPageAligned (lMemsize * 2); // assuming 2 bytes per sample

// read out the data
spcm_dwDefTransfer_i64 (hDrv, SPCM_BUF_DATA, SPCM_DIR_CARDTOPC, 0, pvData, 0, 2 * lMemsize);
spcm_dwSetParam_i32 (hDrv, SPC_M2CMD, M2CMD_DATA_STARTDMA | M2CMD_DATA_WAITDMA);

// ... Use the data here for analysis/calculation/storage

// delete our own buffer in case we have created one
if (qwContBufLen < (2 * lMemsize))
    vFreeMemPageAligned (pvData, lMemsize * 2);
```

Abbreviations

Table 221: Abbreviations used throughout the Spectrum documents

Abbreviation	Long Name	Description
s	Second	
ms	Milli Second	1/1000 second; 1 ms is the time between two samples when running at 1 kS/s
us (µs)	Micro Second	1/1000000 second or 1/1000 milli second; 1 us is the time between two samples when running at 1 MS/s
ns	Nano Second	1/1000000000 second or 1/1000 micro second; 1 ns is the time between two samples when running at 1 GS/s
ps	Pico Second	1/1000000000000 second or 1/1000 nano second; 100 ps is the time between two samples when running at 10 GS/s
fs	Femto Second	1/1000000000000000 second or 1/1000 pico second
S	Sample	One sample represents one data word that has been acquired on the same time position. Each sample consist of either one byte (8 bit resolution) or two bytes (12, 14 and 16 bit resolution)
B	Byte	The smallest storage unit
Hz	Hertz	1 Hertz is one event/sample per second
PCIe	PCI Express	The PCI Express bus is a point to point connection allowing full speed for every single slot. The Express bus is freely scaling and is available with 1 lane (x1), 4 lanes (x4), 8 lanes (x8) and 16 lanes (x16)
PXI	PCI eXtensions for Instrumentation	Based on the CompactPCI 3U standard the PXI (PCI eXtensions for Instrumentation) enhancement was defined especially for the measurement user. In this specification additional lines for measurement purposes are defined.
PXIe	PXI Express	PXI Express or PXIe is a subset of the PXI standard that replaces PXI's parallel data bus with a high speed serial interface.
AWG	Arbitrary Waveform Generator	A method of producing arbitrary shaped waveforms by replaying a stream of digital samples and performing a digital-to-analog conversion.
DDS	Direct Digital Synthesis	A method of producing an analog waveform, typically a sine wave, by generating a time-varying signal in digital form and then performing a digital-to-analog conversion.
PLL	Phase Lock Loop	A clock device which generates a new clock phase-locked to a given reference clock.
LED	Light-Emitting Diode	A semiconductor device that emits light and is often used as a status light or indicator.
API	Application Programming Interface	A type of software interface, offering a service to access/control specific hardware or other pieces of software.
CPU	Central Processing Unit	The central processor of a computer/PC system.
GPU	Graphics Processing Unit	An co-processor specifically tailored for fast and efficient and massively parallel calculations of certain data structures. Often, but not exclusively, located on a separate PCIe graphics card or co-processing card. s
CUDA	Compute Unified Device Architecture	A proprietary API for Nvidia GPUs to perform "general purpose" as in non-graphic related processing on GPUs rather than the CPU.
DMA	Direct Memory Access	A method to transfer data directly between a device (card) and PC memory.
RDMA	Remote Direct Memory Access	A method to transfer data directly between two devices (cards).
RMA	Return Manufacturer Authorization	
WEEE	Waste Electrical and Electronic Equipment)	
Prefixed:		
k	Kilo	1000 (10 ³) e.g. kHz = 1000 Hertz
M	Mega	1000000 (10 ⁶)
G	Giga	1000000000 (10 ⁹)
T	Tera	1000000000000 (10 ¹²)
Ki	Kibi	1024 (2 ¹⁰) e.g. 1 KiB = 1024 Byte
Mi	Mebi	1024 x 1024 (2 ²⁰) e.g. 1 MiB = 1024 KiB
Gi	Gibi	1024 x 1024 x 1024 (2 ³⁰) e.g. 1 GiB = 1024 MiB
Ti	Tebi	1024 x 1024 x 1024 x 1024 (2 ⁴⁰) e.g. 1 TiB = 1024 GiB

List Of Figures

Image 1: M4i card showing mounted star-hub and sync bus connector.....	18
Image 2: M4i card showing mounted digital option.....	18
Image 3: M4i card backside showing type plate location and content.....	19
Image 4: Mounting M4i PCIe card into connector.....	30
Image 5: M4i card slot retention with perforation.....	31
Image 6: M4i card additional power connection usage.....	31
Image 7: M4i card with digital option mechanical installation and position of screws.....	32
Image 8: M4i cards with star-hub ex installed and connecting cables.....	32
Image 9: Installation of PXle cards with connector handling and mounting screws.....	33
Image 10: Windows Device Manager showing a new Spectrum card.....	34
Image 11: Spectrum Driver Installer Welcome Screen.....	34
Image 12: Spectrum Driver Installer - Progress.....	35
Image 13: Spectrum Driver Installer - finished.....	35
Image 14: Windows Device Manager showing properly installed Spectrum card.....	35
Image 15: Device Manager showing a new Spectrum card.....	39
Image 16: Spectrum Kernel Driver, API Library and Software structure.....	41
Image 17: Spectrum Control Center Installer.....	41
Image 18: Spectrum Control Center showing detail card information.....	42
Image 19: Spectrum Control Center - entering an IP address for a NETBOX.....	42
Image 20: Spectrum Control Center: wake on LAN for a cached card.....	42
Image 21: Netbox Monitor activation.....	43
Image 22: Device Identification.....	43
Image 23: Spectrum Control Center: detailed hardware information on installed card.....	44
Image 24: Spectrum Control Center - showing firmware information of an installed card.....	44
Image 25: Spectrum Control Center - showing software license information of an installed card.....	45
Image 26: Spectrum Control Center - showing driver information details.....	45
Image 27: Spectrum Control Center - adding a demo card to the system.....	46
Image 28: Spectrum Control Center - feature update, code entry.....	46
Image 29: Spectrum Control Center - software license install.....	46
Image 30: Spectrum Control Center - running an on-board calibration.....	46
Image 31: Spectrum Control Center - performing memory test.....	47
Image 32: Spectrum Control Center - running a transfer speed test of one card.....	47
Image 33: Spectrum Control Center - activate debug logging for support cases.....	48
Image 34: Spectrum Control Center - using device mapping.....	48
Image 35: Spectrum Control Center - doing a firmware update for one device.....	49
Image 36: Spectrum Control Center - selecting a firmware configuration for one card.....	49
Image 37: SBench 6 overview of main functionality with demo data.....	50
Image 38: SBench 6 overview of main functionality with demo data.....	51
Image 39: Structure of the Delphi examples.....	60
Image 40: LabVIEW driver oscilloscope example.....	67
Image 41: Spectrum MATLAB driver structure.....	67
Image 42: GPU usage with SCAPP SDK: data transfer options.....	68
Image 43: Spectrum API: using the input offset shifting to optimize the usage of the input range.....	81
Image 44: Spectrum API: effects of different input offset setting.....	82
Image 45: Spectrum API: input offset registers and available register settings.....	82
Image 46: Acquisition cards: graphical overview of acquisition status and card command interaction.....	88
Image 47: Generation cards: graphical overview of generation status and card command interaction.....	88
Image 48: standard acquisition mode and pretrigger/posttrigger/trigger relation.....	91
Image 49: Overview of buffer handling for DMA transfers showing and the interaction with the DMA engine.....	94
Image 50: M4i/M4x clock section overview.....	100
Image 51: Trigger Engine Overview. Red marked parts not available on all card types.....	105
Image 52: trigger engine overview with trigger OR mask shown.....	106
Image 53: trigger engine OR mask details.....	106
Image 54: trigger engine overview with trigger AND mask shown.....	107
Image 55: trigger engine AND mask details.....	107
Image 56: trigger engine overview with marked trigger delay stage.....	110
Image 57: trigger engine overview with marked main external trigger Ext0/Trg0.....	111
Image 58: trigger engine overview with external trigger Ext1 marked.....	112
Image 59: trigger engine overview with channel trigger section marked.....	117
Image 60: trigger overview with multi-purpose lines marked.....	129
Image 61: Drawing of Multiple Recording acquisition.....	132
Image 62: drawing of Multiple Recording Acquisition with Timestamps.....	134
Image 63: Drawing of Gated Sampling mode.....	136
Image 64: Drawing of Gated Sampling mode and Timestamp positions.....	138
Image 65: drawing of timestamp acquisition in standard mode in relation to card start and trigger detection.....	150
Image 66: drawing of timestamp acquisition in start-reset mode in relation to card start and trigger detection.....	150
Image 67: drawing of timestamp acquisition in refclock mode in relation to card start and trigger detection.....	151
Image 68: Overview of acquisition data, ABA data and timestamp data DMA transfer.....	152
Image 69: drawing of Multiple Recording Acquisition with Timestamps.....	157
Image 70: Drawing of Gated Sampling mode and Timestamp positions.....	158

Image 71: Drawing of ABA mode.....	159
Image 72: overview of ABA mode data acquisition with slow A-data and fast B-data	160
Image 73: Overview of acquisition data, ABA data and timestamp data DMA transfer	163
Image 74: Drawing of ABA mode.....	166
Image 75: Overview of remote server option interaction in comparison to NETBOX devices.....	168
Image 76: Windows screenshot: finding a remote Spectrum device like digitizerNETBOX	169
Image 77: overview block diagram of multi-purpose I/O lines and pulse generators	171
Image 78: overview block diagram of the pulse generator	172
Image 79: timing diagram illustrating the basic pulse parameters	173
Image 80: timing diagram illustrating delaying a pulse generator output	174
Image 81: timing diagram illustrating the pulse generator triggered output mode.....	175
Image 82: timing diagram illustrating the pulse generator single-shot triggered output mode	175
Image 83: timing diagram illustrating the pulse generator gated output mode	175
Image 84: block average FPGA option block diagram	185
Image 85: block average FPGA option - principle of operation.....	185
Image 86: simplified block diagram of FPGA structure with signal processing firmware block	186
Image 87: timing diagram of block average acquisition	186
Image 89: Overview of waveform block statistics information results	190
Image 88: block statistics FPGA option block diagram	190
Image 90: simplified block diagram of FPGA structure with signal processing firmware block	191
Image 91: timing diagram of block statistics acquisition.....	191
Image 92: electrical structure of multi-purpose I/O lines.....	198
Image 93: electrical structure of clock inputs and potential interfacing circuits.....	198
Image 94: electrical structure of clock outputs and potential interfacing circuits.....	198
Image 95: setting up continuous memory buffer in Spectrum Control Center	203

List Of Tables

Table 1: Symbols and Safety Labels	10
Table 2: Packing List M4i card (PCI Express)	13
Table 3: Packing List M4x card (PXI Express)	13
Table 4: list of C/C++ header files in driver	52
Table 5: C/C++ type declarations for drivers and examples	54
Table 6: C/C++ type naming convention throughout drivers and examples	54
Table 7: Spectrum driver API functions overview and differentiation between 32 bit and 64 bit registers	56
Table 8: Spectrum API: Command register and basic commands	69
Table 9: Spectrum API: Card Type Register	72
Table 10: Spectrum API: hardware and PCB version register overview	72
Table 11: Spectrum API: extension module hardware and PCB version register	73
Table 12: Spectrum API: register for reading back the PXIe card slot number	73
Table 13: Spectrum API: Register overview of firmware versions	73
Table 14: Spectrum API: Register overview of reading current firmware	73
Table 15: Spectrum API: production date register	74
Table 16: Spectrum API: calibration date register	74
Table 17: Spectrum API: hardware serial number register	74
Table 18: Spectrum API: maximum sampling rate register	74
Table 19: Spectrum API: installed memory registers	75
Table 20: Spectrum API: Feature Register and available feature flags	75
Table 21: Spectrum API: Extended feature register and available extended feature flags	76
Table 22: Spectrum API: register overview of miscellaneous cards information	76
Table 23: Spectrum API: register card function type and possible types	76
Table 24: Spectrum API: register driver type information and possible driver types	76
Table 25: Spectrum API: driver version read register	77
Table 26: Spectrum API: kernel driver version read register	77
Table 27: Spectrum API: custom modification register and different bitmasks to split the register in various hardware parts	77
Table 28: Spectrum API: command register and reset command	77
Table 29: Spectrum API: channel enable register and register settings	79
Table 30: Spectrum API: channel count register	79
Table 31: Spectrum API: registers for reading the installed input ranges from card EEPROM	80
Table 32: Spectrum API: input range settings register and available vales depending on installed low-voltage option	81
Table 33: Spectrum API: AC/DC compensation register for offset settings with an AC coupled signal	82
Table 34: Spectrum API: register to read the analog input features and the meaning of the feature flags	82
Table 35: Spectrum API: AC/DC setup registers and available register settings	83
Table 36: Spectrum API: anti-aliasing filter setup register	83
Table 37: Spectrum API: automatic offset compensation register and valid register settings	84
Table 38: Spectrum API: loading and storing calibration values to the EEPROM	84
Table 39: Spectrum API: read out when last on-board calibration has been engaged	84
Table 40: Spectrum API: card mode and read out of available card mode software registers	85
Table 41: Spectrum API: possible values for the card mode register. Description of the different card modes	86
Table 42: Spectrum API: card command register and different commands with descriptions	86
Table 43: Spectrum API: timeout definition register	87
Table 44: Spectrum API: card status register and possible status values with descriptions of the status	88
Table 45: Spectrum API: memory test register	90
Table 46: Spectrum API: Command register and commands for DMA transfers	90
Table 47: Spectrum API: status register and status codes for DMA data transfer	90
Table 48: Spectrum API: card mode register and standard single mode setup	91
Table 49: Spectrum API: memory size and posttrigger registers for standard single mode	91
Table 50: Spectrum API: card mode register and standard FIFO mode setup	92
Table 51: Spectrum API: setup registers for standard FIFO mode	92
Table 52: Spectrum API: Limits of pre trigger, post trigger and memory size	93
Table 53: Spectrum API: registers for DMA buffer handling	94
Table 54: Spectrum API: content of DMA buffer handling registers for different use cases	95
Table 55: M4i and M4x cards data organization	98
Table 56: Spectrum API: data conversion registers and valid register settings	99
Table 57: Spectrum API: clock mode register and available clock modes	100
Table 58: Spectrum API: samplerate register	101
Table 59: Spectrum API: clock mode register and internal clock mode	101
Table 60: Spectrum API: clock output and clock output frequency register	101
Table 61: Spectrum API: clock mode register and quartz 2 settings	102
Table 62: Spectrum API: clock output and clock output frequency register	102
Table 63: Spectrum API: clock oversampling readout register	102
Table 64: Spectrum API: clock mode register and external reference clock setup	102
Table 65: Spectrum API: reference clock register and available settings	102
Table 66: Spectrum API: clock output and clock output frequency register	103
Table 67: Spectrum API: clock mode register and PXI reference clock usage	103
Table 68: Spectrum API: general trigger OR mask register and available settings	106
Table 69: Spectrum API: channel trigger OR mask registers and available settings	107
Table 70: Spectrum API: general trigger AND mask registers and available settings	108

Table 71: Spectrum API: channel trigger AND mask registers and available settings	108
Table 72: Spectrum API: software register and register setting for software trigger	109
Table 73: Spectrum API: command register and force trigger command	109
Table 74: Spectrum API: command register and trigger enable/disable command	109
Table 75: Spectrum API: trigger delay registers and available settings	110
Table 76: Spectrum API: trigger counter register and register return values	110
Table 77: Spectrum API: external trigger Ext0 registers and register settings	111
Table 78: Spectrum API: external trigger Ext0 OR mask settings	111
Table 79: Spectrum API: external trigger Ext0 input termination	111
Table 80: Spectrum API: external trigger Ext0 input coupling	112
Table 81: Spectrum API: external trigger Ext1 registers and register settings	112
Table 82: Spectrum API: external trigger Ext1 OR mask settings	112
Table 83: Spectrum API: external trigger available settings for trigger levels	112
Table 84: Spectrum API: external trigger OR mask and AND mask register and settings	113
Table 85: Spectrum API: external register mode setup for trigger on positive edge	113
Table 86: Spectrum API: external register mode setup for trigger on negative edge	113
Table 87: Spectrum API: external trigger register mode setup for trigger on positive and negative edge	114
Table 88: Spectrum API: external trigger register mode setup for trigger re-arm on positive edge	114
Table 89: Spectrum API: external trigger register mode setup for trigger re-arm on negative edge	114
Table 90: Spectrum API: external trigger register mode setup for window trigger for entering signals	115
Table 91: Spectrum API: external trigger register mode setup for window trigger for leaving signals	115
Table 92: Spectrum API: external trigger register mode setup for high level trigger	115
Table 93: Spectrum API: external trigger register mode setup for low level trigger	116
Table 94: Spectrum API: external trigger register mode setup for in window trigger	116
Table 95: Spectrum API: external trigger register mode setup for outside window trigger	116
Table 96: Spectrum API: channel trigger OR mask register	117
Table 97: Spectrum API: channel trigger mode registers and available mode settings	117
Table 98: Spectrum API: trigger level count register	119
Table 99: Spectrum API: channel trigger OR mask register	119
Table 100: Spectrum API: channel trigger register settings for positive edge trigger	119
Table 101: Spectrum API: channel trigger register settings for negative edge trigger	119
Table 102: Spectrum API: channel trigger register settings for positive and negative edge trigger	120
Table 103: Spectrum API: channel trigger register settings for re-arm trigger on positive edge	120
Table 104: Spectrum API: channel trigger register settings for re-arm trigger on negative edge	120
Table 105: Spectrum API: channel trigger register settings for window trigger for entering signals	121
Table 106: Spectrum API: channel trigger register settings for window trigger for leaving signals	121
Table 107: Spectrum API: channel trigger register settings for high level trigger	121
Table 108: Spectrum API: channel trigger register settings for low level trigger	122
Table 109: Spectrum API: channel trigger register settings for in-window trigger	122
Table 110: Spectrum API: channel trigger register settings for outside-window trigger	122
Table 111: Spectrum API: register settings for channel hysteresis trigger on positive edge	123
Table 112: Spectrum API: register settings for channel hysteresis trigger on negative edge	123
Table 113: Spectrum API: register settings for channel hysteresis re-arm trigger on positive edge	123
Table 114: Spectrum API: register settings for channel hysteresis re-arm trigger on negative edge	124
Table 115: Spectrum API: register settings for high-level channel hysteresis trigger	124
Table 116: Spectrum API: register settings for low-level channel hysteresis trigger	124
Table 117: trigger overview with PXI trigger lines marked	126
Table 118: Spectrum API: PXI trigger register and available register settings	126
Table 119: Spectrum API: PXI trigger mask register and available register settings	127
Table 120: Spectrum API: multi-purpose I/O lines registers and available register settings	129
Table 121: Spectrum API: asynchronous I/O register settings of the multi-purpose I/O registers	130
Table 122: Spectrum API: additional trigger output register for compatibility with older hardware	130
Table 123: Spectrum API: software registers for Multiple Recording mode setup	132
Table 124: Spectrum API: card mode register and multiple recording settings	132
Table 125: Spectrum API: memory and loop registers with related multiple recording settings	132
Table 126: Spectrum API: card mode register and multiple replay FIFO mode settings	132
Table 127: Spectrum API: loops register settings when using Multiple Replay FIFO mode	133
Table 128: Spectrum API: Limits of pre trigger, post trigger and memory size	133
Table 129: Spectrum API: registers and settings for Gated Sampling mode	136
Table 130: Spectrum API: card mode register and settings for Gated Sampling standard mode	136
Table 131: Spectrum API: memsize and loops register and register settings for Gated Replay mode	136
Table 132: Spectrum API: card mode register and Gated Sampling FIFO mode settings	136
Table 133: Spectrum API: Gated Sampling FIFO mode loops register settings	136
Table 134: Spectrum API: Limits of pre trigger, post trigger and memory size	137
Table 135: Spectrum API: gate end alignment in Gated Sampling mode	138
Table 136: Spectrum API: reading out the Gated Sampling or Gated Replay gate-end alignment value	138
Table 137: Spectrum API: trigger mask registers and available register settings	139
Table 138: Spectrum API: trigger register settings for trigger on positive edge	139
Table 139: Spectrum API: trigger register settings for trigger on negative edge	139
Table 140: Spectrum API: trigger register settings for re-arm trigger on positive edge	140
Table 141: Spectrum API: trigger register settings for re-arm trigger on negative edge	140
Table 142: Spectrum API: trigger register settings for window trigger on entering signals	140

Table 143: Spectrum API: trigger register settings for window trigger on leaving signals.....	141
Table 144: Spectrum API: trigger register settings for high-level trigger	141
Table 145: Spectrum API: trigger register settings for low-level trigger	141
Table 146: Spectrum API: trigger register settings for in-window trigger	142
Table 147: Spectrum API: trigger register settings for outside-window trigger	142
Table 148: Spectrum API: channel trigger OR mask register	143
Table 149: Spectrum API: trigger register mode and level setup for trigger on positive edge	143
Table 150: Spectrum API: trigger register mode and level setup for trigger on high level	143
Table 151: Spectrum API: trigger register mode and level setup for trigger on negative edge	143
Table 152: Spectrum API: trigger register mode and level setup for trigger on low level.....	144
Table 153: Spectrum API: trigger register mode and level setup for trigger on positive edge with re-arm level	144
Table 154: Spectrum API: trigger register mode and level setup for trigger on negative edge with re-arm level	144
Table 155: Spectrum API: trigger register mode and level setup for trigger on signal entering window	145
Table 156: Spectrum API: trigger register mode and level setup for trigger on signal leaving window	145
Table 157: Spectrum API: trigger register mode and level setup for trigger on signal inside window	145
Table 158: Spectrum API: trigger register mode and level setup for trigger on signal outside window	146
Table 159: Spectrum API: trigger register mode and level setup for trigger on positive edge with hysteresis	146
Table 160: Spectrum API: trigger register mode and level setup for trigger on high level with hysteresis	146
Table 161: Spectrum API: trigger register mode and level setup for trigger on negative edge with hysteresis	147
Table 162: Spectrum API: trigger register mode and level setup for trigger on low level with hysteresis	147
Table 163: Spectrum API: trigger register mode and level setup for trigger on positive edge with re-arm level and hysteresis	147
Table 164: Spectrum API: trigger register mode and level setup for trigger on negative edge with re-arm level and hysteresis	148
Table 165: Spectrum API: timestamp related register and available timestamp commands	149
Table 166: Spectrum API: timestamp commands for standard mode	150
Table 167: Spectrum API: timestamp commands for star-reset mode	151
Table 168: Spectrum API: timestamp commands for refclock mode	151
Table 169: Spectrum API: extra DMA commands (ABA and Timestamp)	152
Table 170: Spectrum API: extra DMA status (ABA and Timestamp)	153
Table 171: Spectrum API: ABA and Timestamp DMA buffer handling registers	153
Table 172: Spectrum API: timestamp sample format for standard mode	155
Table 173: Spectrum API: timestamp sample format for extended mode	156
Table 174: Spectrum API: timestamp extra data word format	156
Table 175: Spectrum API: timestamp data format register	156
Table 176: Spectrum API: gate end alignment in Gated Sampling mode	157
Table 177: Spectrum API: reading out the Gated Sampling or Gated Replay gate-end alignment value	158
Table 178: Spectrum API: timestamp command register and ABA mode settings	159
Table 179: Spectrum API: ABA mode relevant registers and register settings	160
Table 180: Spectrum API: card mode programming register and setup for ABA mode	161
Table 181: Spectrum API: memory size register and available register settings	161
Table 182: Spectrum API: card mode programming register and setup for ABA FIFO mode	161
Table 183: Spectrum API: loops programming register and available register settings	161
Table 184: Spectrum API: Limits of pre trigger, post trigger and memory size	161
Table 185: Spectrum API: extra DMA commands (ABA and Timestamp)	163
Table 186: Spectrum API: extra DMA status (ABA and Timestamp)	163
Table 187: Spectrum API: ABA and Timestamp DMA buffer handling registers	164
Table 188: Spectrum API: timestamp command register and ABA mode settings	166
Table 189: Spectrum API: pulse generator clock frequency read register	172
Table 190: Spectrum API: pulse generator enable registers	173
Table 191: Spectrum API: pulse generator length/period register	173
Table 192: Spectrum API: pulse generator HIGH time registers	173
Table 193: Spectrum API: pulse generator loops/pulse repetition registers	174
Table 194: Spectrum API: pulse generator delay/phase shift registers	174
Table 195: Spectrum API: pulse generator mode registers with their available settings	174
Table 196: Spectrum API: pulse generator trigger MUX1 registers with their available settings	175
Table 197: Spectrum API: pulse generator trigger MUX2 registers with their available settings	176
Table 198: Spectrum API: pulse generator command register for trigger forcing by software	176
Table 199: Spectrum API: pulse generator additional configuration registers with the available settings	176
Table 200: Spectrum API: XIO lines and mode software registers with their reduced to the settings required for outputting pulses	177
Table 201: star-hub clock overview diagram	179
Table 202: Spectrum API: star-hub related registers for reading detected connections	180
Table 203: Spectrum API: synchronization enable mask register	181
Table 204: Spectrum API: star-hub synchronization commands	182
Table 205: Spectrum API: clock mode register and settings for SH Direct mode	183
Table 206: Spectrum API: software registers and register settings for programming the block average mode	186
Table 207: Spectrum API: card mode registers and register settings for standard lock average mode	187
Table 208: Spectrum API: card mode registers and register settings for FIFO block average mode	187
Table 209: Spectrum API: block average mode loop register and register settings	187
Table 210: Spectrum API: block average mode output sample format	188
Table 211: Spectrum API: block average mode data organization	189
Table 212: Spectrum API: software registers and register settings for programming the block statistics mode	191
Table 213: Spectrum API: card mode registers and register settings for standard block statistics mode	192
Table 214: Spectrum API: card mode registers and register settings for FIFO block statistics mode	192

Table 215: Spectrum API: block statistics mode loop register and register settings.....	192
Table 216: Spectrum API: block statistics mode data organization	193
Table 217: Spectrum API: driver error codes and error description	195
Table 218: Spectrum API: temperature read-out registers of internal temperature sensors	197
Table 219: card status LED color and blink coding.....	200
Table 220: Spectrum API: card identification LED register	200
Table 221: Abbreviations used throughout the Spectrum documents.....	204



Spectrum Instrumentation GmbH

Ahrensfelder Weg 13-17 | 22927 Grosshansdorf | Germany

Phone +49 (0)4102-69 56-0 | Fax +49 (0)4102-69 56-66

info@spec.de



Spectrum Instrumentation Corp

401 Hackensack Ave, 4th Floor | Hackensack, NJ 07601 | USA

Phone +1 (201) 562-1999 | Fax +1 (201) 342-7598

sales@spectrum-instrumentation.com



spectrum-instrumentation.com